

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP103125\
 Data File : PP076248.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2025 13:21
 Operator : YP\AJ
 Sample : Q3500-01 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 459

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 11/03/2025
 Supervised By :Yogesh Patel 11/03/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 23:19:49 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 24 15:40:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.641	3.771	3501274	23222638	2.450m	3.509m#
2)	SA Decachlor...	10.431	8.788	2928811	6740521	2.721m	0.820 #
Target Compounds							
26)	L6 AR-1254-1	6.649	0.000	2791013	0	34.934	N.D. d#
27)	L6 AR-1254-2	6.866	0.000	1835580	0	18.359	N.D. d#
28)	L6 AR-1254-3	7.229	0.000	2016576	0	19.399	N.D. d#
29)	L6 AR-1254-4	7.512	0.000	1319847	0	15.785	N.D. d#
30)	L6 AR-1254-5	7.927	0.000	3060313	0	33.420	N.D. d#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP103125\
Data File : PP076248.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2025 13:21
Operator : YP\AJ
Sample : Q3500-01 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
459


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/03/2025
Supervised By :Yogesh Patel 11/03/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 23:19:49 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 24 15:40:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

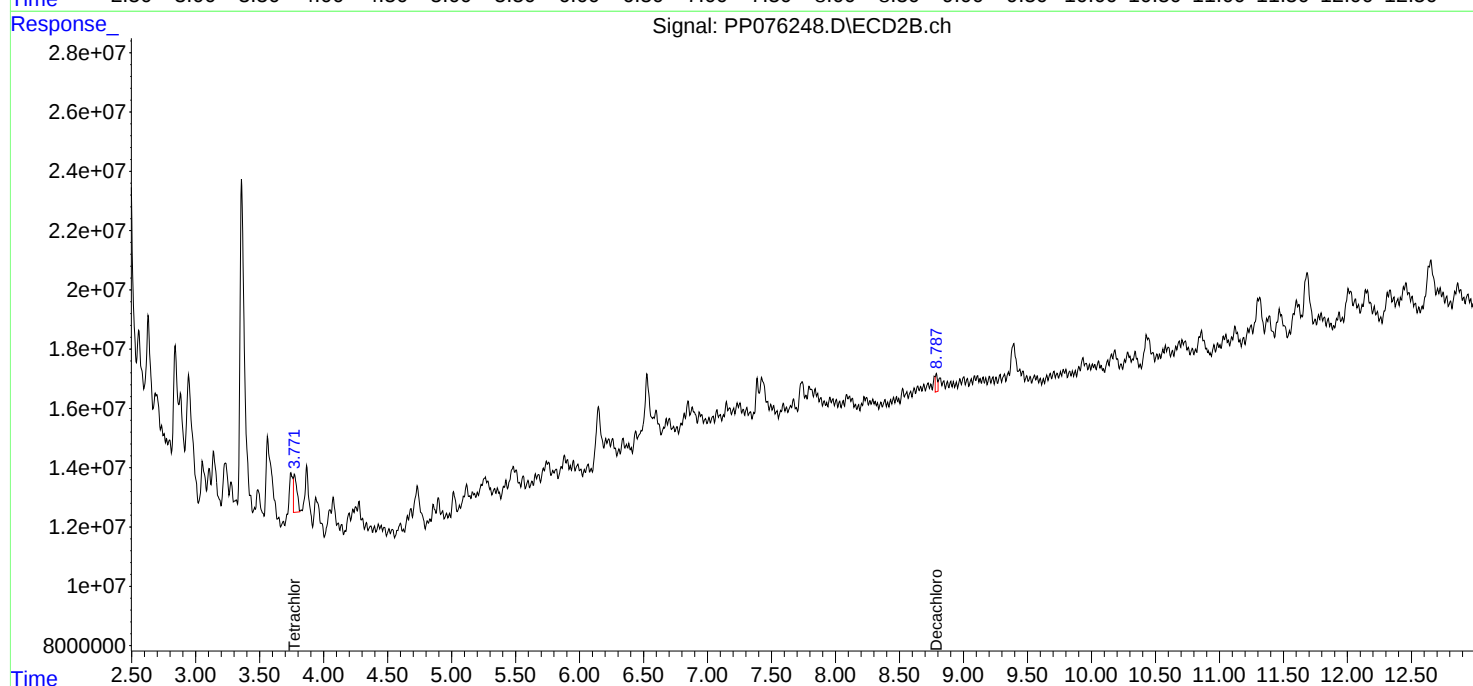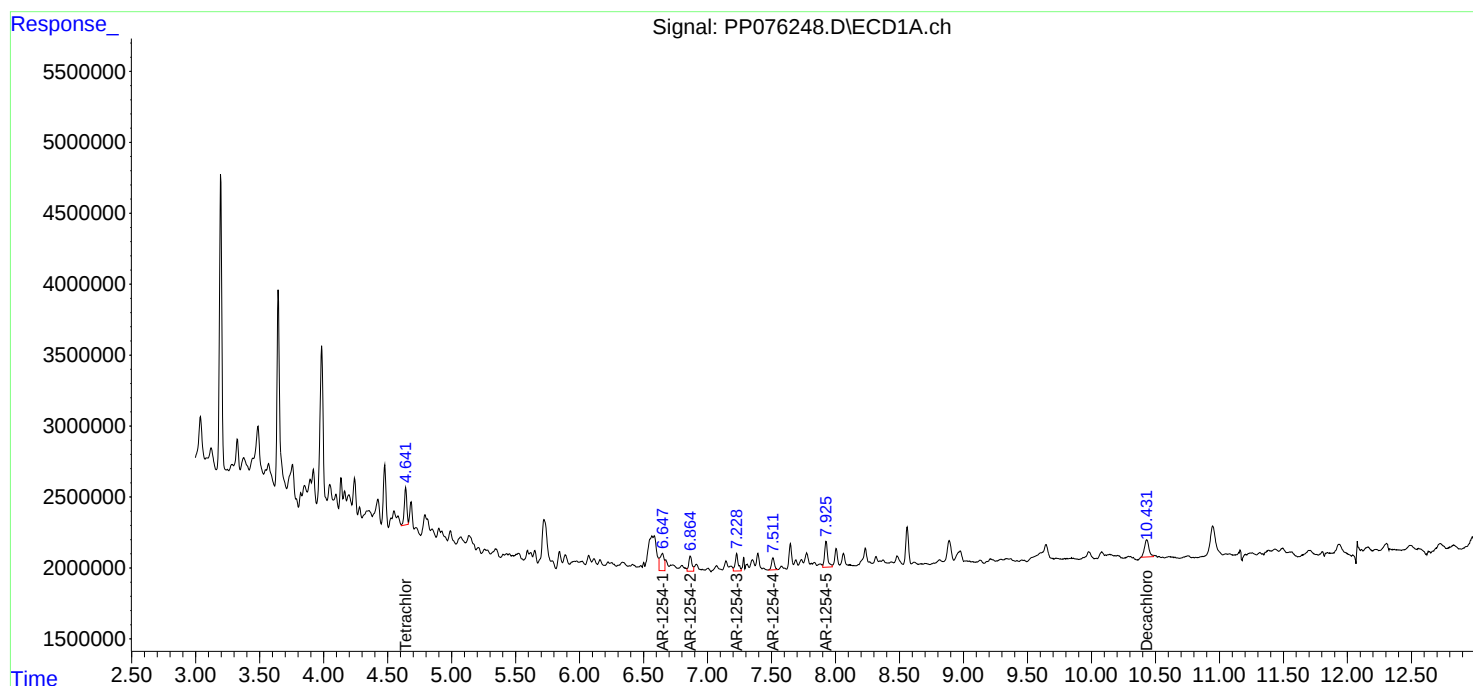

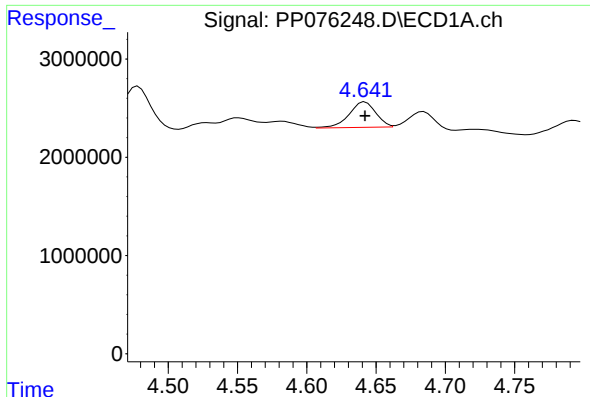


#1 Tetrachloro-m-xylene

R.T.: 4.641 min
Delta R.T.: -0.001 min
Response: 3501274
Conc: 2.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
459


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/03/2025
Supervised By :Yogesh Patel 11/03/2025

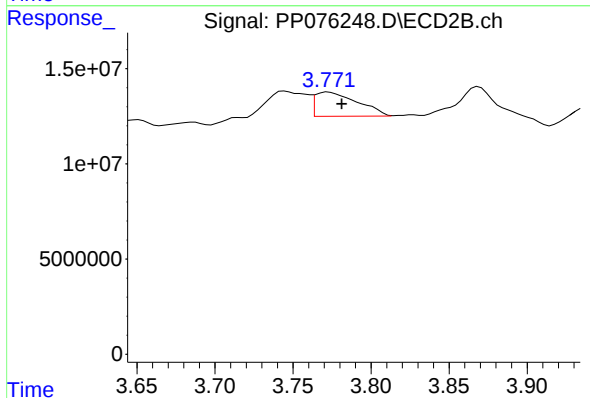


#1 Tetrachloro-m-xylene

R.T.: 3.771 min
Delta R.T.: -0.010 min
Response: 23222638
Conc: 3.51 ng/ml m

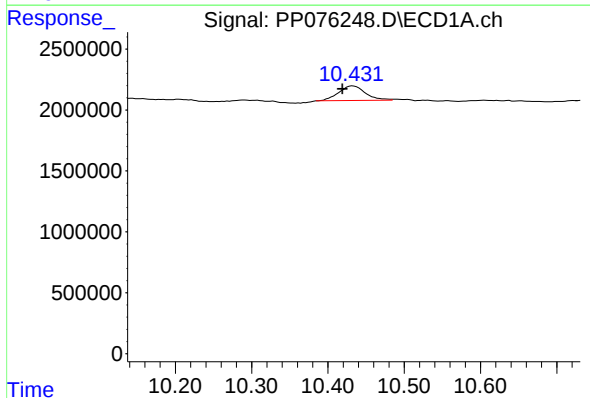

#2 Decachlorobiphenyl

R.T.: 10.431 min
Delta R.T.: 0.012 min
Response: 2928811
Conc: 2.72 ng/ml m

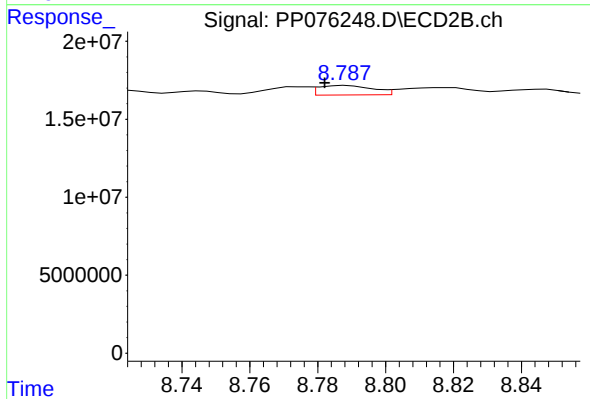

#2 Decachlorobiphenyl

R.T.: 8.788 min
Delta R.T.: 0.006 min
Response: 6740521
Conc: 0.82 ng/ml