

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110120\
 Data File : PP031008.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Oct 2020 15:40
 Operator : DD\AJ
 Sample : MDL-AR1262-S-2
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-AR1262-S-2

Manual Integrations
 APPROVED

Ankita
 11/2/2020 3:00:06 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 02:43:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\AR1262PP110120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 31 02:26:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.802	4.079	1042816	905177	16.346	15.669
2)	SA Decachlor...	10.690	9.411	620661	667701	16.713	16.886
Target Compounds							
36)	L8 AR-1262-1	8.420	7.509	52150	54829	22.219	21.001
37)	L8 AR-1262-2	8.964	8.019	86486	93652	20.421	19.886
38)	L8 AR-1262-3	9.265	8.307	62217	38892	20.832	19.584m
39)	L8 AR-1262-4	9.350	8.369	44677	75184	18.271m	20.791
40)	L8 AR-1262-5	9.980	8.867	23888	31733	15.273	19.257 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110120\
Data File : PP031008.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Oct 2020 15:40
Operator : DD\AJ
Sample : MDL-AR1262-S-2
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
MDL-AR1262-S-2


Manual Integrations
APPROVED

Ankita
11/2/2020 3:00:06 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 02:43:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\AR1262PP110120.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 31 02:26:29 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

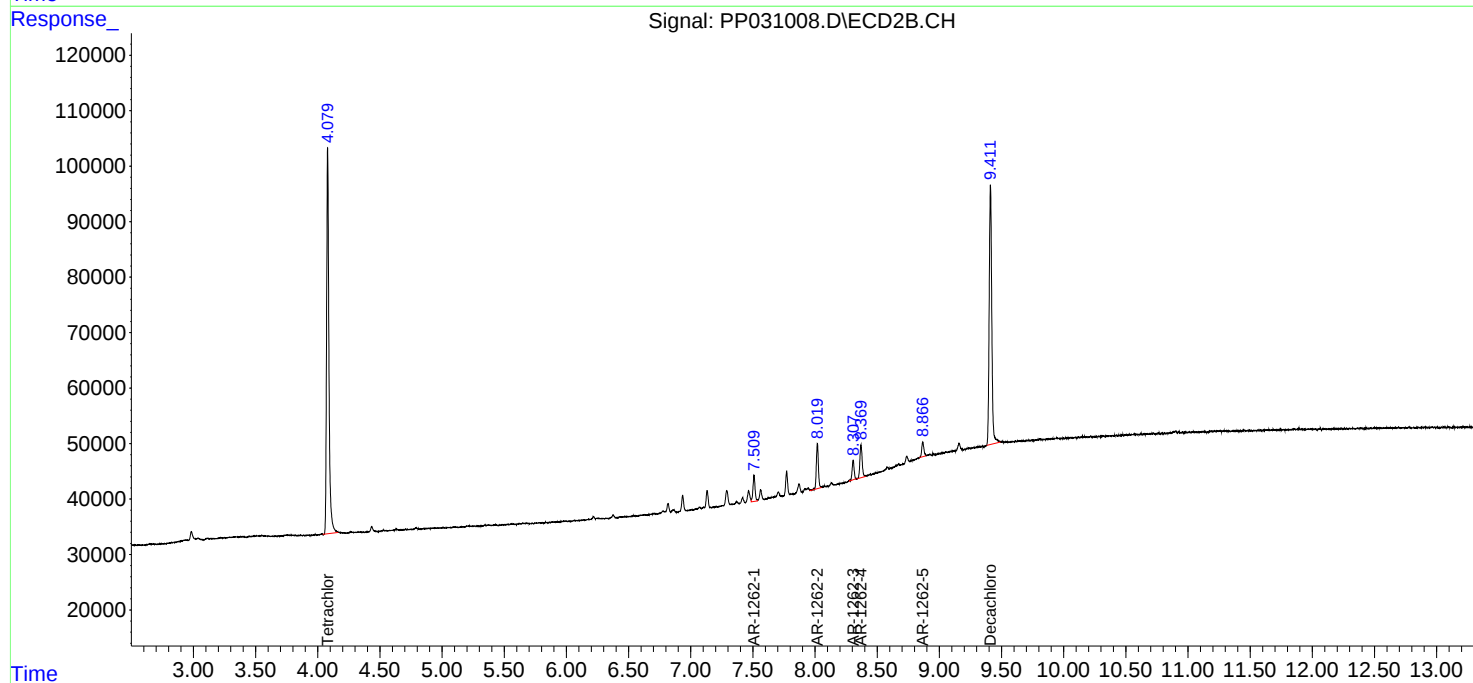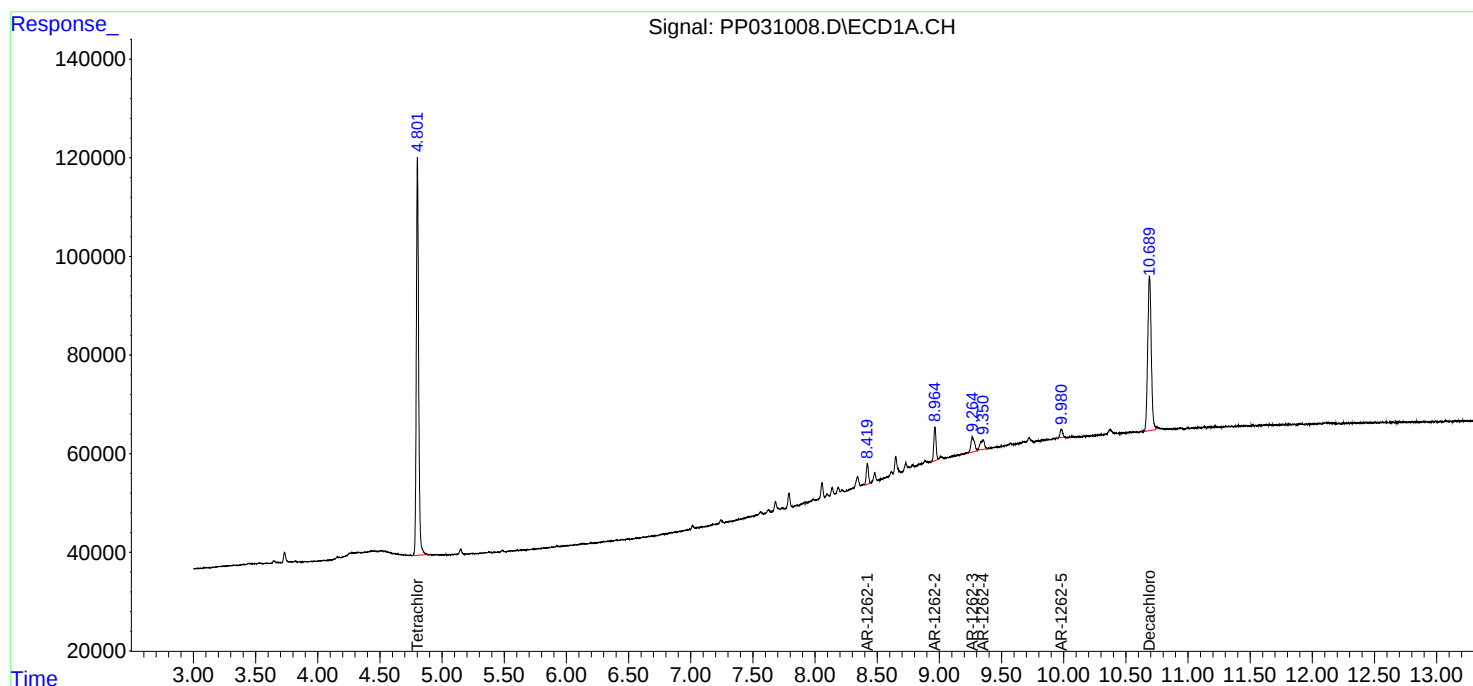

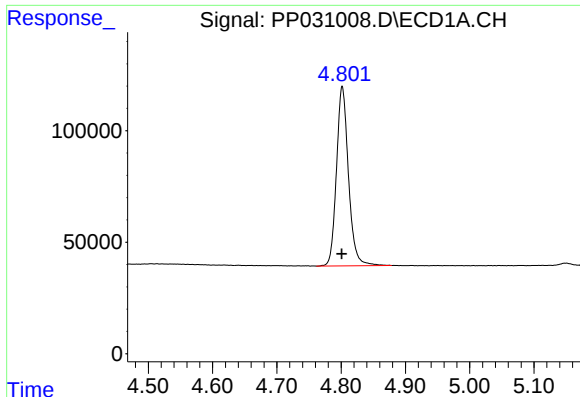


#1 Tetrachloro-m-xylene

R.T.: 4.802 min
Delta R.T.: 0.000 min
Response: 1042816
Conc: 16.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-AR1262-S-2


Manual Integrations
APPROVED

Ankita
11/2/2020 3:00:06 PM

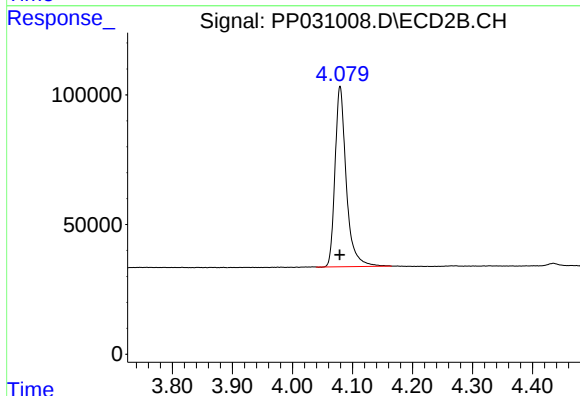


#1 Tetrachloro-m-xylene

R.T.: 4.079 min
Delta R.T.: 0.000 min
Response: 905177
Conc: 15.67 ng/ml

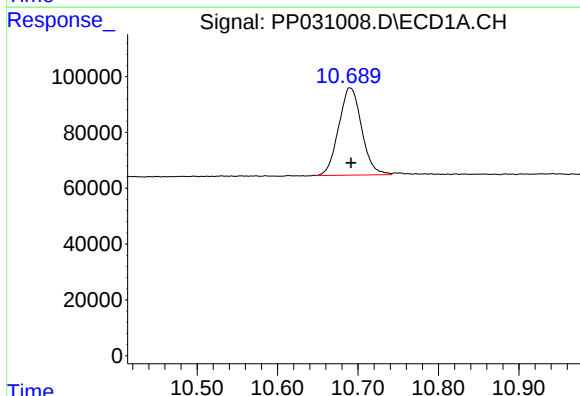


#2 Decachlorobiphenyl

R.T.: 10.690 min
Delta R.T.: -0.002 min
Response: 620661
Conc: 16.71 ng/ml

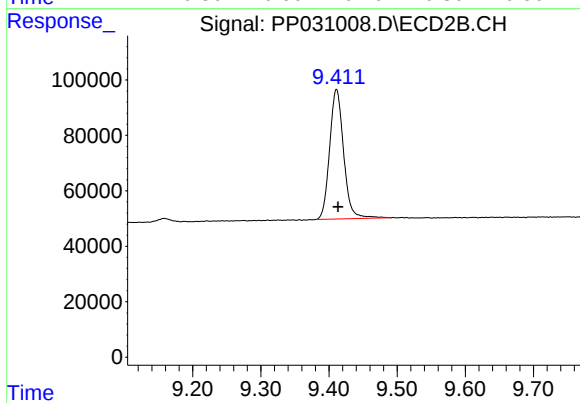

#2 Decachlorobiphenyl

R.T.: 9.411 min
Delta R.T.: -0.002 min
Response: 667701
Conc: 16.89 ng/ml

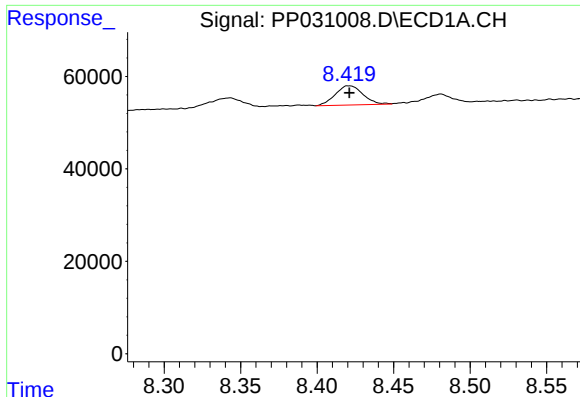


#36 AR-1262-1

R.T.: 8.420 min
Delta R.T.: 0.000 min
Response: 52150
Conc: 22.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-AR1262-S-2


Manual Integrations
APPROVED

Ankita
11/2/2020 3:00:06 PM

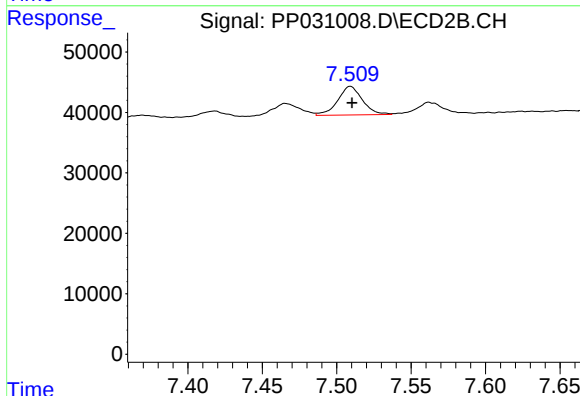


#36 AR-1262-1

R.T.: 7.509 min
Delta R.T.: -0.001 min
Response: 54829
Conc: 21.00 ng/ml

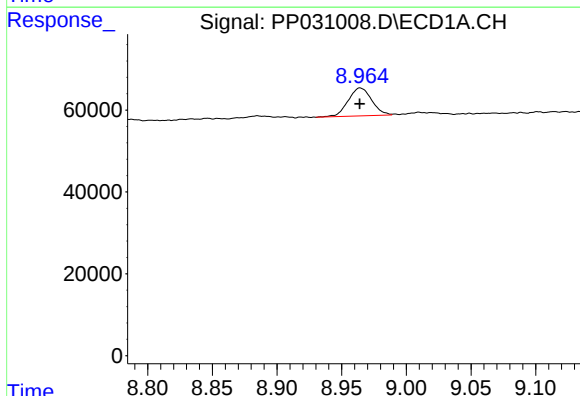


#37 AR-1262-2

R.T.: 8.964 min
Delta R.T.: 0.000 min
Response: 86486
Conc: 20.42 ng/ml

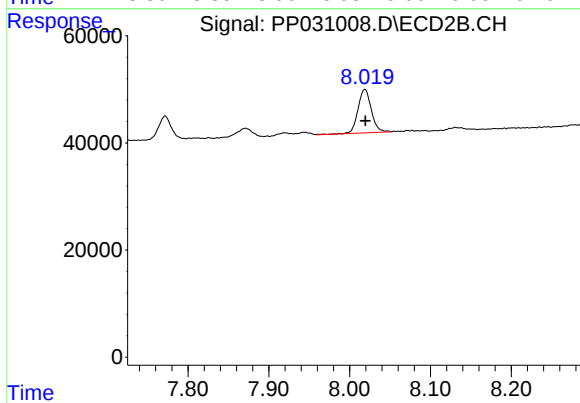

#37 AR-1262-2

R.T.: 8.019 min
Delta R.T.: 0.000 min
Response: 93652
Conc: 19.89 ng/ml

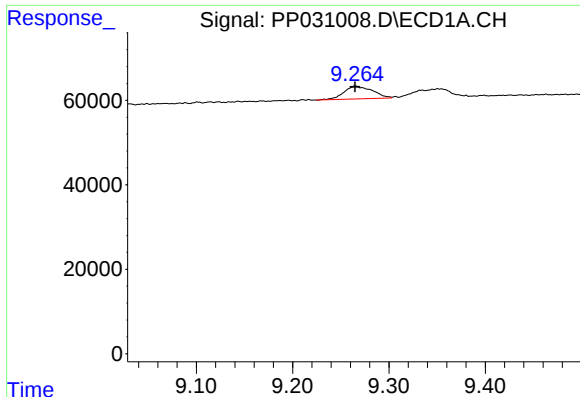


#38 AR-1262-3

R.T.: 9.265 min
Delta R.T.: 0.000 min
Response: 62217
Conc: 20.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-AR1262-S-2


Manual Integrations
APPROVED

Ankita
11/2/2020 3:00:06 PM

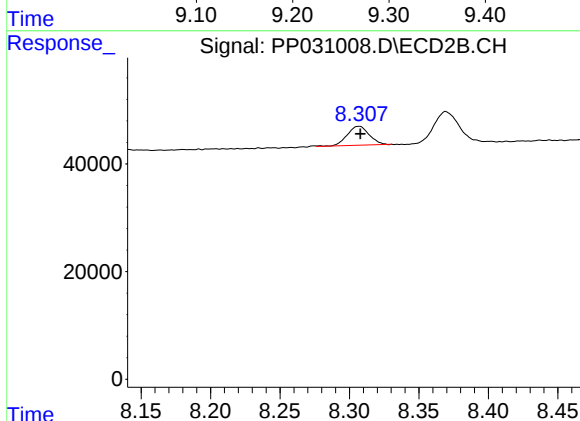


#38 AR-1262-3

R.T.: 8.307 min
Delta R.T.: -0.001 min
Response: 38892
Conc: 19.58 ng/ml m

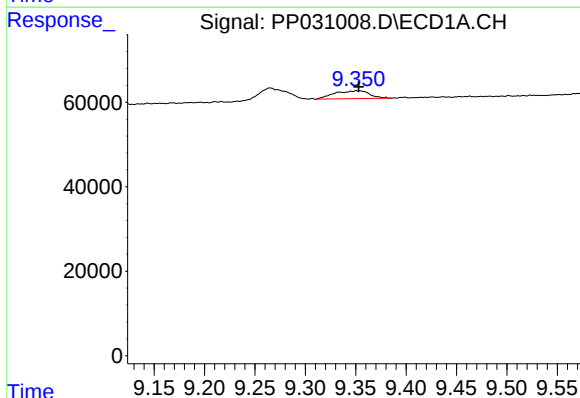


#39 AR-1262-4

R.T.: 9.350 min
Delta R.T.: -0.003 min
Response: 44677
Conc: 18.27 ng/ml m

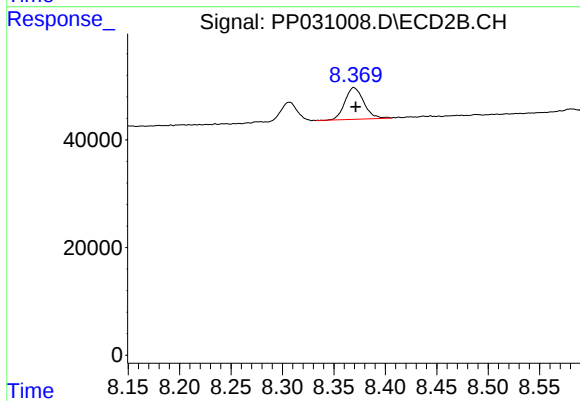

#39 AR-1262-4

R.T.: 8.369 min
Delta R.T.: -0.002 min
Response: 75184
Conc: 20.79 ng/ml

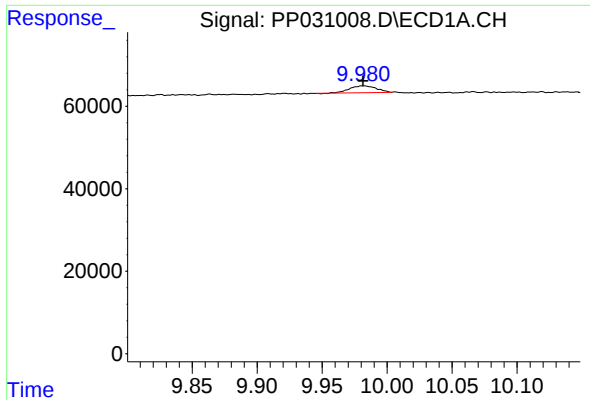


#40 AR-1262-5

R.T.: 9.980 min
Delta R.T.: -0.001 min
Response: 23888
Conc: 15.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-AR1262-S-2

Manual Integrations
APPROVED

Ankita
11/2/2020 3:00:06 PM

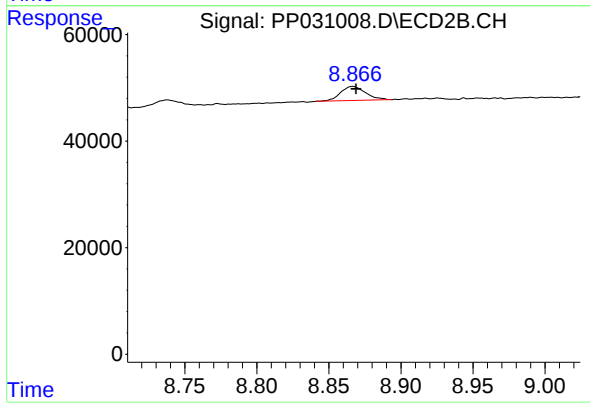

#40 AR-1262-5

R.T.: 8.867 min
Delta R.T.: -0.002 min
Response: 31733
Conc: 19.26 ng/ml