

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110120\
 Data File : PP031016.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Oct 2020 17:54
 Operator : DD\AJ
 Sample : MDL-AR1262-W-8
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-AR1262-W-8

Manual Integrations
 APPROVED

Ankita
 11/2/2020 3:00:16 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 02:44:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\AR1262PP110120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 31 02:26:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.801	4.078	992264	875304	15.553	15.152
2) SA Decachlor...	10.688	9.408	626962	666418	16.882	16.853
Target Compounds						
36) L8 AR-1262-1	8.419	7.506	52963	55419	22.565	21.227
37) L8 AR-1262-2	8.962	8.016	86972	93355	20.536	19.823
38) L8 AR-1262-3	9.264	8.303	65533	44551	21.942m	22.434m
39) L8 AR-1262-4	9.351	8.368	66699	75674	27.277	20.926
40) L8 AR-1262-5	9.978	8.865	33439	29641	21.380	17.988

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110120\
Data File : PP031016.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Oct 2020 17:54
Operator : DD\AJ
Sample : MDL-AR1262-W-8
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
MDL-AR1262-W-8


Manual Integrations
APPROVED

Ankita
11/2/2020 3:00:16 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 02:44:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\AR1262PP110120.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 31 02:26:29 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

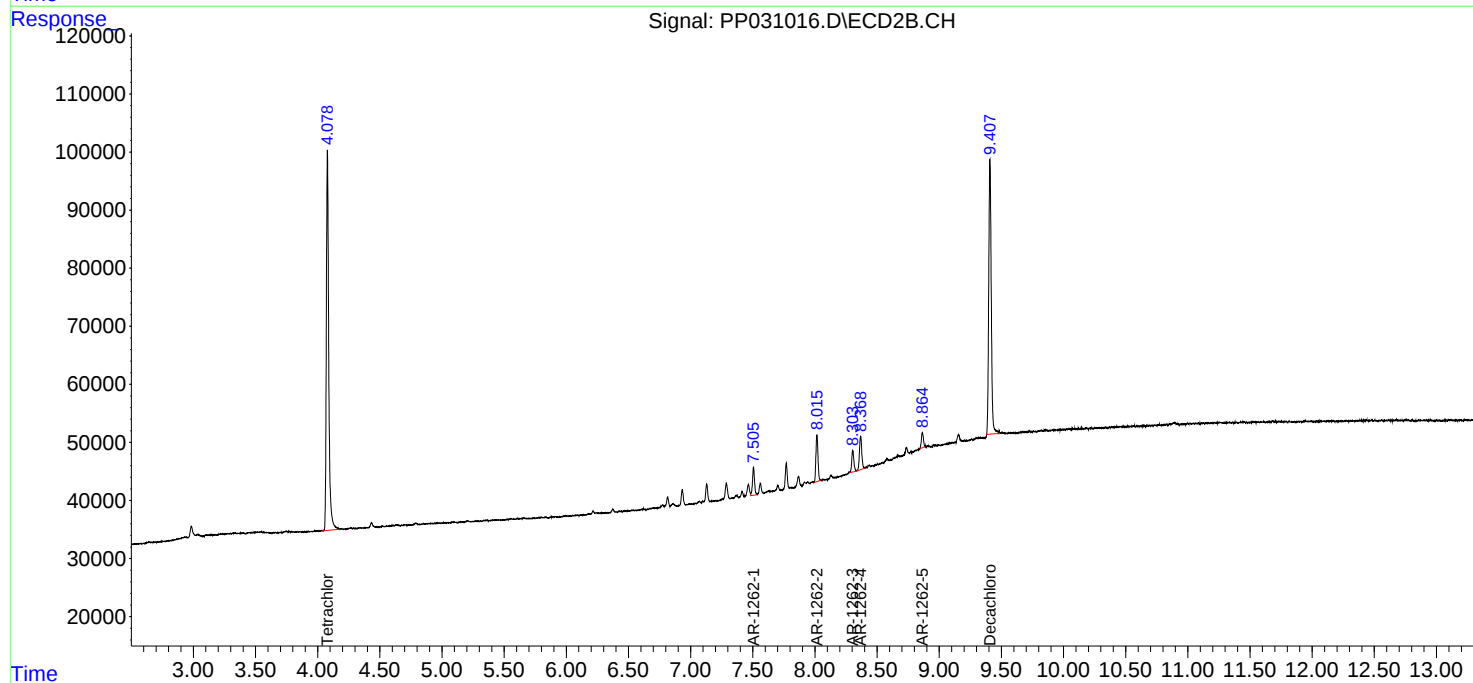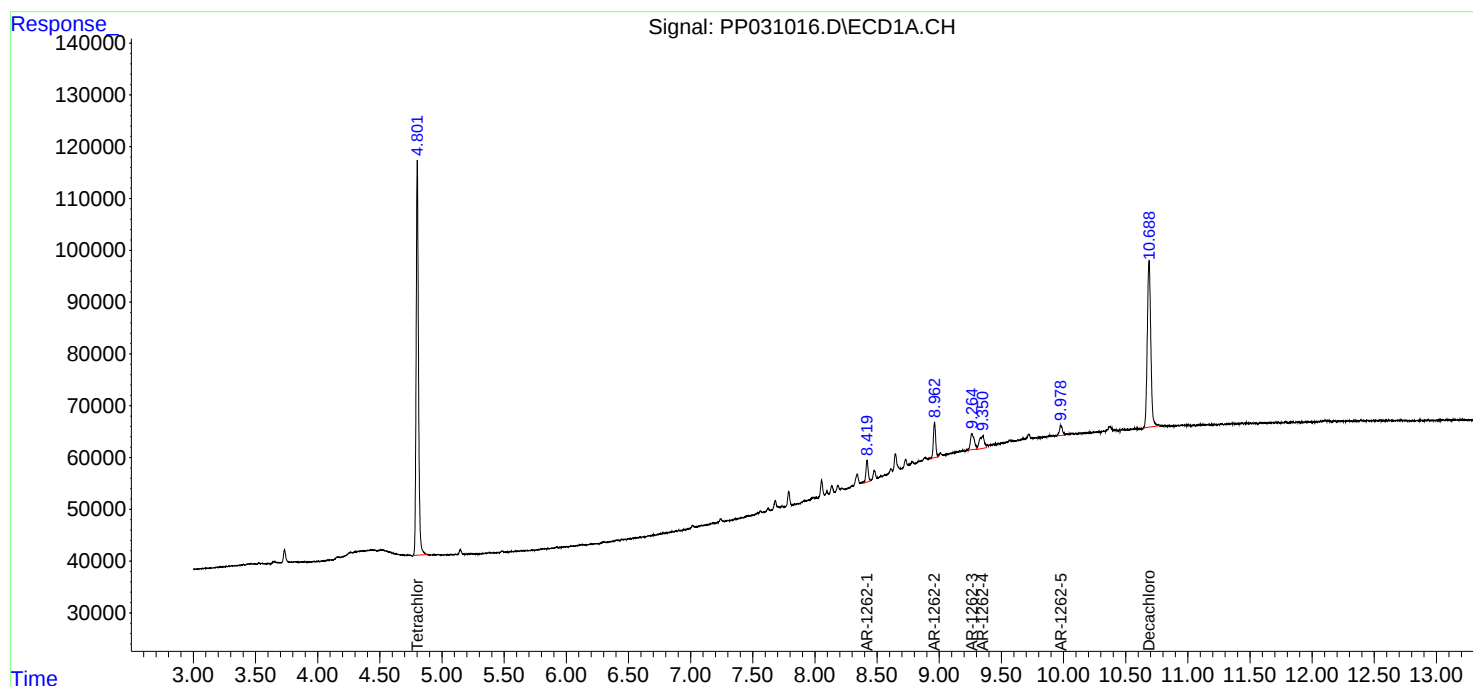

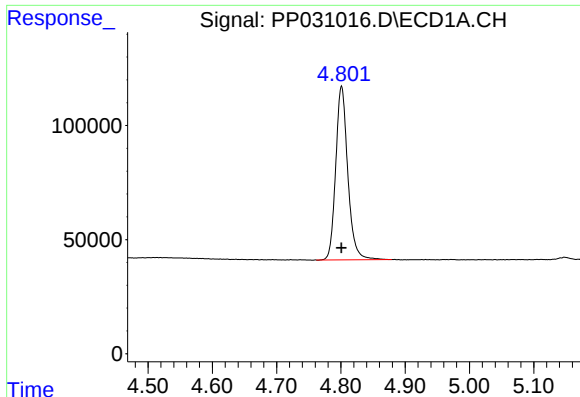


#1 Tetrachloro-m-xylene

R.T.: 4.801 min
Delta R.T.: 0.000 min
Response: 992264
Conc: 15.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-AR1262-W-8


Manual Integrations
APPROVED

Ankita
11/2/2020 3:00:16 PM

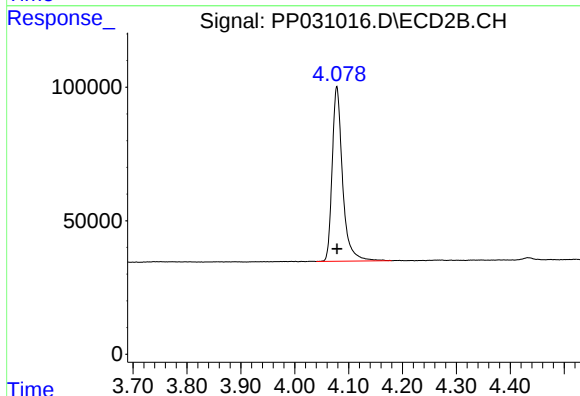


#1 Tetrachloro-m-xylene

R.T.: 4.078 min
Delta R.T.: 0.000 min
Response: 875304
Conc: 15.15 ng/ml

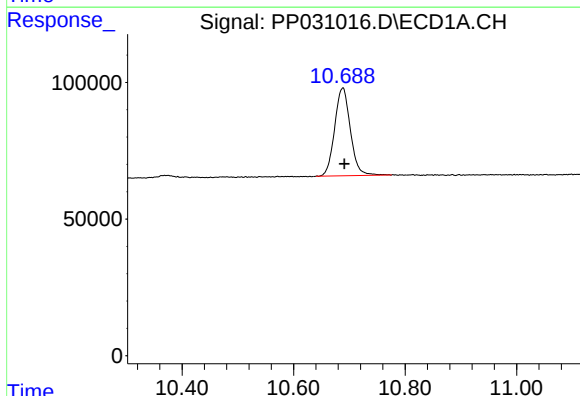


#2 Decachlorobiphenyl

R.T.: 10.688 min
Delta R.T.: -0.003 min
Response: 626962
Conc: 16.88 ng/ml

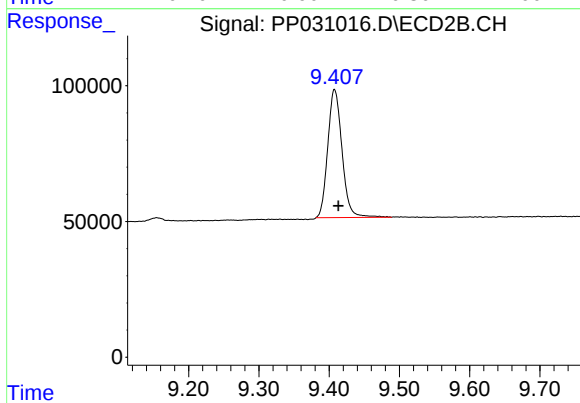

#2 Decachlorobiphenyl

R.T.: 9.408 min
Delta R.T.: -0.006 min
Response: 666418
Conc: 16.85 ng/ml

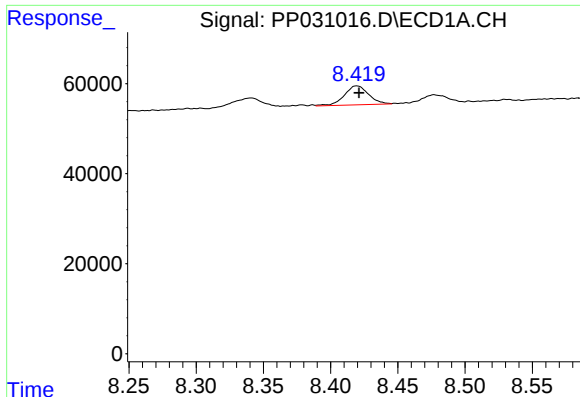


#36 AR-1262-1

R.T.: 8.419 min
Delta R.T.: -0.002 min
Response: 52963
Conc: 22.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-AR1262-W-8


Manual Integrations
APPROVED

Ankita
11/2/2020 3:00:16 PM

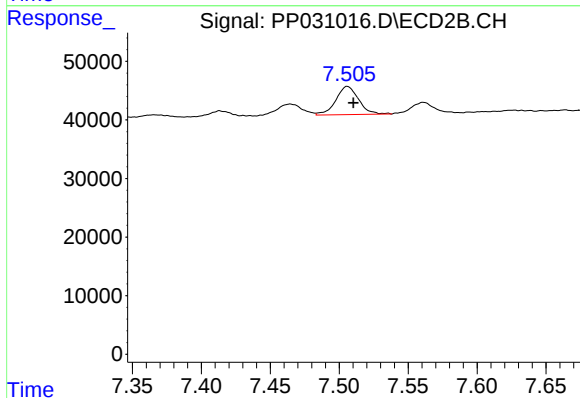


#36 AR-1262-1

R.T.: 7.506 min
Delta R.T.: -0.004 min
Response: 55419
Conc: 21.23 ng/ml

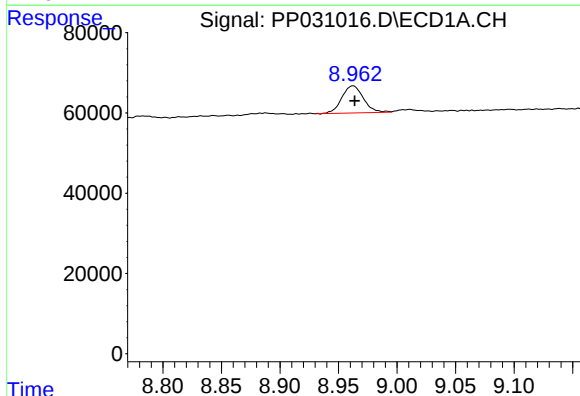


#37 AR-1262-2

R.T.: 8.962 min
Delta R.T.: -0.002 min
Response: 86972
Conc: 20.54 ng/ml

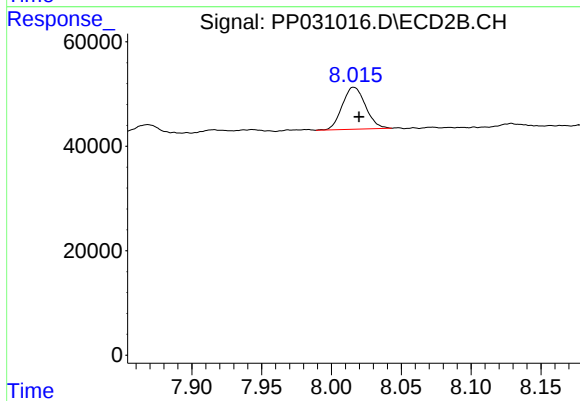

#37 AR-1262-2

R.T.: 8.016 min
Delta R.T.: -0.004 min
Response: 93355
Conc: 19.82 ng/ml

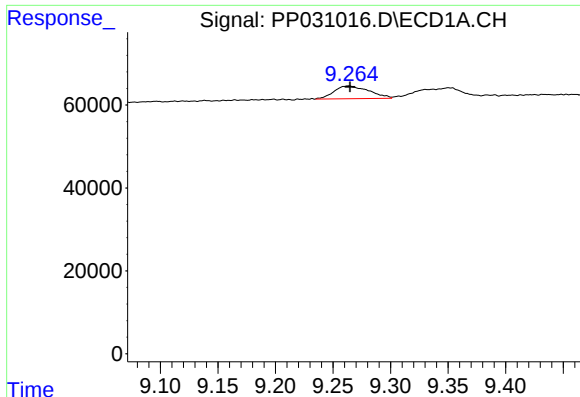


#38 AR-1262-3

R.T.: 9.264 min
Delta R.T.: -0.001 min
Response: 65533
Conc: 21.94 ng/ml m

Instrument :
ECD_P
ClientSampleId :
MDL-AR1262-W-8


Manual Integrations
APPROVED

Ankita
11/2/2020 3:00:16 PM

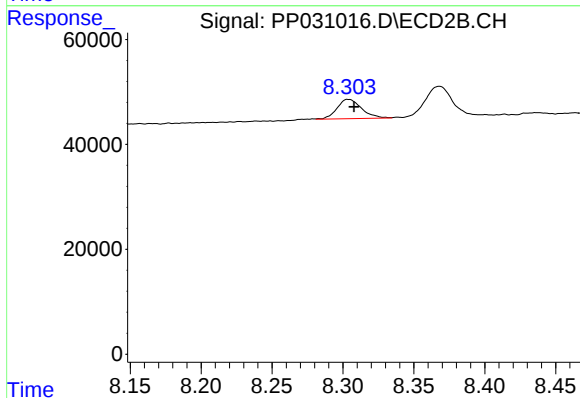


#38 AR-1262-3

R.T.: 8.303 min
Delta R.T.: -0.005 min
Response: 44551
Conc: 22.43 ng/ml m

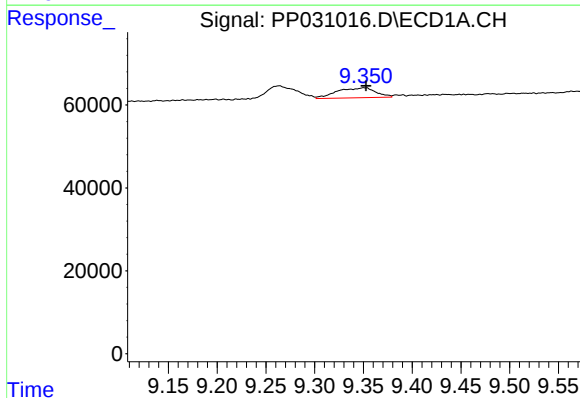


#39 AR-1262-4

R.T.: 9.351 min
Delta R.T.: -0.002 min
Response: 66699
Conc: 27.28 ng/ml

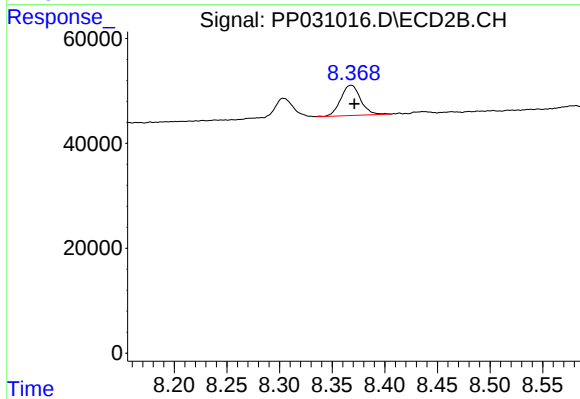

#39 AR-1262-4

R.T.: 8.368 min
Delta R.T.: -0.003 min
Response: 75674
Conc: 20.93 ng/ml

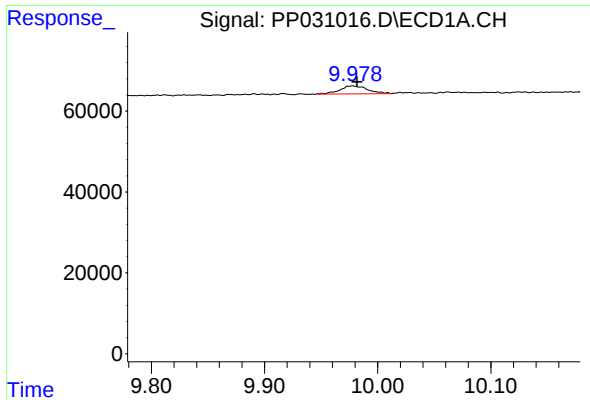


#40 AR-1262-5

R.T.: 9.978 min
Delta R.T.: -0.004 min
Response: 33439
Conc: 21.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-AR1262-W-8

Manual Integrations
APPROVED

Ankita
11/2/2020 3:00:16 PM

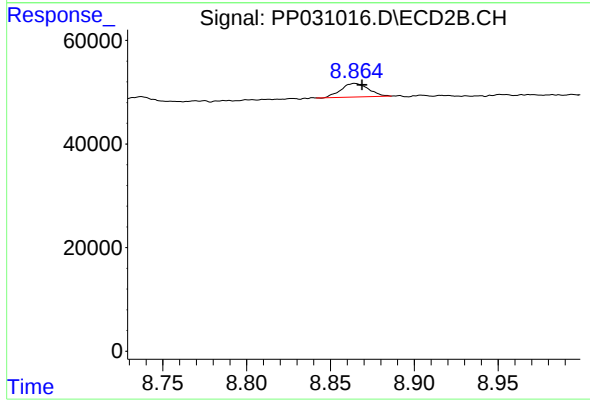

#40 AR-1262-5

R.T.: 8.865 min
Delta R.T.: -0.004 min
Response: 29641
Conc: 17.99 ng/ml