

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110120\
 Data File : PP031017.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Oct 2020 18:11
 Operator : DD\AJ
 Sample : MDL-AR1262-W-9
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-AR1262-W-9

Manual Integrations
 APPROVED

Ankita
 11/2/2020 3:00:34 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 02:45:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\AR1262PP110120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 31 02:26:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.801	4.078	1027612	894077	16.107	15.476
2) SA Decachlor...	10.688	9.408	616893	649993	16.611	16.438
Target Compounds						
36) L8 AR-1262-1	8.421	7.507	52894	54055	22.536	20.705
37) L8 AR-1262-2	8.964	8.016	87700	97375	20.708	20.677
38) L8 AR-1262-3	9.265	8.304	60751	40373	20.341	20.330m
39) L8 AR-1262-4	9.352	8.368	50071	76868	20.477m	21.257
40) L8 AR-1262-5	9.979	8.864	33127	32969	21.180	20.007

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110120\
Data File : PP031017.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Oct 2020 18:11
Operator : DD\AJ
Sample : MDL-AR1262-W-9
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
MDL-AR1262-W-9


Manual Integrations
APPROVED

Ankita
11/2/2020 3:00:34 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 02:45:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\AR1262PP110120.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 31 02:26:29 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

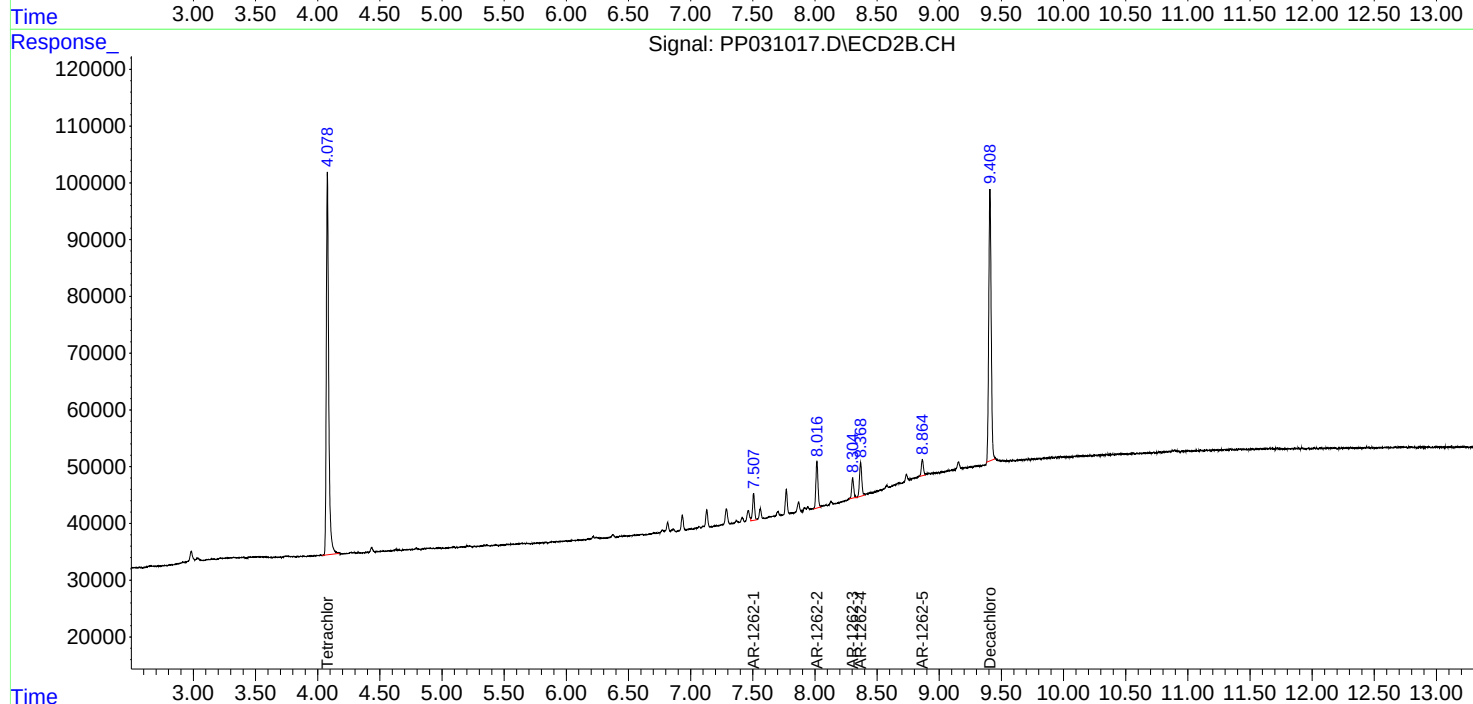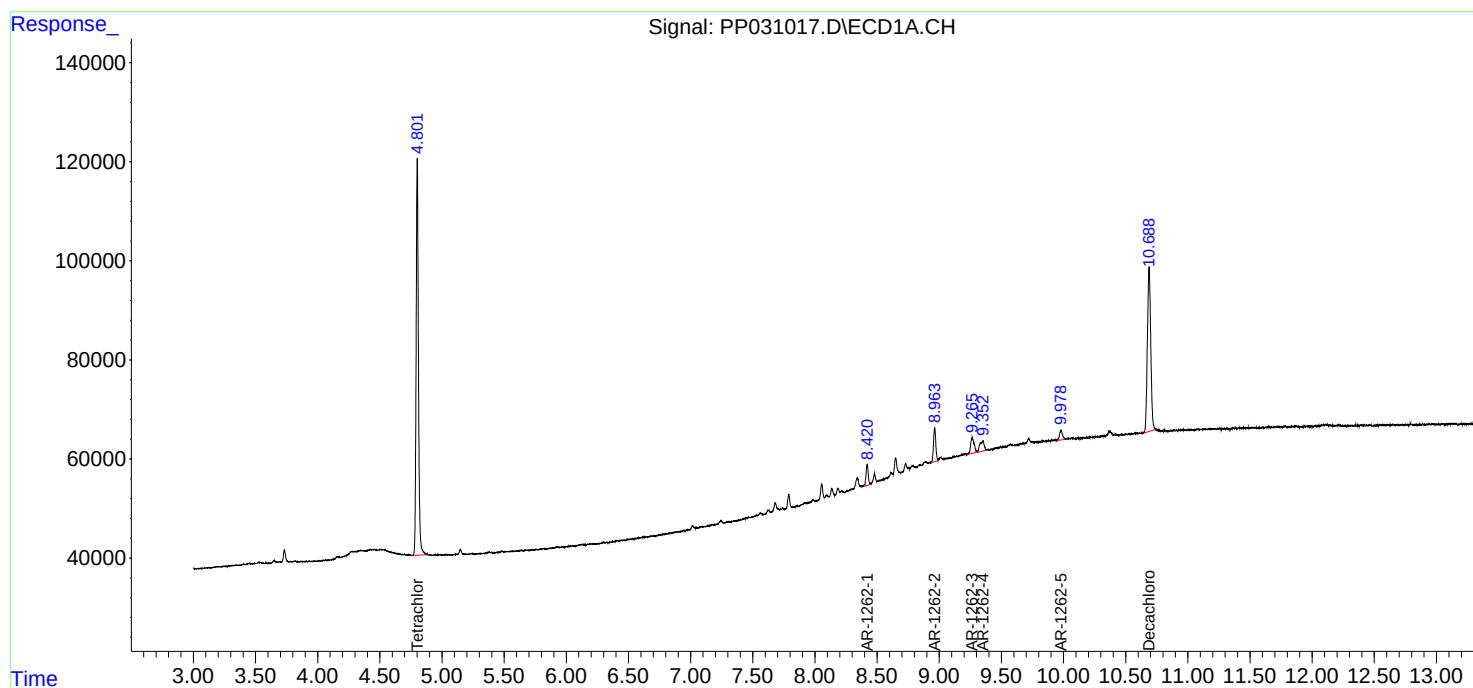

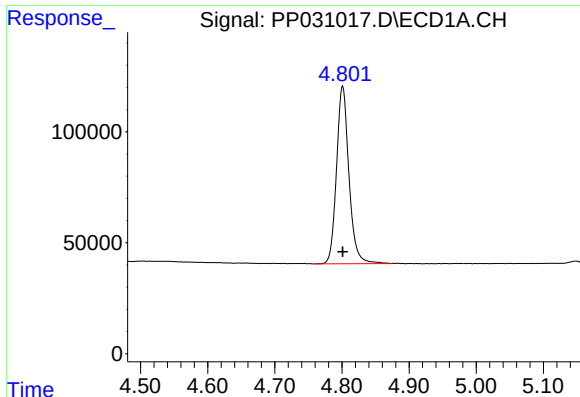


#1 Tetrachloro-m-xylene

R.T.: 4.801 min
Delta R.T.: 0.000 min
Response: 1027612
Conc: 16.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-AR1262-W-9


Manual Integrations
APPROVED

Ankita
11/2/2020 3:00:34 PM

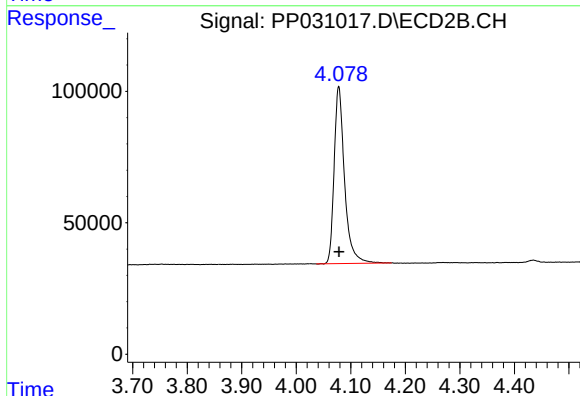


#1 Tetrachloro-m-xylene

R.T.: 4.078 min
Delta R.T.: 0.000 min
Response: 894077
Conc: 15.48 ng/ml

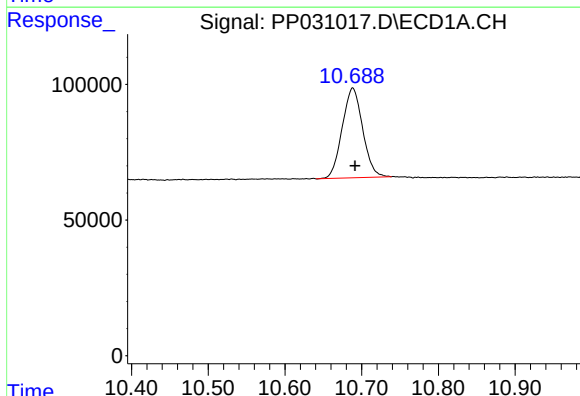


#2 Decachlorobiphenyl

R.T.: 10.688 min
Delta R.T.: -0.003 min
Response: 616893
Conc: 16.61 ng/ml

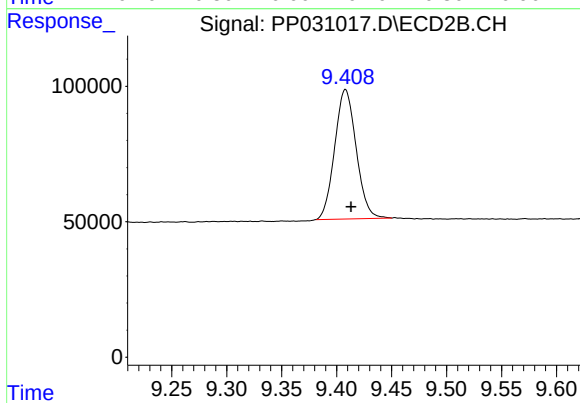

#2 Decachlorobiphenyl

R.T.: 9.408 min
Delta R.T.: -0.005 min
Response: 649993
Conc: 16.44 ng/ml

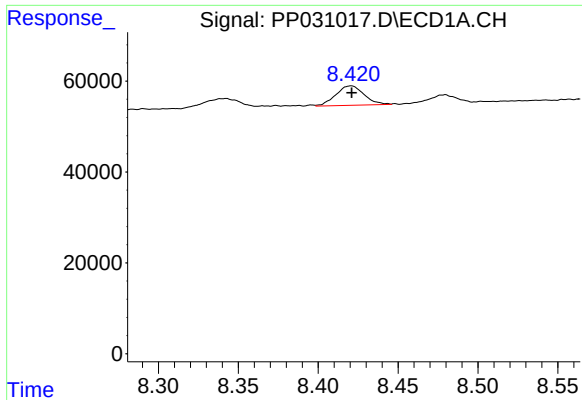


#36 AR-1262-1

R.T.: 8.421 min
Delta R.T.: 0.000 min
Response: 52894
Conc: 22.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-AR1262-W-9


Manual Integrations
APPROVED

Ankita
11/2/2020 3:00:34 PM

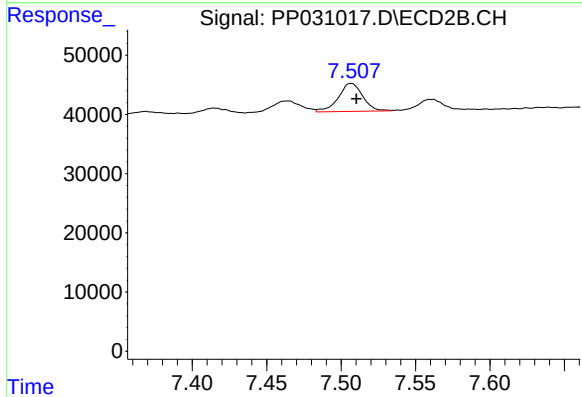


#36 AR-1262-1

R.T.: 7.507 min
Delta R.T.: -0.003 min
Response: 54055
Conc: 20.71 ng/ml

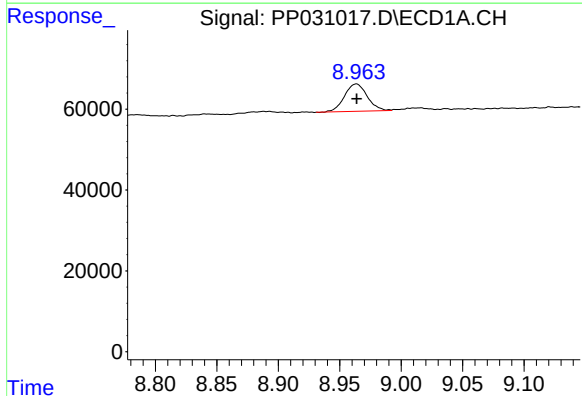


#37 AR-1262-2

R.T.: 8.964 min
Delta R.T.: 0.000 min
Response: 87700
Conc: 20.71 ng/ml

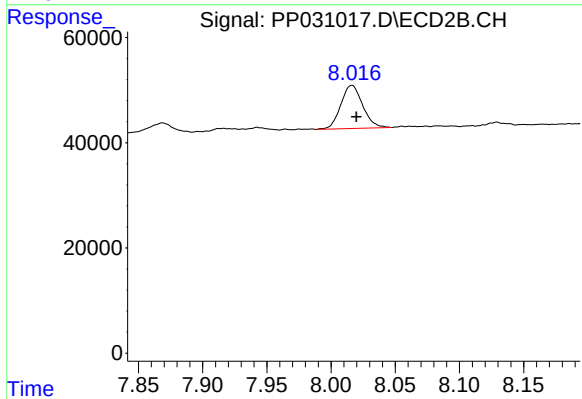

#37 AR-1262-2

R.T.: 8.016 min
Delta R.T.: -0.003 min
Response: 97375
Conc: 20.68 ng/ml

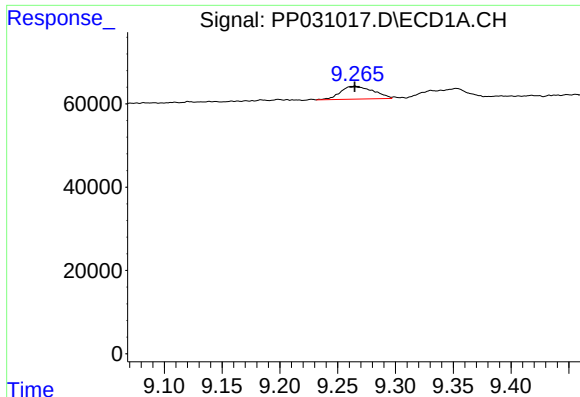


#38 AR-1262-3

R.T.: 9.265 min
Delta R.T.: 0.000 min
Response: 60751
Conc: 20.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-AR1262-W-9


Manual Integrations
APPROVED

Ankita
11/2/2020 3:00:34 PM

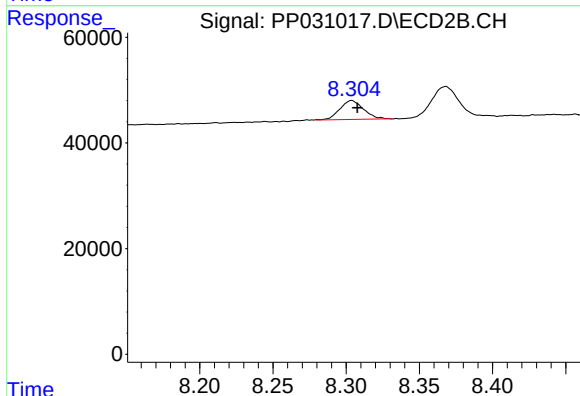


#38 AR-1262-3

R.T.: 8.304 min
Delta R.T.: -0.004 min
Response: 40373
Conc: 20.33 ng/ml m

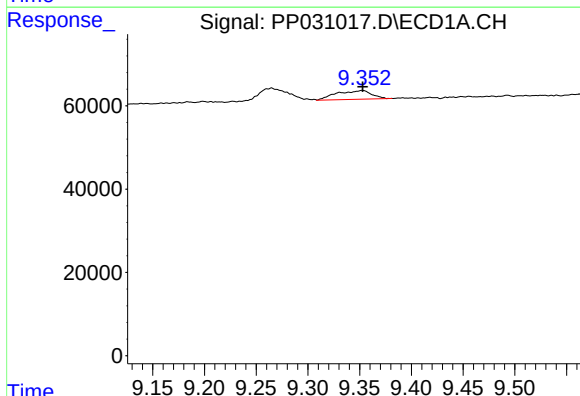


#39 AR-1262-4

R.T.: 9.352 min
Delta R.T.: 0.000 min
Response: 50071
Conc: 20.48 ng/ml m

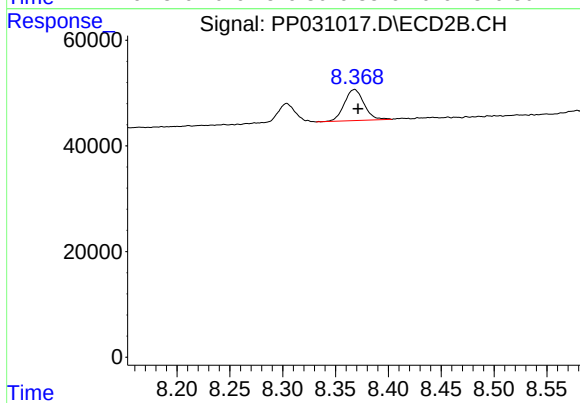

#39 AR-1262-4

R.T.: 8.368 min
Delta R.T.: -0.003 min
Response: 76868
Conc: 21.26 ng/ml

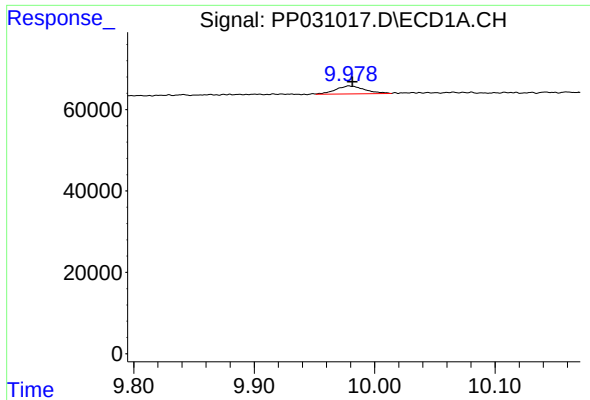


#40 AR-1262-5

R.T.: 9.979 min
Delta R.T.: -0.003 min
Response: 33127
Conc: 21.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-AR1262-W-9

Manual Integrations
APPROVED

Ankita
11/2/2020 3:00:34 PM

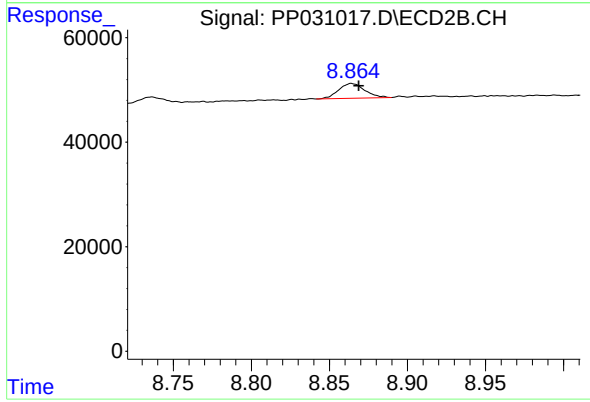

#40 AR-1262-5

R.T.: 8.864 min
Delta R.T.: -0.005 min
Response: 32969
Conc: 20.01 ng/ml