

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110120\
 Data File : PP031021.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Oct 2020 19:17
 Operator : DD\AJ
 Sample : MDL-AR1268-W-10
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-AR1268-W-10

Manual Integrations
 APPROVED

Ankita
 11/2/2020 3:00:35 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 02:52:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\AR1268PP110120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 31 02:37:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.800	4.078	1017261	901741	17.070	17.131
2) SA Decachlor...	10.687	9.407	682352	742810	11.891	11.765
Target Compounds						
41) L9 AR-1268-1	9.261	8.304	118381	126989	24.303	23.606m
42) L9 AR-1268-2	9.352	8.368	110524	118765	22.819	22.498
43) L9 AR-1268-3	9.569	8.578	94547	105532	23.367	23.932
44) L9 AR-1268-4	9.977	8.864	31093	37010	19.359	20.577
45) L9 AR-1268-5	10.369	9.154	277853	294010	21.617	20.572

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110120\
Data File : PP031021.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Oct 2020 19:17
Operator : DD\AJ
Sample : MDL-AR1268-W-10
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
MDL-AR1268-W-10


Manual Integrations
APPROVED

Ankita
11/2/2020 3:00:35 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 02:52:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\AR1268PP110120.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 31 02:37:11 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

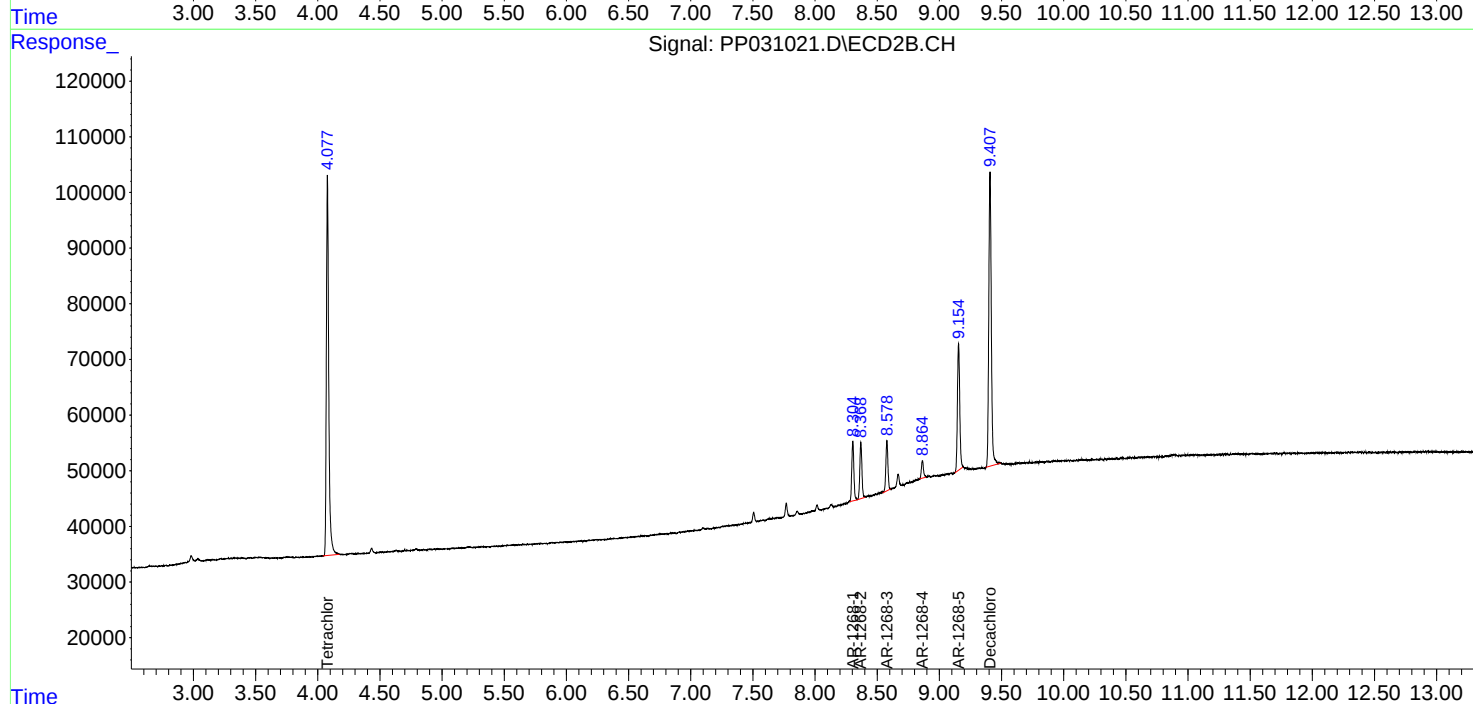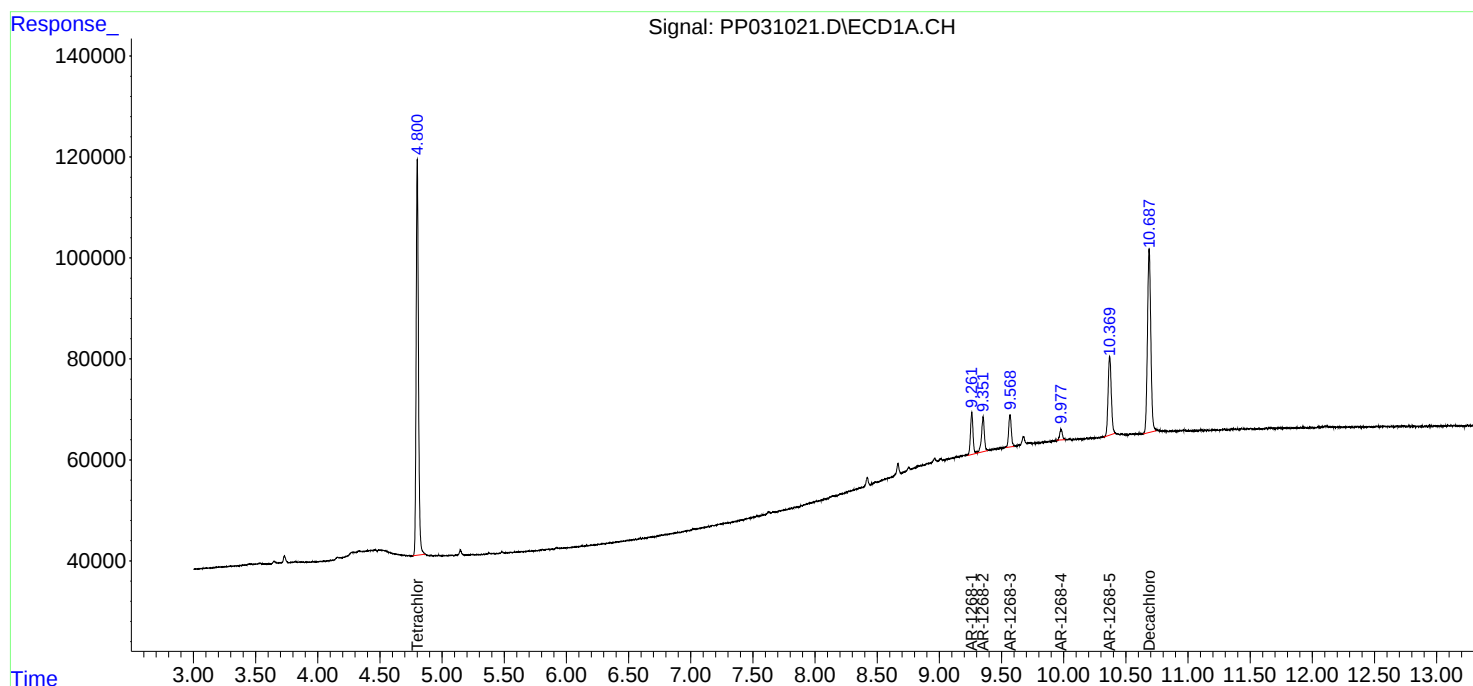

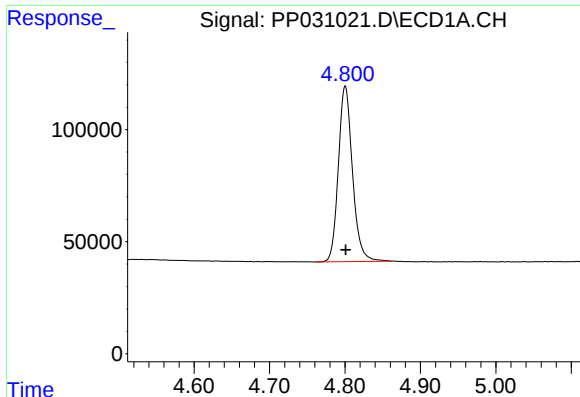


#1 Tetrachloro-m-xylene

R.T.: 4.800 min
Delta R.T.: 0.000 min
Response: 1017261
Conc: 17.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-AR1268-W-10


Manual Integrations
APPROVED

Ankita
11/2/2020 3:00:35 PM

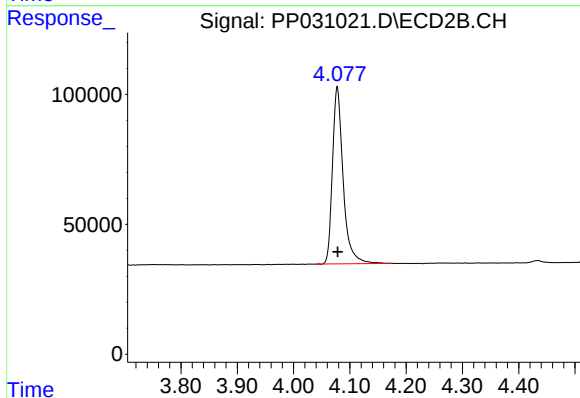


#1 Tetrachloro-m-xylene

R.T.: 4.078 min
Delta R.T.: -0.001 min
Response: 901741
Conc: 17.13 ng/ml

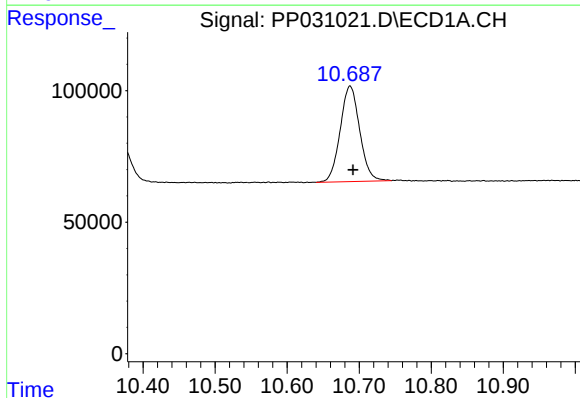


#2 Decachlorobiphenyl

R.T.: 10.687 min
Delta R.T.: -0.004 min
Response: 682352
Conc: 11.89 ng/ml

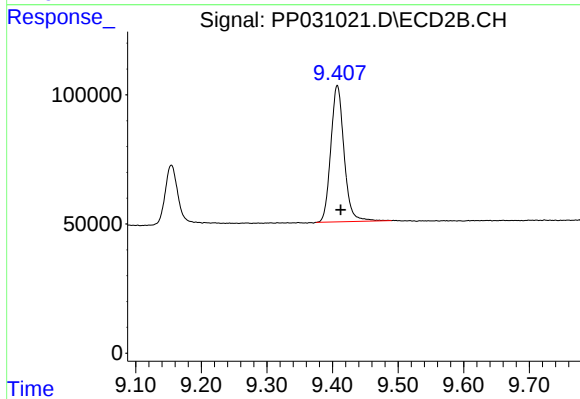

#2 Decachlorobiphenyl

R.T.: 9.407 min
Delta R.T.: -0.005 min
Response: 742810
Conc: 11.77 ng/ml

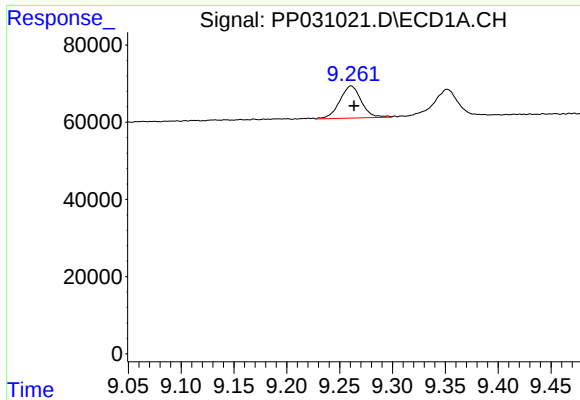


#41 AR-1268-1

R.T.: 9.261 min
Delta R.T.: -0.003 min
Response: 118381
Conc: 24.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-AR1268-W-10


Manual Integrations
APPROVED

Ankita
11/2/2020 3:00:35 PM

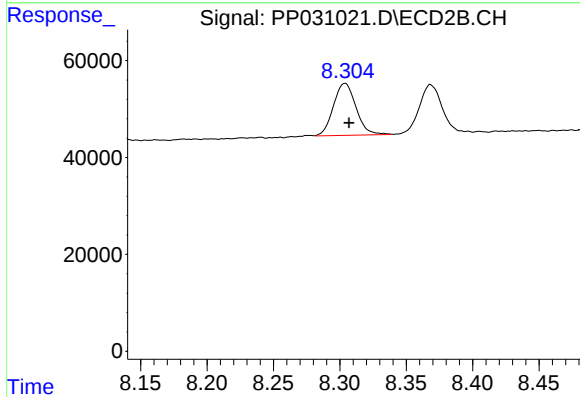


#41 AR-1268-1

R.T.: 8.304 min
Delta R.T.: -0.003 min
Response: 126989
Conc: 23.61 ng/ml m

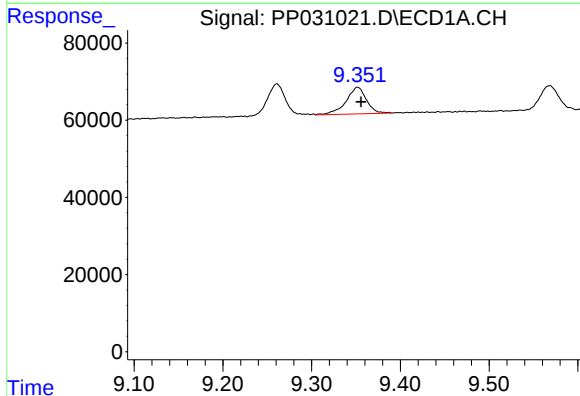


#42 AR-1268-2

R.T.: 9.352 min
Delta R.T.: -0.004 min
Response: 110524
Conc: 22.82 ng/ml

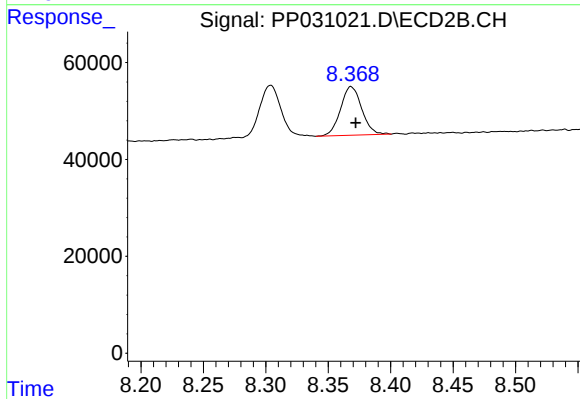

#42 AR-1268-2

R.T.: 8.368 min
Delta R.T.: -0.004 min
Response: 118765
Conc: 22.50 ng/ml

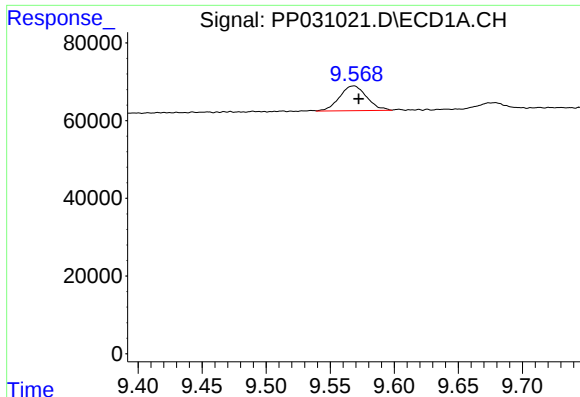


#43 AR-1268-3

R.T.: 9.569 min
Delta R.T.: -0.004 min
Response: 94547
Conc: 23.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-AR1268-W-10


Manual Integrations
APPROVED

Ankita
11/2/2020 3:00:35 PM

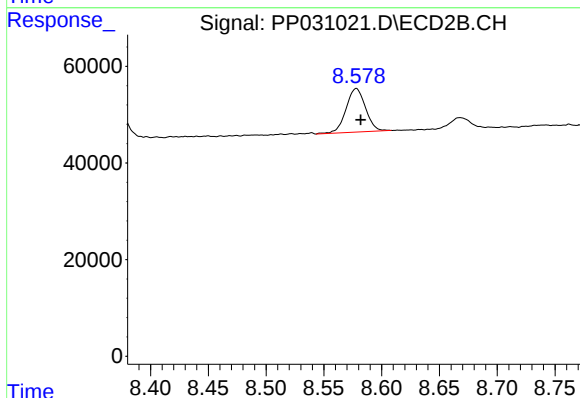


#43 AR-1268-3

R.T.: 8.578 min
Delta R.T.: -0.004 min
Response: 105532
Conc: 23.93 ng/ml

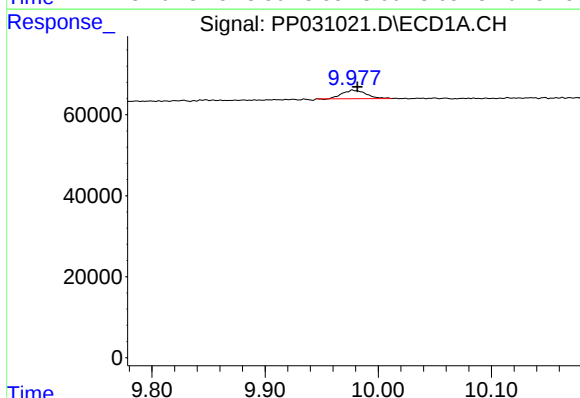


#44 AR-1268-4

R.T.: 9.977 min
Delta R.T.: -0.004 min
Response: 31093
Conc: 19.36 ng/ml

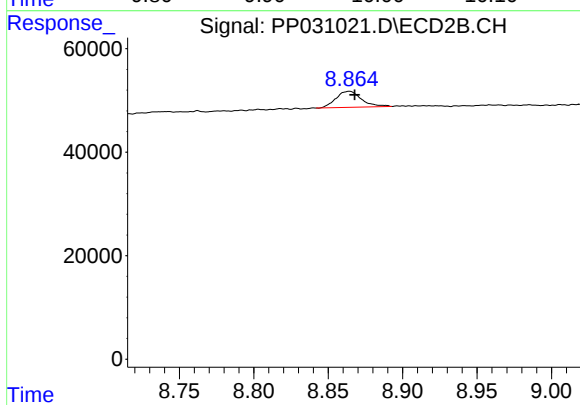

#44 AR-1268-4

R.T.: 8.864 min
Delta R.T.: -0.004 min
Response: 37010
Conc: 20.58 ng/ml

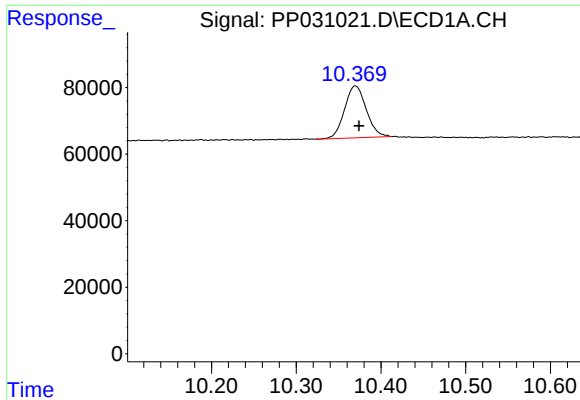


#45 AR-1268-5

R.T.: 10.369 min
Delta R.T.: -0.005 min
Response: 277853
Conc: 21.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-AR1268-W-10

Manual Integrations
APPROVED

Ankita
11/2/2020 3:00:35 PM

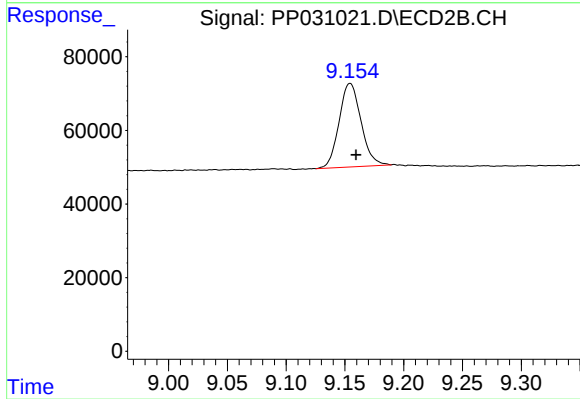

#45 AR-1268-5

R.T.: 9.154 min
Delta R.T.: -0.005 min
Response: 294010
Conc: 20.57 ng/ml