

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110122\
 Data File : PS020992.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2022 17:15
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 05:08:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 31 10:07:57 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.409	6.848	1140.7E6	776.9E6	546.553	561.667
Target Compounds							
3) T	4-Nitroph...	6.249	0.000	6460742	0	4.296	N.D. #
5) T	DICAMBA	6.624f	7.010	8673435	5862018	<MDL	<MDL #
6) T	MCP	6.739	7.071f	6239385	3892984	<MDL	<MDL #
7) T	MCPA	6.776f	0.000	8275314	0	<MDL	N.D. #
8) T	DICHLORPROP	7.206f	7.660	552315	12422469	<MDL	8.067 #
9) T	2,4-D	0.000	7.875f	0	2310688	N.D.	1.234
10) T	Pentachlo...	7.579	8.373	2911449	5569591	<MDL	<MDL #
11) T	2,4,5-TP ...	8.136	8.753	58058636	15203246	4.370	1.694 #
12) T	2,4,5-T	8.397	9.110	53266492	15514851	4.003	1.799 #
13) T	2,4-DB	8.821f	9.617	1585521	11069765	<MDL	9.946 #
14) T	DINOSEB	9.983	9.954	382742	5187093	<MDL	<MDL #
15) T	Picloram	9.749	10.927	10325021	113.7E6	<MDL	8.962 #
16) T	DCPA	10.244	10.830f	6724511	329.4E6	<MDL	30.846 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110122\
Data File : PS020992.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2022 17:15
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 05:08:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
Quant Title : 8080.M
QLast Update : Mon Oct 31 10:07:57 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

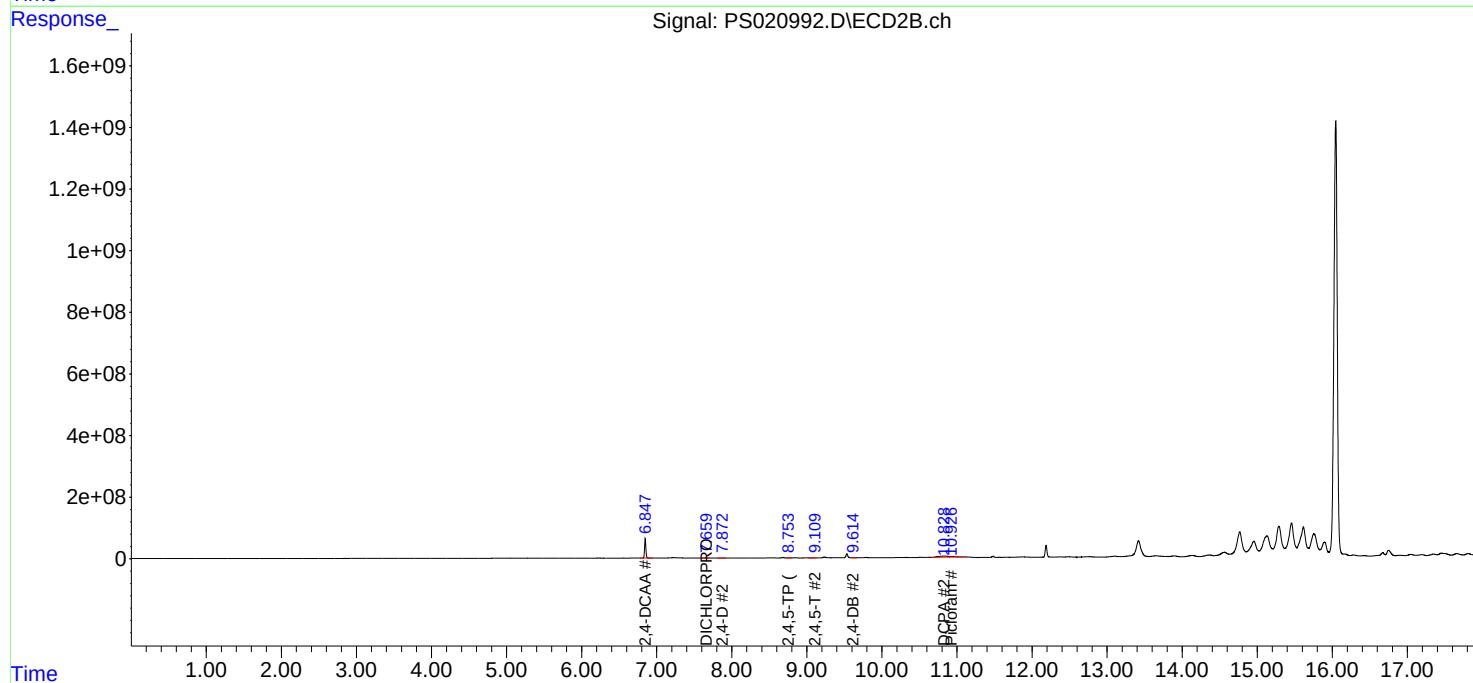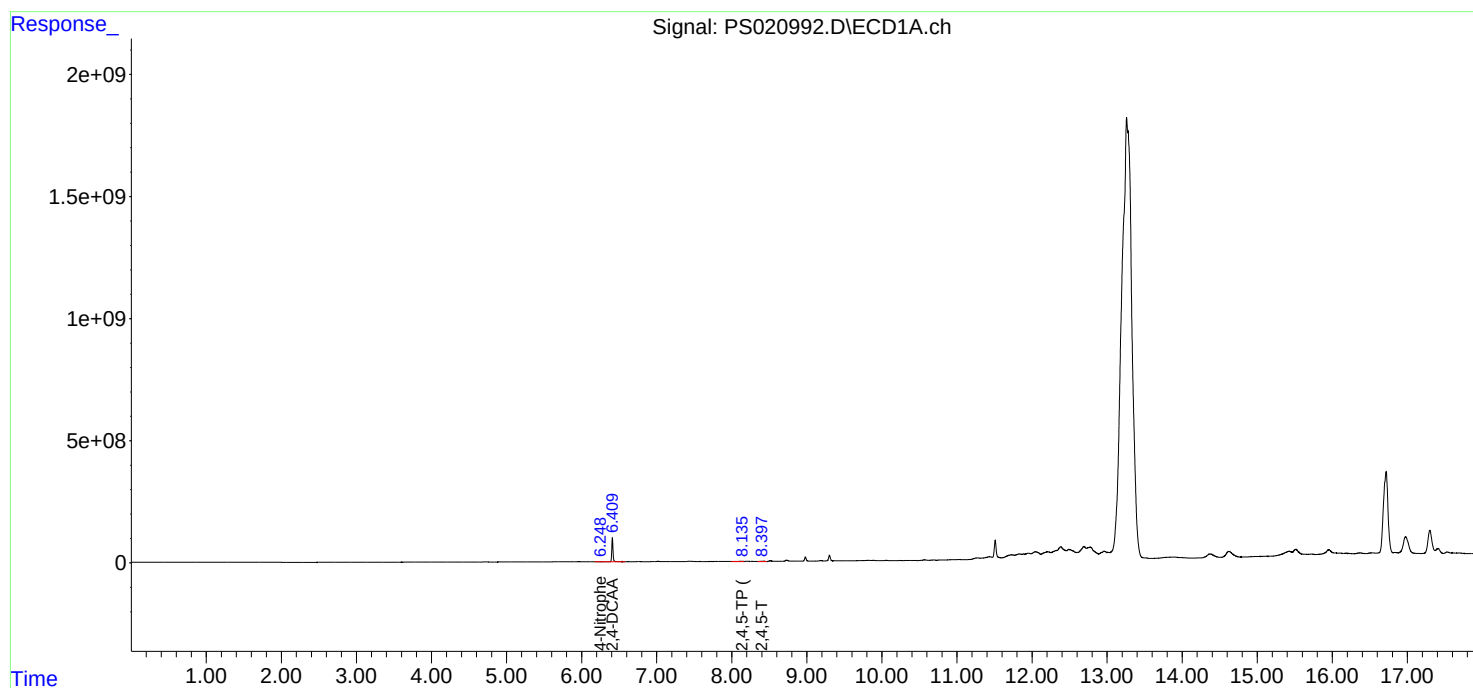


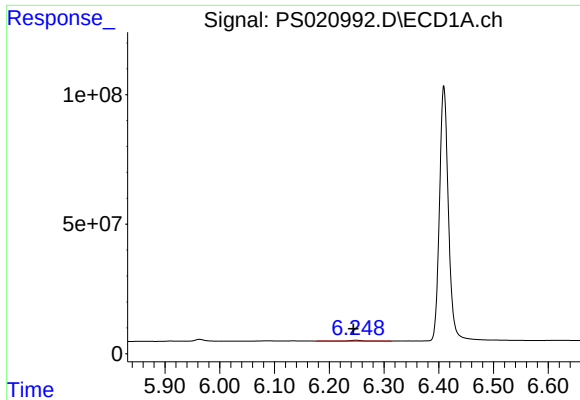

#3 4-Nitrophenol


R.T.: 6.249 min
Delta R.T.: 0.004 min
Response: 6460742
Conc: 4.30 ng/ml

Instrument :
ECD_P
ClientSampleId :

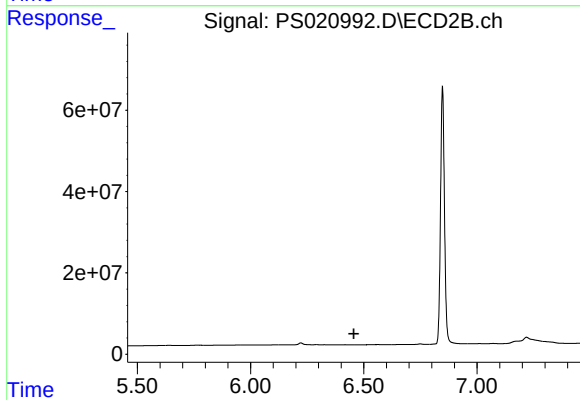


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.456 min
Response: 0
Conc: N.D.

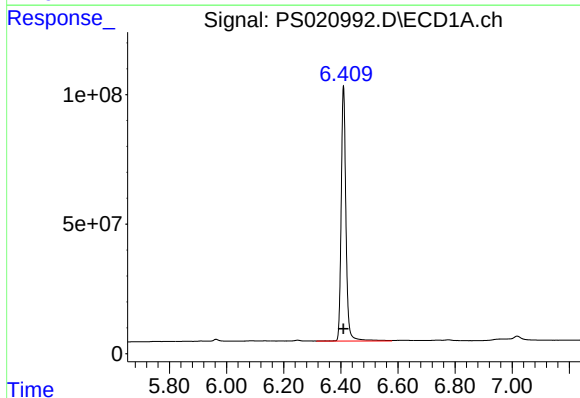


#4 2,4-DCAA

R.T.: 6.409 min
Delta R.T.: 0.000 min
Response: 1140698256
Conc: 546.55 ng/ml

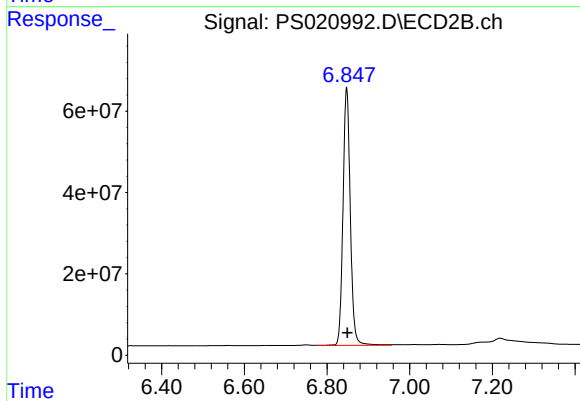

#4 2,4-DCAA


R.T.: 6.848 min
Delta R.T.: -0.002 min
Response: 776867680
Conc: 561.67 ng/ml

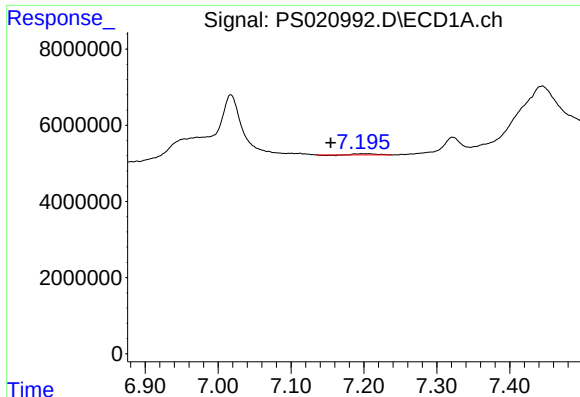

#8 DICHLORPROP


R.T.: 7.206 min
Delta R.T.: 0.052 min
Response: 552315
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

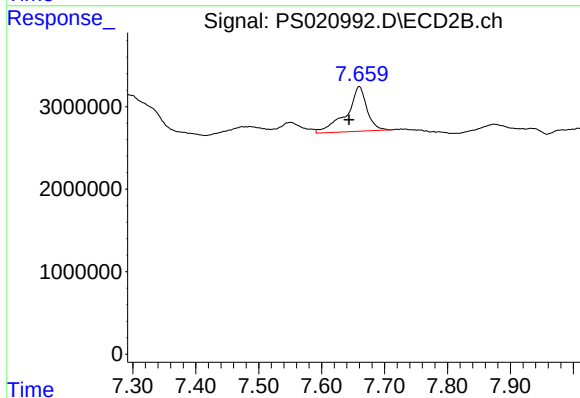


#8 DICHLORPROP

R.T.: 7.660 min
Delta R.T.: 0.016 min
Response: 12422469
Conc: 8.07 ng/ml

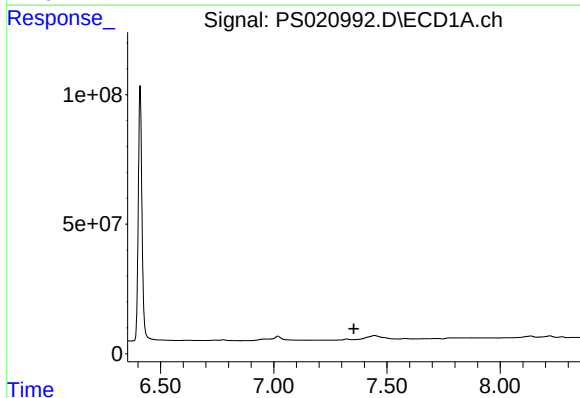


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.353 min
Response: 0
Conc: N.D.

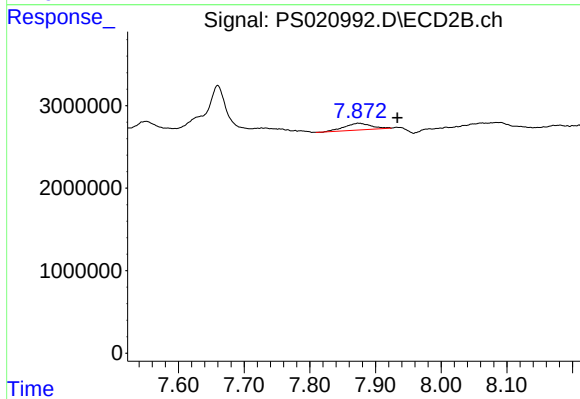

#9 2,4-D


R.T.: 7.875 min
Delta R.T.: -0.059 min
Response: 2310688
Conc: 1.23 ng/ml

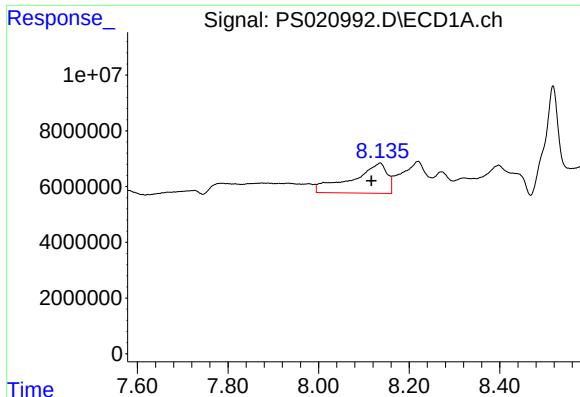

#11 2,4,5-TP (SILVEX)


R.T.: 8.136 min
Delta R.T.: 0.019 min
Response: 58058636
Conc: 4.37 ng/ml

Instrument :
ECD_P
ClientSampleId :

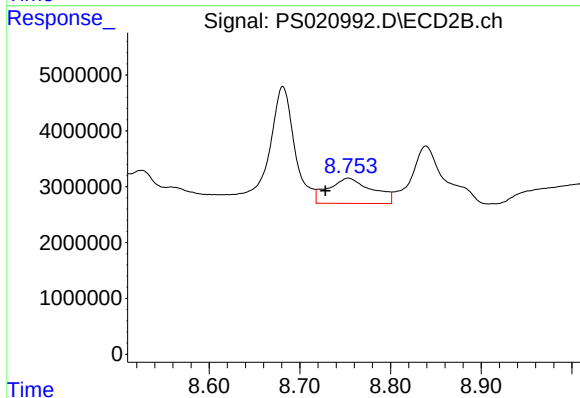


#11 2,4,5-TP (SILVEX)

R.T.: 8.753 min
Delta R.T.: 0.025 min
Response: 15203246
Conc: 1.69 ng/ml

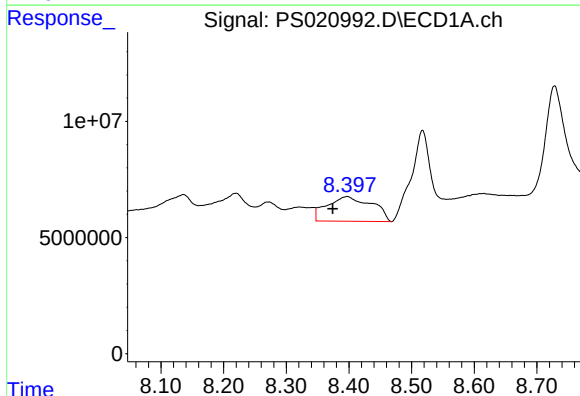


#12 2,4,5-T

R.T.: 8.397 min
Delta R.T.: 0.023 min
Response: 53266492
Conc: 4.00 ng/ml

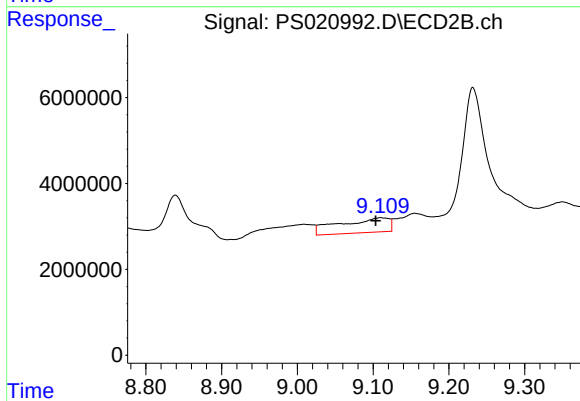

#12 2,4,5-T


R.T.: 9.110 min
Delta R.T.: 0.007 min
Response: 15514851
Conc: 1.80 ng/ml

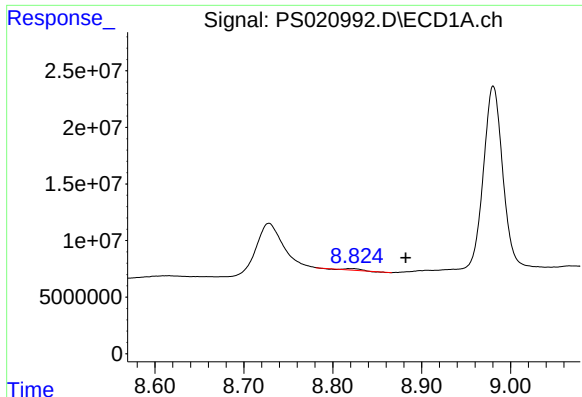

#13 2,4-DB


R.T.: 8.821 min
Delta R.T.: -0.061 min
Response: 1585521
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

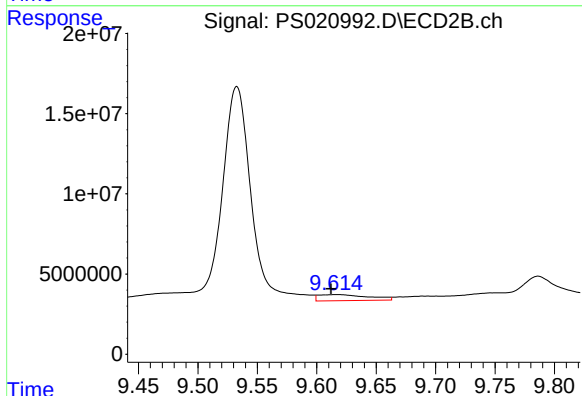


#13 2,4-DB

R.T.: 9.617 min
Delta R.T.: 0.005 min
Response: 11069765
Conc: 9.95 ng/ml

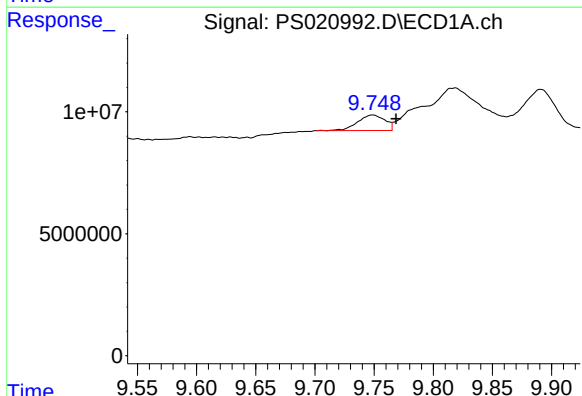


#15 Picloram

R.T.: 9.749 min
Delta R.T.: -0.020 min
Response: 10325021
Conc: N.D.

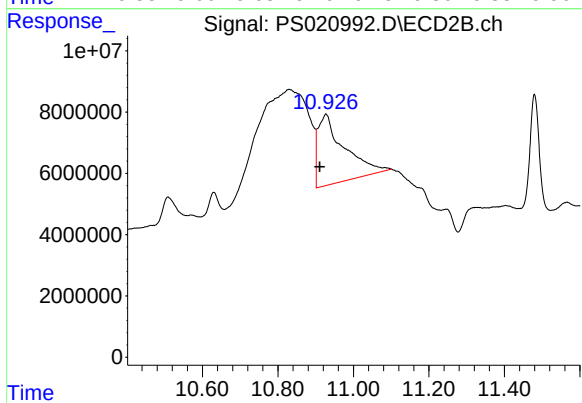

#15 Picloram


R.T.: 10.927 min
Delta R.T.: 0.017 min
Response: 113709862
Conc: 8.96 ng/ml

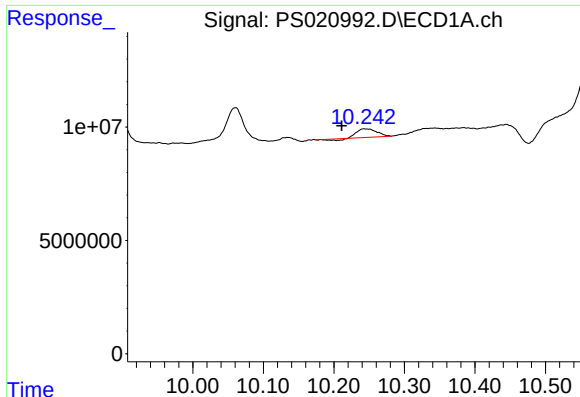

#16 DCPA

R.T.: 10.244 min
Delta R.T.: 0.033 min
Response: 6724511
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

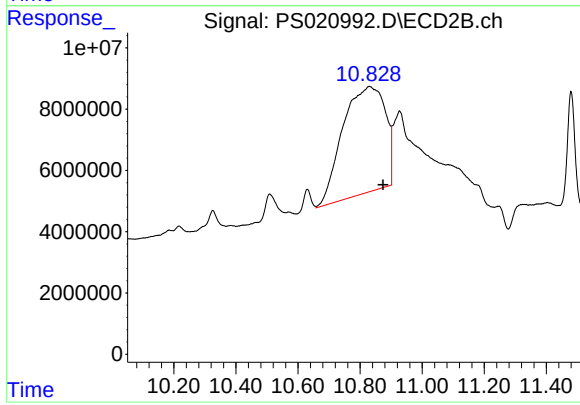

#16 DCPA

R.T.: 10.830 min
Delta R.T.: -0.044 min
Response: 329369041
Conc: 30.85 ng/ml