

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110122\
 Data File : PP052936.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2022 17:35
 Operator : YP\AJ
 Sample : N5352-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CMS-WATERPIT-1028

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 22:48:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 27 04:46:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.412	3.657	29460184	28468051	13.332	15.149
2) SA Decachlor...	10.218	8.738	21448975	26638779	16.898	15.884

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110122\
Data File : PP052936.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2022 17:35
Operator : YP\AJ
Sample : N5352-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
CMS-WATERPIT-1028

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 22:48:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 27 04:46:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

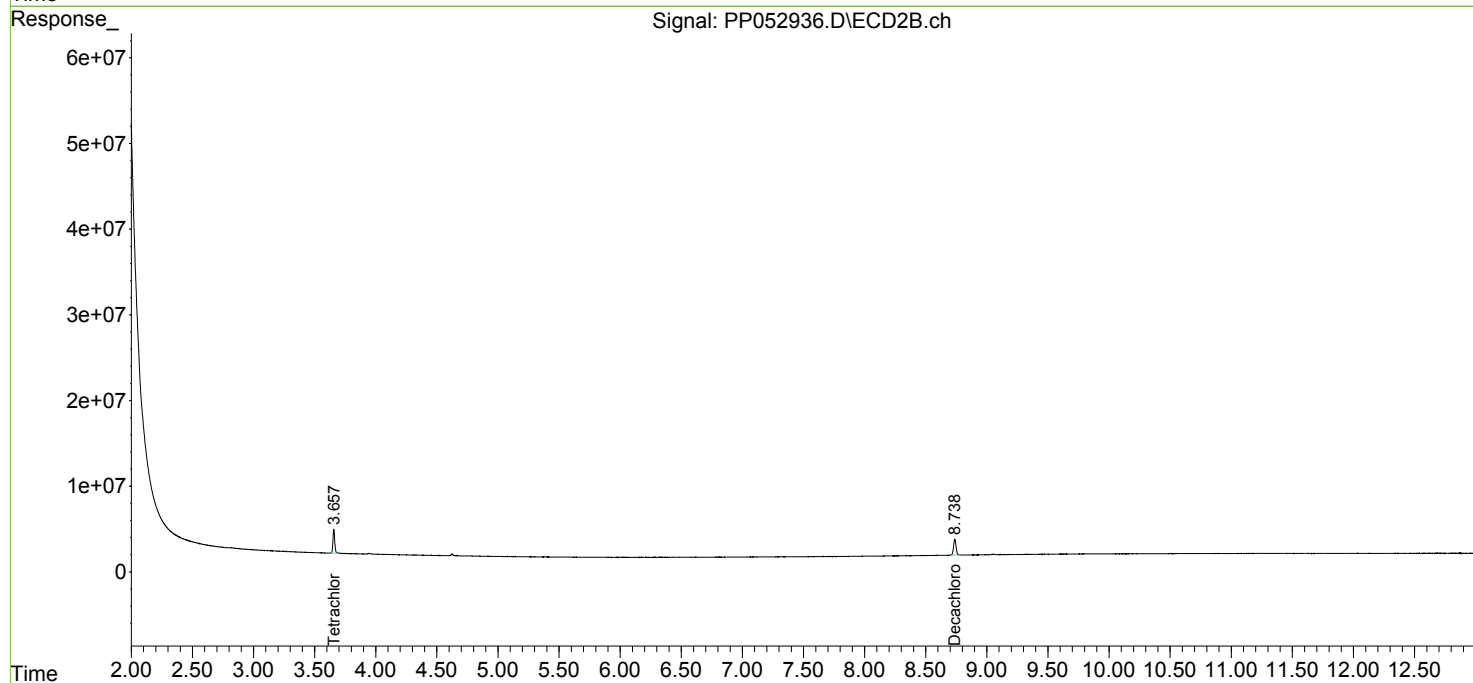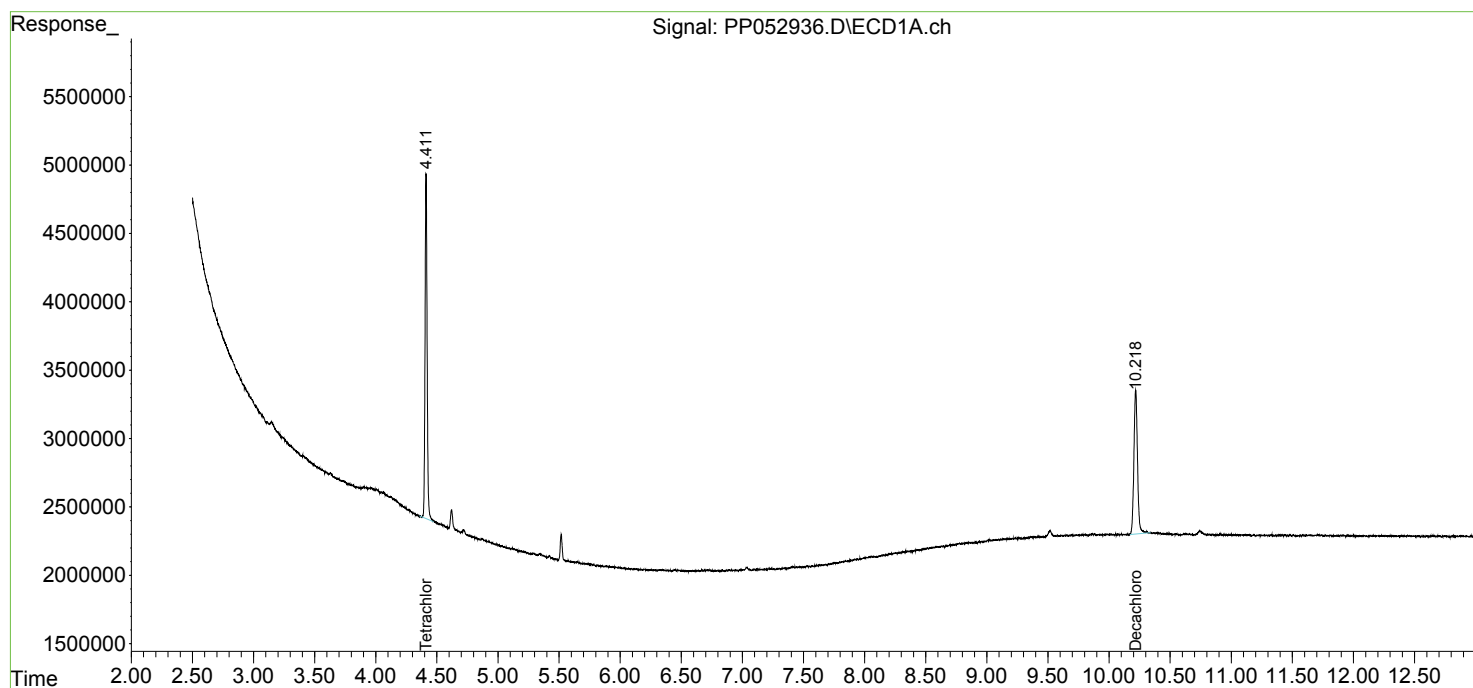


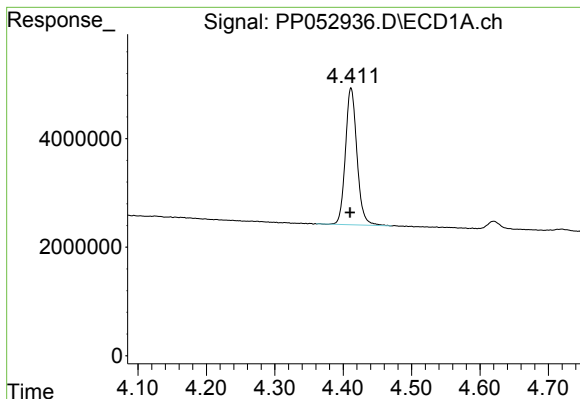

#1 Tetrachloro-m-xylene


R.T.: 4.412 min
Delta R.T.: 0.002 min
Response: 29460184
Conc: 13.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
CMS-WATERPIT-1028

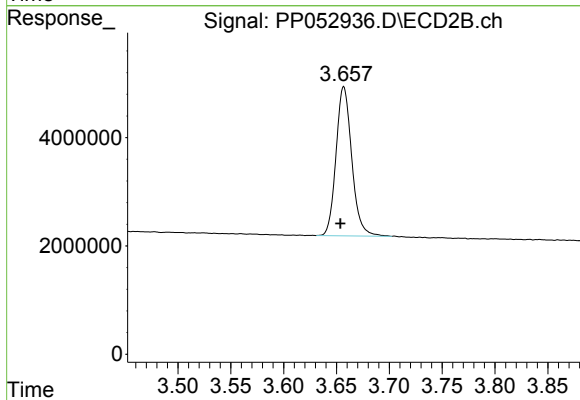


#1 Tetrachloro-m-xylene

R.T.: 3.657 min
Delta R.T.: 0.003 min
Response: 28468051
Conc: 15.15 ng/ml

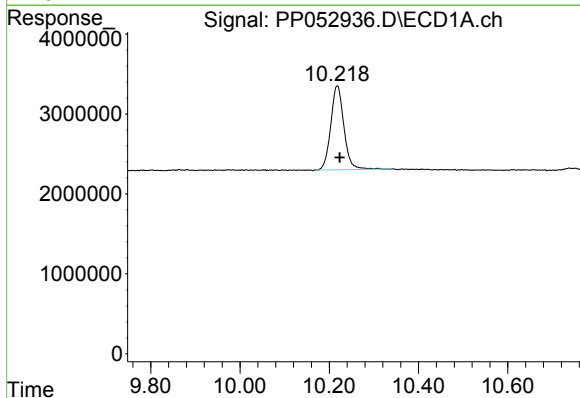

#2 Decachlorobiphenyl

R.T.: 10.218 min
Delta R.T.: -0.006 min
Response: 21448975
Conc: 16.90 ng/ml

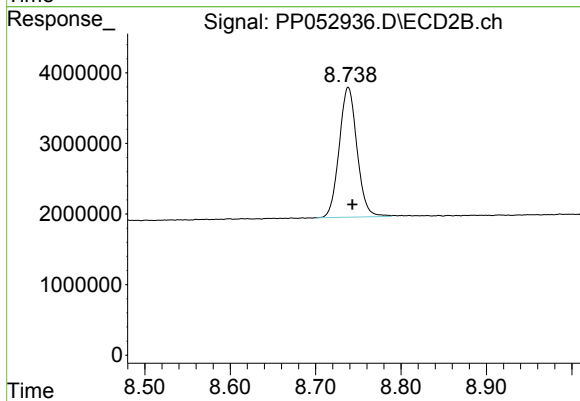

#2 Decachlorobiphenyl

R.T.: 8.738 min
Delta R.T.: -0.005 min
Response: 26638779
Conc: 15.88 ng/ml