

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110220\
 Data File : PP031025.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Nov 2020 9:01
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 01:31:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\AR1262PP110120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 31 02:26:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.791	4.076	2018	3168	0.032	0.055 #
Target Compounds							
36)	L8 AR-1262-1	8.419	0.000	5967	0	2.542	N.D. #
39)	L8 AR-1262-4	9.380f	0.000	2962	0	1.211	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110220\
Data File : PP031025.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Nov 2020 9:01
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 01:31:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\AR1262PP110120.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 31 02:26:29 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

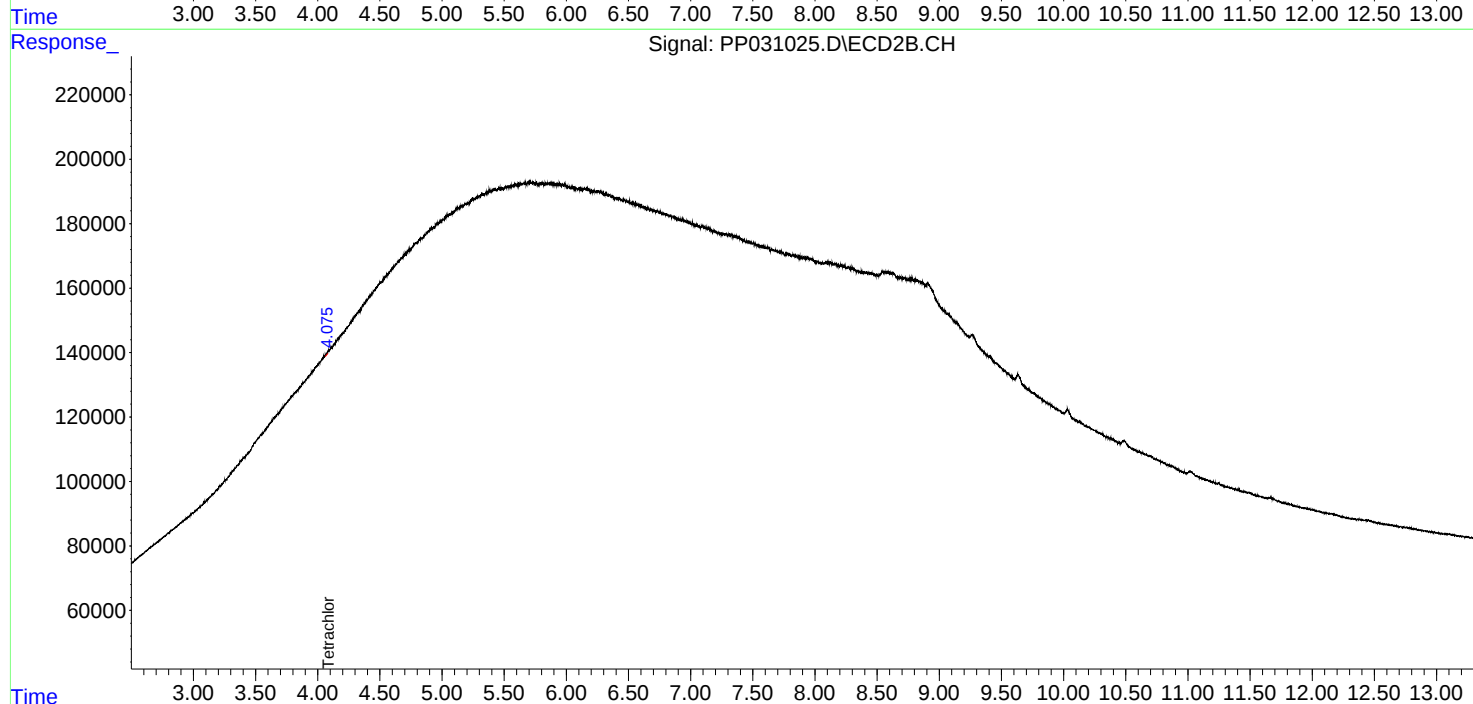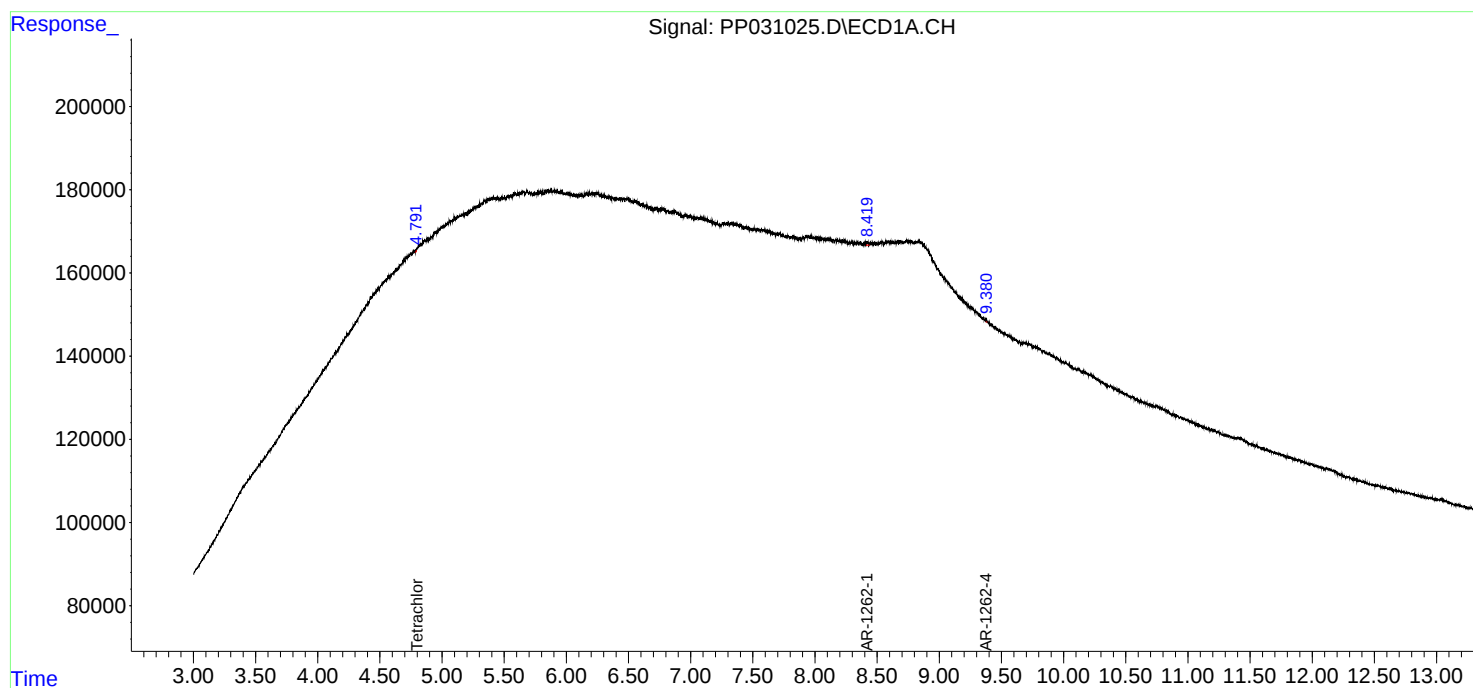


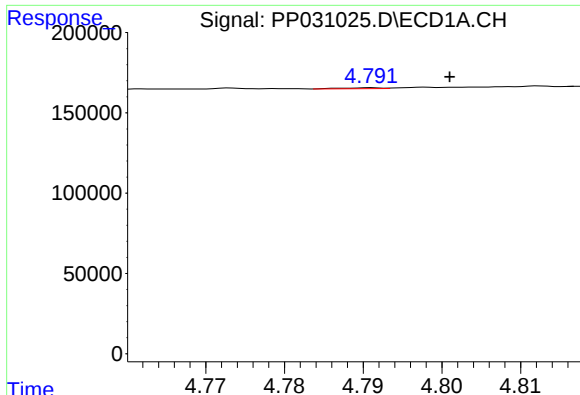

#1 Tetrachloro-m-xylene


R.T.: 4.791 min
Delta R.T.: -0.010 min
Response: 2018
Conc: 0.03 ng/ml

Instrument :
ECD_P
ClientSampleId :

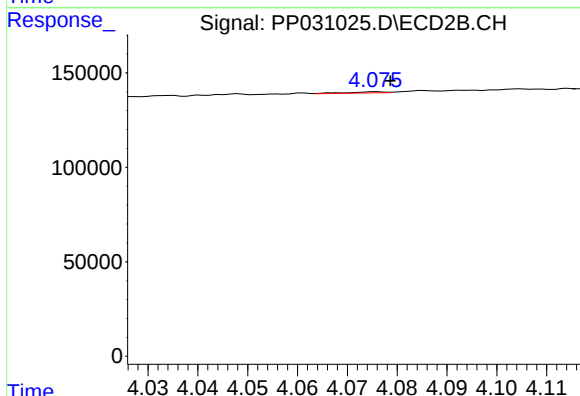


#1 Tetrachloro-m-xylene

R.T.: 4.076 min
Delta R.T.: -0.003 min
Response: 3168
Conc: 0.05 ng/ml

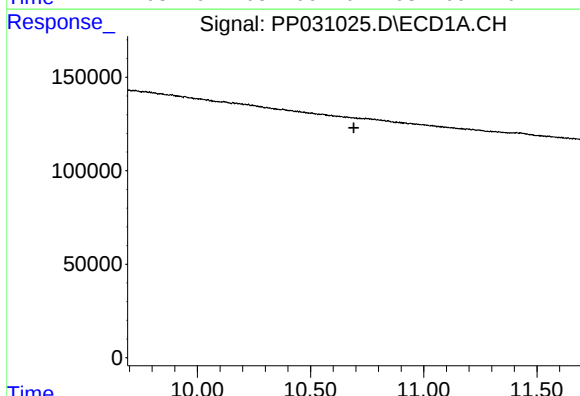


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.691 min
Response: 0
Conc: N.D.

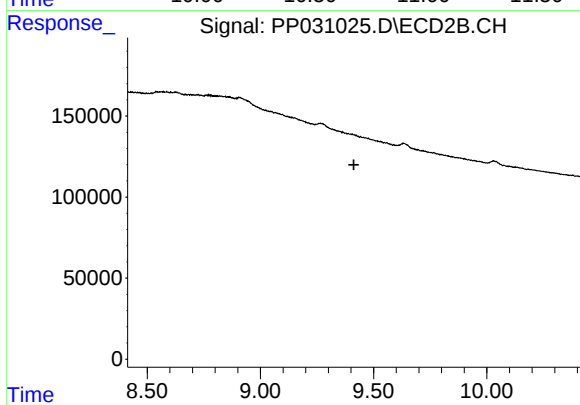

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 9.413 min
Response: 0
Conc: N.D.

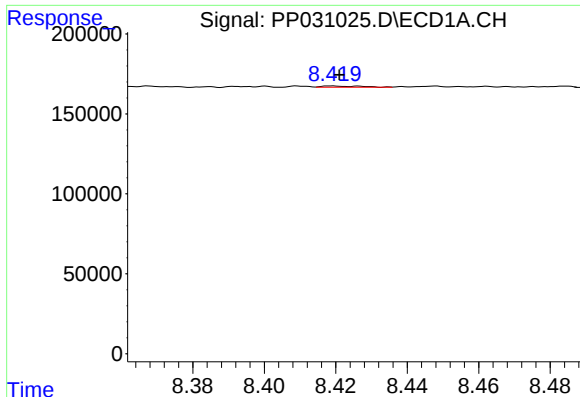

#36 AR-1262-1


R.T.: 8.419 min
Delta R.T.: -0.002 min
Response: 5967
Conc: 2.54 ng/ml

Instrument :
ECD_P
ClientSampleId :

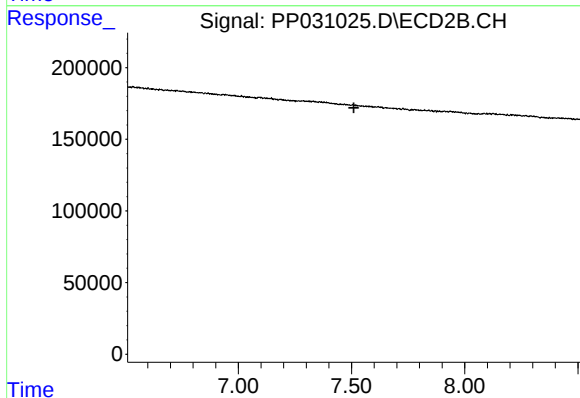


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.510 min
Response: 0
Conc: N.D.

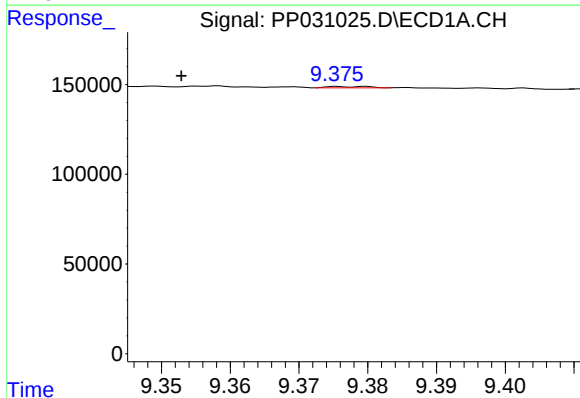

#39 AR-1262-4

R.T.: 9.380 min
Delta R.T.: 0.027 min
Response: 2962
Conc: 1.21 ng/ml

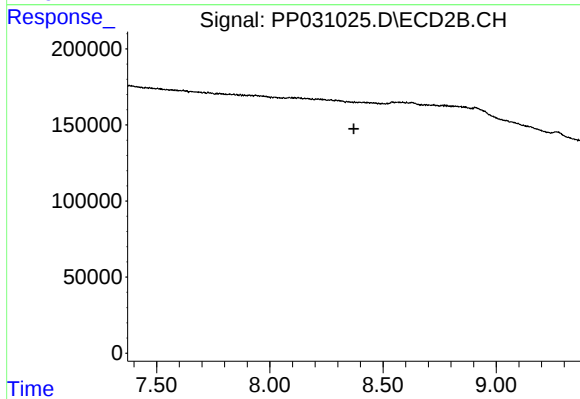

#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 8.371 min
Response: 0
Conc: N.D.