

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110220\
 Data File : PP031033.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Nov 2020 13:00
 Operator : DD\AJ
 Sample : MDL-AR1268-W-11
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-AR1268-W-11

Manual Integrations
 APPROVED

Ankita
 11/3/2020 3:30:09 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 01:35:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\AR1268PP110120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 31 02:37:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.801	4.078	1062563	932343	17.830	17.712
2) SA Decachlor...	10.691	9.410	671760	739949	11.706	11.720
Target Compounds						
41) L9 AR-1268-1	9.263	8.304	121171	120019	24.875	22.310m
42) L9 AR-1268-2	9.354	8.370	118774	114655	24.522	21.719
43) L9 AR-1268-3	9.572	8.579	94694	109201	23.403	24.764
44) L9 AR-1268-4	9.983	8.866	37711	40035	23.480	22.259
45) L9 AR-1268-5	10.374	9.156	285221	314099	22.190	21.978

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110220\
Data File : PP031033.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Nov 2020 13:00
Operator : DD\AJ
Sample : MDL-AR1268-W-11
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
MDL-AR1268-W-11


Manual Integrations
APPROVED

Ankita
11/3/2020 3:30:09 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 01:35:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\AR1268PP110120.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 31 02:37:11 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

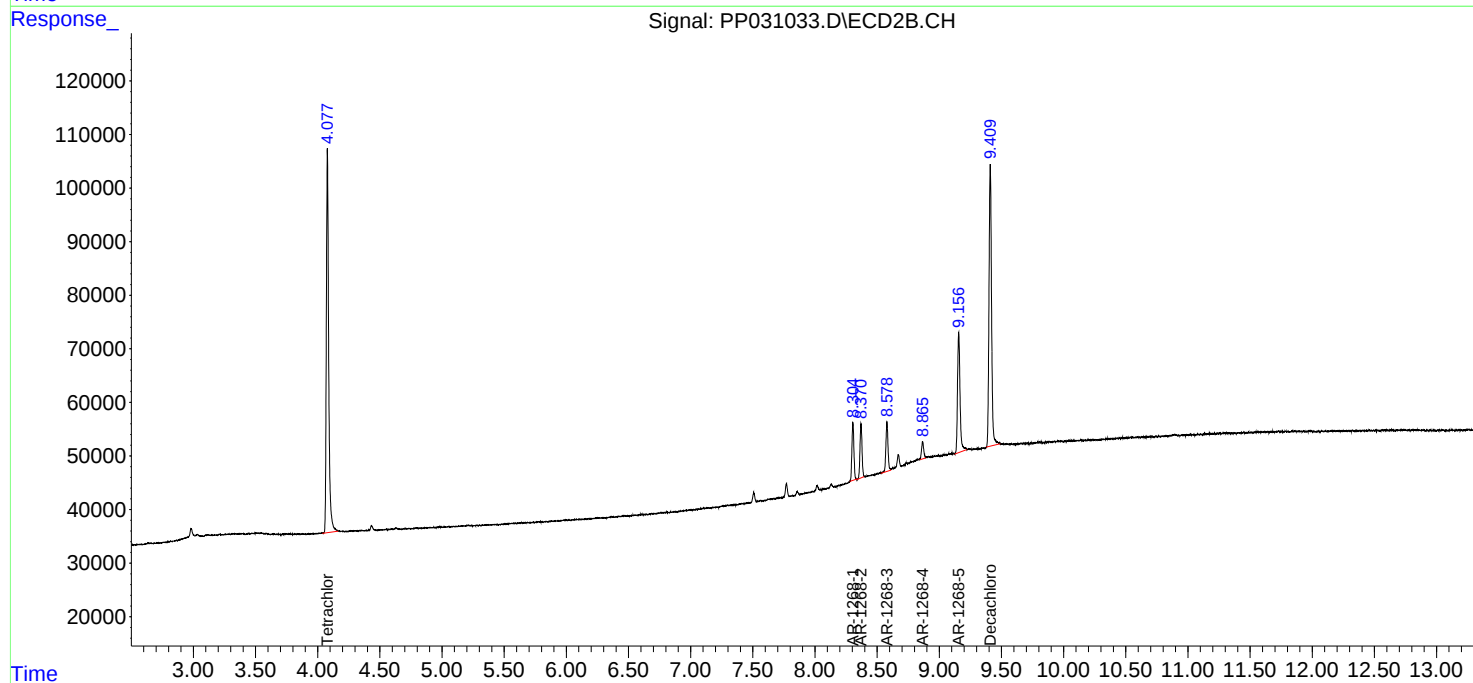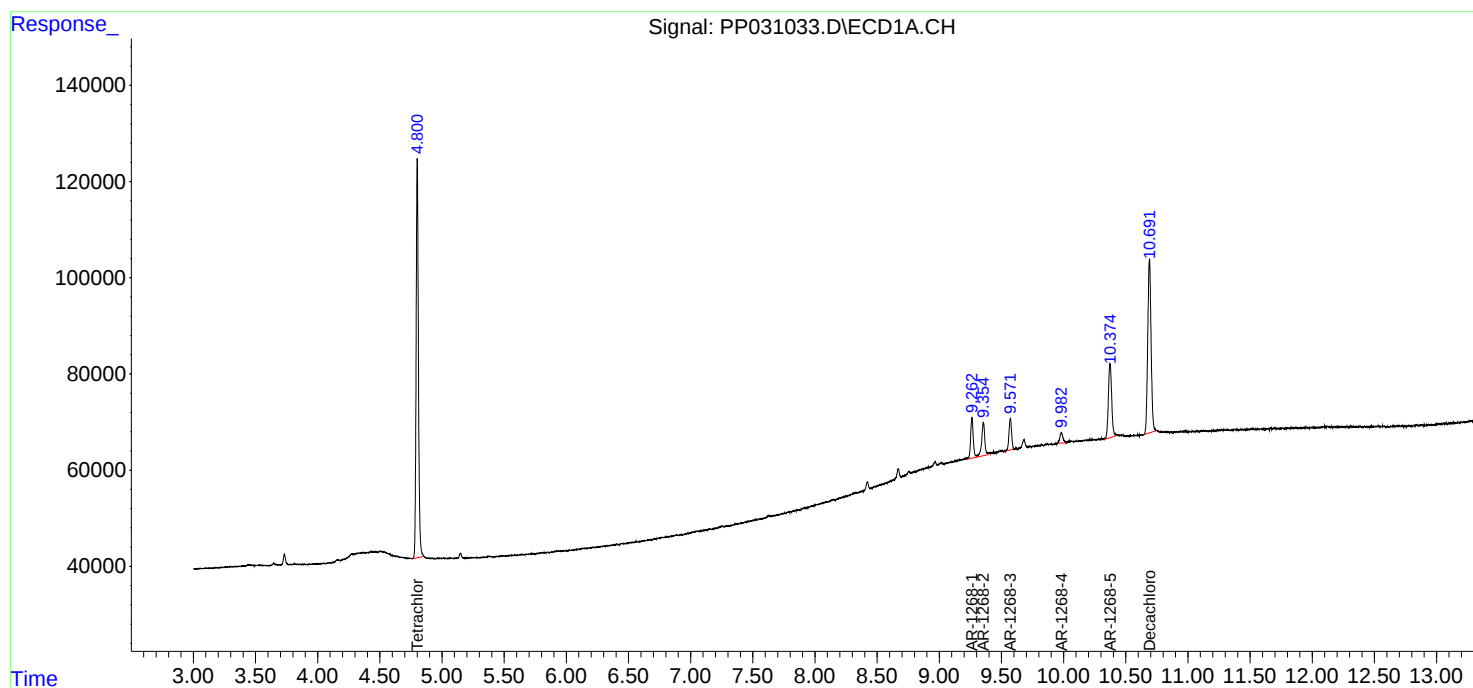

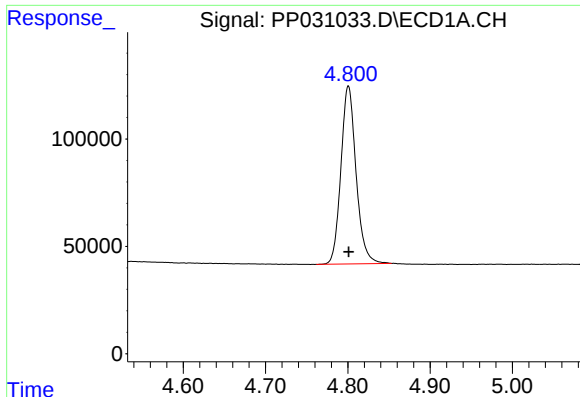


#1 Tetrachloro-m-xylene

R.T.: 4.801 min
Delta R.T.: 0.000 min
Response: 1062563
Conc: 17.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-AR1268-W-11


Manual Integrations
APPROVED

Ankita
11/3/2020 3:30:09 PM

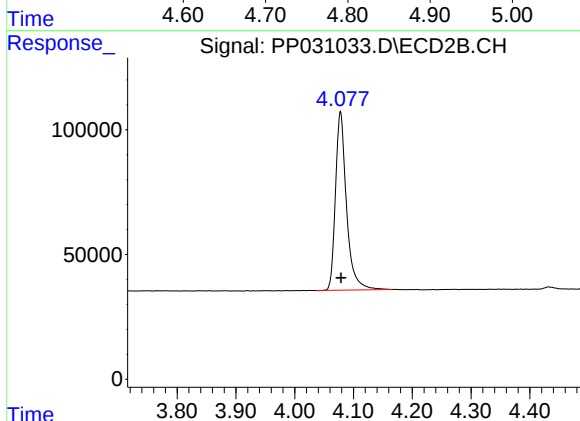


#1 Tetrachloro-m-xylene

R.T.: 4.078 min
Delta R.T.: 0.000 min
Response: 932343
Conc: 17.71 ng/ml

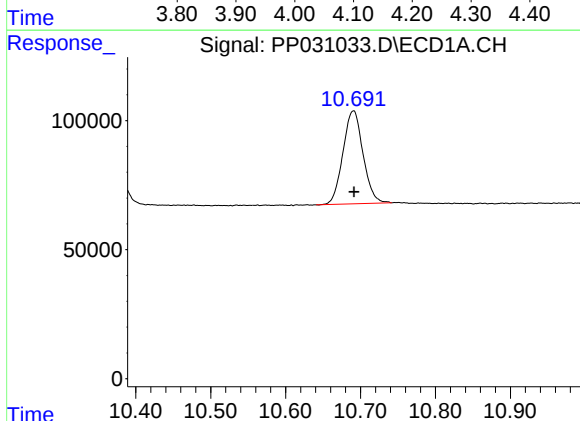


#2 Decachlorobiphenyl

R.T.: 10.691 min
Delta R.T.: 0.000 min
Response: 671760
Conc: 11.71 ng/ml

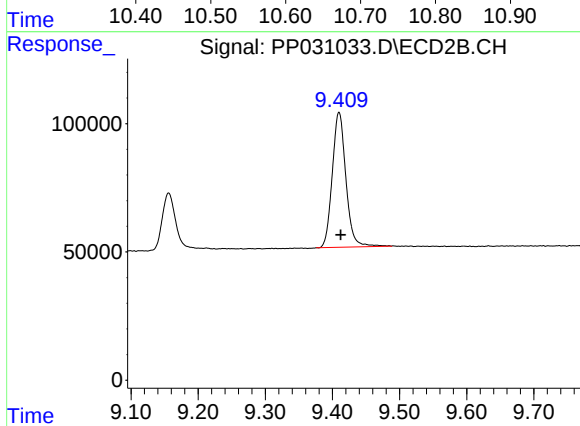

#2 Decachlorobiphenyl

R.T.: 9.410 min
Delta R.T.: -0.002 min
Response: 739949
Conc: 11.72 ng/ml

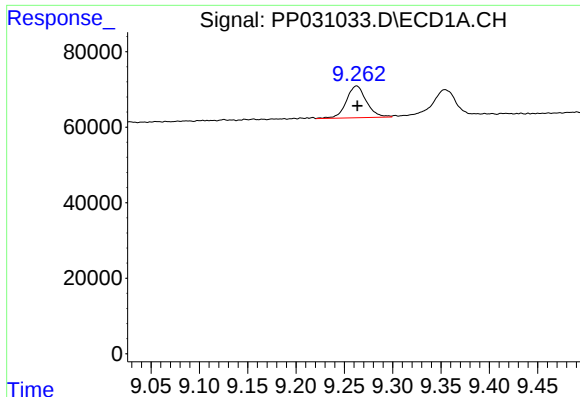


#41 AR-1268-1

R.T.: 9.263 min
Delta R.T.: 0.000 min
Response: 121171
Conc: 24.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-AR1268-W-11


Manual Integrations
APPROVED

Ankita
11/3/2020 3:30:09 PM

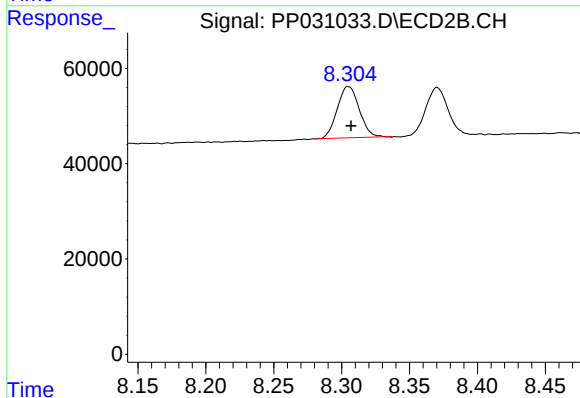


#41 AR-1268-1

R.T.: 8.304 min
Delta R.T.: -0.003 min
Response: 120019
Conc: 22.31 ng/ml m

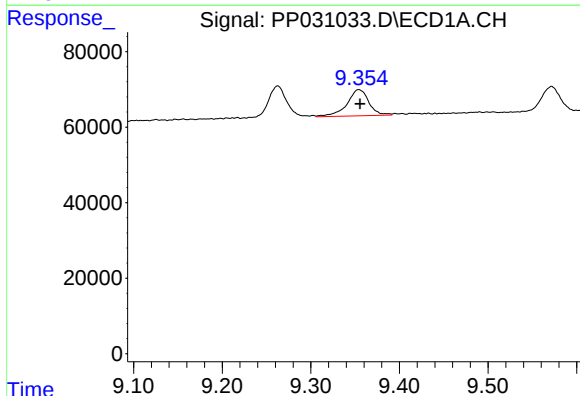


#42 AR-1268-2

R.T.: 9.354 min
Delta R.T.: -0.001 min
Response: 118774
Conc: 24.52 ng/ml

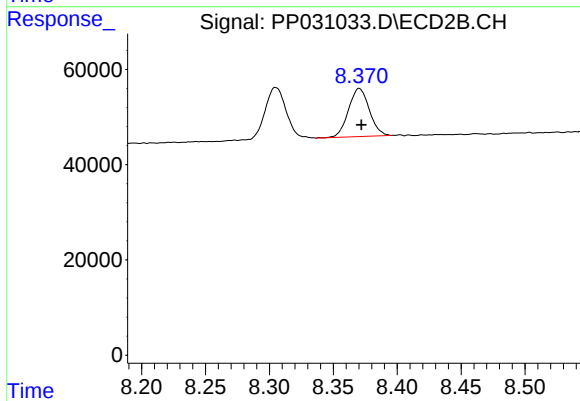

#42 AR-1268-2

R.T.: 8.370 min
Delta R.T.: -0.002 min
Response: 114655
Conc: 21.72 ng/ml

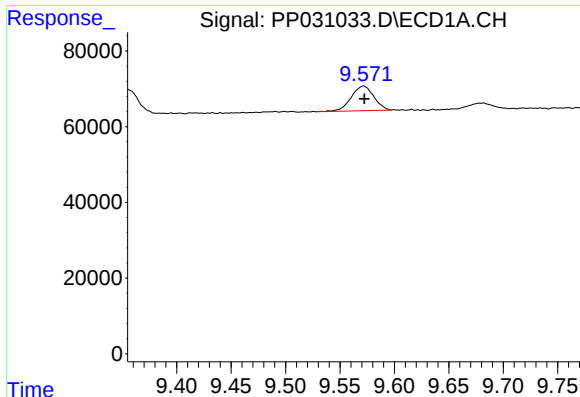


#43 AR-1268-3

R.T.: 9.572 min
Delta R.T.: 0.000 min
Response: 94694
Conc: 23.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-AR1268-W-11


Manual Integrations
APPROVED

Ankita
11/3/2020 3:30:09 PM

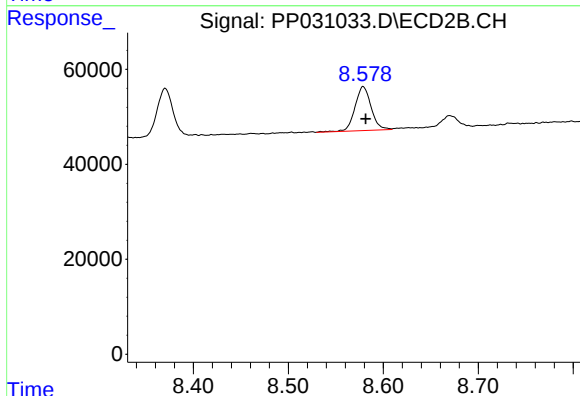


#43 AR-1268-3

R.T.: 8.579 min
Delta R.T.: -0.003 min
Response: 109201
Conc: 24.76 ng/ml

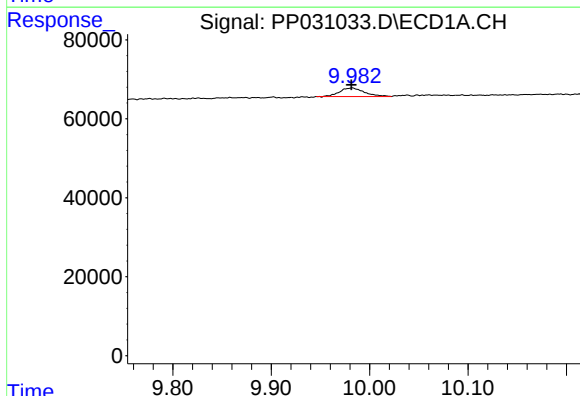


#44 AR-1268-4

R.T.: 9.983 min
Delta R.T.: 0.001 min
Response: 37711
Conc: 23.48 ng/ml

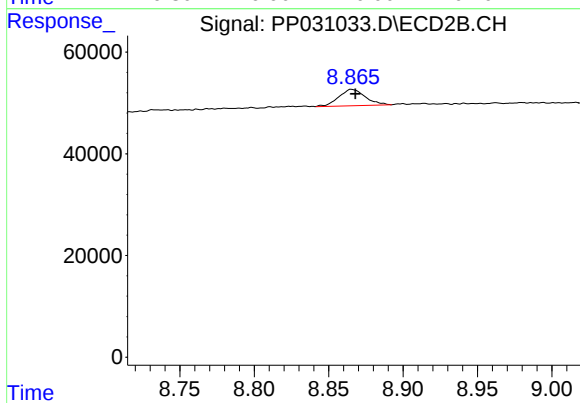

#44 AR-1268-4

R.T.: 8.866 min
Delta R.T.: -0.002 min
Response: 40035
Conc: 22.26 ng/ml

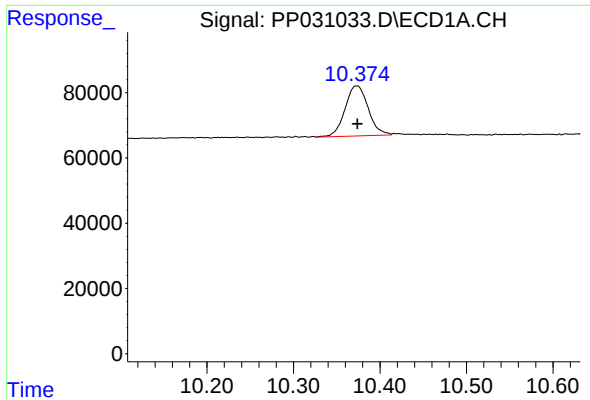


#45 AR-1268-5

R.T.: 10.374 min
Delta R.T.: 0.000 min
Response: 285221
Conc: 22.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-AR1268-W-11

Manual Integrations
APPROVED

Ankita
11/3/2020 3:30:09 PM

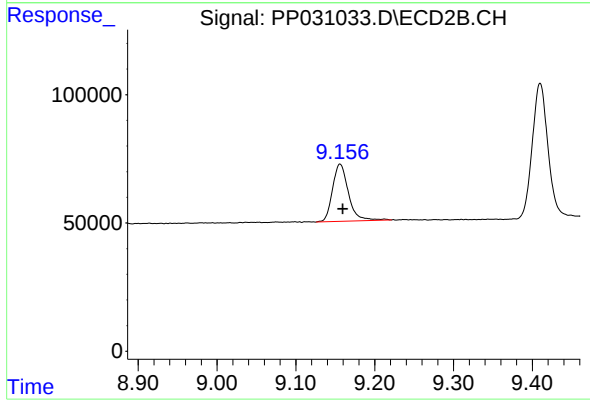

#45 AR-1268-5

R.T.: 9.156 min
Delta R.T.: -0.003 min
Response: 314099
Conc: 21.98 ng/ml