

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110220\
 Data File : PP031040.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Nov 2020 15:00
 Operator : DD\AJ
 Sample : MDL-AR1262-S-4
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-AR1262-S-4

Manual Integrations
 APPROVED

Ankita
 11/3/2020 3:30:14 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 01:33:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\AR1262PP110120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 31 02:26:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.801	4.078	1345301	1174725	21.087	20.335
2) SA Decachlor...	10.693	9.410	779699	825146	20.995	20.867
Target Compounds						
36) L8 AR-1262-1	8.421	7.508	65417	73765	27.871m	28.255
37) L8 AR-1262-2	8.965	8.017	114613	127995	27.062	27.179
38) L8 AR-1262-3	9.266	8.306	86642	55317	29.010m	27.855
39) L8 AR-1262-4	9.354	8.370	64170	96523	26.243m	26.692
40) L8 AR-1262-5	9.983	8.868	37737	40733	24.127	24.719

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110220\
Data File : PP031040.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Nov 2020 15:00
Operator : DD\AJ
Sample : MDL-AR1262-S-4
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
MDL-AR1262-S-4


Manual Integrations
APPROVED

Ankita
11/3/2020 3:30:14 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 01:33:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\AR1262PP110120.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 31 02:26:29 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

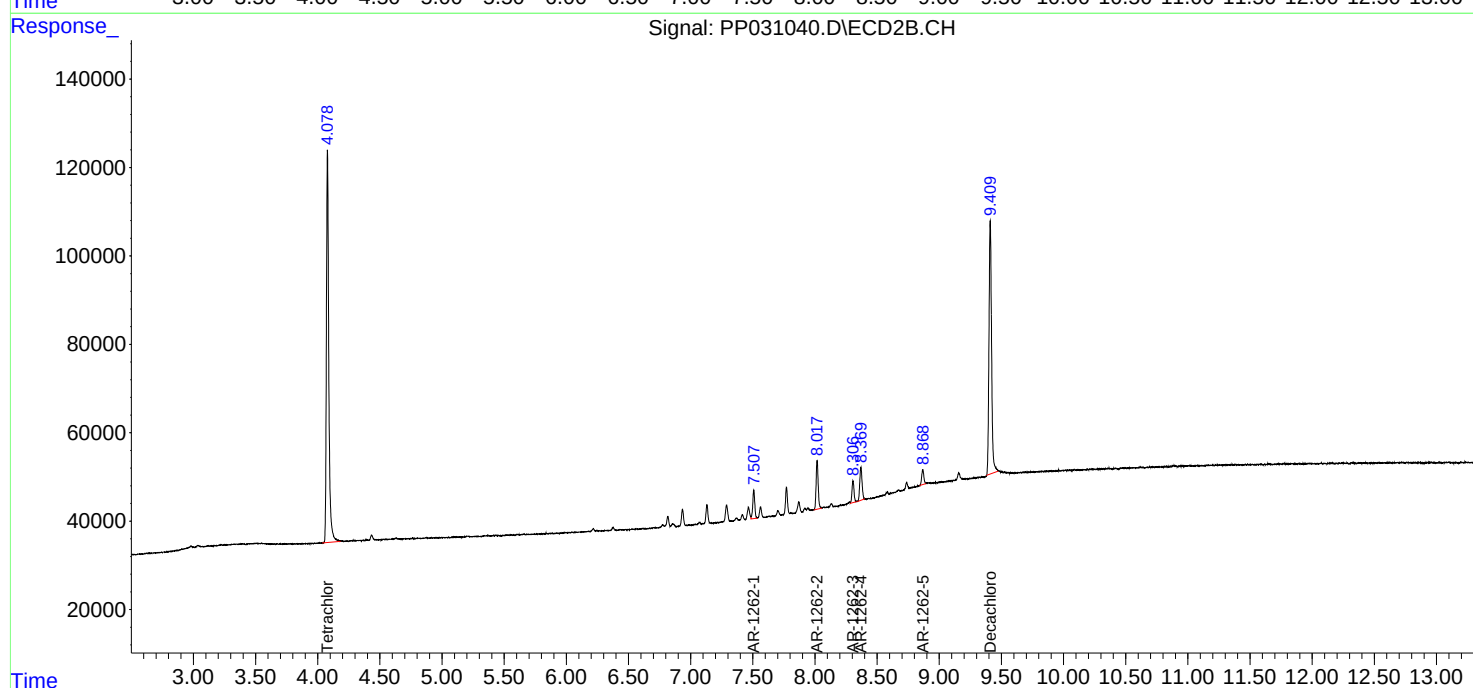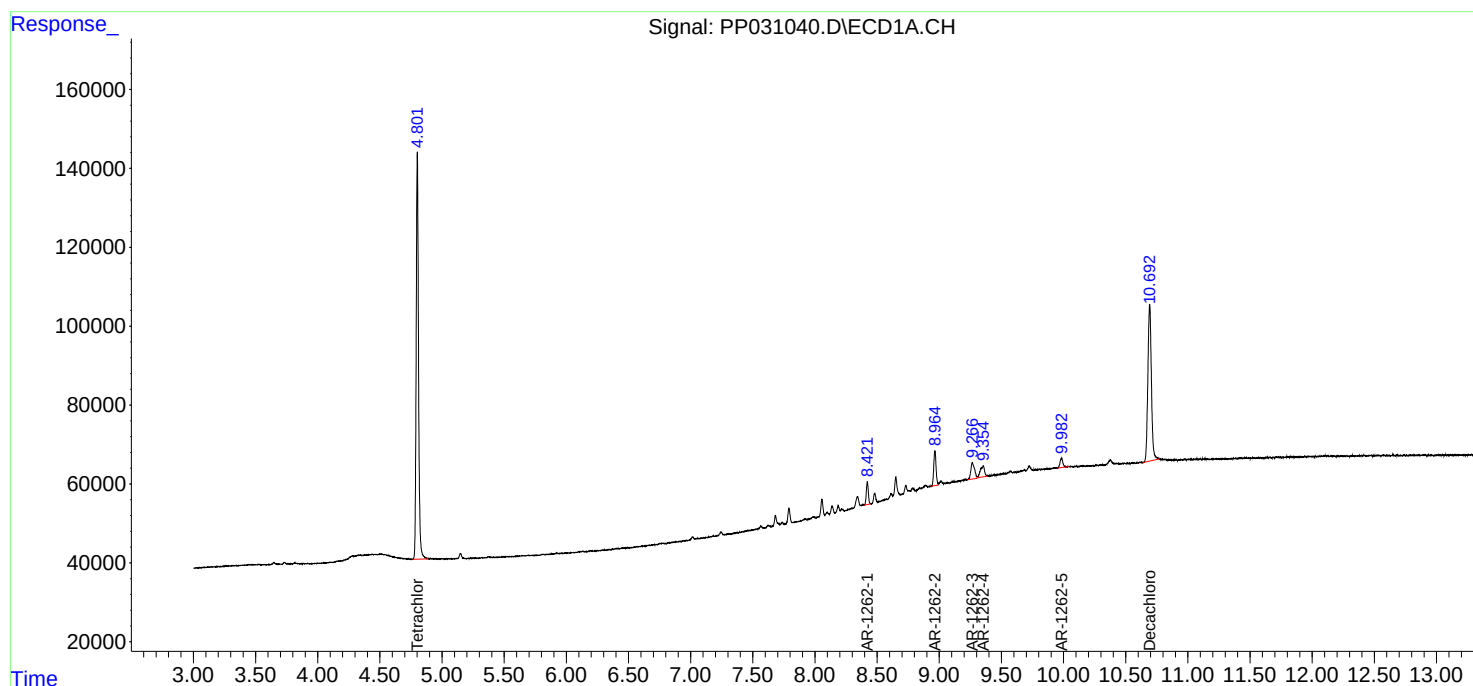

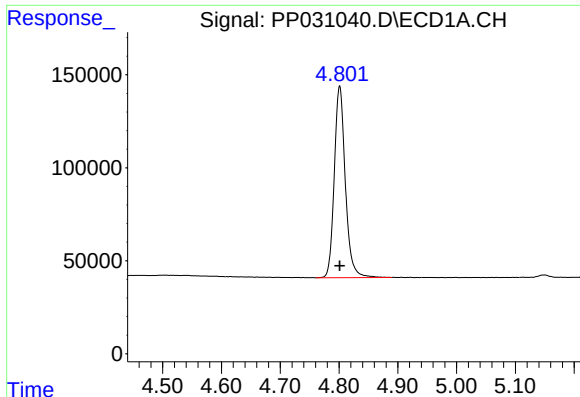


#1 Tetrachloro-m-xylene

R.T.: 4.801 min
Delta R.T.: 0.000 min
Response: 1345301
Conc: 21.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-AR1262-S-4


Manual Integrations
APPROVED

Ankita
11/3/2020 3:30:14 PM

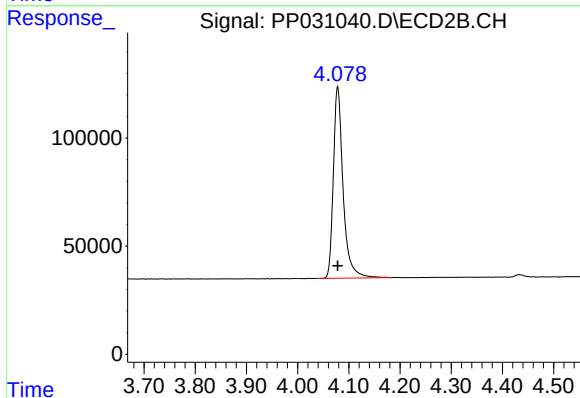


#1 Tetrachloro-m-xylene

R.T.: 4.078 min
Delta R.T.: 0.000 min
Response: 1174725
Conc: 20.33 ng/ml

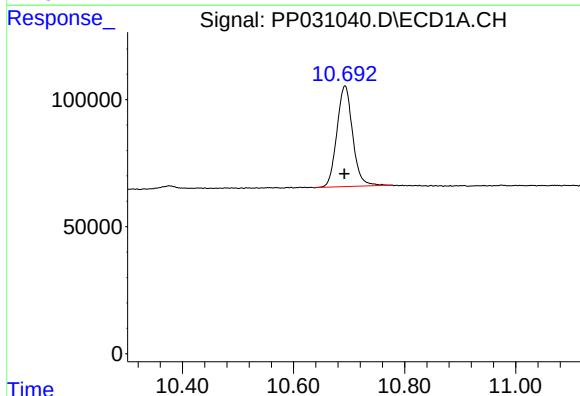


#2 Decachlorobiphenyl

R.T.: 10.693 min
Delta R.T.: 0.001 min
Response: 779699
Conc: 21.00 ng/ml

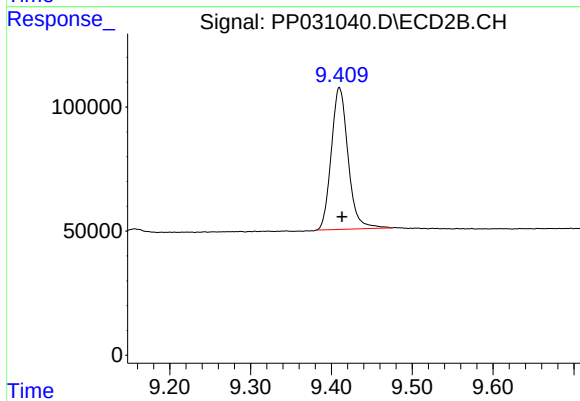

#2 Decachlorobiphenyl

R.T.: 9.410 min
Delta R.T.: -0.003 min
Response: 825146
Conc: 20.87 ng/ml

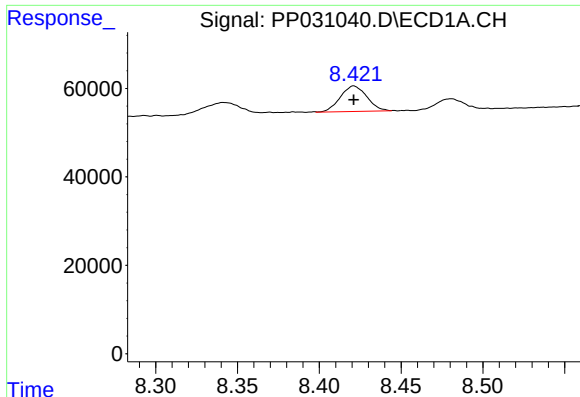


#36 AR-1262-1

R.T.: 8.421 min
Delta R.T.: 0.000 min
Response: 65417
Conc: 27.87 ng/ml m

Instrument :
ECD_P
ClientSampleId :
MDL-AR1262-S-4


Manual Integrations
APPROVED

Ankita
11/3/2020 3:30:14 PM

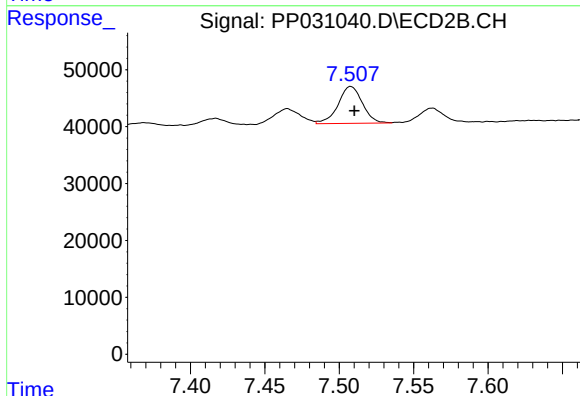


#36 AR-1262-1

R.T.: 7.508 min
Delta R.T.: -0.002 min
Response: 73765
Conc: 28.25 ng/ml

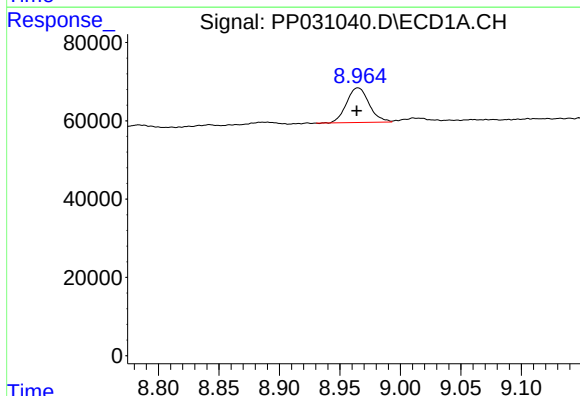


#37 AR-1262-2

R.T.: 8.965 min
Delta R.T.: 0.001 min
Response: 114613
Conc: 27.06 ng/ml

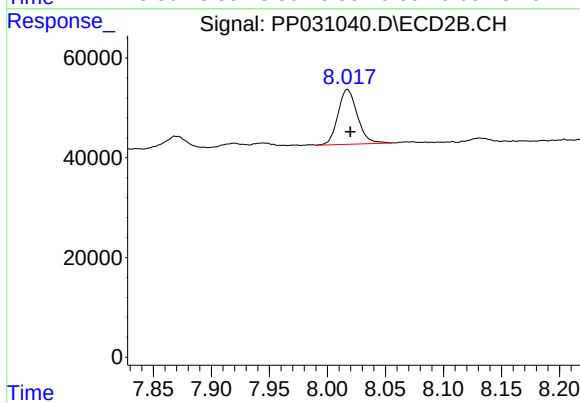

#37 AR-1262-2

R.T.: 8.017 min
Delta R.T.: -0.002 min
Response: 127995
Conc: 27.18 ng/ml

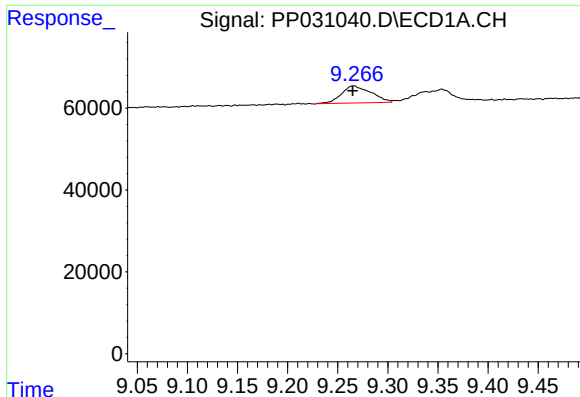


#38 AR-1262-3

R.T.: 9.266 min
Delta R.T.: 0.001 min
Response: 86642
Conc: 29.01 ng/ml m

Instrument :
ECD_P
ClientSampleId :
MDL-AR1262-S-4


Manual Integrations
APPROVED

Ankita
11/3/2020 3:30:14 PM

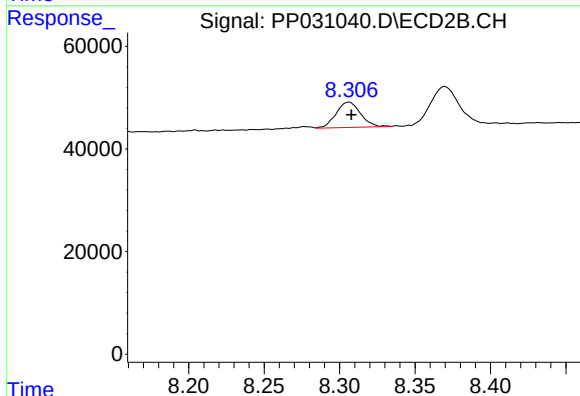


#38 AR-1262-3

R.T.: 8.306 min
Delta R.T.: -0.002 min
Response: 55317
Conc: 27.85 ng/ml

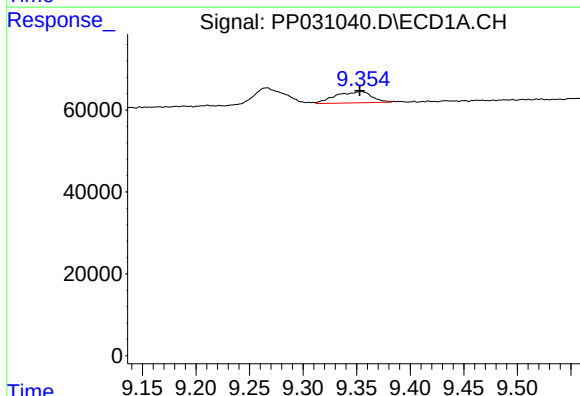


#39 AR-1262-4

R.T.: 9.354 min
Delta R.T.: 0.000 min
Response: 64170
Conc: 26.24 ng/ml m

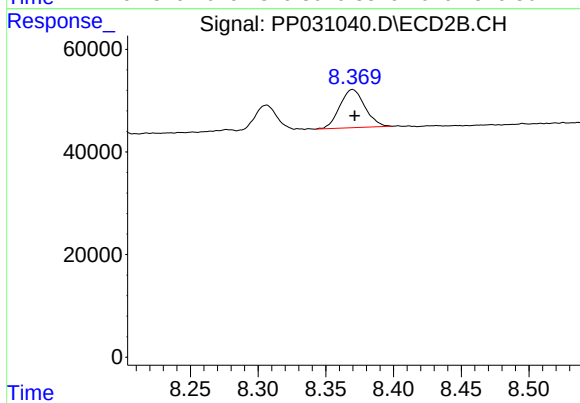

#39 AR-1262-4

R.T.: 8.370 min
Delta R.T.: -0.002 min
Response: 96523
Conc: 26.69 ng/ml

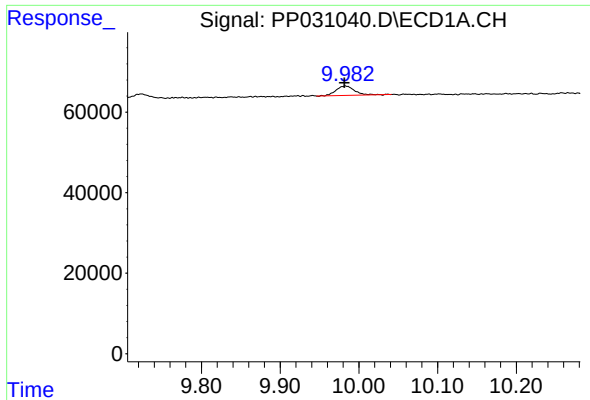


#40 AR-1262-5

R.T.: 9.983 min
Delta R.T.: 0.001 min
Response: 37737
Conc: 24.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-AR1262-S-4

Manual Integrations
APPROVED

Ankita
11/3/2020 3:30:14 PM

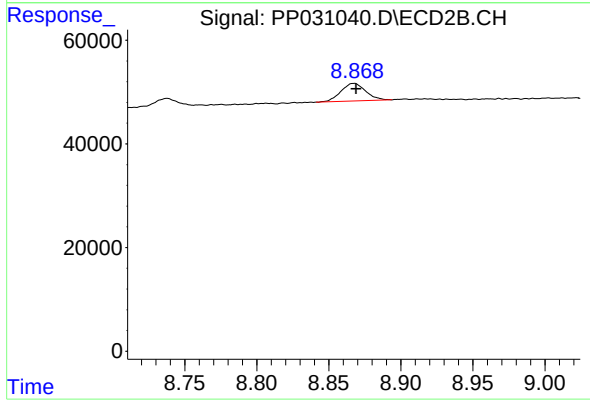

#40 AR-1262-5

R.T.: 8.868 min
Delta R.T.: -0.001 min
Response: 40733
Conc: 24.72 ng/ml