

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110220\
 Data File : PP031041.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Nov 2020 15:18
 Operator : DD\AJ
 Sample : MDL-AR1262-S-5
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-AR1262-S-5

Manual Integrations
 APPROVED

Ankita
 11/3/2020 3:30:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 15:21:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\AR1268PP110120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 31 02:37:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.805	4.078	1420599	1243527	23.838	23.624
2)	SA Decachlor...	10.695	9.412	818391	895649	14.261	14.186
Target Compounds							
41)	L9 AR-1268-1	9.269	8.307	90077	59863	18.492	11.128 #
42)	L9 AR-1268-2	9.355	8.371	69725	103168	14.395	19.543 #
44)	L9 AR-1268-4	9.984	8.868	38756	41747	24.130	23.211
45)	L9 AR-1268-5	10.377	9.158	11668	21884	0.908	1.531 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110220\
Data File : PP031041.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Nov 2020 15:18
Operator : DD\AJ
Sample : MDL-AR1262-S-5
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
MDL-AR1262-S-5


Manual Integrations
APPROVED

Ankita
11/3/2020 3:30:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 15:21:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\AR1268PP110120.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 31 02:37:11 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

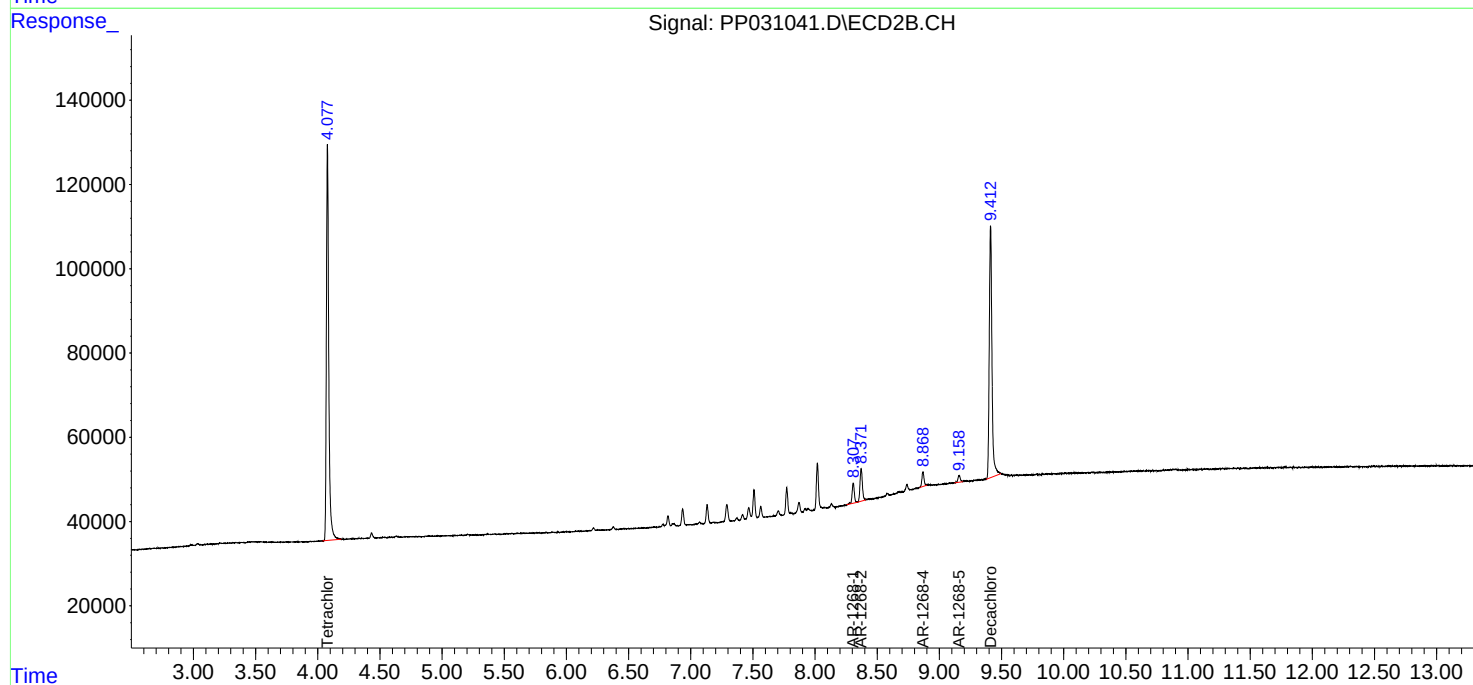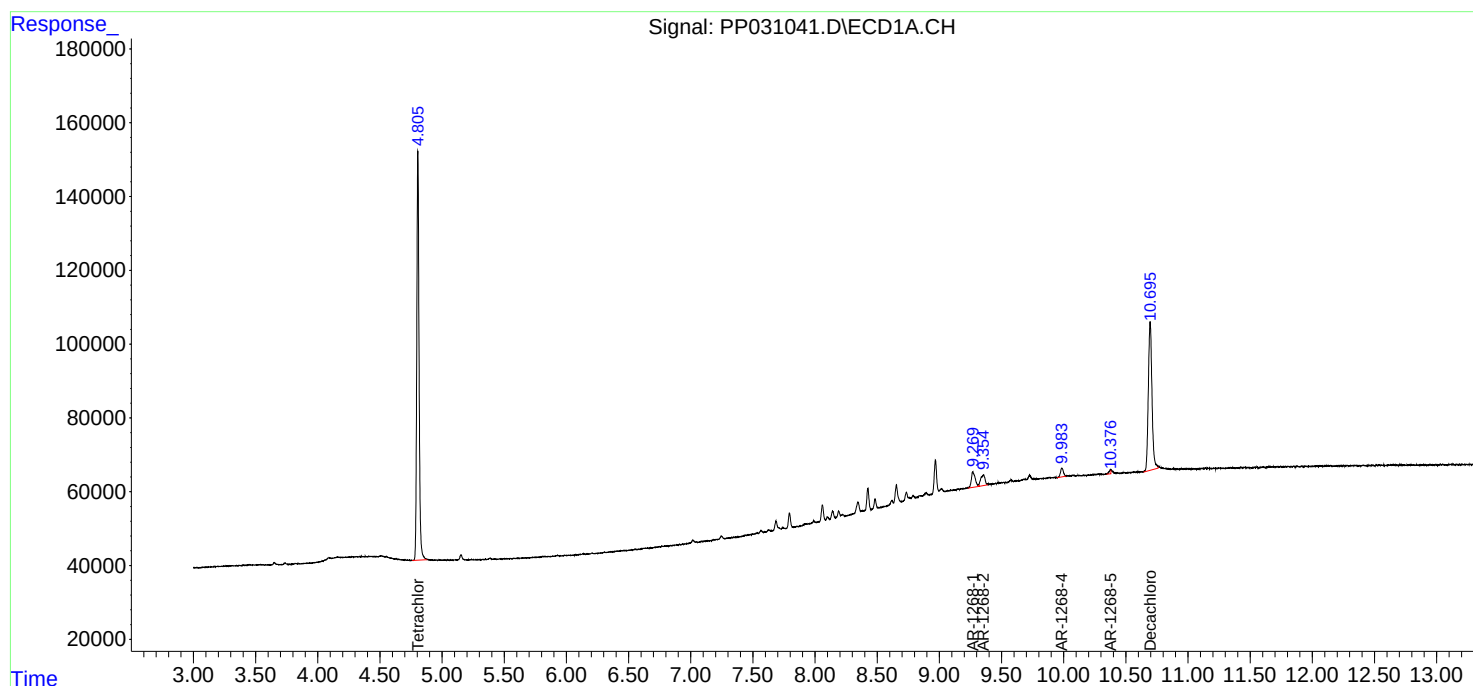

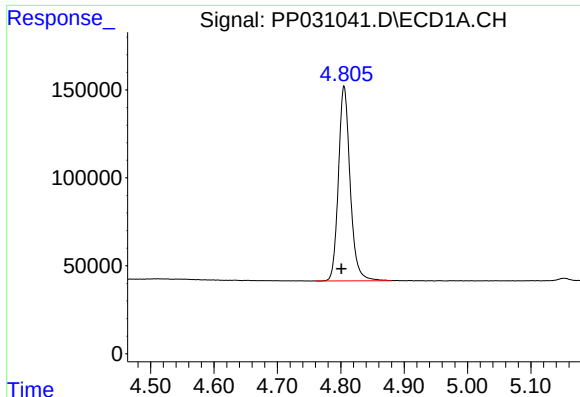


#1 Tetrachloro-m-xylene

R.T.: 4.805 min
Delta R.T.: 0.004 min
Response: 1420599
Conc: 23.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-AR1262-S-5


Manual Integrations
APPROVED

Ankita
11/3/2020 3:30:15 PM

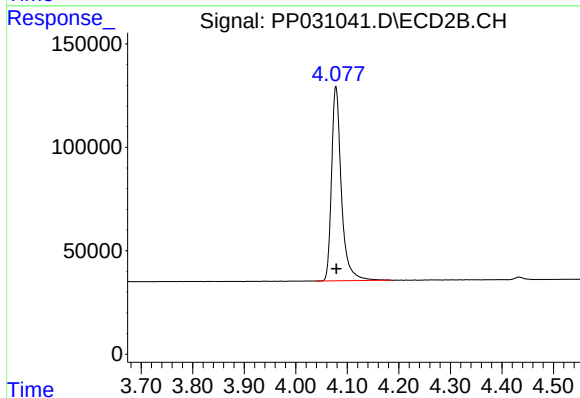


#1 Tetrachloro-m-xylene

R.T.: 4.078 min
Delta R.T.: 0.000 min
Response: 1243527
Conc: 23.62 ng/ml

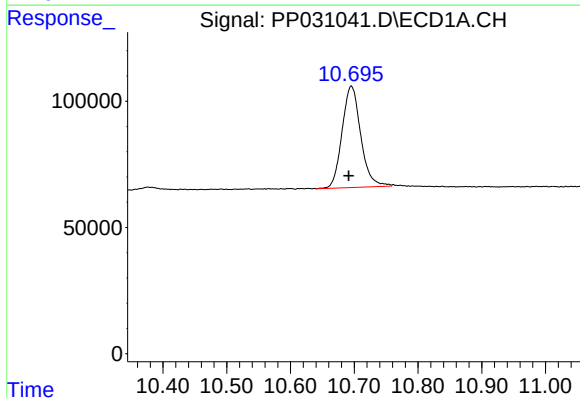


#2 Decachlorobiphenyl

R.T.: 10.695 min
Delta R.T.: 0.004 min
Response: 818391
Conc: 14.26 ng/ml

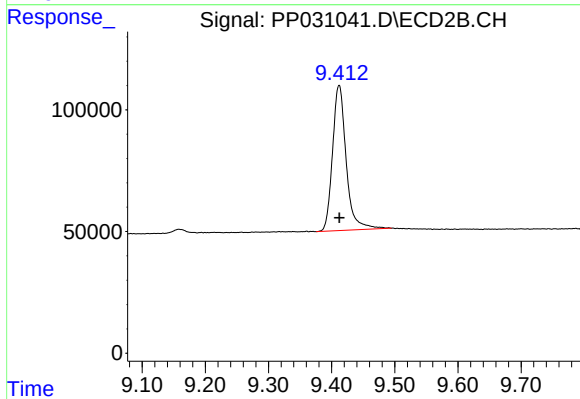

#2 Decachlorobiphenyl

R.T.: 9.412 min
Delta R.T.: 0.000 min
Response: 895649
Conc: 14.19 ng/ml

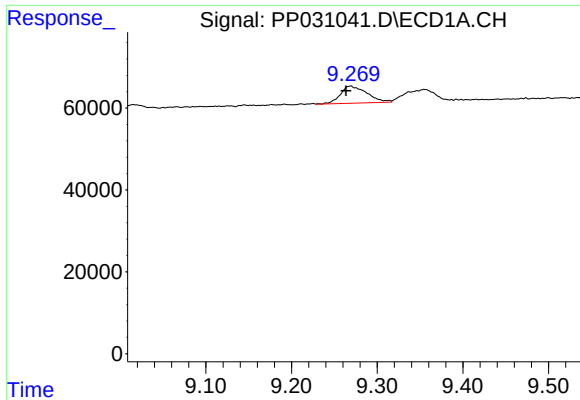


#41 AR-1268-1

R.T.: 9.269 min
Delta R.T.: 0.006 min
Response: 90077
Conc: 18.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-AR1262-S-5


Manual Integrations
APPROVED

Ankita
11/3/2020 3:30:15 PM

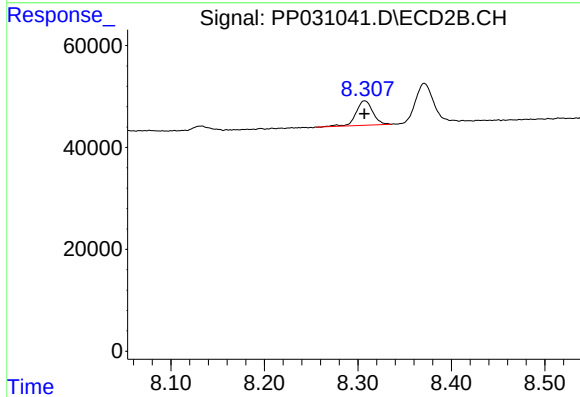


#41 AR-1268-1

R.T.: 8.307 min
Delta R.T.: 0.000 min
Response: 59863
Conc: 11.13 ng/ml

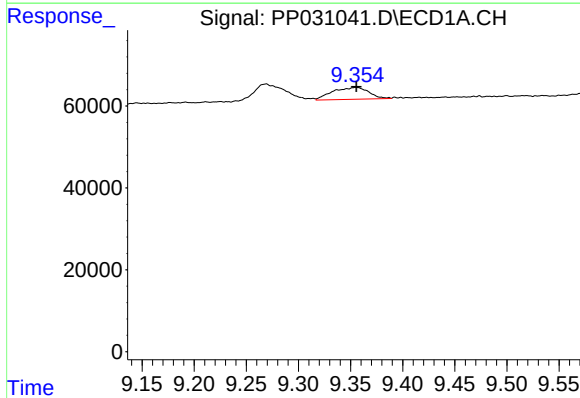


#42 AR-1268-2

R.T.: 9.355 min
Delta R.T.: 0.000 min
Response: 69725
Conc: 14.40 ng/ml

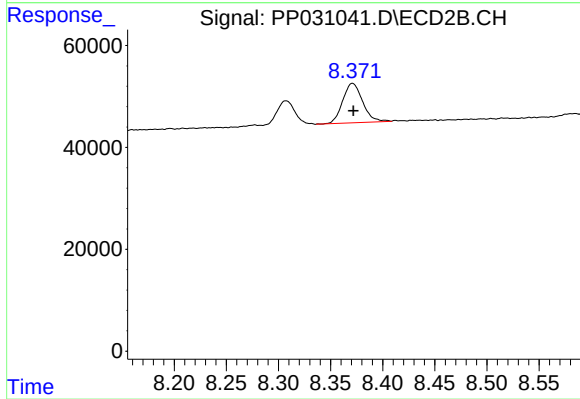

#42 AR-1268-2

R.T.: 8.371 min
Delta R.T.: -0.001 min
Response: 103168
Conc: 19.54 ng/ml

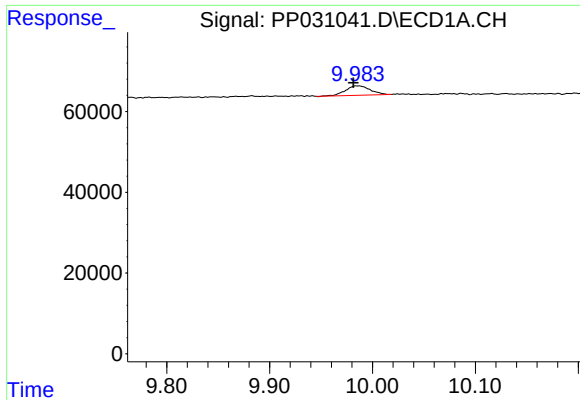


#44 AR-1268-4

R.T.: 9.984 min
Delta R.T.: 0.002 min
Response: 38756
Conc: 24.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-AR1262-S-5


Manual Integrations
APPROVED

Ankita
11/3/2020 3:30:15 PM

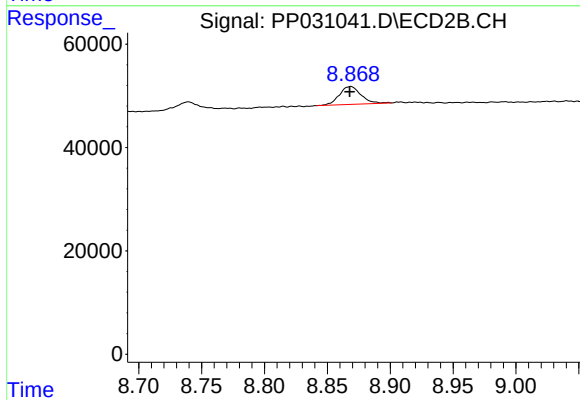


#44 AR-1268-4

R.T.: 8.868 min
Delta R.T.: 0.000 min
Response: 41747
Conc: 23.21 ng/ml

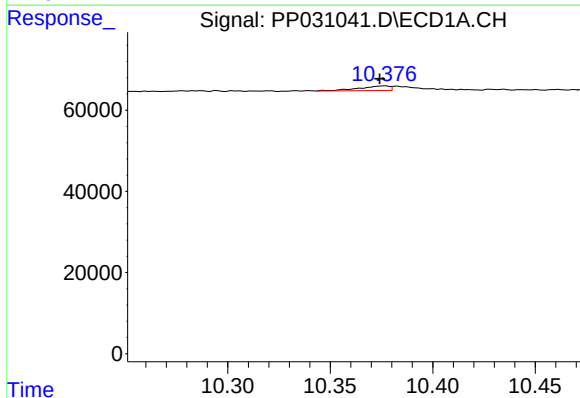

#45 AR-1268-5

R.T.: 10.377 min
Delta R.T.: 0.003 min
Response: 11668
Conc: 0.91 ng/ml

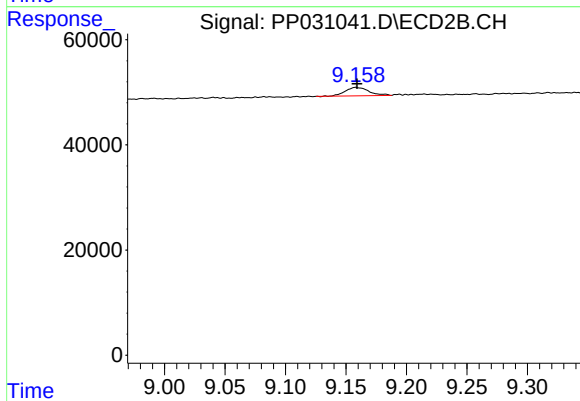

#45 AR-1268-5

R.T.: 9.158 min
Delta R.T.: -0.001 min
Response: 21884
Conc: 1.53 ng/ml