

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110222\
 Data File : PP052976.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2022 10:57
 Operator : YP\AJ
 Sample : N5379-07DL 50X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 135ADL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/03/2022
 Supervised By :Ankita Jodhani 11/03/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 15:30:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 27 04:46:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
26)	L6	AR-1254-1	6.440	5.565	6691807 11457721	88.159 106.699
27)	L6	AR-1254-2	6.660	5.714	17224261 15978473	154.110 167.167
28)	L6	AR-1254-3	7.028	6.124	32079744 41861515	288.202 273.989
29)	L6	AR-1254-4	7.315	6.354	39360436 46294264	558.935 509.881
30)	L6	AR-1254-5	7.735	6.778	67491006 100.9E6	857.212m 725.303

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110222\
Data File : PP052976.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2022 10:57
Operator : YP\AJ
Sample : N5379-07DL 50X
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
135ADL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/03/2022
Supervised By :Ankita Jodhani 11/03/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 15:30:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 27 04:46:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

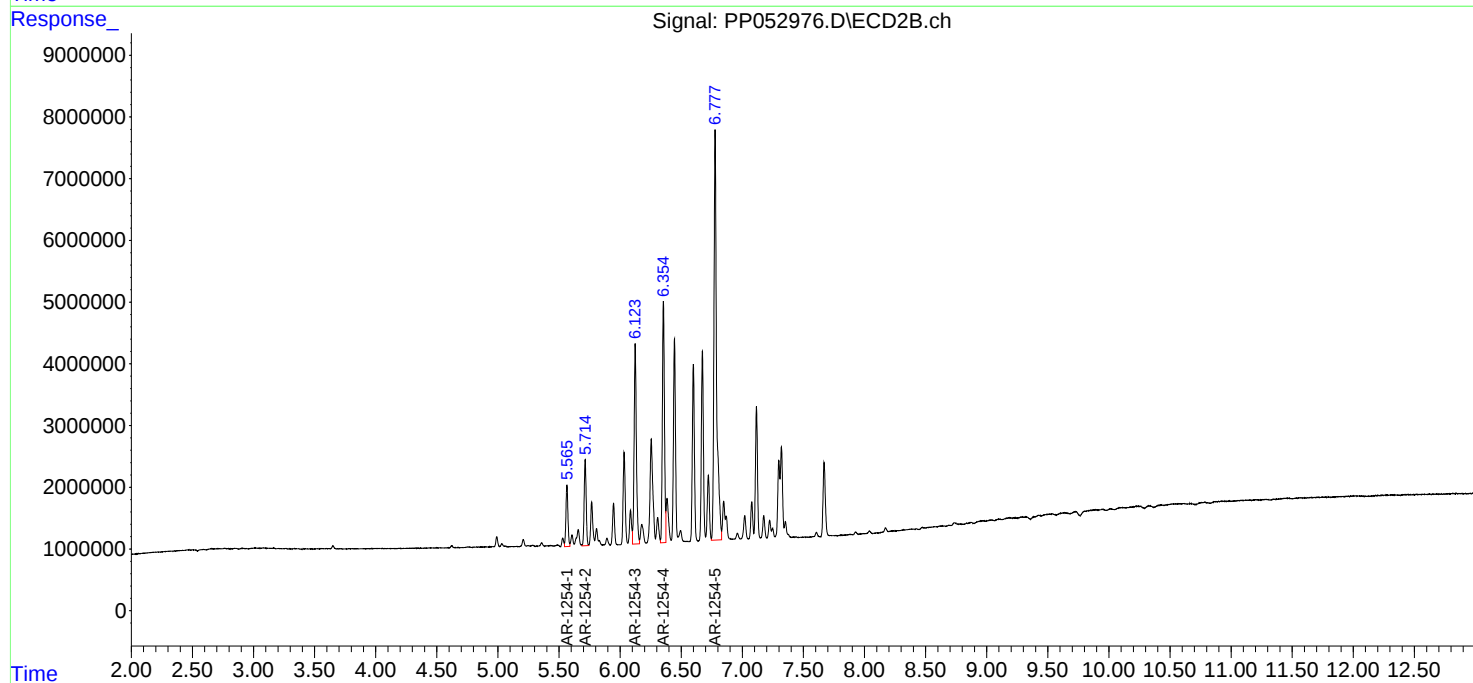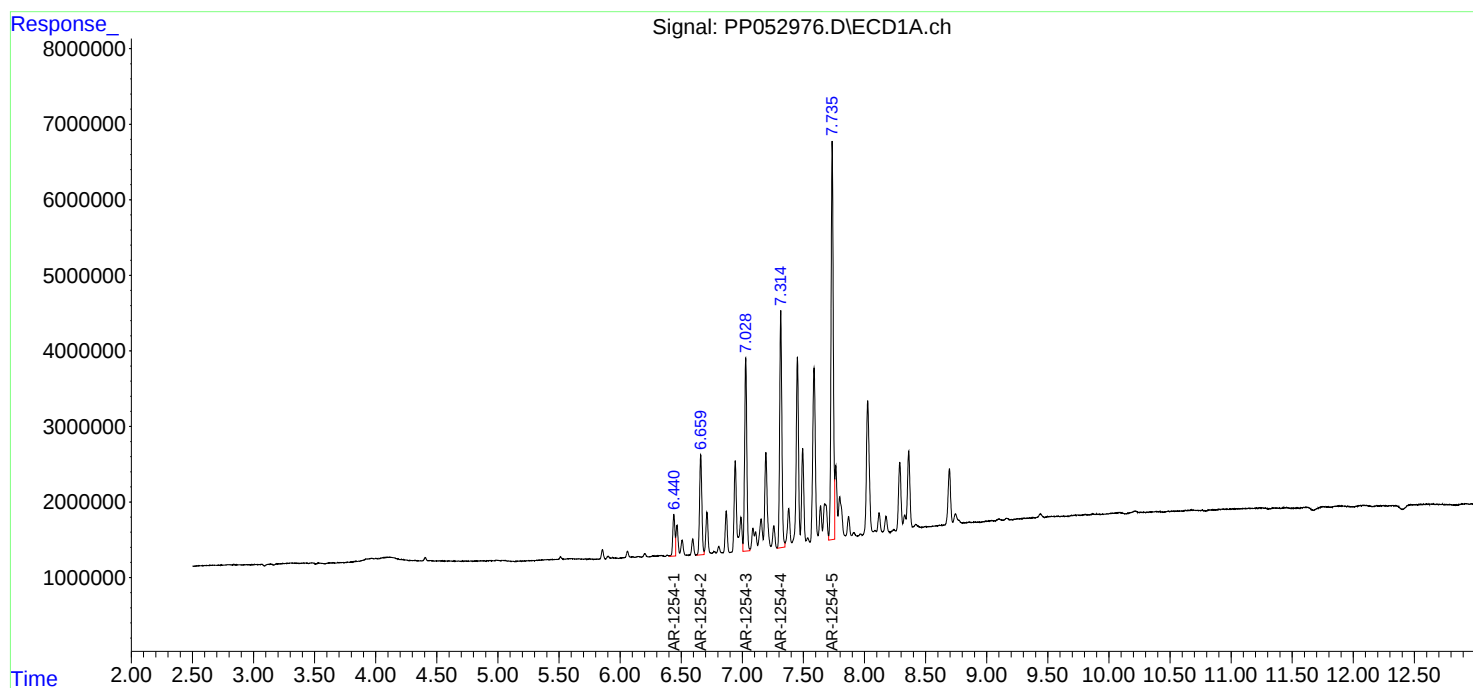

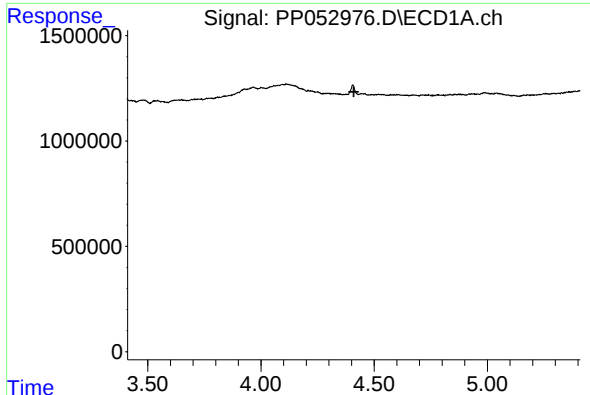

#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.410 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
135ADL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/03/2022
Supervised By :Ankita Jodhani 11/03/2022

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.654 min
Response: 0
Conc: N.D.

#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.224 min
Response: 0
Conc: N.D.

#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.743 min
Response: 0
Conc: N.D.

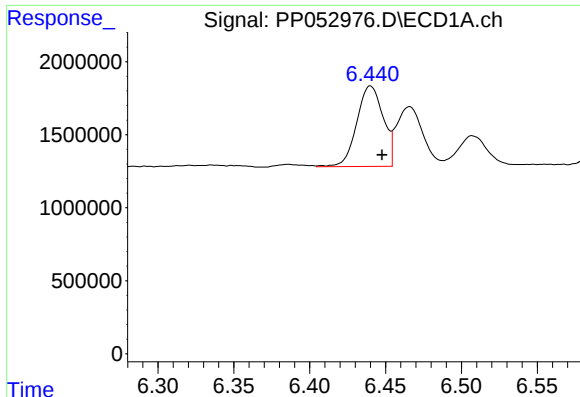


#26 AR-1254-1

R.T.: 6.440 min
Delta R.T.: -0.007 min
Response: 6691807
Conc: 88.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
135ADL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/03/2022
Supervised By :Ankita Jodhani 11/03/2022

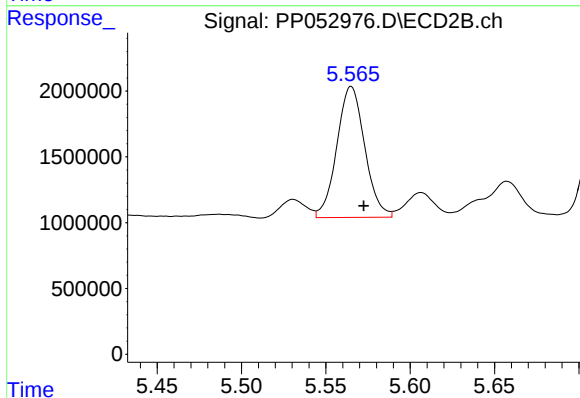


#26 AR-1254-1

R.T.: 5.565 min
Delta R.T.: -0.007 min
Response: 11457721
Conc: 106.70 ng/ml

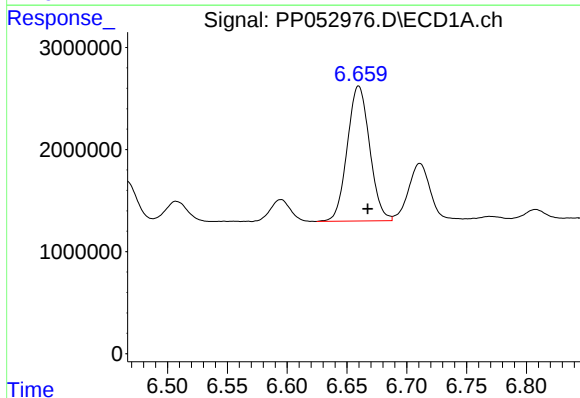


#27 AR-1254-2

R.T.: 6.660 min
Delta R.T.: -0.007 min
Response: 17224261
Conc: 154.11 ng/ml

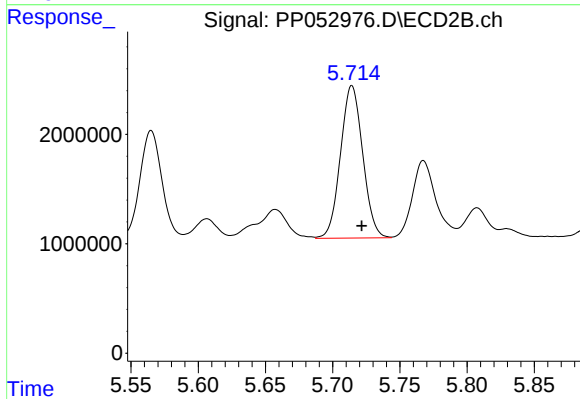

#27 AR-1254-2

R.T.: 5.714 min
Delta R.T.: -0.008 min
Response: 15978473
Conc: 167.17 ng/ml

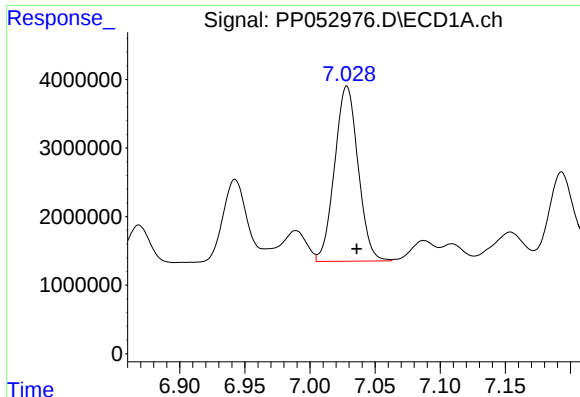


#28 AR-1254-3

R.T.: 7.028 min
Delta R.T.: -0.008 min
Response: 32079744
Conc: 288.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
135ADL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/03/2022
Supervised By :Ankita Jodhani 11/03/2022

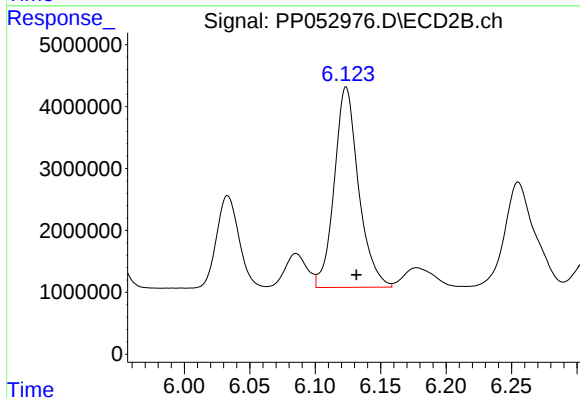


#28 AR-1254-3

R.T.: 6.124 min
Delta R.T.: -0.008 min
Response: 41861515
Conc: 273.99 ng/ml

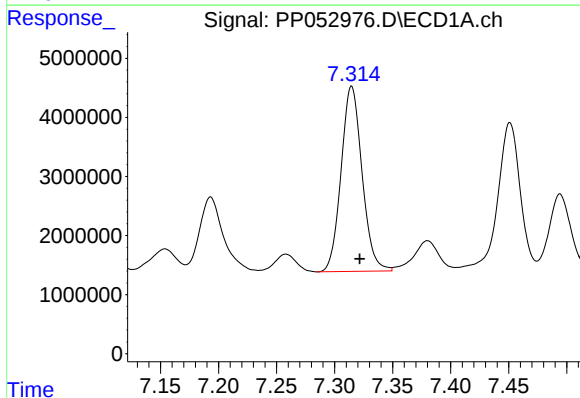


#29 AR-1254-4

R.T.: 7.315 min
Delta R.T.: -0.007 min
Response: 39360436
Conc: 558.94 ng/ml

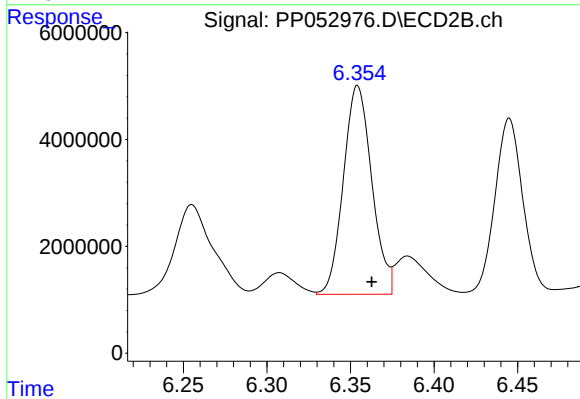

#29 AR-1254-4

R.T.: 6.354 min
Delta R.T.: -0.008 min
Response: 46294264
Conc: 509.88 ng/ml

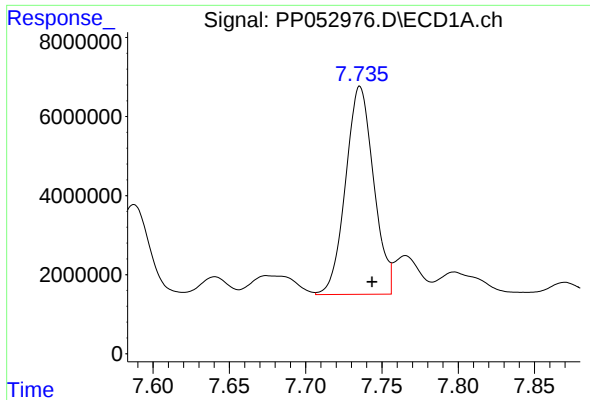


#30 AR-1254-5

R.T.: 7.735 min
Delta R.T.: -0.008 min
Response: 67491006
Conc: 857.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
135ADL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/03/2022
Supervised By :Ankita Jodhani 11/03/2022

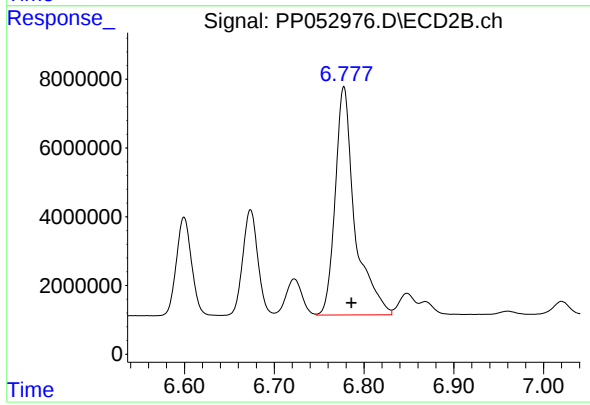

#30 AR-1254-5

R.T.: 6.778 min
Delta R.T.: -0.008 min
Response: 100910826
Conc: 725.30 ng/ml