

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110320\
 Data File : PP031054.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Nov 2020 2:48
 Operator : DD\AJ
 Sample : MDL-AR1262-S-7
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-AR1262-S-7

Manual Integrations
 APPROVED

Ankita
 11/3/2020 3:31:18 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 05:06:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\AR1262PP110120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 31 02:26:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.799	4.076	1455880	1267795	22.820	21.946
2) SA Decachlor...	10.689	9.409	838981	897735	22.591	22.703
Target Compounds						
36) L8 AR-1262-1	8.420	7.506	76901	81271	32.764	31.130
37) L8 AR-1262-2	8.962	8.016	126183	138428	29.794	29.394
38) L8 AR-1262-3	9.267	8.303	77358	56536	25.901m	28.468m
39) L8 AR-1262-4	9.353	8.367	65036	109919	26.597m	30.396
40) L8 AR-1262-5	9.980	8.865	41341	43262	26.432	26.254

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110320\
Data File : PP031054.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Nov 2020 2:48
Operator : DD\AJ
Sample : MDL-AR1262-S-7
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
MDL-AR1262-S-7


Manual Integrations
APPROVED

Ankita
11/3/2020 3:31:18 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 05:06:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\AR1262PP110120.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 31 02:26:29 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

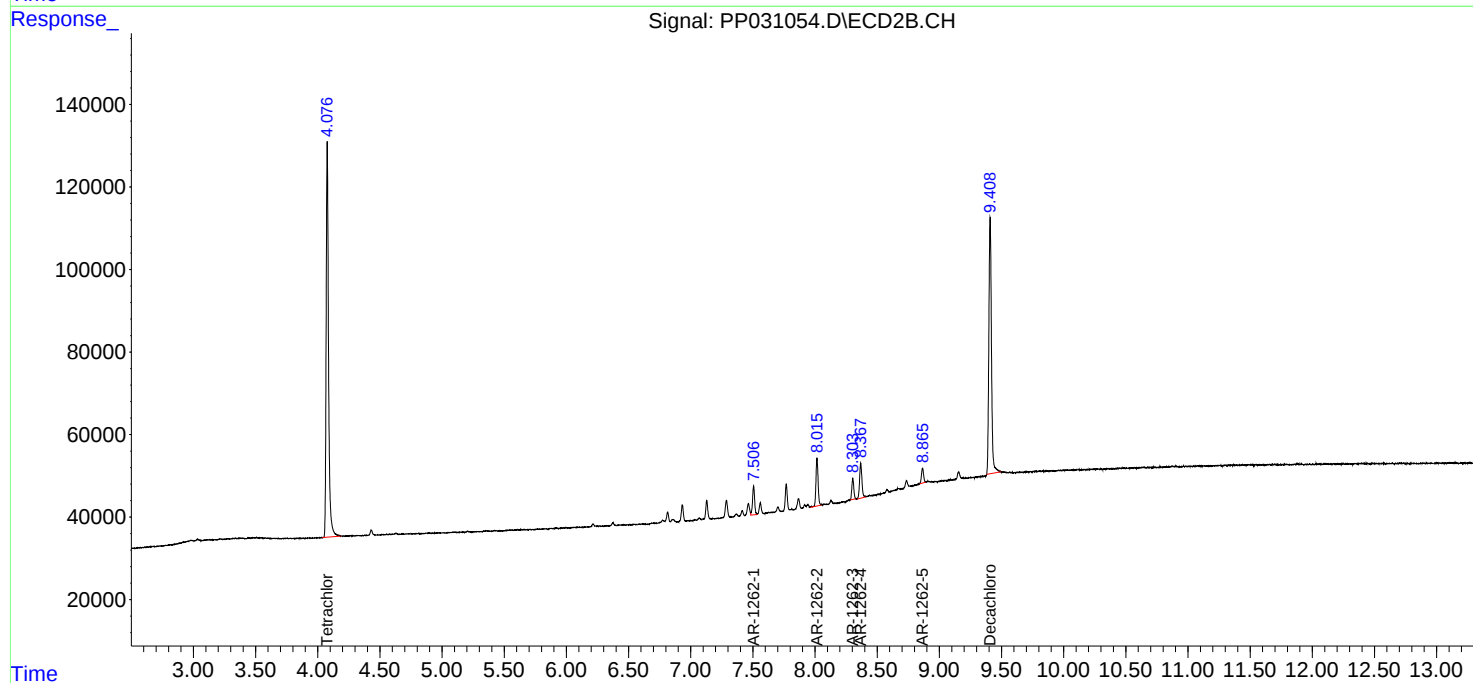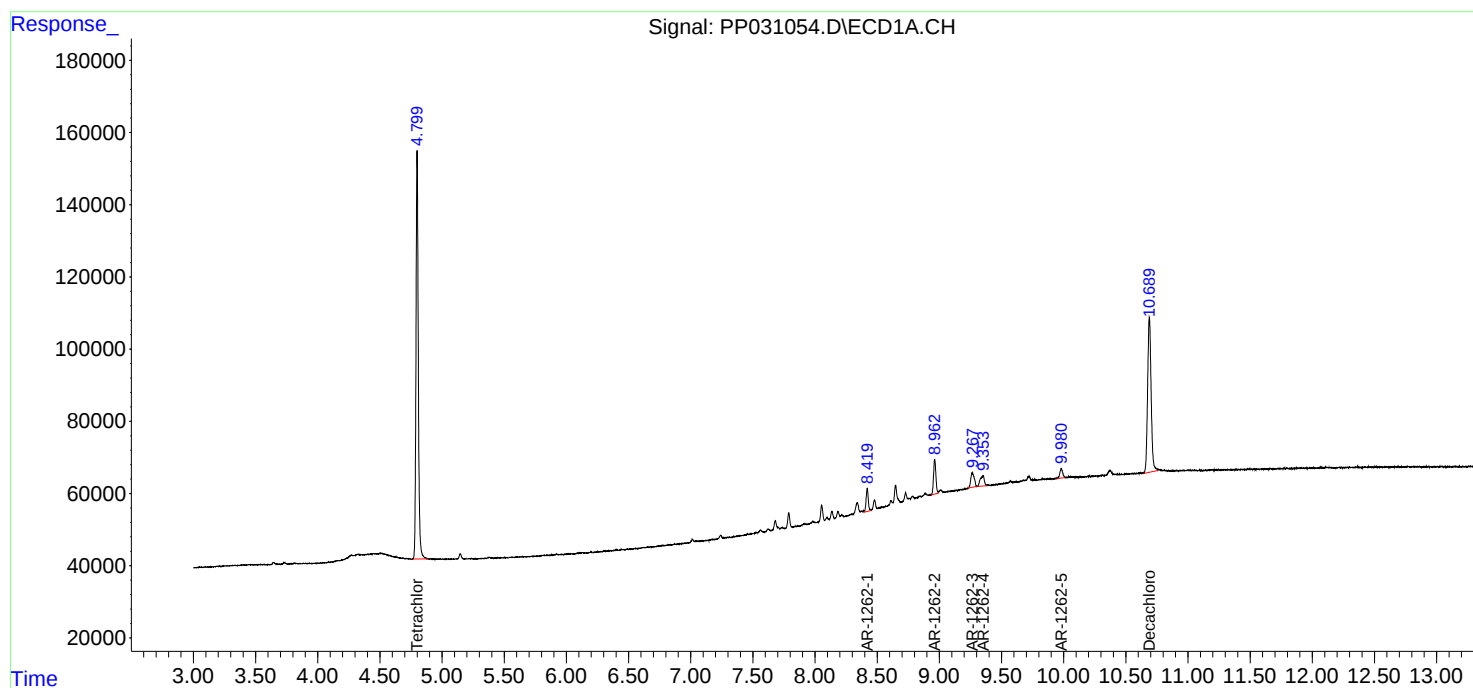

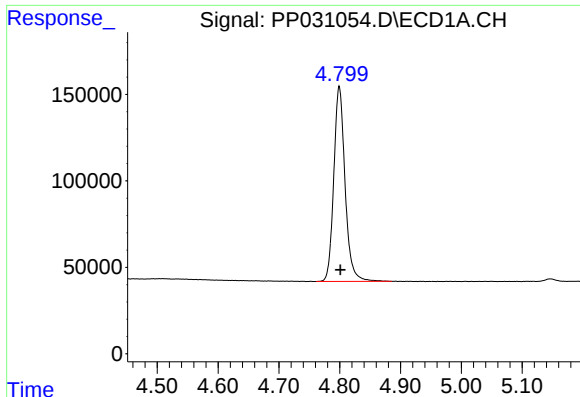


#1 Tetrachloro-m-xylene

R.T.: 4.799 min
Delta R.T.: -0.002 min
Response: 1455880
Conc: 22.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-AR1262-S-7


Manual Integrations
APPROVED

Ankita
11/3/2020 3:31:18 PM

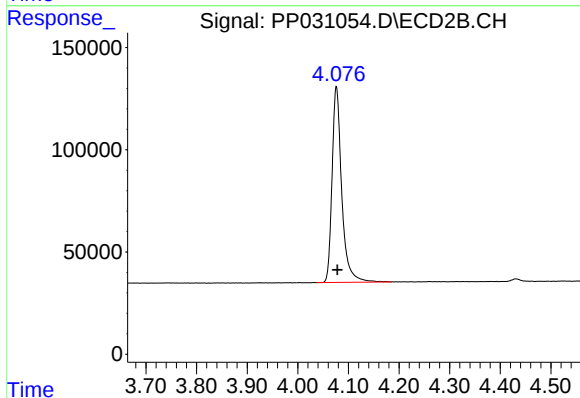


#1 Tetrachloro-m-xylene

R.T.: 4.076 min
Delta R.T.: -0.002 min
Response: 1267795
Conc: 21.95 ng/ml

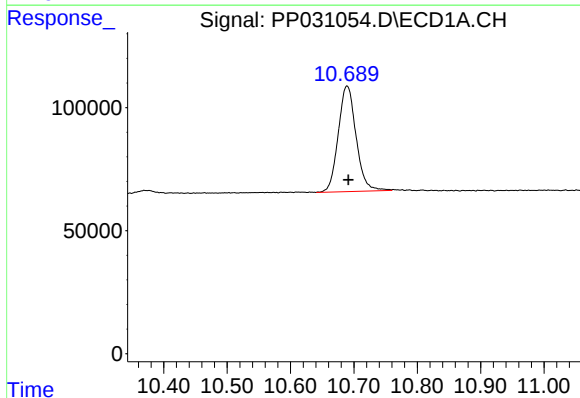


#2 Decachlorobiphenyl

R.T.: 10.689 min
Delta R.T.: -0.002 min
Response: 838981
Conc: 22.59 ng/ml

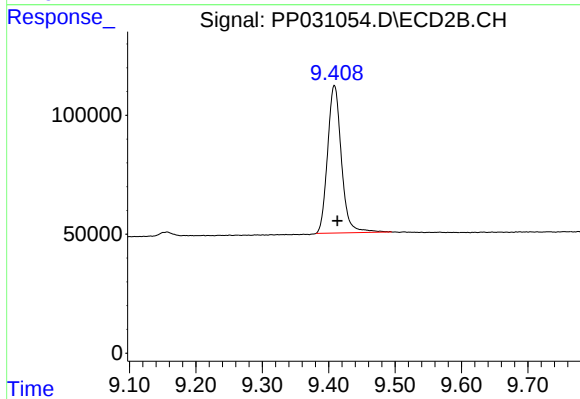

#2 Decachlorobiphenyl

R.T.: 9.409 min
Delta R.T.: -0.005 min
Response: 897735
Conc: 22.70 ng/ml

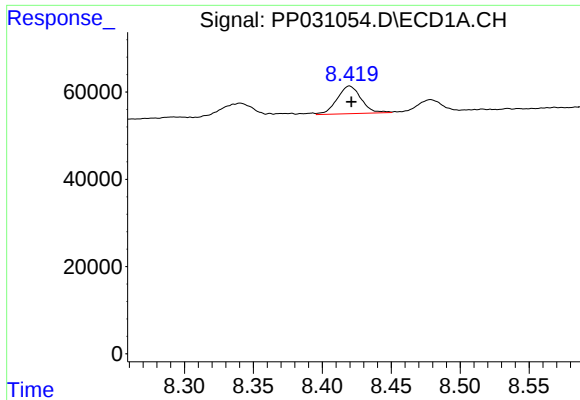


#36 AR-1262-1

R.T.: 8.420 min
Delta R.T.: -0.001 min
Response: 76901
Conc: 32.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-AR1262-S-7


Manual Integrations
APPROVED

Ankita
11/3/2020 3:31:18 PM

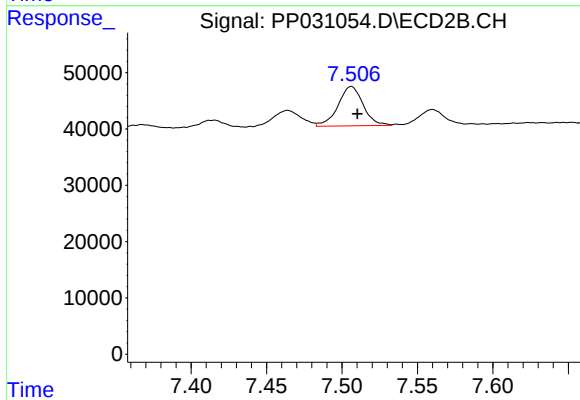


#36 AR-1262-1

R.T.: 7.506 min
Delta R.T.: -0.004 min
Response: 81271
Conc: 31.13 ng/ml

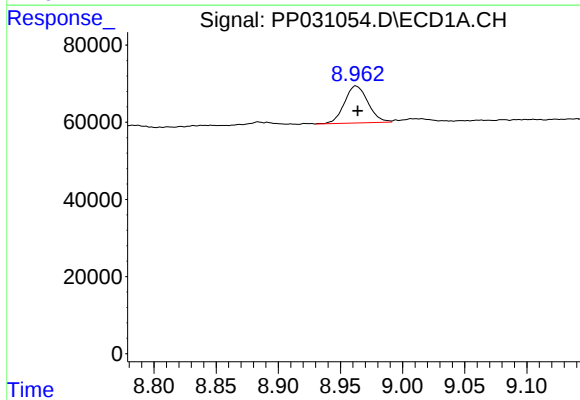


#37 AR-1262-2

R.T.: 8.962 min
Delta R.T.: -0.002 min
Response: 126183
Conc: 29.79 ng/ml

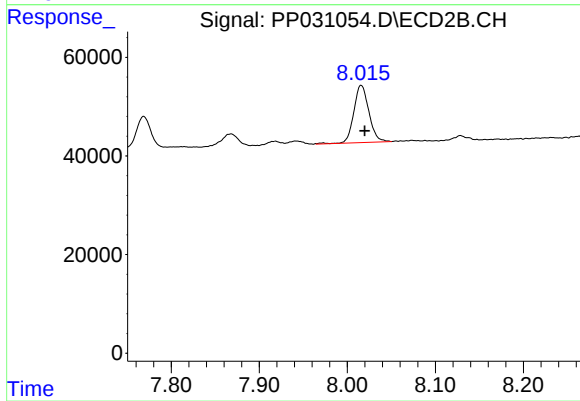

#37 AR-1262-2

R.T.: 8.016 min
Delta R.T.: -0.004 min
Response: 138428
Conc: 29.39 ng/ml

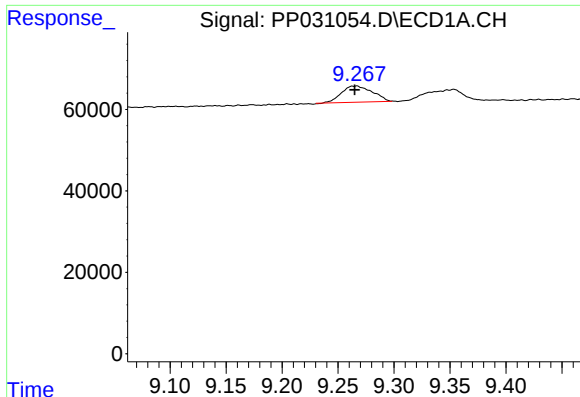


#38 AR-1262-3

R.T.: 9.267 min
Delta R.T.: 0.002 min
Response: 77358
Conc: 25.90 ng/ml m

Instrument :
ECD_P
ClientSampleId :
MDL-AR1262-S-7


Manual Integrations
APPROVED

Ankita
11/3/2020 3:31:18 PM

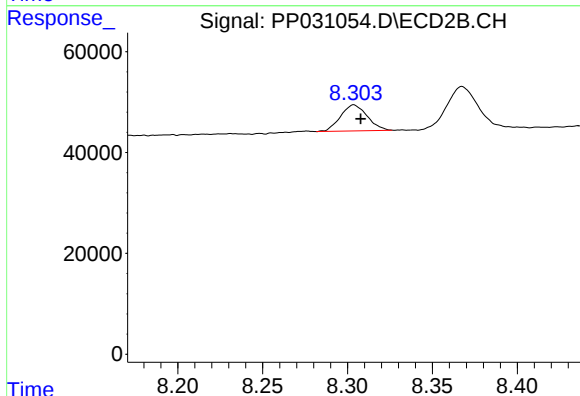


#38 AR-1262-3

R.T.: 8.303 min
Delta R.T.: -0.005 min
Response: 56536
Conc: 28.47 ng/ml m

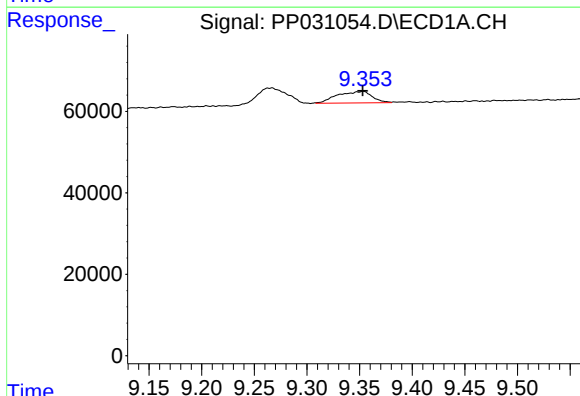


#39 AR-1262-4

R.T.: 9.353 min
Delta R.T.: 0.000 min
Response: 65036
Conc: 26.60 ng/ml m

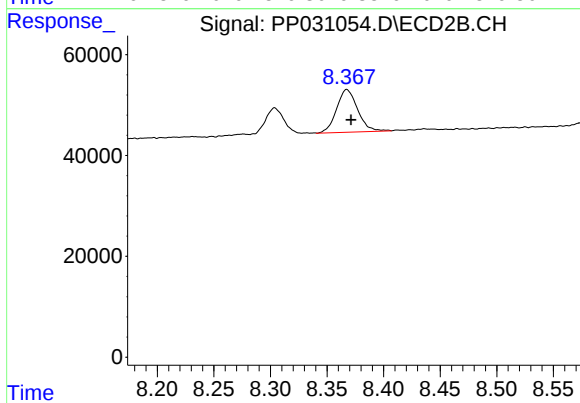

#39 AR-1262-4

R.T.: 8.367 min
Delta R.T.: -0.004 min
Response: 109919
Conc: 30.40 ng/ml

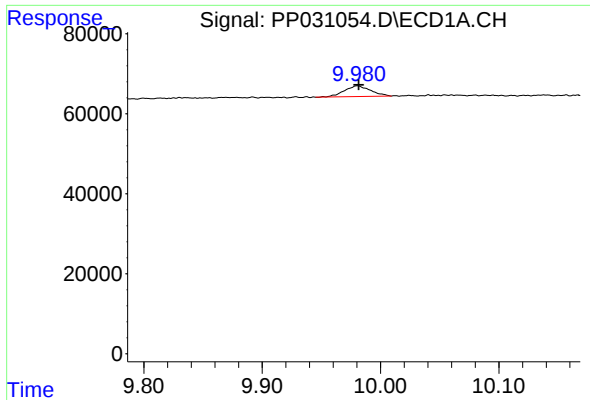


#40 AR-1262-5

R.T.: 9.980 min
Delta R.T.: -0.001 min
Response: 41341
Conc: 26.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-AR1262-S-7

Manual Integrations
APPROVED

Ankita
11/3/2020 3:31:18 PM

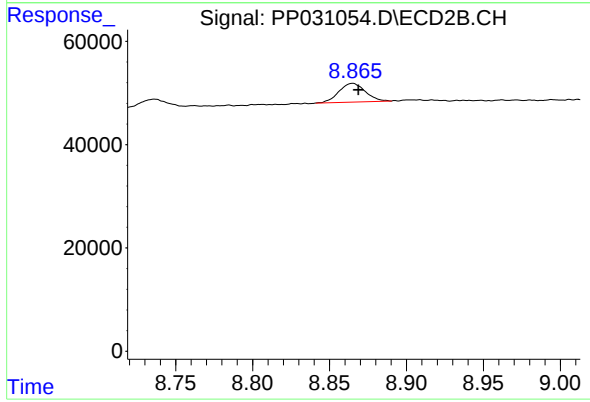

#40 AR-1262-5

R.T.: 8.865 min
Delta R.T.: -0.004 min
Response: 43262
Conc: 26.25 ng/ml