

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110320\
 Data File : PP031058.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Nov 2020 3:54
 Operator : DD\AJ
 Sample : MDL-PCB-BL-W-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-PCB-BL-W-14

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 05:06:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\AR1262PP110120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 31 02:26:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.799	4.077	1237100	1075873	19.391	18.623
2) SA Decachlor...	10.689	9.408	721825	769805	19.437	19.468

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110320\
Data File : PP031058.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Nov 2020 3:54
Operator : DD\AJ
Sample : MDL-PCB-BL-W-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-PCB-BL-W-14

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 05:06:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\AR1262PP110120.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 31 02:26:29 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

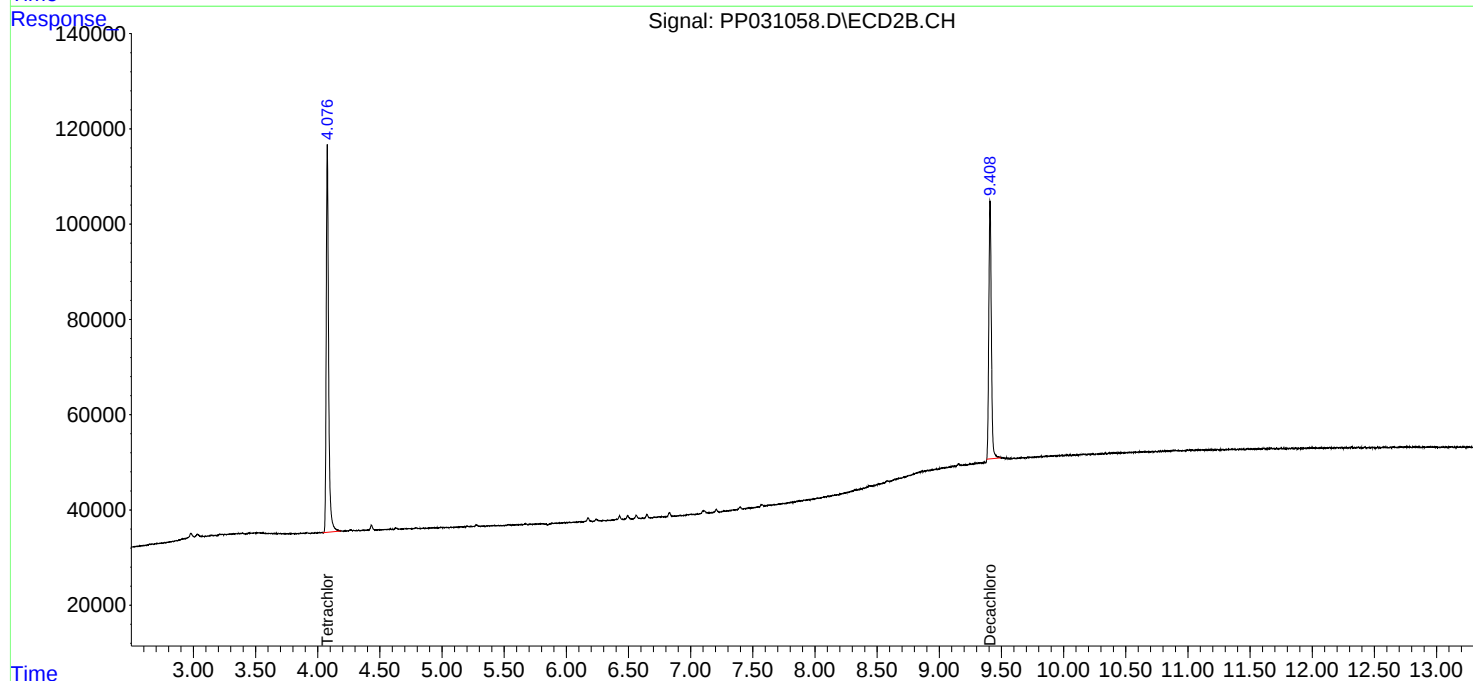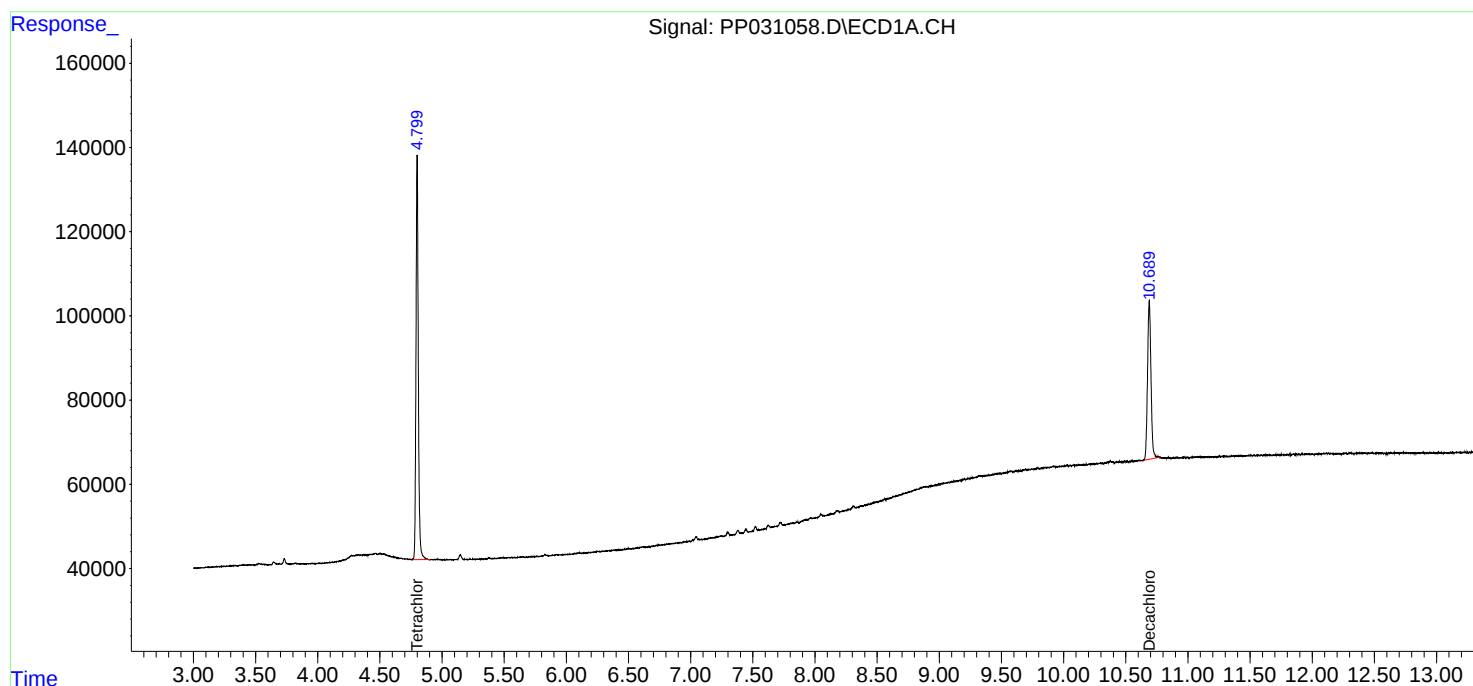


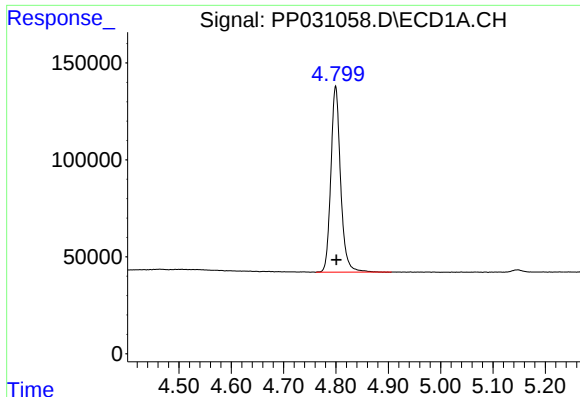

#1 Tetrachloro-m-xylene


R.T.: 4.799 min
Delta R.T.: -0.002 min
Response: 1237100
Conc: 19.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-PCB-BL-W-14

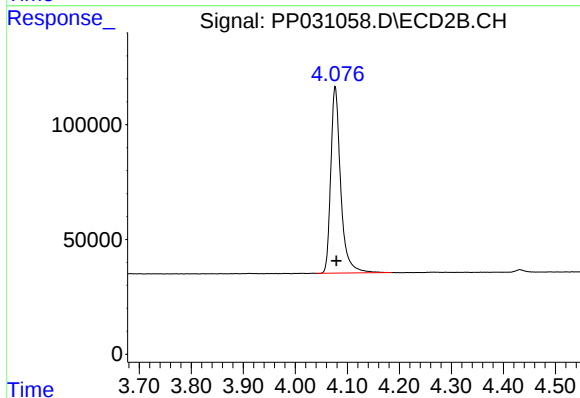


#1 Tetrachloro-m-xylene

R.T.: 4.077 min
Delta R.T.: -0.002 min
Response: 1075873
Conc: 18.62 ng/ml

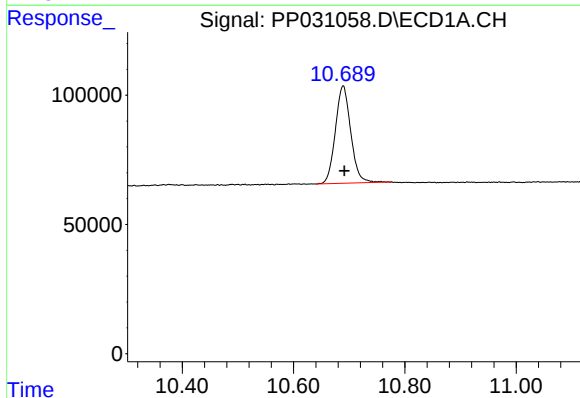

#2 Decachlorobiphenyl

R.T.: 10.689 min
Delta R.T.: -0.002 min
Response: 721825
Conc: 19.44 ng/ml

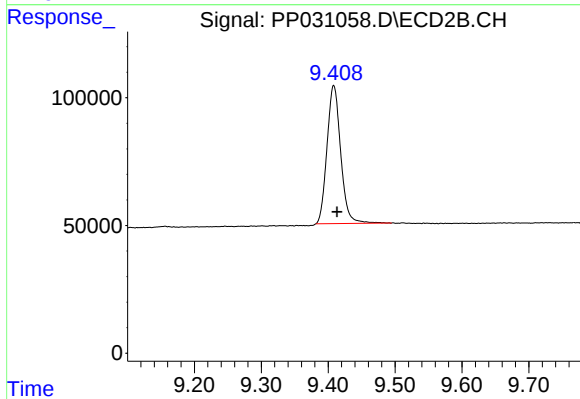

#2 Decachlorobiphenyl

R.T.: 9.408 min
Delta R.T.: -0.005 min
Response: 769805
Conc: 19.47 ng/ml