

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110320\
 Data File : PP031065.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Nov 2020 9:18
 Operator : DD\AJ
 Sample : MDL-PCB-BL-W-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-PCB-BL-W-14

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 11:23:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\AR1268PP110120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 31 02:37:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.799	4.076	1260182	1096673	21.147	20.834
2)	SA Decachlor...	10.689	9.406	738663	806853	12.872	12.780

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110320\
Data File : PP031065.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Nov 2020 9:18
Operator : DD\AJ
Sample : MDL-PCB-BL-W-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-PCB-BL-W-14

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 11:23:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\AR1268PP110120.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 31 02:37:11 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

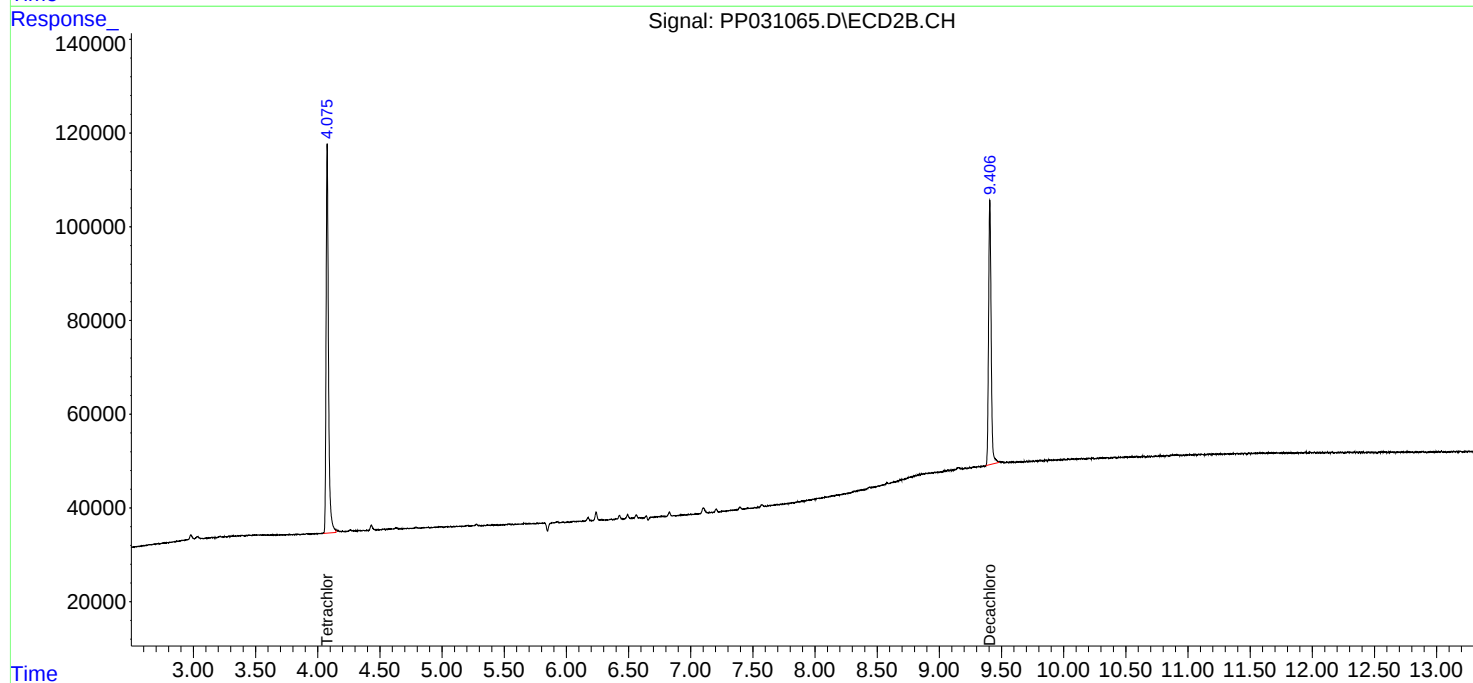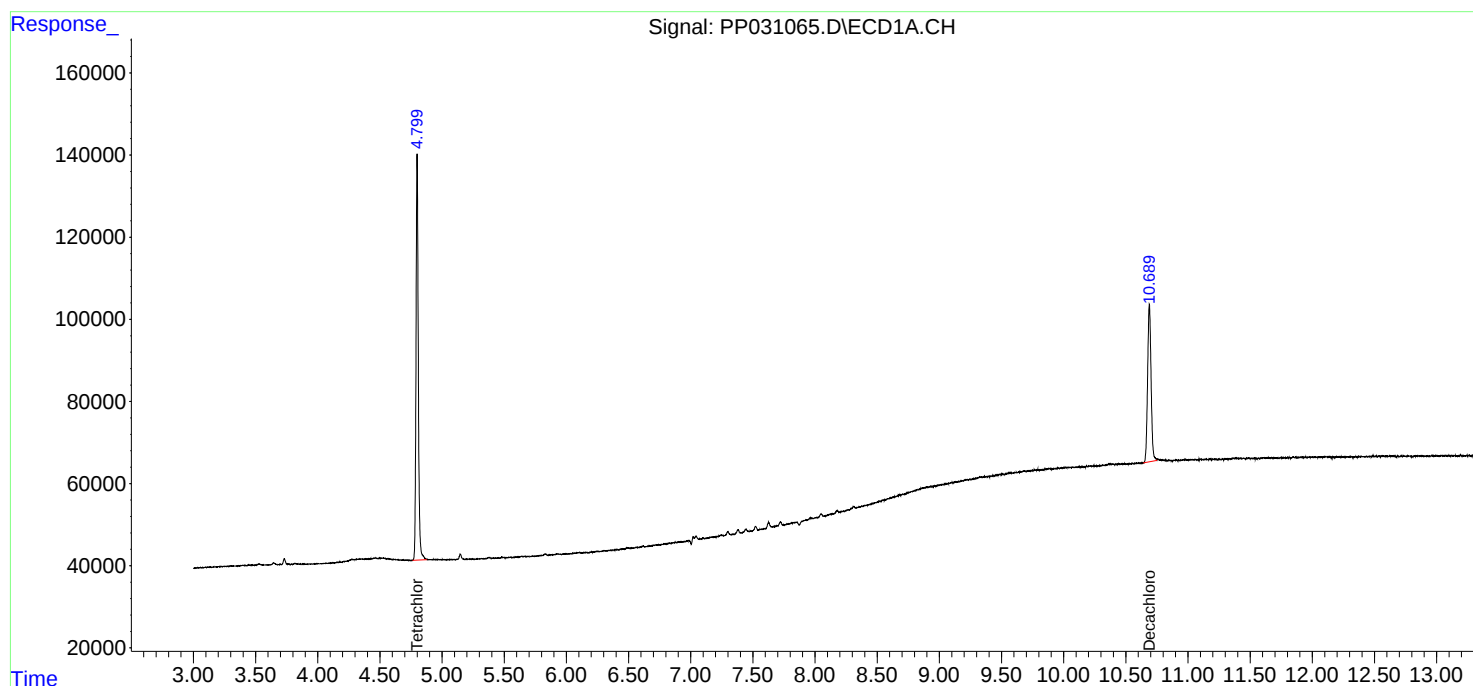


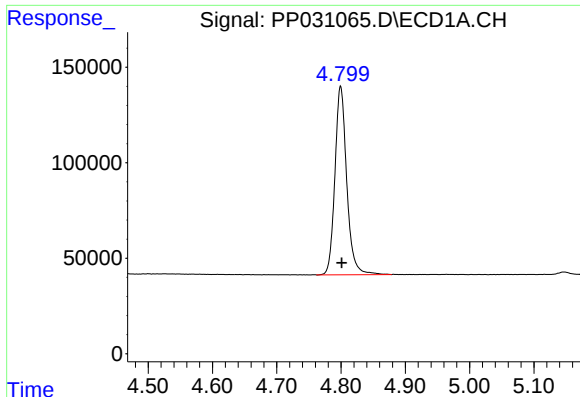

#1 Tetrachloro-m-xylene


R.T.: 4.799 min
Delta R.T.: -0.002 min
Response: 1260182
Conc: 21.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-PCB-BL-W-14

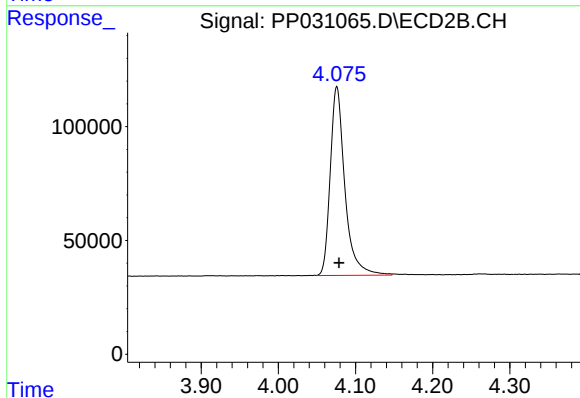


#1 Tetrachloro-m-xylene

R.T.: 4.076 min
Delta R.T.: -0.003 min
Response: 1096673
Conc: 20.83 ng/ml

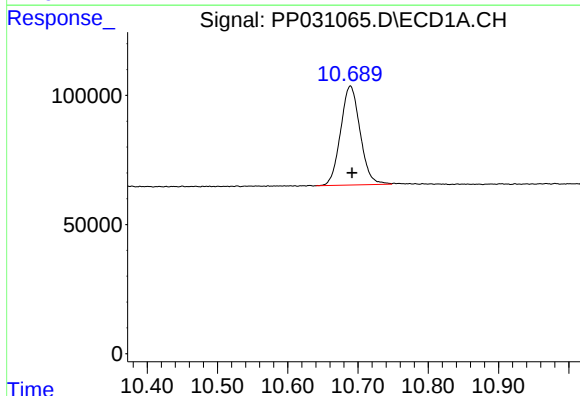

#2 Decachlorobiphenyl

R.T.: 10.689 min
Delta R.T.: -0.002 min
Response: 738663
Conc: 12.87 ng/ml

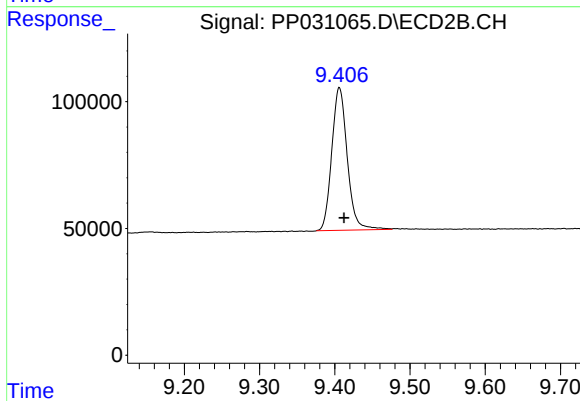

#2 Decachlorobiphenyl

R.T.: 9.406 min
Delta R.T.: -0.006 min
Response: 806853
Conc: 12.78 ng/ml