

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110420\
 Data File : PP031103.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Nov 2020 14:15
 Operator : DD\AJ
 Sample : L4214-07
 Misc : AR1248 LOD 25 PPB
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2020

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 05:02:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 04 08:24:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.800	4.075	940630	890150	14.083	13.392
2)	SA Decachlor...	10.682	9.399	587249	655460	14.687	15.697
Target Compounds							
3)	L1 AR-1016-1	6.105	5.335	23861	20443	12.255	11.019
4)	L1 AR-1016-2	6.129	5.356	27173	19525	9.519	7.183
5)	L1 AR-1016-3	6.195	5.550	13491	12525	7.745	9.888 #
6)	L1 AR-1016-4	6.299	5.600	13099	25213	9.065	27.339 #
7)	L1 AR-1016-5	6.614	5.830	34919	31570	28.011	24.053
9)	L2 AR-1221-2	5.148	4.432	12307	9229	27.400	22.244
12)	L3 AR-1232-2	5.815	5.356	10181	19525	16.766	18.373
13)	L3 AR-1232-3	6.129	5.550	27173	12525	24.324	24.429
14)	L3 AR-1232-4	6.299	5.644	13099	28762	23.080	65.855 #
15)	L3 AR-1232-5	6.399	5.830	25697	31570	74.159	65.376
16)	L4 AR-1242-1	6.105	5.335	23861	20443	17.761	15.885
17)	L4 AR-1242-2	6.129	5.356	27173	19525	13.914	10.456
18)	L4 AR-1242-3	6.195	5.550	13491	12525	11.062	13.340
19)	L4 AR-1242-4	6.299	5.644	13099	28762	12.929	33.167 #
20)	L4 AR-1242-5	7.079	6.210	42002	40461	44.015	40.644
21)	L5 AR-1248-1	6.105	5.335	23861	20443	24.745	22.093
22)	L5 AR-1248-2	6.399	5.600	25697	25213	22.218	22.877
23)	L5 AR-1248-3	6.614	5.644	34919	28762	24.542	23.764
24)	L5 AR-1248-4	7.040	5.830	42012	31570	27.565	21.391
25)	L5 AR-1248-5	7.079	6.253	42002	30167	27.686	23.886
26)	L6 AR-1254-1	7.010	6.210	35346	40461	25.175	20.573
27)	L6 AR-1254-2	7.242	6.368	46190	14143	22.159	8.607 #
28)	L6 AR-1254-3	7.619	6.790	58144	17860	25.192	6.522 #
29)	L6 AR-1254-4	7.913	7.029	20372	11714	12.443	7.259 #
30)	L6 AR-1254-5	8.345	7.465	2758	970	1.634	0.443 #
31)	L7 AR-1260-1	7.788	6.938	3043	6918	1.657	3.452 #
32)	L7 AR-1260-2	0.000	7.121	0	869	N.D.	0.371 #
33)	L7 AR-1260-3	8.437f	7.274	2011	4978	1.222	2.189 #
34)	L7 AR-1260-4	8.638	0.000	1702	0	0.915	N.D. #
35)	L7 AR-1260-5	8.964	8.008	11884	2124	3.152	0.472 #
36)	L8 AR-1262-1	8.437f	7.520f	2011	687	1.001	0.296 #
37)	L8 AR-1262-2	8.964	8.008	11884	2124	3.270	0.512 #
38)	L8 AR-1262-3	9.261	0.000	5459	0	2.112	N.D. #
39)	L8 AR-1262-4	9.356	8.357	3705	3930	1.799	1.238 #
40)	L8 AR-1262-5	9.955f	0.000	34014	0	24.012	N.D. #
41)	L9 AR-1268-1	9.261	0.000	5459	0	1.250	N.D. #
42)	L9 AR-1268-2	9.356	8.357	3705	3930	0.862	0.826
43)	L9 AR-1268-3	9.579	8.588	23731	1010	6.562	0.252 #
44)	L9 AR-1268-4	9.955f	0.000	34014	0	21.475	N.D. #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110420\
Data File : PP031103.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Nov 2020 14:15
Operator : DD\AJ
Sample : L4214-07
Misc : AR1248 LOD 25 PPB
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 05:02:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 04 08:24:38 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
45) L9	AR-1268-5	10.388f	9.151	62537	2357	5.229	0.176 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110420\
Data File : PP031103.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Nov 2020 14:15
Operator : DD\AJ
Sample : L4214-07
Misc : AR1248 LOD 25 PPB
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 05:02:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 04 08:24:38 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

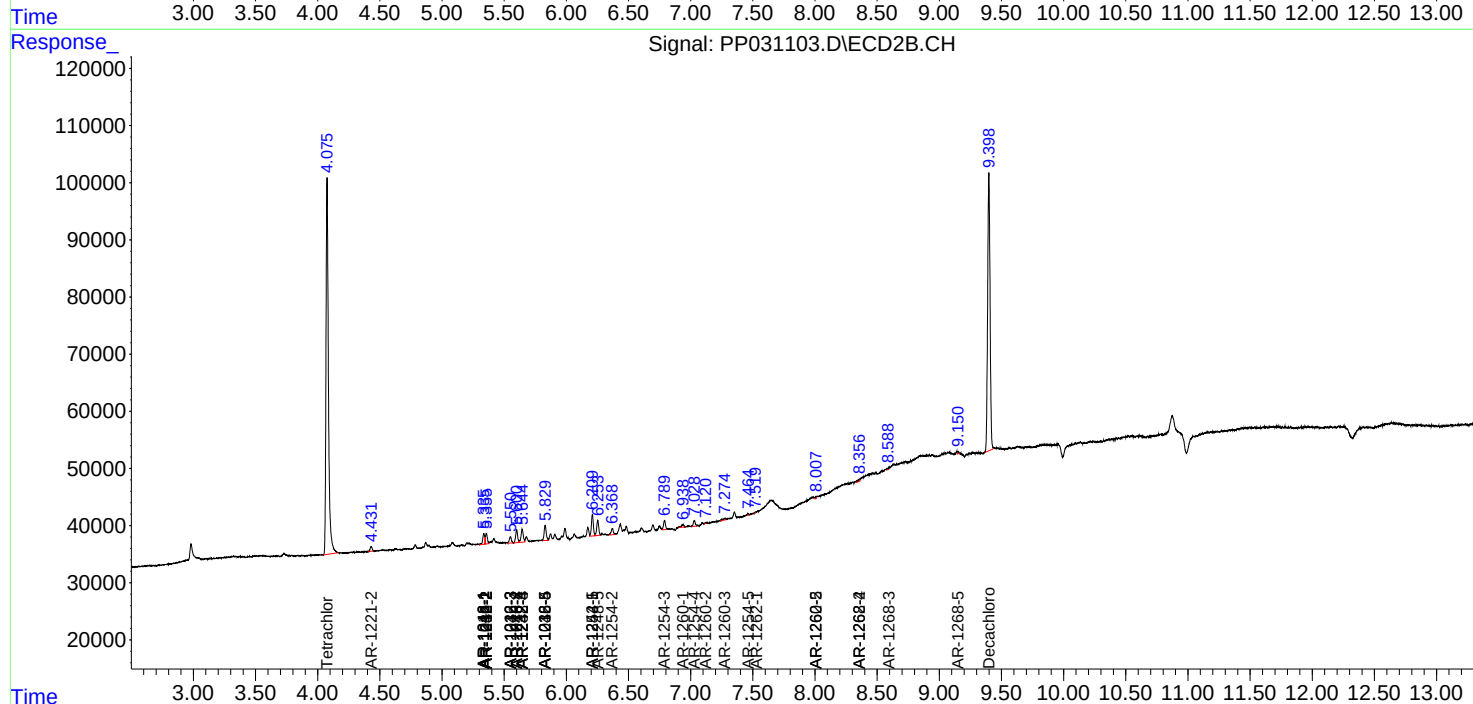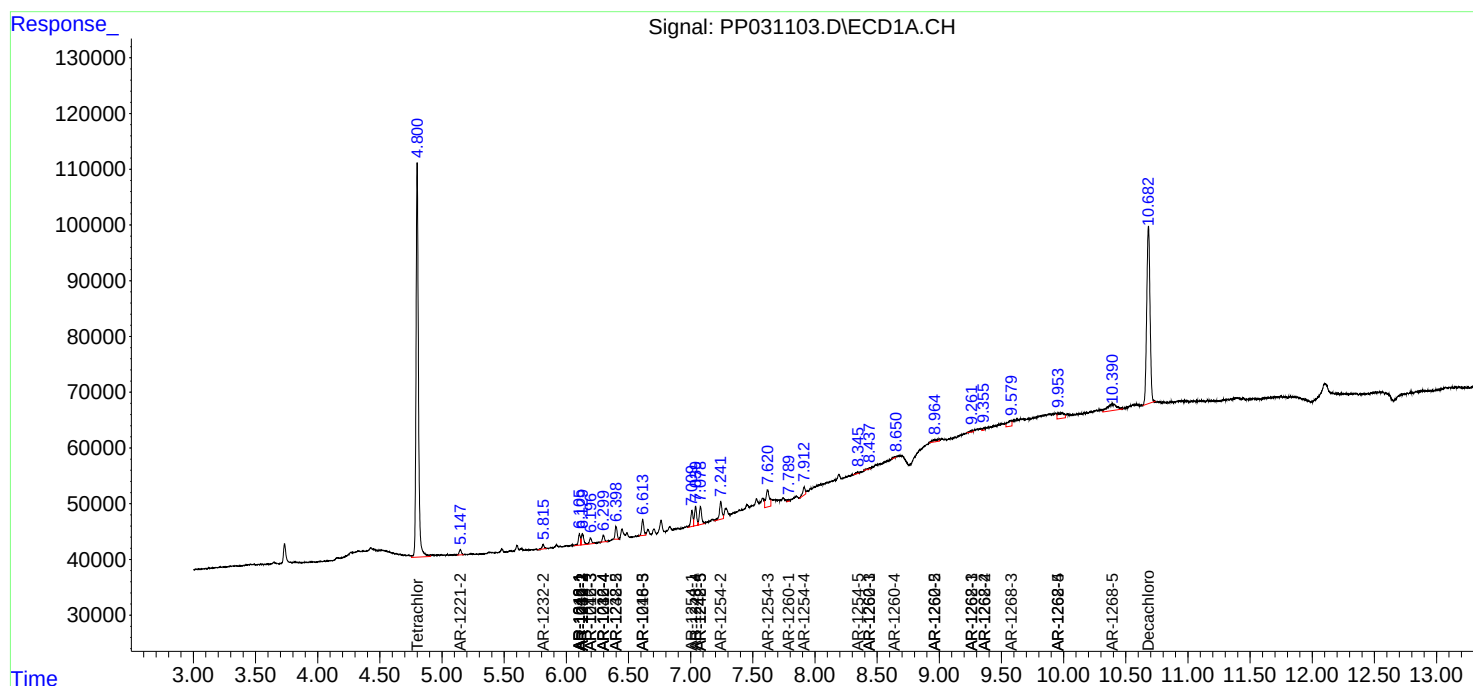


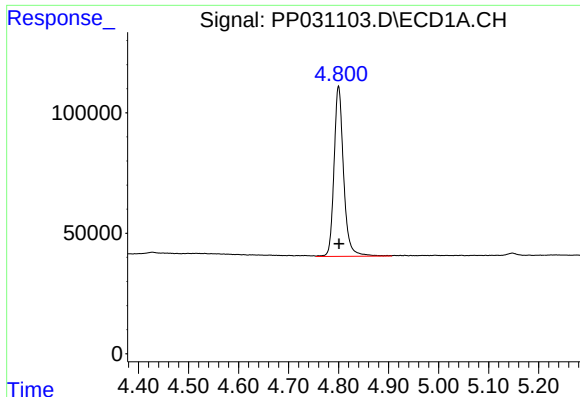

#1 Tetrachloro-m-xylene


R.T.: 4.800 min
Delta R.T.: -0.001 min
Response: 940630
Conc: 14.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

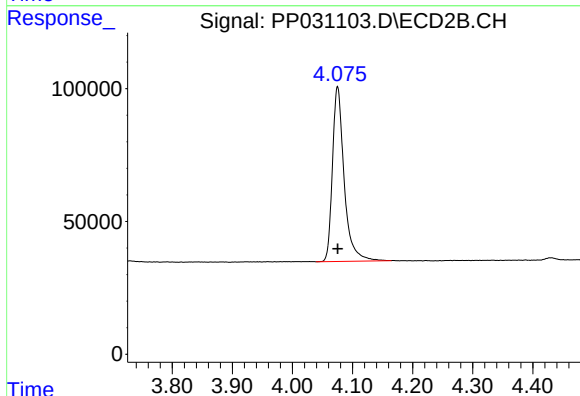


#1 Tetrachloro-m-xylene

R.T.: 4.075 min
Delta R.T.: 0.000 min
Response: 890150
Conc: 13.39 ng/ml

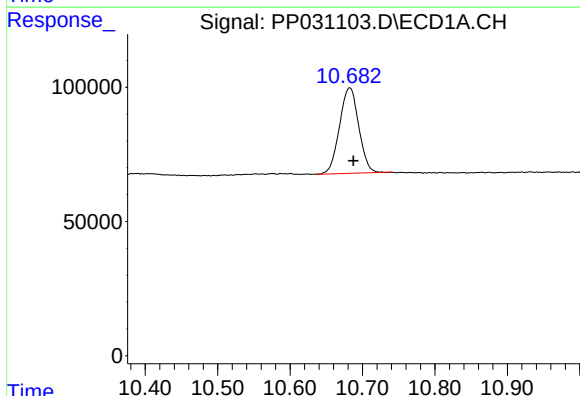


#2 Decachlorobiphenyl

R.T.: 10.682 min
Delta R.T.: -0.005 min
Response: 587249
Conc: 14.69 ng/ml

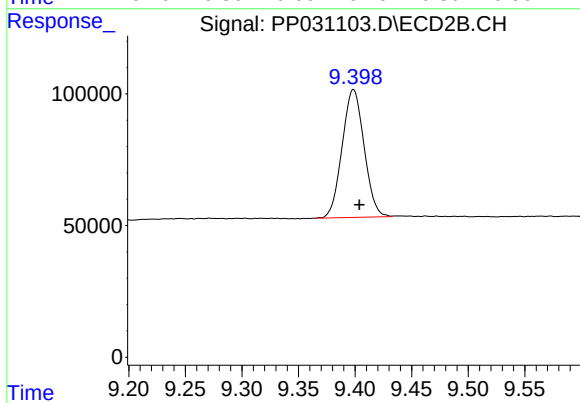

#2 Decachlorobiphenyl


R.T.: 9.399 min
Delta R.T.: -0.005 min
Response: 655460
Conc: 15.70 ng/ml

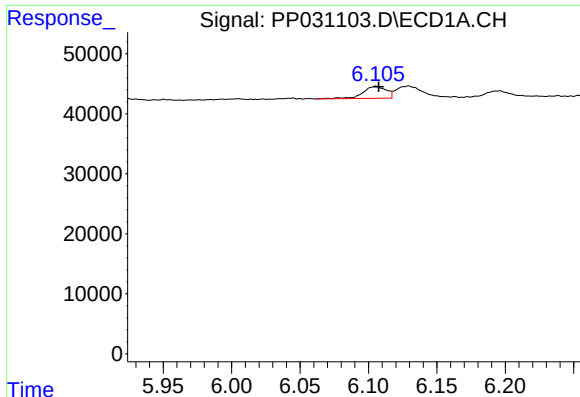

#3 AR-1016-1


R.T.: 6.105 min
Delta R.T.: -0.002 min
Response: 23861
Conc: 12.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

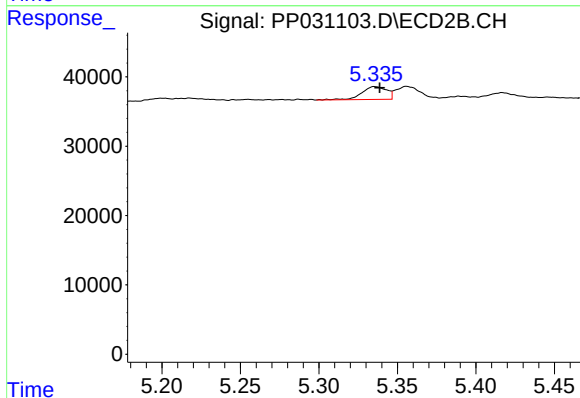


#3 AR-1016-1

R.T.: 5.335 min
Delta R.T.: -0.003 min
Response: 20443
Conc: 11.02 ng/ml

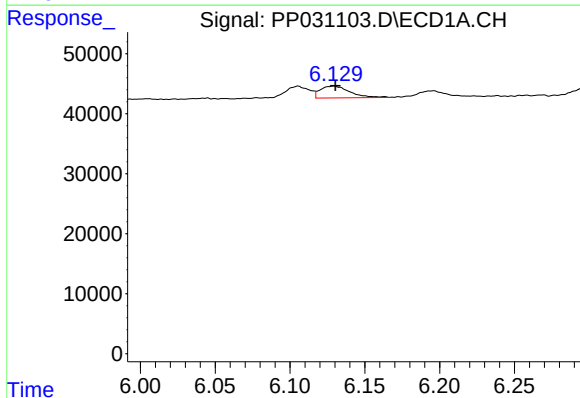


#4 AR-1016-2

R.T.: 6.129 min
Delta R.T.: -0.001 min
Response: 27173
Conc: 9.52 ng/ml

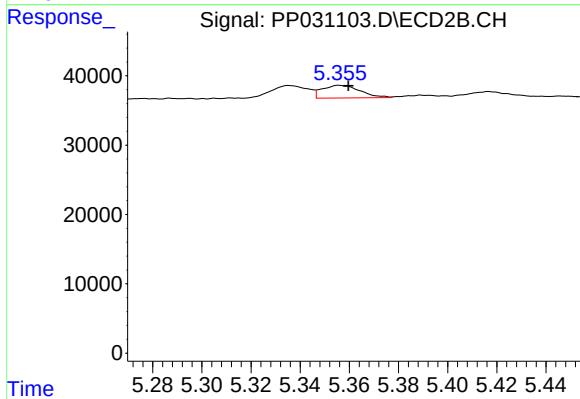

#4 AR-1016-2


R.T.: 5.356 min
Delta R.T.: -0.004 min
Response: 19525
Conc: 7.18 ng/ml

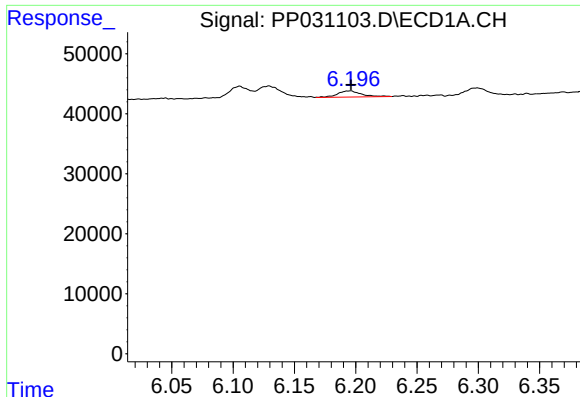

#5 AR-1016-3


R.T.: 6.195 min
Delta R.T.: 0.000 min
Response: 13491
Conc: 7.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

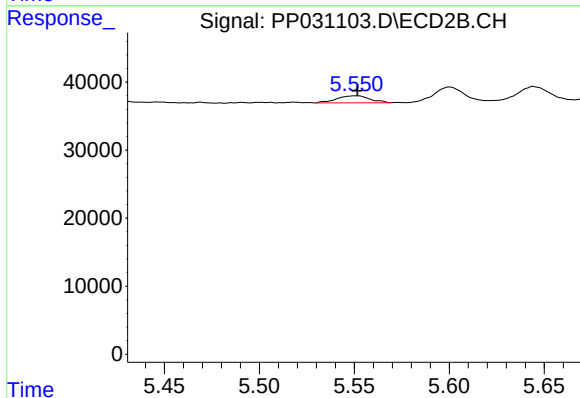


#5 AR-1016-3

R.T.: 5.550 min
Delta R.T.: -0.001 min
Response: 12525
Conc: 9.89 ng/ml

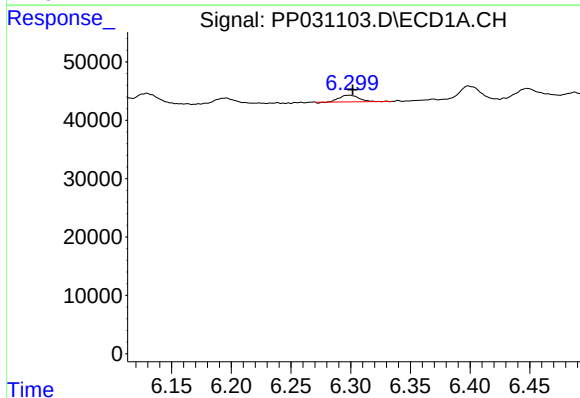


#6 AR-1016-4

R.T.: 6.299 min
Delta R.T.: -0.003 min
Response: 13099
Conc: 9.07 ng/ml

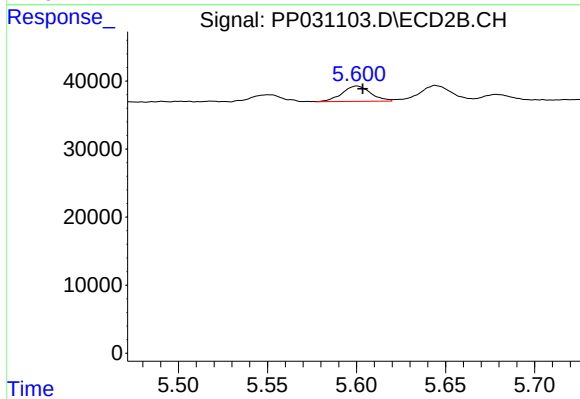

#6 AR-1016-4


R.T.: 5.600 min
Delta R.T.: -0.003 min
Response: 25213
Conc: 27.34 ng/ml

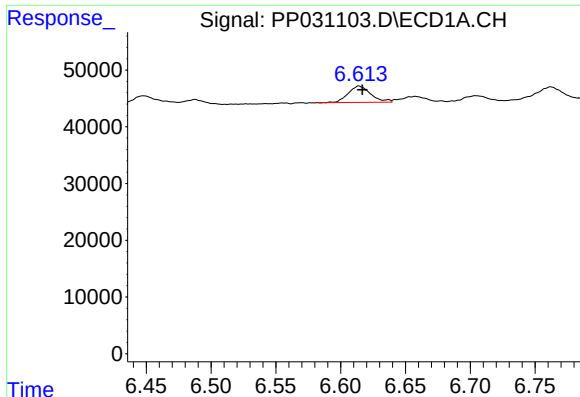

#7 AR-1016-5


R.T.: 6.614 min
Delta R.T.: -0.003 min
Response: 34919
Conc: 28.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

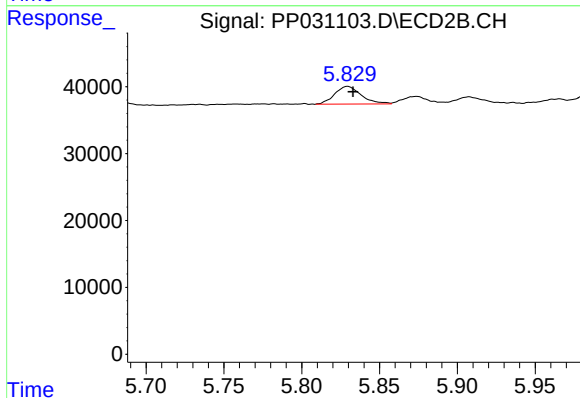


#7 AR-1016-5

R.T.: 5.830 min
Delta R.T.: -0.004 min
Response: 31570
Conc: 24.05 ng/ml

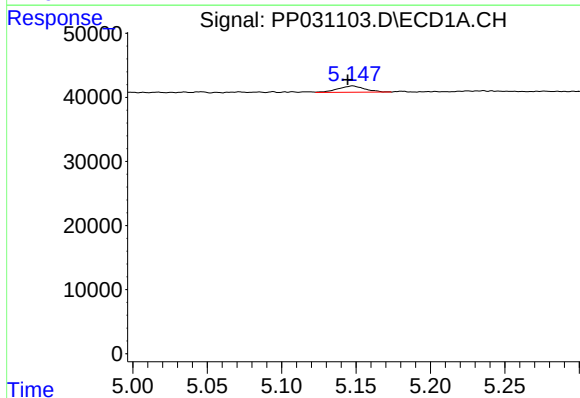


#9 AR-1221-2

R.T.: 5.148 min
Delta R.T.: 0.003 min
Response: 12307
Conc: 27.40 ng/ml

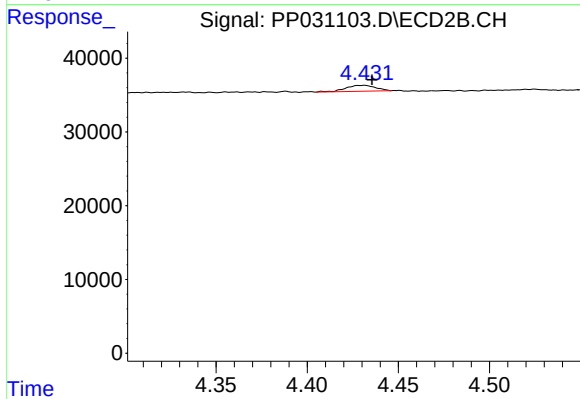

#9 AR-1221-2


R.T.: 4.432 min
Delta R.T.: -0.004 min
Response: 9229
Conc: 22.24 ng/ml

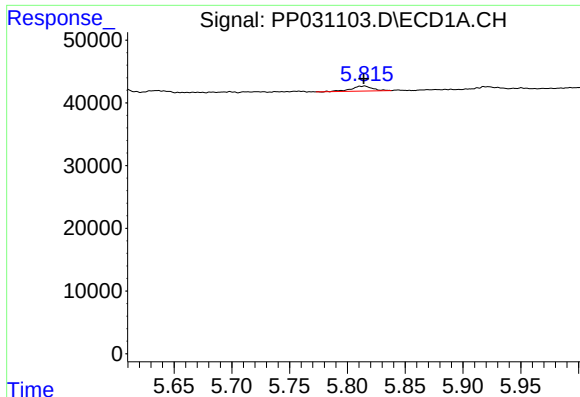

#12 AR-1232-2


R.T.: 5.815 min
Delta R.T.: 0.000 min
Response: 10181
Conc: 16.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

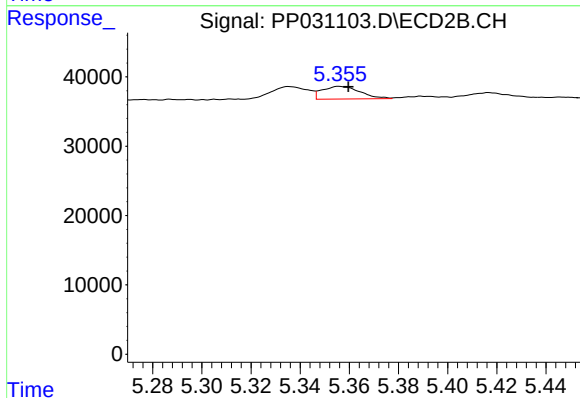


#12 AR-1232-2

R.T.: 5.356 min
Delta R.T.: -0.004 min
Response: 19525
Conc: 18.37 ng/ml

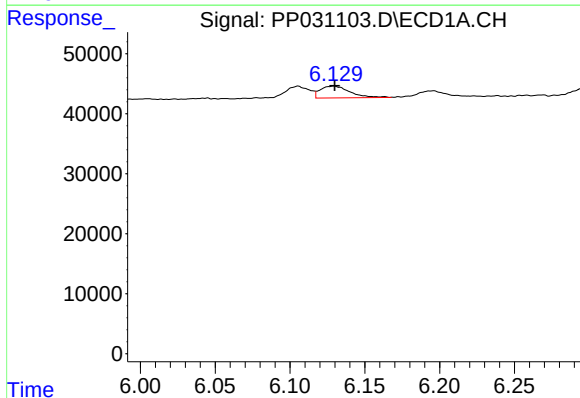


#13 AR-1232-3

R.T.: 6.129 min
Delta R.T.: 0.000 min
Response: 27173
Conc: 24.32 ng/ml

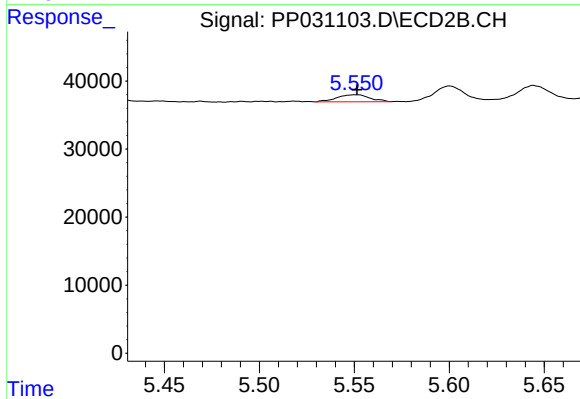

#13 AR-1232-3


R.T.: 5.550 min
Delta R.T.: -0.001 min
Response: 12525
Conc: 24.43 ng/ml

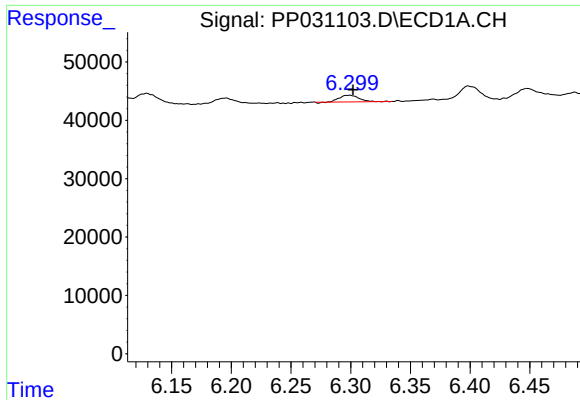

#14 AR-1232-4


R.T.: 6.299 min
Delta R.T.: -0.003 min
Response: 13099
Conc: 23.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

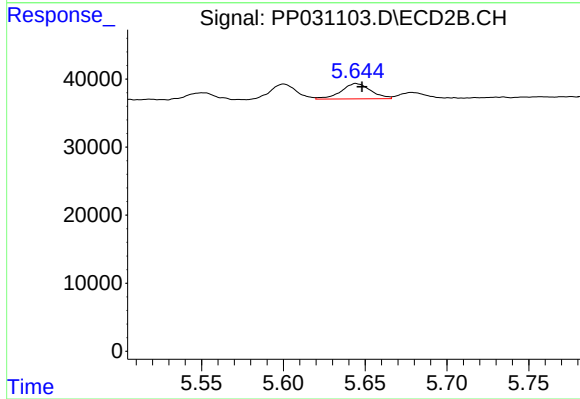


#14 AR-1232-4

R.T.: 5.644 min
Delta R.T.: -0.004 min
Response: 28762
Conc: 65.85 ng/ml

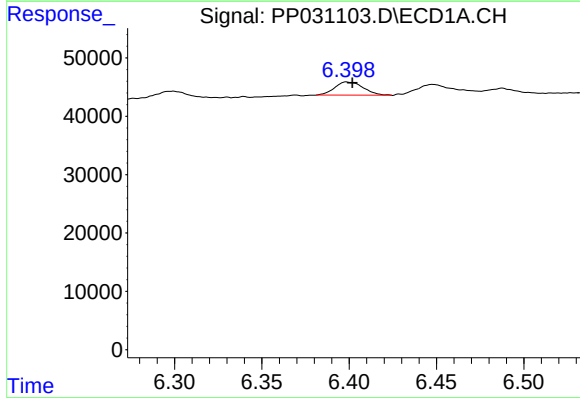


#15 AR-1232-5

R.T.: 6.399 min
Delta R.T.: -0.003 min
Response: 25697
Conc: 74.16 ng/ml

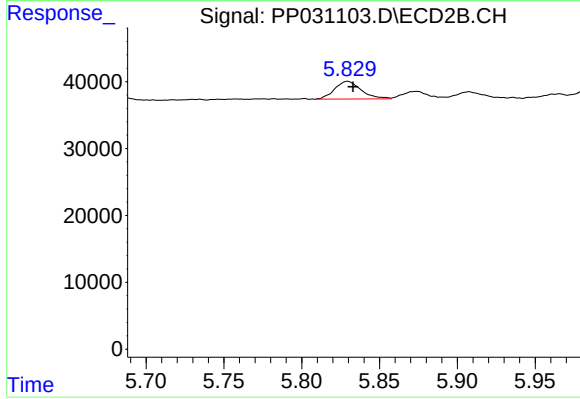

#15 AR-1232-5


R.T.: 5.830 min
Delta R.T.: -0.003 min
Response: 31570
Conc: 65.38 ng/ml

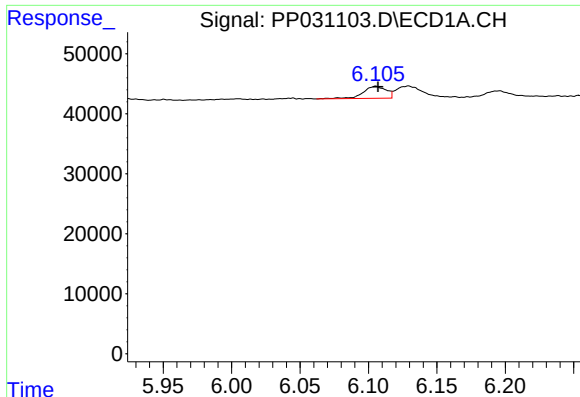

#16 AR-1242-1


R.T.: 6.105 min
Delta R.T.: -0.002 min
Response: 23861
Conc: 17.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

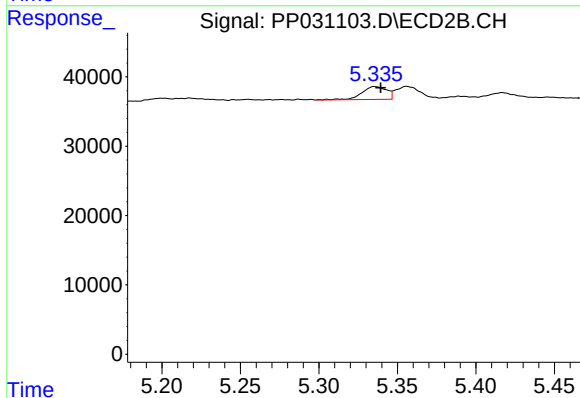


#16 AR-1242-1

R.T.: 5.335 min
Delta R.T.: -0.004 min
Response: 20443
Conc: 15.88 ng/ml

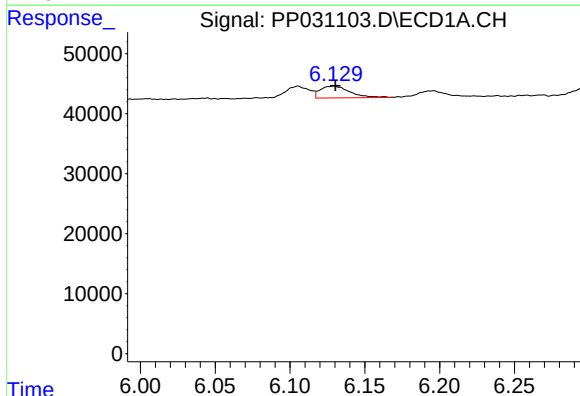


#17 AR-1242-2

R.T.: 6.129 min
Delta R.T.: -0.001 min
Response: 27173
Conc: 13.91 ng/ml

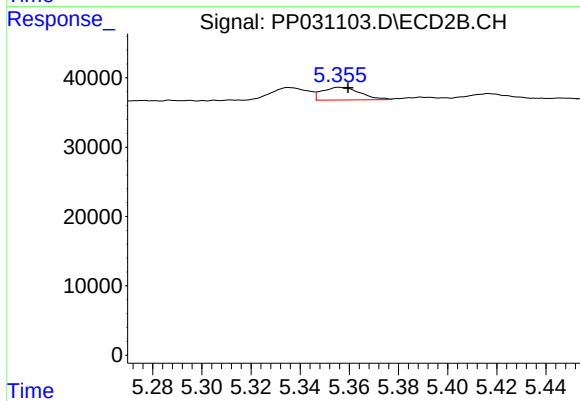

#17 AR-1242-2


R.T.: 5.356 min
Delta R.T.: -0.004 min
Response: 19525
Conc: 10.46 ng/ml

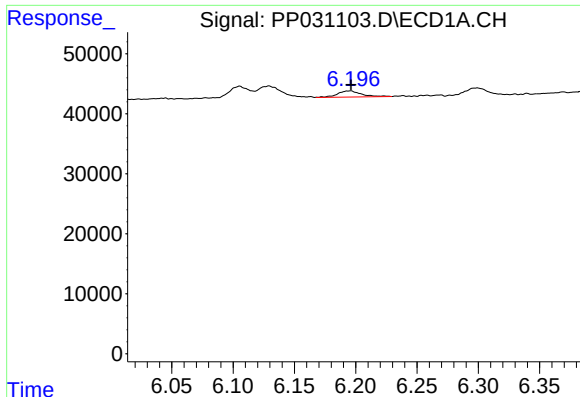

#18 AR-1242-3


R.T.: 6.195 min
Delta R.T.: 0.000 min
Response: 13491
Conc: 11.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

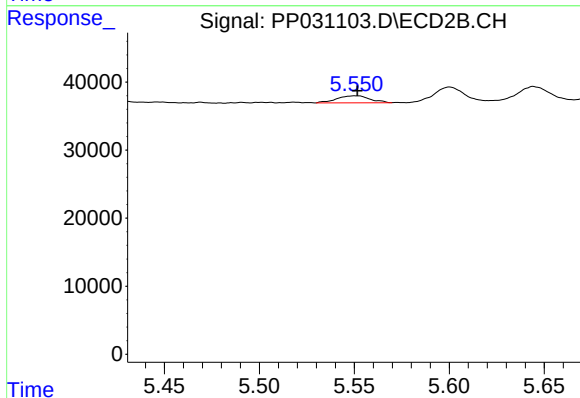


#18 AR-1242-3

R.T.: 5.550 min
Delta R.T.: -0.001 min
Response: 12525
Conc: 13.34 ng/ml

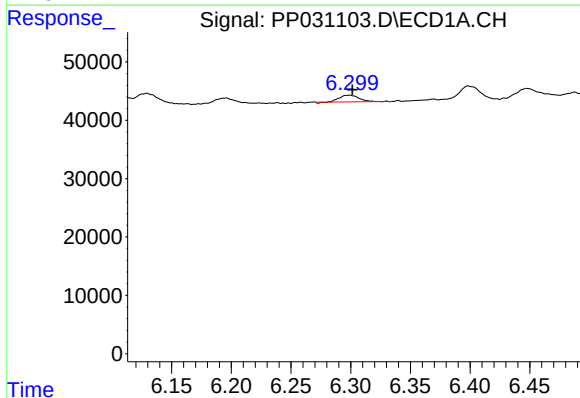


#19 AR-1242-4

R.T.: 6.299 min
Delta R.T.: -0.003 min
Response: 13099
Conc: 12.93 ng/ml

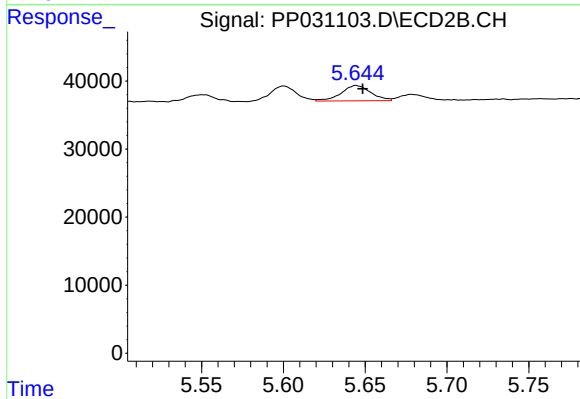

#19 AR-1242-4


R.T.: 5.644 min
Delta R.T.: -0.004 min
Response: 28762
Conc: 33.17 ng/ml

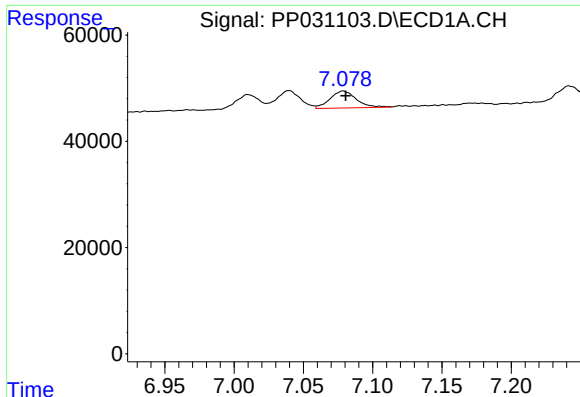

#20 AR-1242-5


R.T.: 7.079 min
Delta R.T.: -0.002 min
Response: 42002
Conc: 44.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

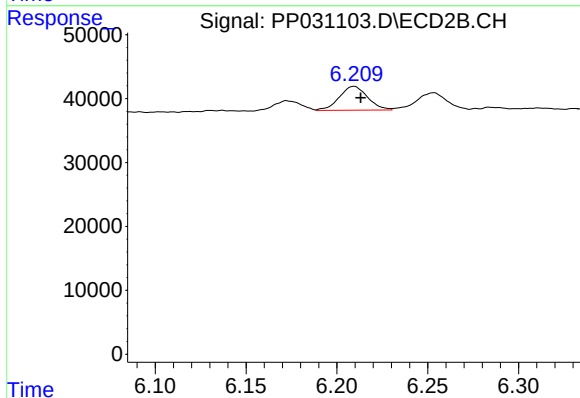


#20 AR-1242-5

R.T.: 6.210 min
Delta R.T.: -0.003 min
Response: 40461
Conc: 40.64 ng/ml

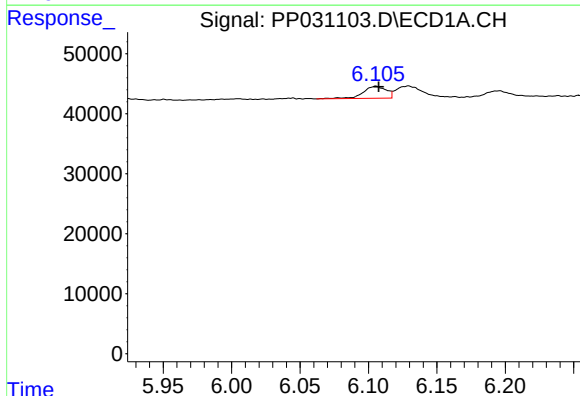


#21 AR-1248-1

R.T.: 6.105 min
Delta R.T.: -0.002 min
Response: 23861
Conc: 24.74 ng/ml

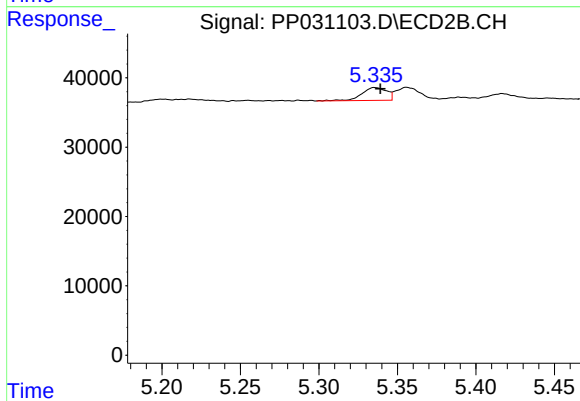

#21 AR-1248-1


R.T.: 5.335 min
Delta R.T.: -0.004 min
Response: 20443
Conc: 22.09 ng/ml

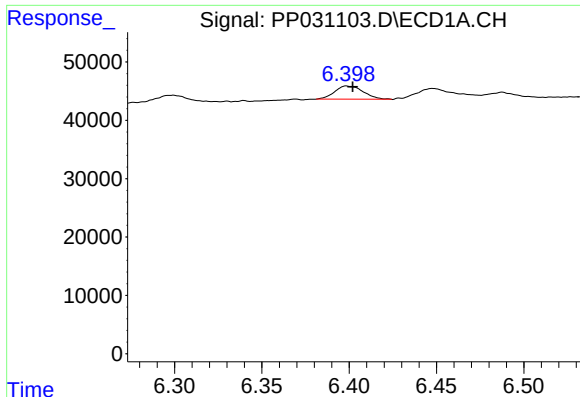

#22 AR-1248-2


R.T.: 6.399 min
Delta R.T.: -0.003 min
Response: 25697
Conc: 22.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

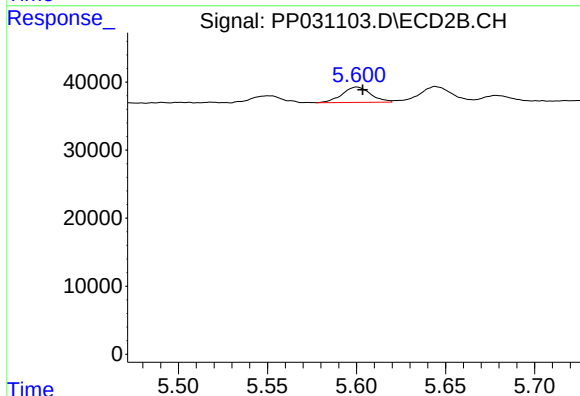


#22 AR-1248-2

R.T.: 5.600 min
Delta R.T.: -0.003 min
Response: 25213
Conc: 22.88 ng/ml

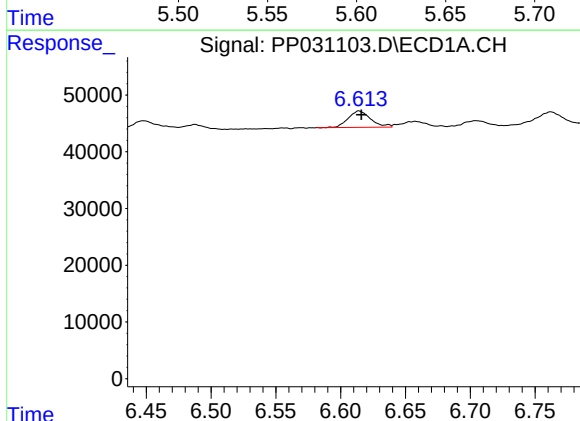


#23 AR-1248-3

R.T.: 6.614 min
Delta R.T.: -0.002 min
Response: 34919
Conc: 24.54 ng/ml

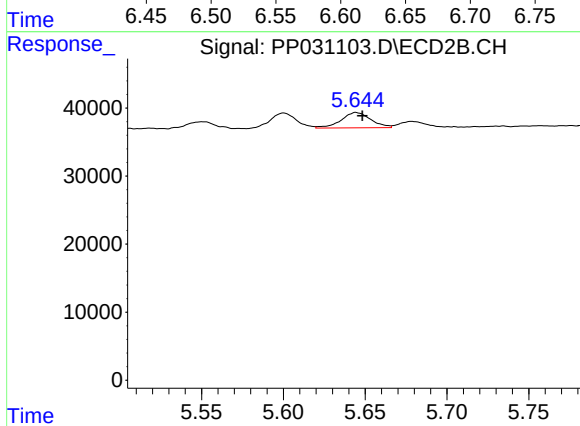

#23 AR-1248-3


R.T.: 5.644 min
Delta R.T.: -0.004 min
Response: 28762
Conc: 23.76 ng/ml

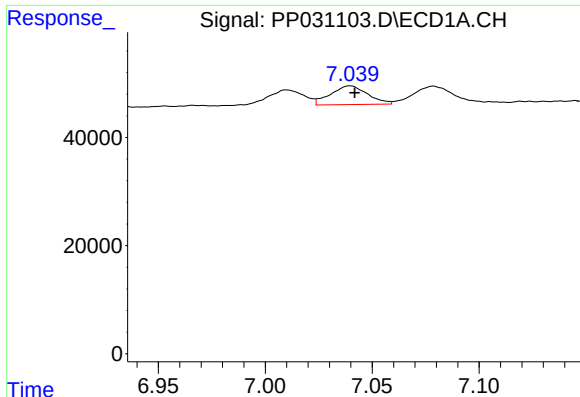

#24 AR-1248-4


R.T.: 7.040 min
Delta R.T.: -0.002 min
Response: 42012
Conc: 27.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

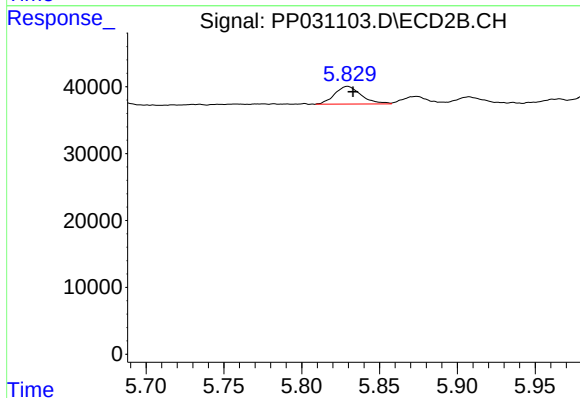


#24 AR-1248-4

R.T.: 5.830 min
Delta R.T.: -0.004 min
Response: 31570
Conc: 21.39 ng/ml

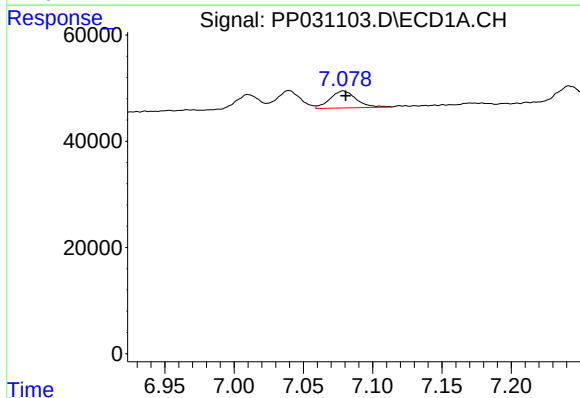


#25 AR-1248-5

R.T.: 7.079 min
Delta R.T.: -0.002 min
Response: 42002
Conc: 27.69 ng/ml

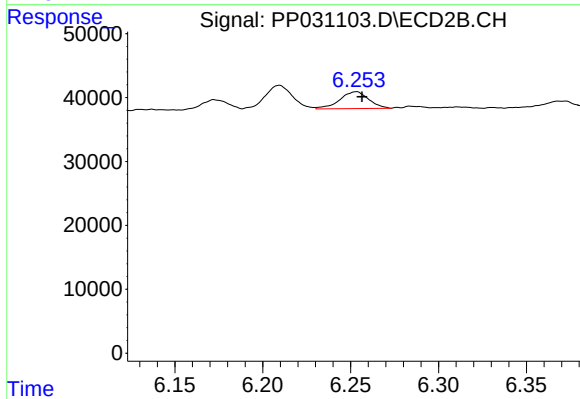

#25 AR-1248-5


R.T.: 6.253 min
Delta R.T.: -0.003 min
Response: 30167
Conc: 23.89 ng/ml

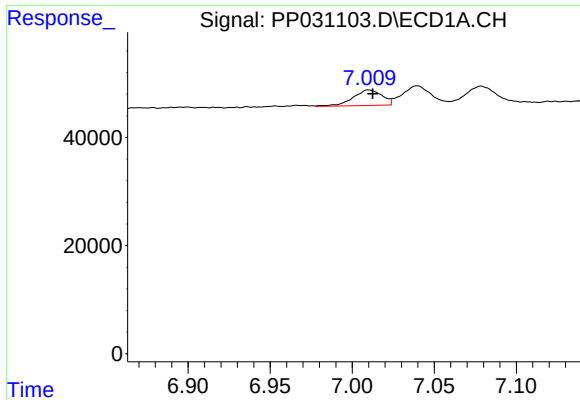

#26 AR-1254-1


R.T.: 7.010 min
Delta R.T.: -0.002 min
Response: 35346
Conc: 25.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

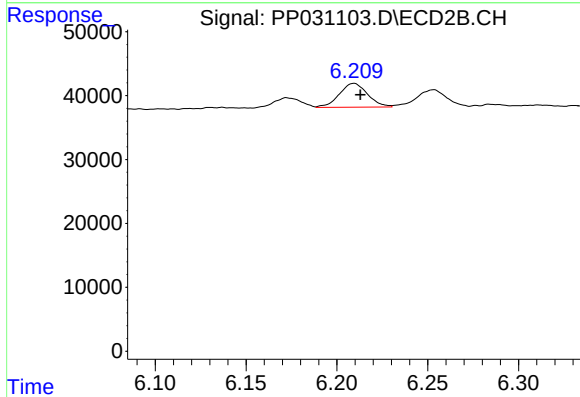


#26 AR-1254-1

R.T.: 6.210 min
Delta R.T.: -0.003 min
Response: 40461
Conc: 20.57 ng/ml

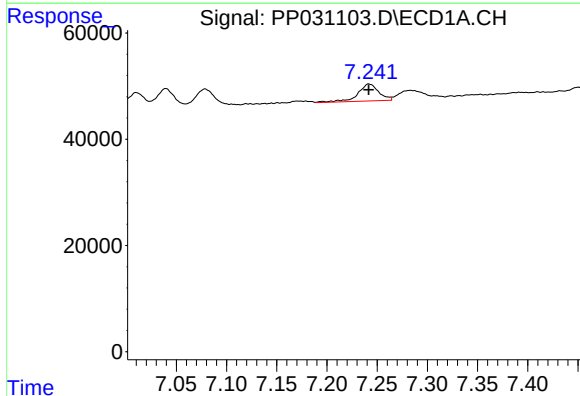


#27 AR-1254-2

R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 46190
Conc: 22.16 ng/ml

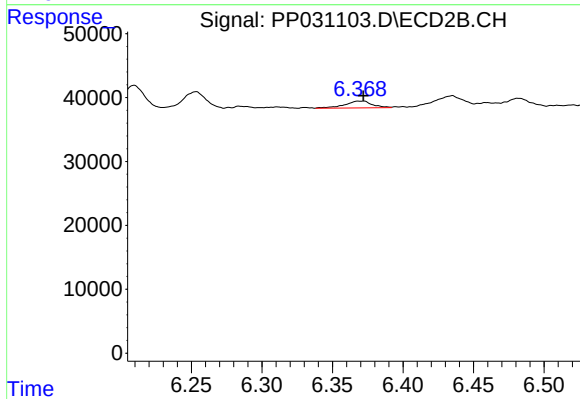

#27 AR-1254-2


R.T.: 6.368 min
Delta R.T.: -0.004 min
Response: 14143
Conc: 8.61 ng/ml

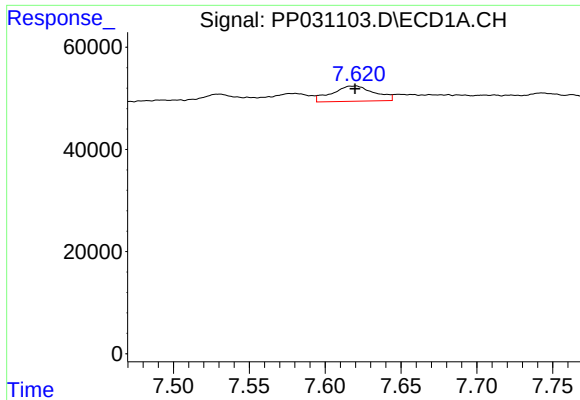

#28 AR-1254-3


R.T.: 7.619 min
Delta R.T.: 0.000 min
Response: 58144
Conc: 25.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

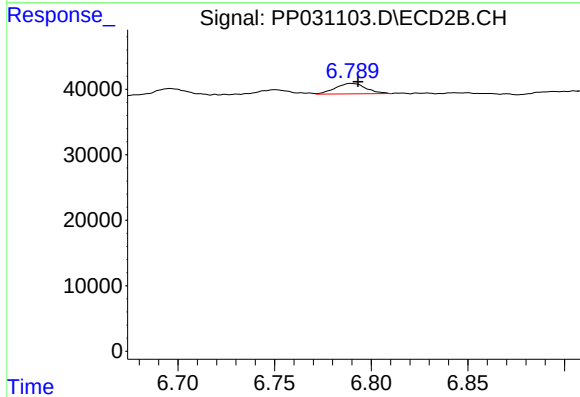


#28 AR-1254-3

R.T.: 6.790 min
Delta R.T.: -0.004 min
Response: 17860
Conc: 6.52 ng/ml

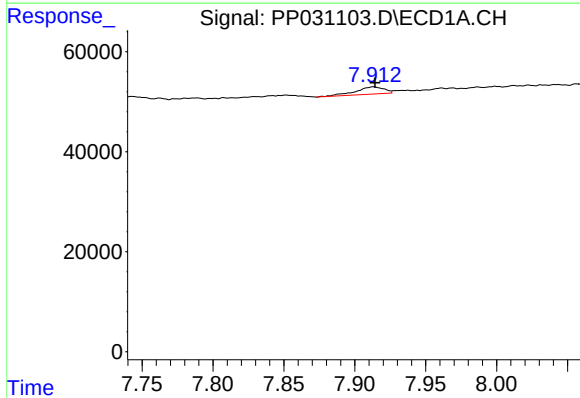


#29 AR-1254-4

R.T.: 7.913 min
Delta R.T.: -0.001 min
Response: 20372
Conc: 12.44 ng/ml

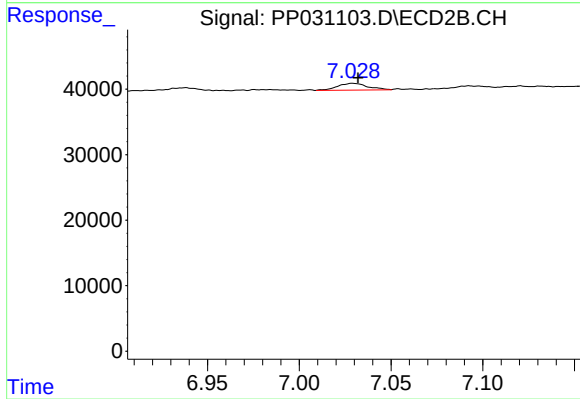

#29 AR-1254-4


R.T.: 7.029 min
Delta R.T.: -0.003 min
Response: 11714
Conc: 7.26 ng/ml

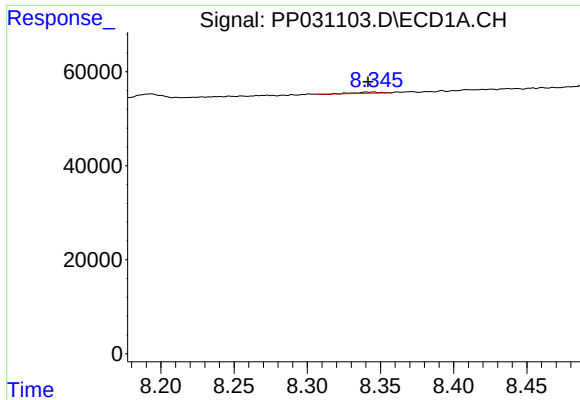

#30 AR-1254-5


R.T.: 8.345 min
Delta R.T.: 0.004 min
Response: 2758
Conc: 1.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

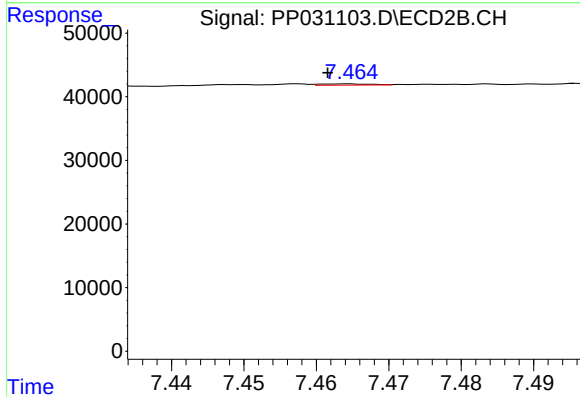


#30 AR-1254-5

R.T.: 7.465 min
Delta R.T.: 0.003 min
Response: 970
Conc: 0.44 ng/ml

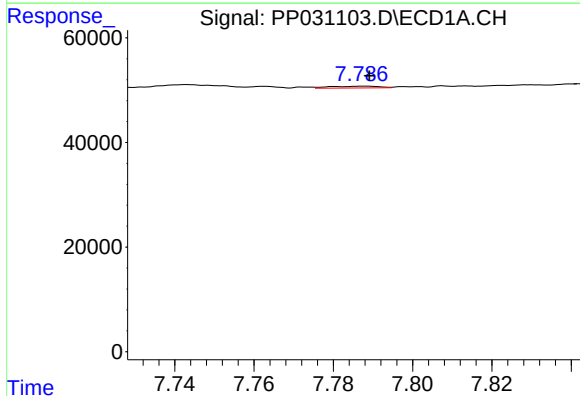


#31 AR-1260-1

R.T.: 7.788 min
Delta R.T.: -0.001 min
Response: 3043
Conc: 1.66 ng/ml

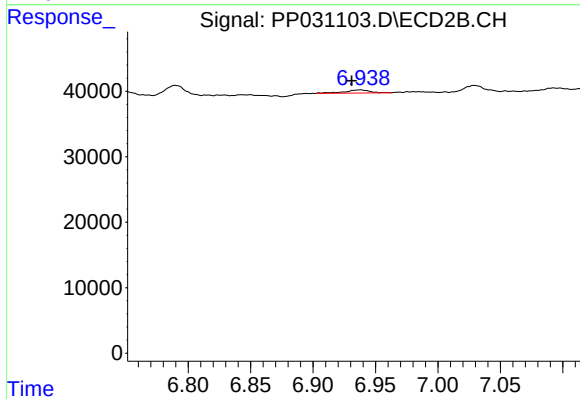

#31 AR-1260-1


R.T.: 6.938 min
Delta R.T.: 0.007 min
Response: 6918
Conc: 3.45 ng/ml

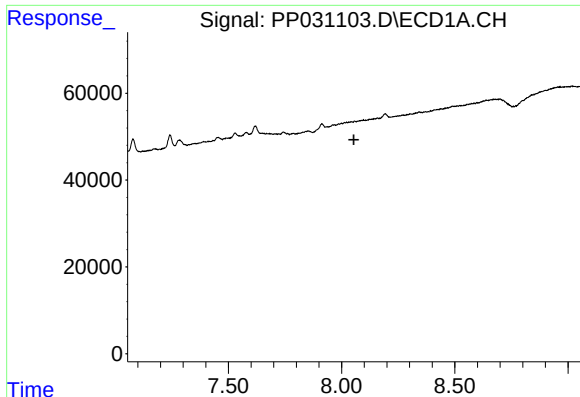

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 8.054 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

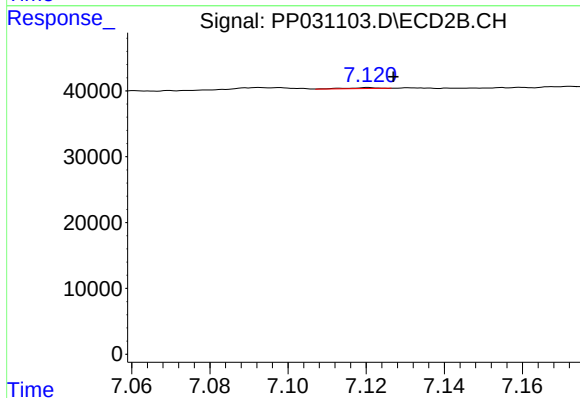


#32 AR-1260-2

R.T.: 7.121 min
Delta R.T.: -0.006 min
Response: 869
Conc: 0.37 ng/ml

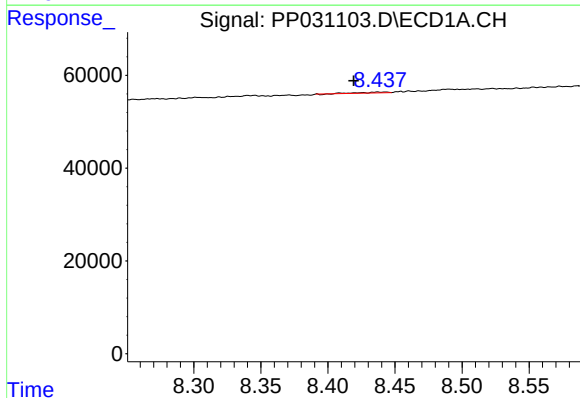


#33 AR-1260-3

R.T.: 8.437 min
Delta R.T.: 0.018 min
Response: 2011
Conc: 1.22 ng/ml

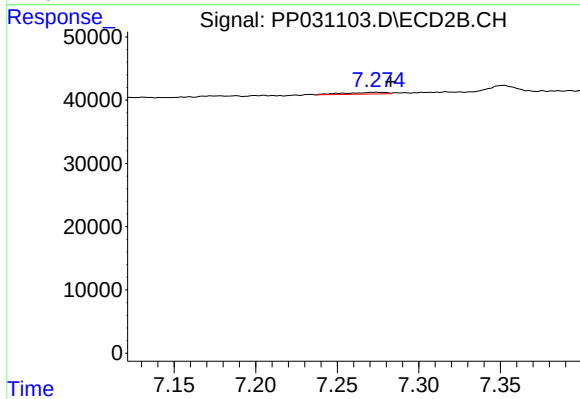

#33 AR-1260-3


R.T.: 7.274 min
Delta R.T.: -0.009 min
Response: 4978
Conc: 2.19 ng/ml

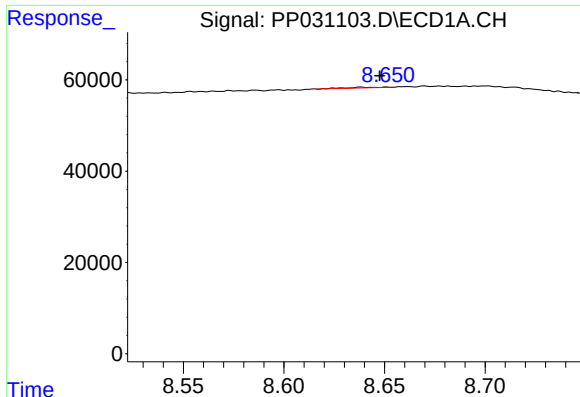

#34 AR-1260-4


R.T.: 8.638 min
Delta R.T.: -0.009 min
Response: 1702
Conc: 0.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

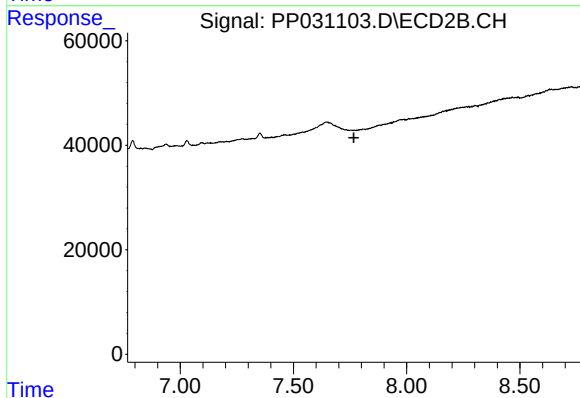


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.767 min
Response: 0
Conc: N.D.

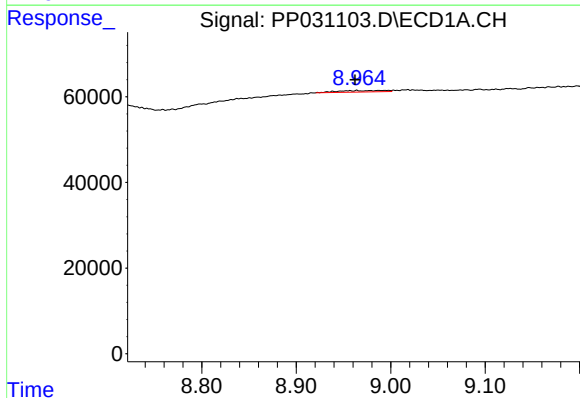


#35 AR-1260-5

R.T.: 8.964 min
Delta R.T.: 0.002 min
Response: 11884
Conc: 3.15 ng/ml

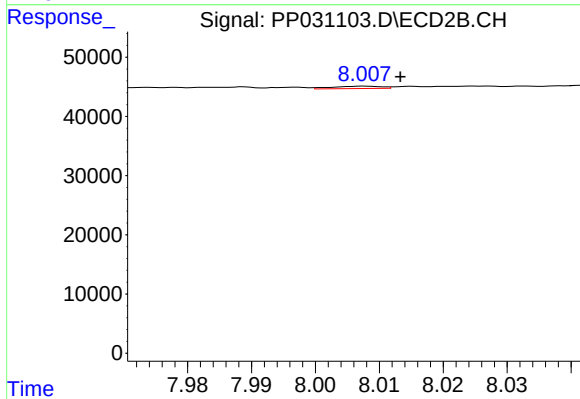

#35 AR-1260-5


R.T.: 8.008 min
Delta R.T.: -0.005 min
Response: 2124
Conc: 0.47 ng/ml

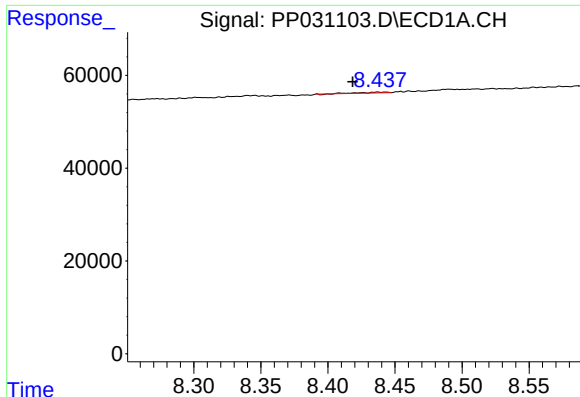

#36 AR-1262-1


R.T.: 8.437 min
Delta R.T.: 0.019 min
Response: 2011
Conc: 1.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

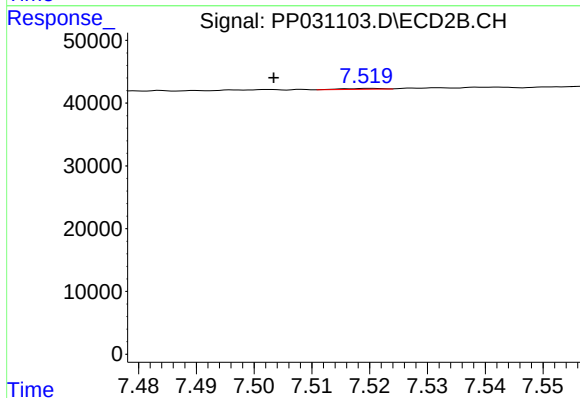


#36 AR-1262-1

R.T.: 7.520 min
Delta R.T.: 0.017 min
Response: 687
Conc: 0.30 ng/ml

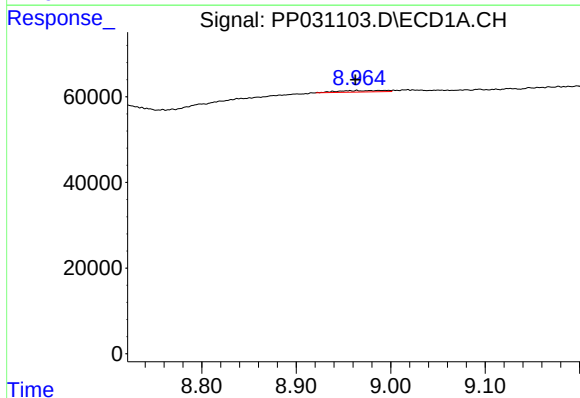


#37 AR-1262-2

R.T.: 8.964 min
Delta R.T.: 0.002 min
Response: 11884
Conc: 3.27 ng/ml

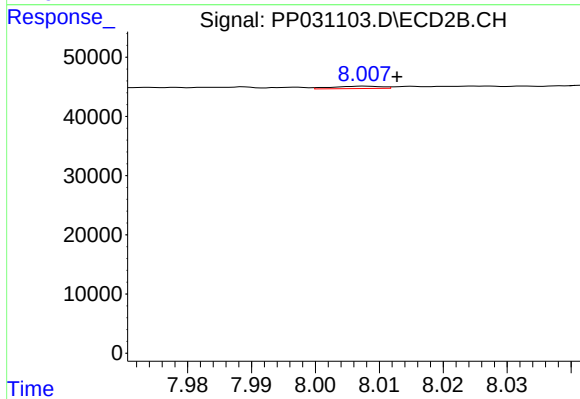

#37 AR-1262-2


R.T.: 8.008 min
Delta R.T.: -0.005 min
Response: 2124
Conc: 0.51 ng/ml

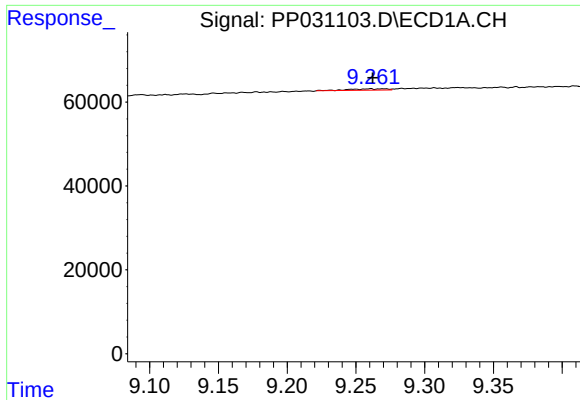

#38 AR-1262-3


R.T.: 9.261 min
Delta R.T.: -0.002 min
Response: 5459
Conc: 2.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

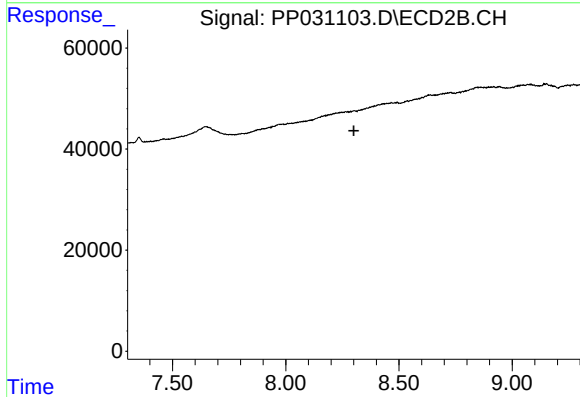


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 8.301 min
Response: 0
Conc: N.D.

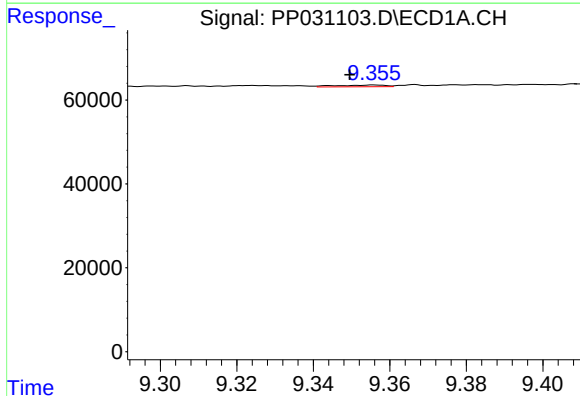


#39 AR-1262-4

R.T.: 9.356 min
Delta R.T.: 0.006 min
Response: 3705
Conc: 1.80 ng/ml

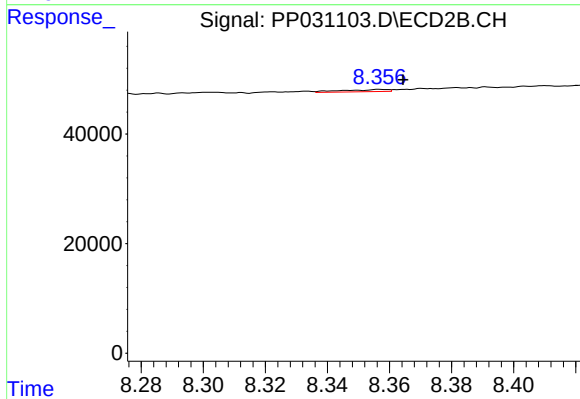

#39 AR-1262-4


R.T.: 8.357 min
Delta R.T.: -0.008 min
Response: 3930
Conc: 1.24 ng/ml

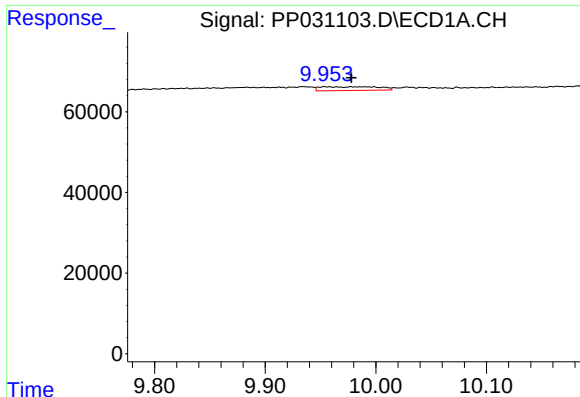

#40 AR-1262-5


R.T.: 9.955 min
Delta R.T.: -0.023 min
Response: 34014
Conc: 24.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

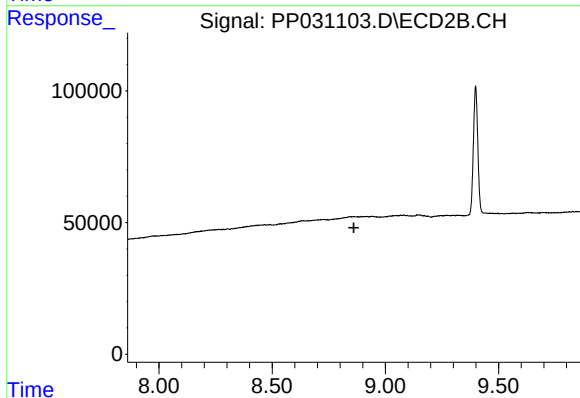


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 8.861 min
Response: 0
Conc: N.D.

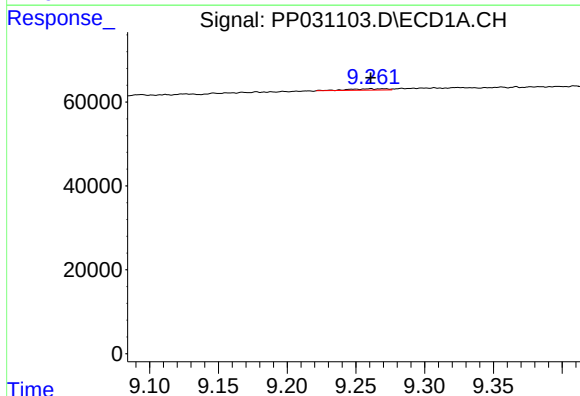


#41 AR-1268-1

R.T.: 9.261 min
Delta R.T.: 0.000 min
Response: 5459
Conc: 1.25 ng/ml

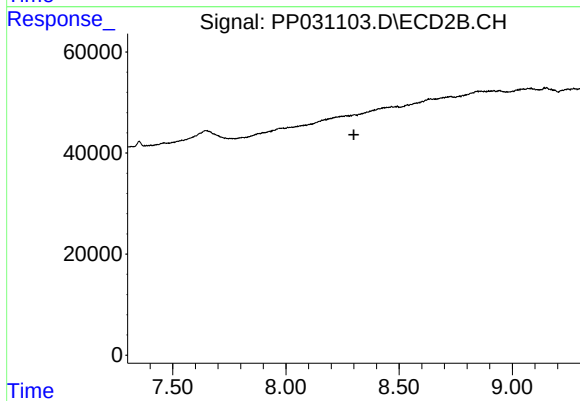

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 8.300 min
Response: 0
Conc: N.D.

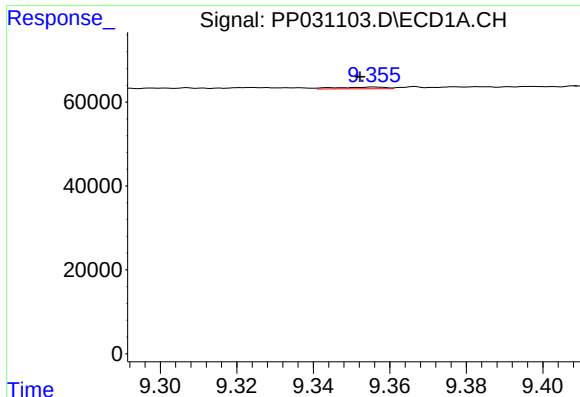

#42 AR-1268-2


R.T.: 9.356 min
Delta R.T.: 0.004 min
Response: 3705
Conc: 0.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

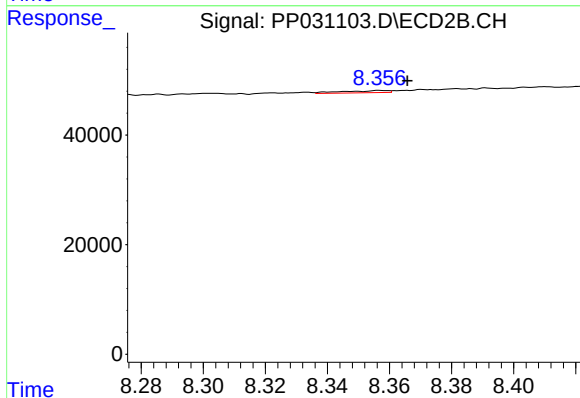


#42 AR-1268-2

R.T.: 8.357 min
Delta R.T.: -0.009 min
Response: 3930
Conc: 0.83 ng/ml

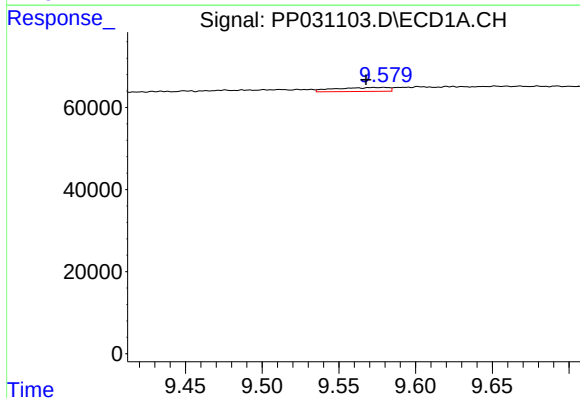


#43 AR-1268-3

R.T.: 9.579 min
Delta R.T.: 0.012 min
Response: 23731
Conc: 6.56 ng/ml

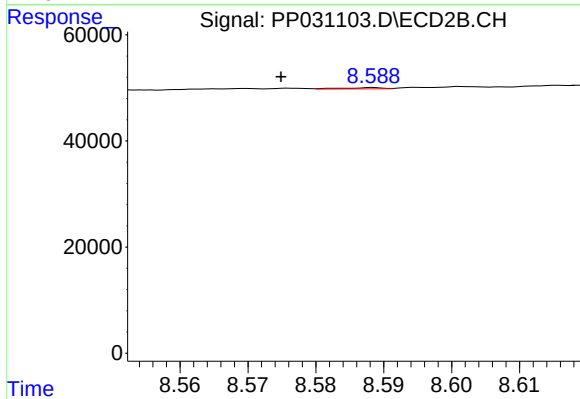

#43 AR-1268-3


R.T.: 8.588 min
Delta R.T.: 0.014 min
Response: 1010
Conc: 0.25 ng/ml

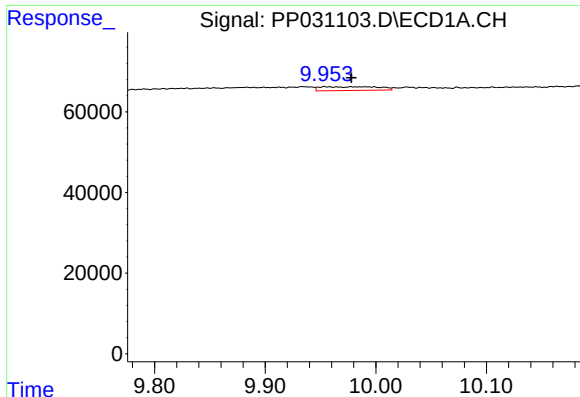

#44 AR-1268-4


R.T.: 9.955 min
Delta R.T.: -0.023 min
Response: 34014
Conc: 21.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

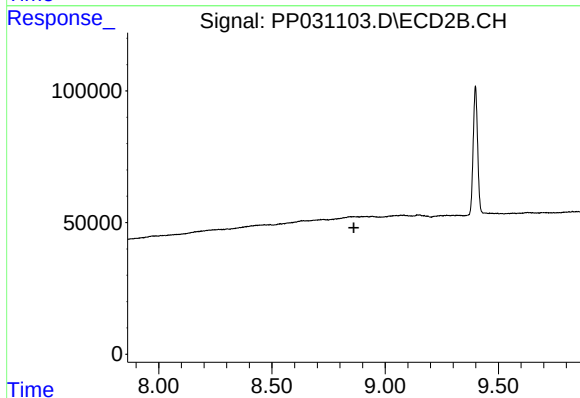


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 8.862 min
Response: 0
Conc: N.D.

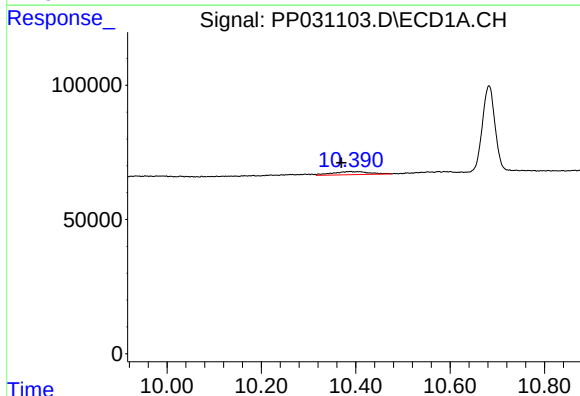

#45 AR-1268-5

R.T.: 10.388 min
Delta R.T.: 0.019 min
Response: 62537
Conc: 5.23 ng/ml

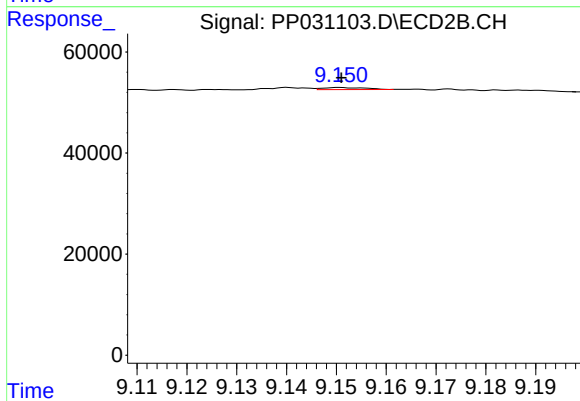

#45 AR-1268-5

R.T.: 9.151 min
Delta R.T.: 0.000 min
Response: 2357
Conc: 0.18 ng/ml