

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110420\
 Data File : PP031143.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Nov 2020 1:38
 Operator : DD\AJ
 Sample : L4214-07
 Misc : AR1232 LOD 40 PPB
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2020

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 05:13:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 04 08:24:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.800	4.074	957328	929025	14.333	13.977
2)	SA Decachlor...	10.681	9.395	607530	675944	15.194	16.188
Target Compounds							
3)	L1 AR-1016-1	6.105	5.335	27400	25031	14.072	13.492
4)	L1 AR-1016-2	6.128	5.356	43201	36268	15.133	13.343
5)	L1 AR-1016-3	6.195	5.547	24420	19590	14.020	15.467
6)	L1 AR-1016-4	6.300	5.601	18853	10536	13.047	11.424
7)	L1 AR-1016-5	6.614	5.827	18059	15609	14.487	11.893
8)	L2 AR-1221-1	5.044	4.334	15360	14520	25.436	25.781
9)	L2 AR-1221-2	5.144	4.431	23445	21025	52.197	50.677
10)	L2 AR-1221-3	5.228	4.522	42713	37920	31.647	28.915
11)	L3 AR-1232-1	5.228	4.522	42713	37920	34.925	31.656
12)	L3 AR-1232-2	5.813	5.356	22901	36268	37.713	34.128
13)	L3 AR-1232-3	6.128	5.547	43201	19590	38.672	38.210
14)	L3 AR-1232-4	6.300	5.642	18853	14876	33.218	34.061
15)	L3 AR-1232-5	6.400	5.827	11203	15609	32.331	32.325
16)	L4 AR-1242-1	6.105	5.335	27400	25031	20.395	19.450
17)	L4 AR-1242-2	6.128	5.356	43201	36268	22.120	19.422
18)	L4 AR-1242-3	6.195	5.547	24420	19590	20.023	20.866
19)	L4 AR-1242-4	6.300	5.642	18853	14876	18.609	17.154
20)	L4 AR-1242-5	7.078	6.208	22466	16536	23.542	16.611 #
21)	L5 AR-1248-1	6.105	5.335	27400	25031	28.414	27.052
22)	L5 AR-1248-2	6.400	5.601	11203	10536	9.686	9.560
23)	L5 AR-1248-3	6.614	5.642	18059	14876	12.693	12.291
24)	L5 AR-1248-4	7.039	5.827	19666	15609	12.904	10.577
25)	L5 AR-1248-5	7.078	6.250	22466	21085	14.808	16.695
26)	L6 AR-1254-1	7.012	6.208	23342	16536	16.625	8.408 #
27)	L6 AR-1254-2	7.243	0.000	26224	0	12.581	N.D. #
28)	L6 AR-1254-3	7.621	0.000	62951	0	27.274	N.D. #
29)	L6 AR-1254-4	7.913	0.000	15857	0	9.686	N.D. #
30)	L6 AR-1254-5	0.000	7.452	0	1514	N.D.	0.691 #
31)	L7 AR-1260-1	7.784	0.000	5195	0	2.828	N.D. #
33)	L7 AR-1260-3	8.416	0.000	2746	0	1.668	N.D. #
34)	L7 AR-1260-4	8.634	0.000	1683	0	0.905	N.D. #
35)	L7 AR-1260-5	0.000	8.014	0	6104	N.D.	1.356 #
36)	L8 AR-1262-1	8.416	7.511	2746	1137	1.367	0.490 #
37)	L8 AR-1262-2	0.000	8.014	0	6104	N.D.	1.472 #
38)	L8 AR-1262-3	9.288f	0.000	7107	0	2.749	N.D. #
39)	L8 AR-1262-4	9.349	8.379	13640	2390	6.625	0.753 #
40)	L8 AR-1262-5	9.967	0.000	4722	0	3.334	N.D. #
41)	L9 AR-1268-1	9.288f	0.000	7107	0	1.627	N.D. #
42)	L9 AR-1268-2	9.349	8.379	13640	2390	3.172	0.503 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110420\
 Data File : PP031143.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Nov 2020 1:38
 Operator : DD\AJ
 Sample : L4214-07
 Misc : AR1232 LOD 40 PPB
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2020

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 05:13:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 04 08:24:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	9.557	8.580	8674	1532	2.398	0.383 #
44) L9	AR-1268-4	9.967	0.000	4722	0	2.981	N.D. #
45) L9	AR-1268-5	10.383	9.146	33968	3912	2.840	0.292 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110420\
Data File : PP031143.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Nov 2020 1:38
Operator : DD\AJ
Sample : L4214-07
Misc : AR1232 LOD 40 PPB
ALS Vial : 50 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 05:13:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 04 08:24:38 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

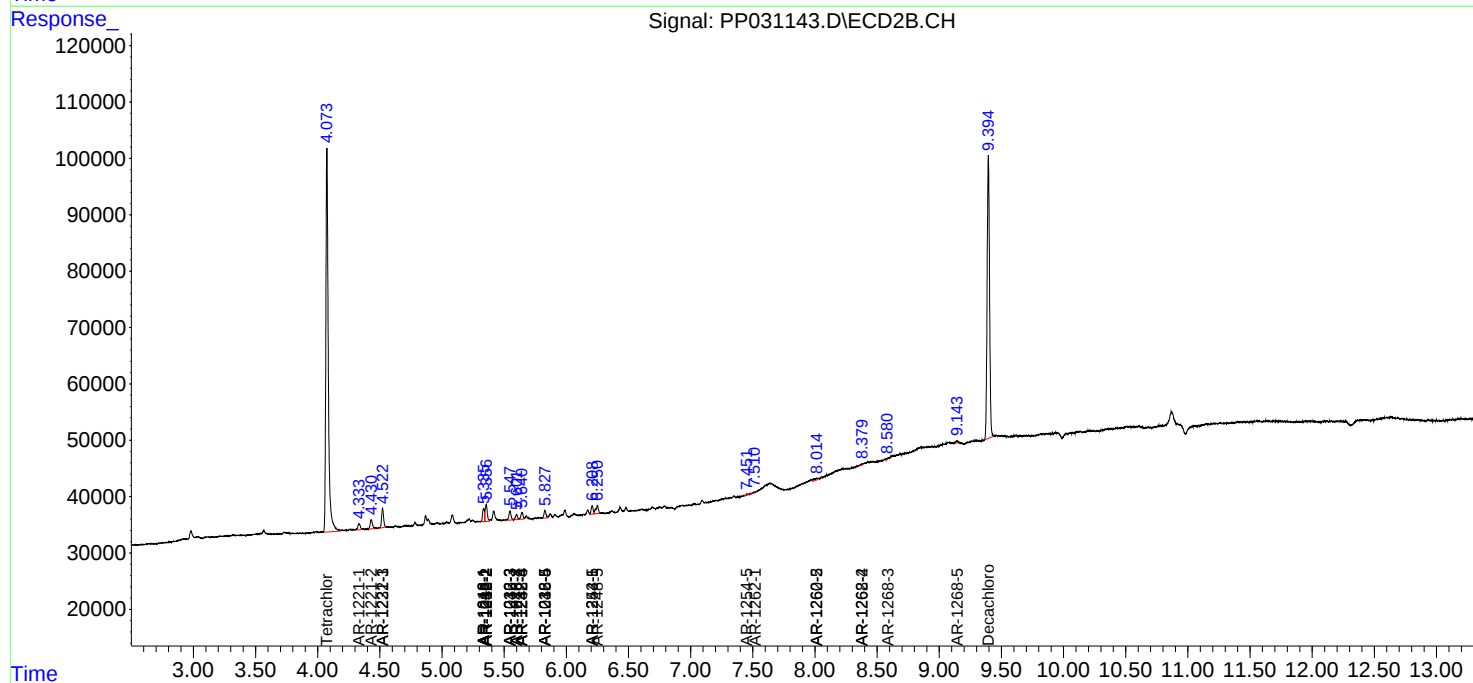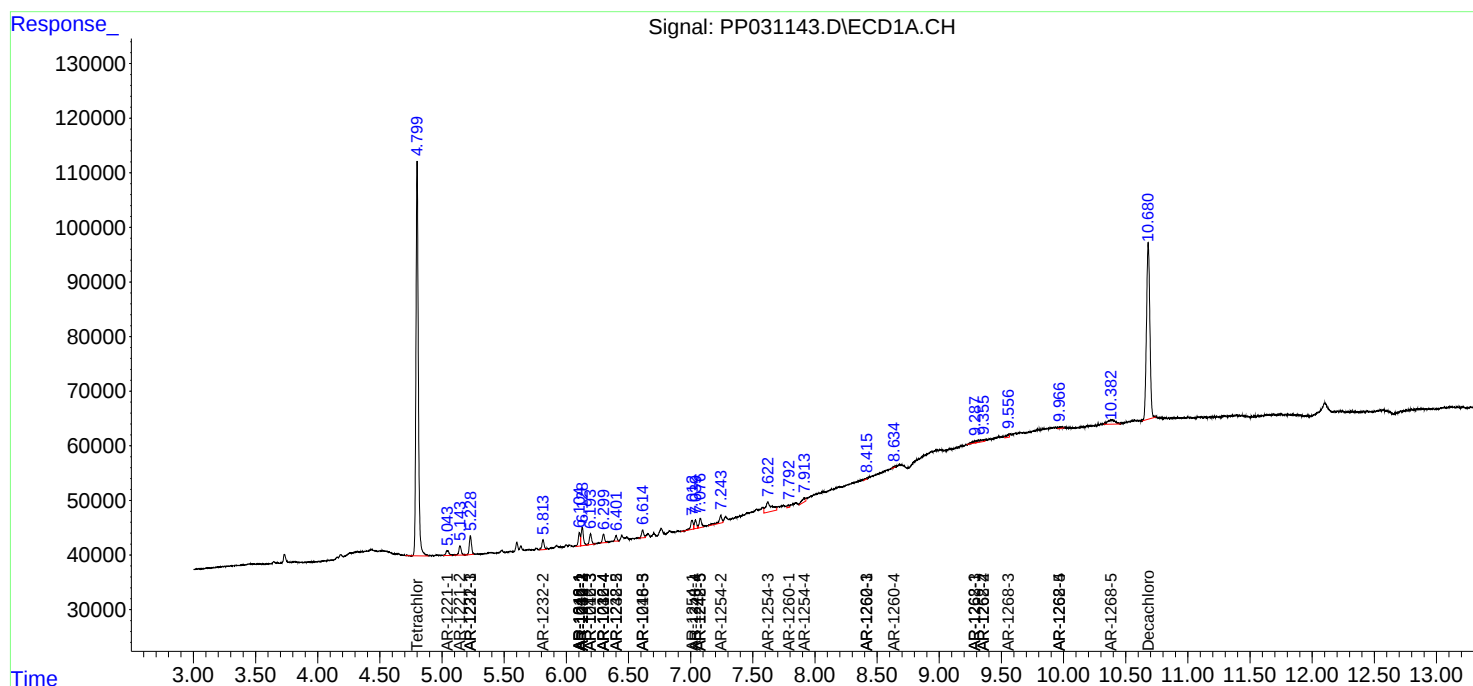


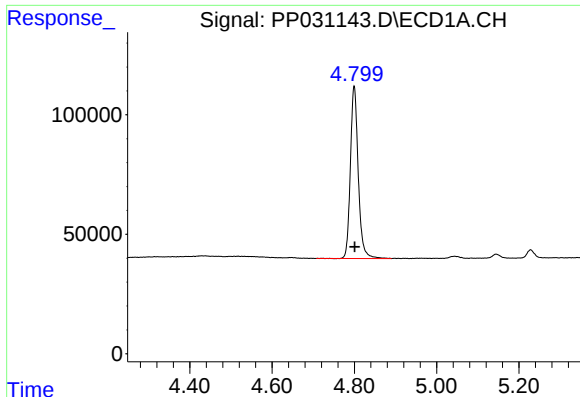

#1 Tetrachloro-m-xylene


R.T.: 4.800 min
Delta R.T.: -0.001 min
Response: 957328
Conc: 14.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

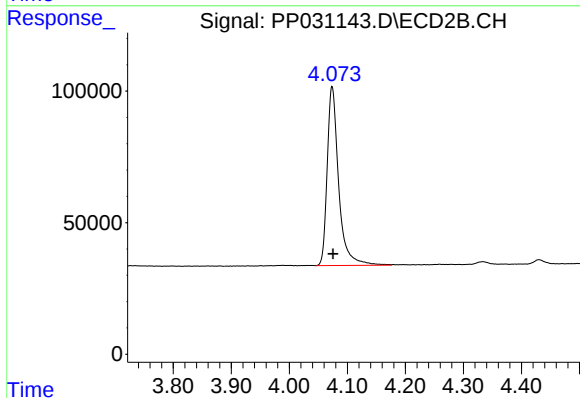


#1 Tetrachloro-m-xylene

R.T.: 4.074 min
Delta R.T.: -0.002 min
Response: 929025
Conc: 13.98 ng/ml

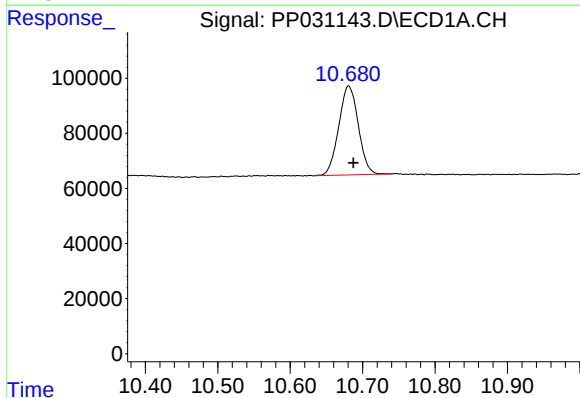


#2 Decachlorobiphenyl

R.T.: 10.681 min
Delta R.T.: -0.007 min
Response: 607530
Conc: 15.19 ng/ml

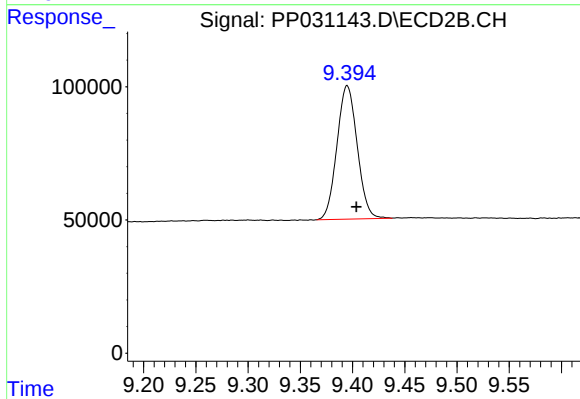

#2 Decachlorobiphenyl


R.T.: 9.395 min
Delta R.T.: -0.009 min
Response: 675944
Conc: 16.19 ng/ml

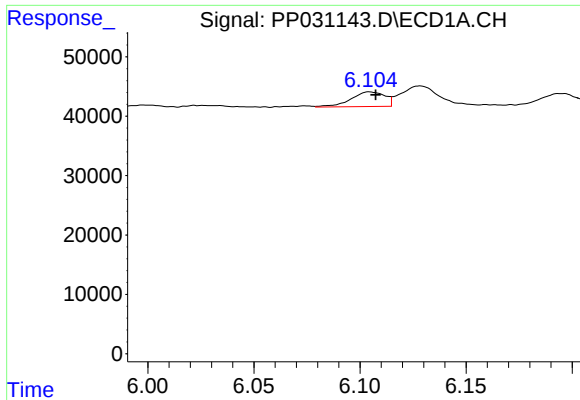

#3 AR-1016-1


R.T.: 6.105 min
Delta R.T.: -0.003 min
Response: 27400
Conc: 14.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

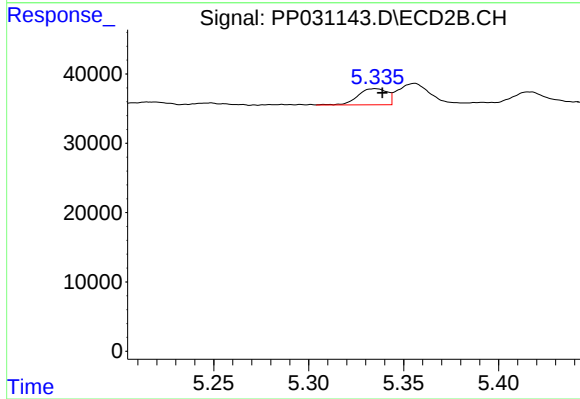


#3 AR-1016-1

R.T.: 5.335 min
Delta R.T.: -0.004 min
Response: 25031
Conc: 13.49 ng/ml

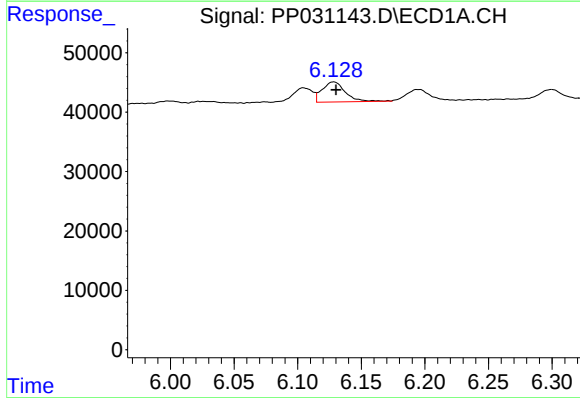


#4 AR-1016-2

R.T.: 6.128 min
Delta R.T.: -0.002 min
Response: 43201
Conc: 15.13 ng/ml

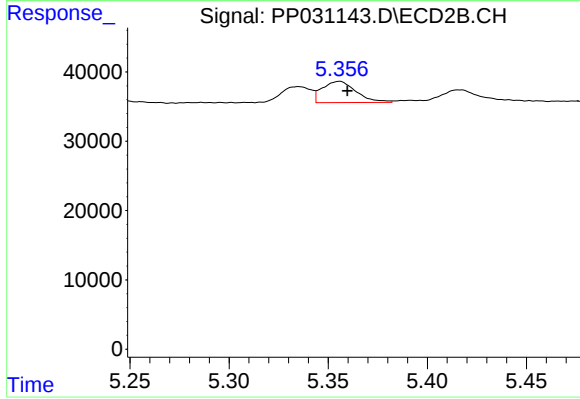

#4 AR-1016-2


R.T.: 5.356 min
Delta R.T.: -0.004 min
Response: 36268
Conc: 13.34 ng/ml

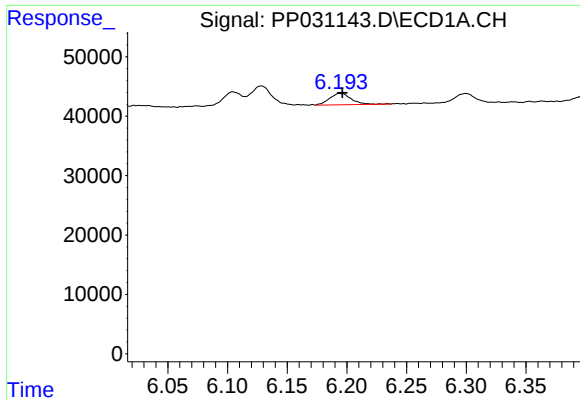

#5 AR-1016-3


R.T.: 6.195 min
Delta R.T.: -0.001 min
Response: 24420
Conc: 14.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

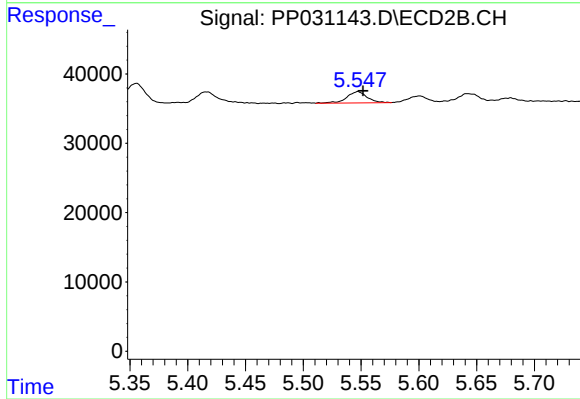


#5 AR-1016-3

R.T.: 5.547 min
Delta R.T.: -0.004 min
Response: 19590
Conc: 15.47 ng/ml

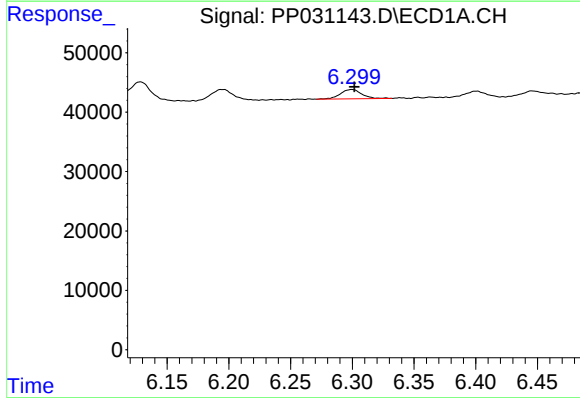


#6 AR-1016-4

R.T.: 6.300 min
Delta R.T.: -0.002 min
Response: 18853
Conc: 13.05 ng/ml

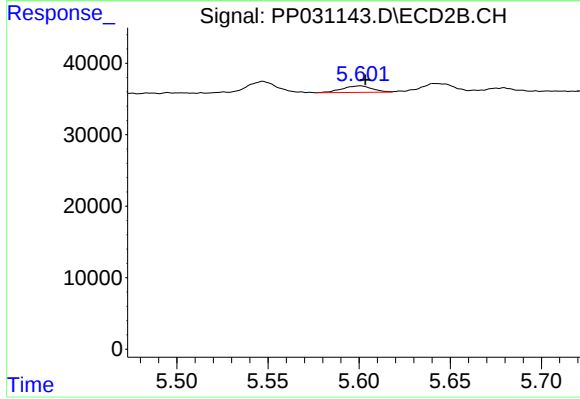

#6 AR-1016-4


R.T.: 5.601 min
Delta R.T.: -0.003 min
Response: 10536
Conc: 11.42 ng/ml

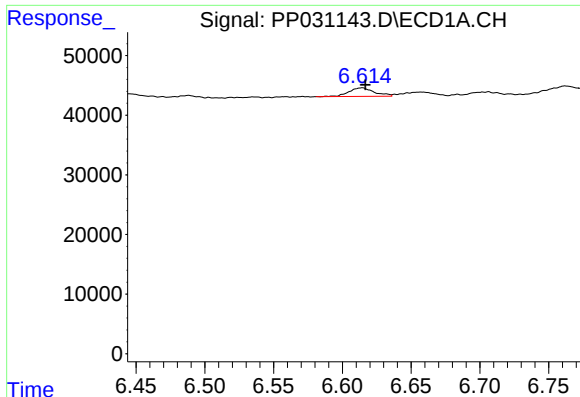

#7 AR-1016-5


R.T.: 6.614 min
Delta R.T.: -0.003 min
Response: 18059
Conc: 14.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

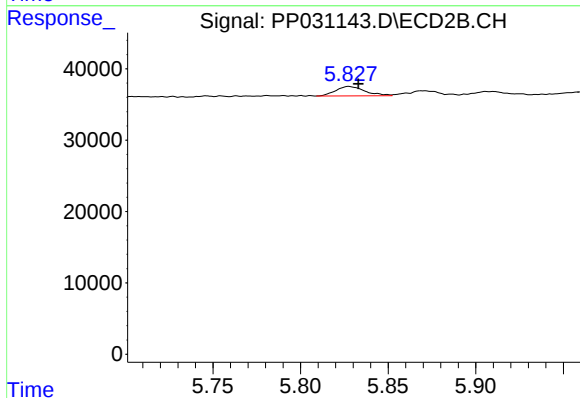


#7 AR-1016-5

R.T.: 5.827 min
Delta R.T.: -0.006 min
Response: 15609
Conc: 11.89 ng/ml

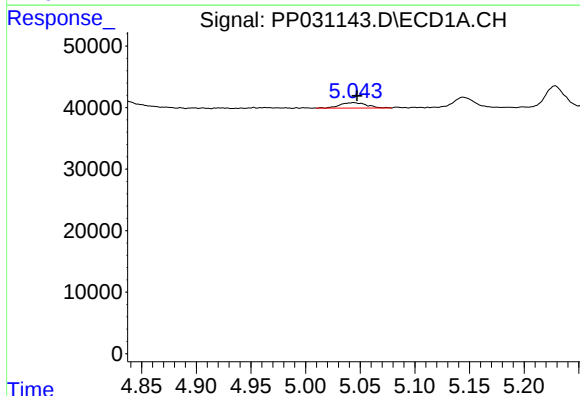


#8 AR-1221-1

R.T.: 5.044 min
Delta R.T.: -0.003 min
Response: 15360
Conc: 25.44 ng/ml

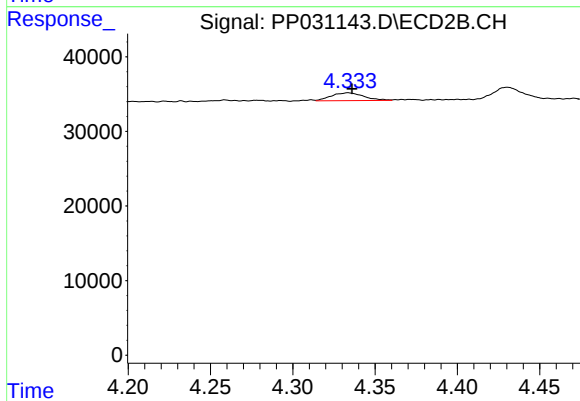

#8 AR-1221-1


R.T.: 4.334 min
Delta R.T.: -0.002 min
Response: 14520
Conc: 25.78 ng/ml

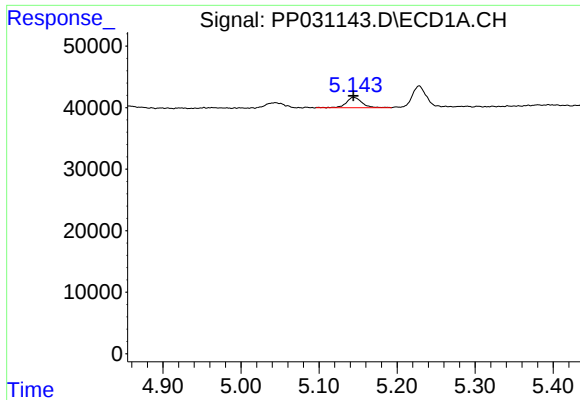

#9 AR-1221-2


R.T.: 5.144 min
Delta R.T.: 0.000 min
Response: 23445
Conc: 52.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

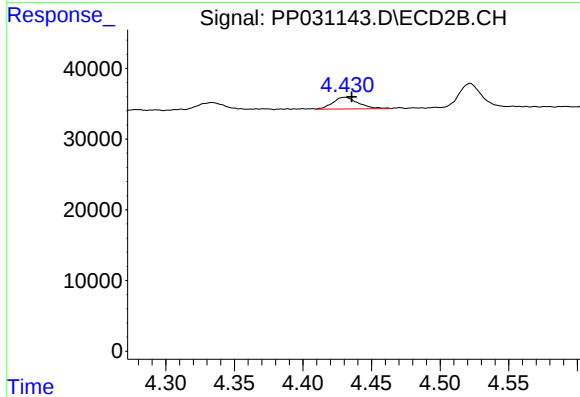


#9 AR-1221-2

R.T.: 4.431 min
Delta R.T.: -0.005 min
Response: 21025
Conc: 50.68 ng/ml

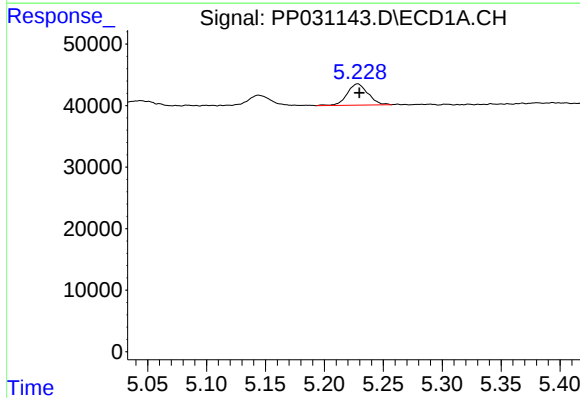


#10 AR-1221-3

R.T.: 5.228 min
Delta R.T.: -0.001 min
Response: 42713
Conc: 31.65 ng/ml

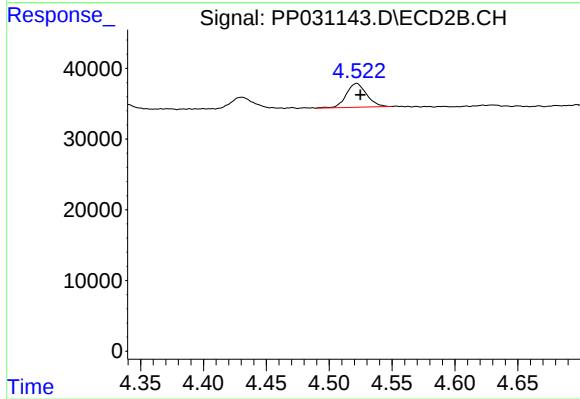

#10 AR-1221-3


R.T.: 4.522 min
Delta R.T.: -0.003 min
Response: 37920
Conc: 28.92 ng/ml

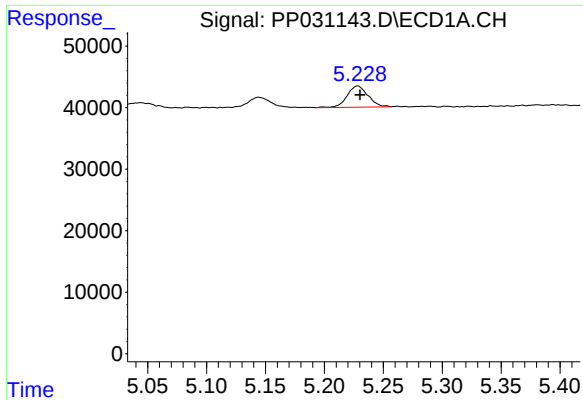

#11 AR-1232-1


R.T.: 5.228 min
Delta R.T.: -0.002 min
Response: 42713
Conc: 34.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

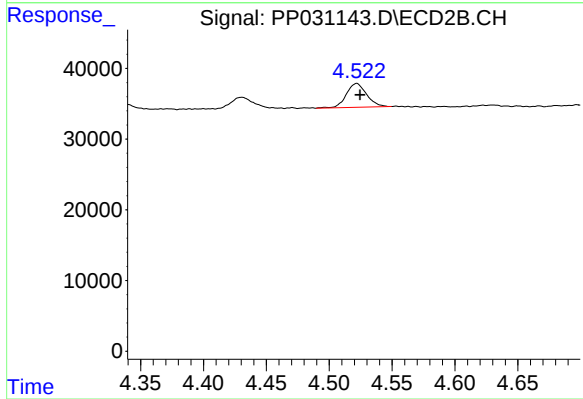


#11 AR-1232-1

R.T.: 4.522 min
Delta R.T.: -0.003 min
Response: 37920
Conc: 31.66 ng/ml

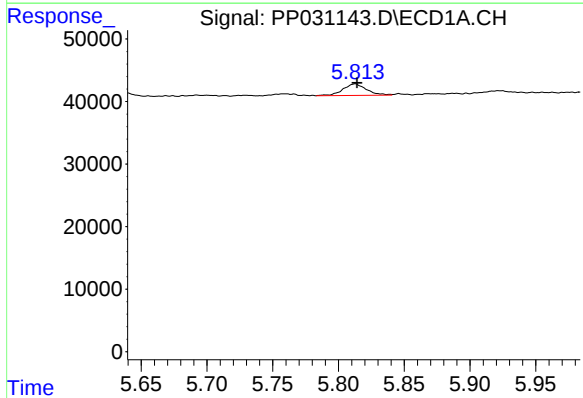


#12 AR-1232-2

R.T.: 5.813 min
Delta R.T.: -0.002 min
Response: 22901
Conc: 37.71 ng/ml

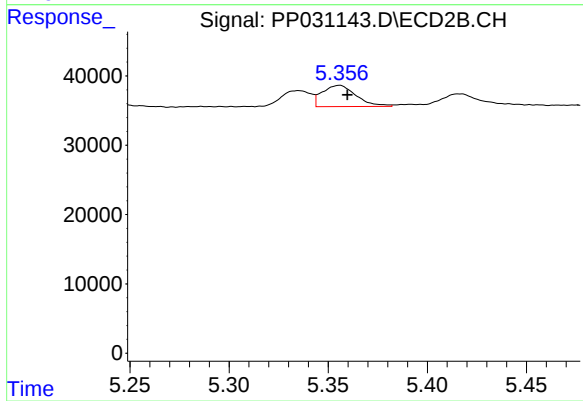

#12 AR-1232-2


R.T.: 5.356 min
Delta R.T.: -0.004 min
Response: 36268
Conc: 34.13 ng/ml

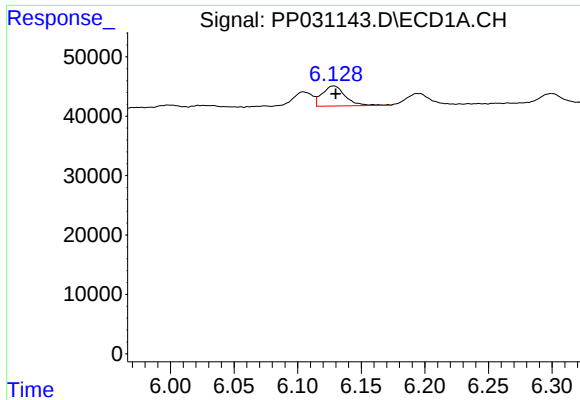

#13 AR-1232-3


R.T.: 6.128 min
Delta R.T.: -0.002 min
Response: 43201
Conc: 38.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

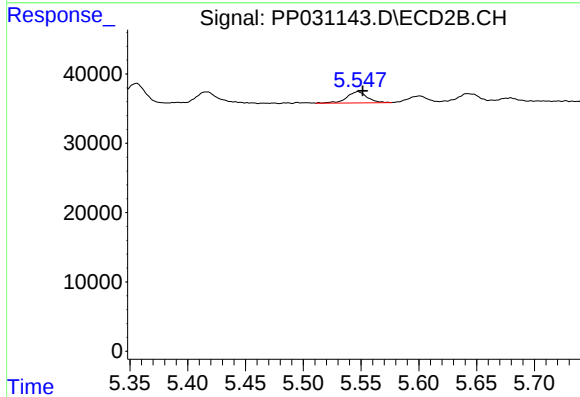


#13 AR-1232-3

R.T.: 5.547 min
Delta R.T.: -0.004 min
Response: 19590
Conc: 38.21 ng/ml

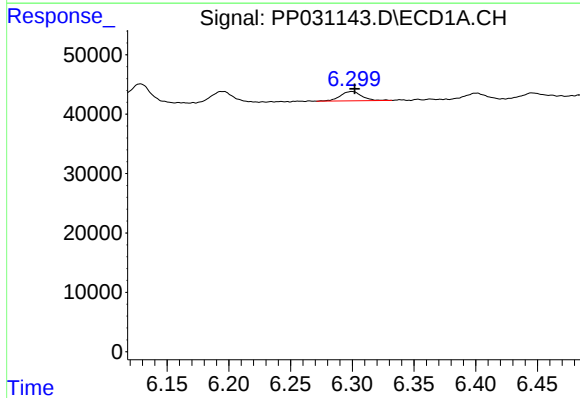


#14 AR-1232-4

R.T.: 6.300 min
Delta R.T.: -0.002 min
Response: 18853
Conc: 33.22 ng/ml

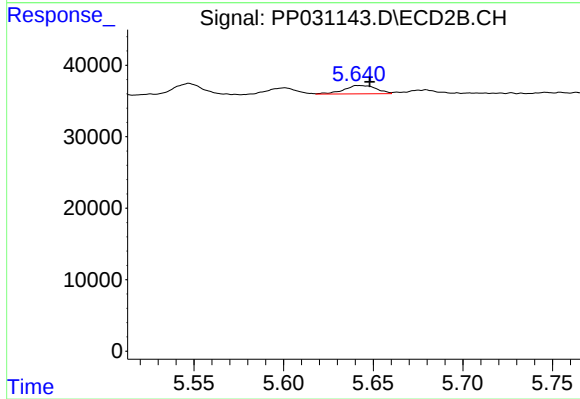

#14 AR-1232-4


R.T.: 5.642 min
Delta R.T.: -0.007 min
Response: 14876
Conc: 34.06 ng/ml

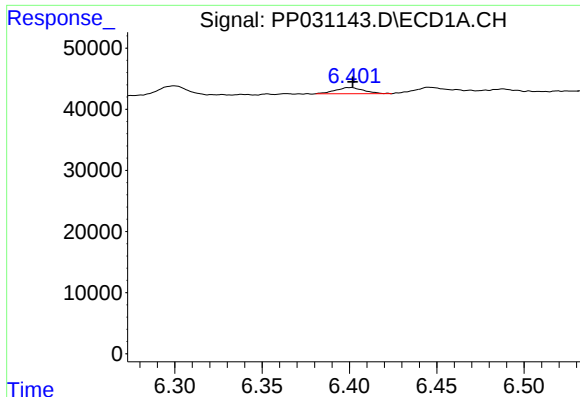

#15 AR-1232-5


R.T.: 6.400 min
Delta R.T.: -0.001 min
Response: 11203
Conc: 32.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

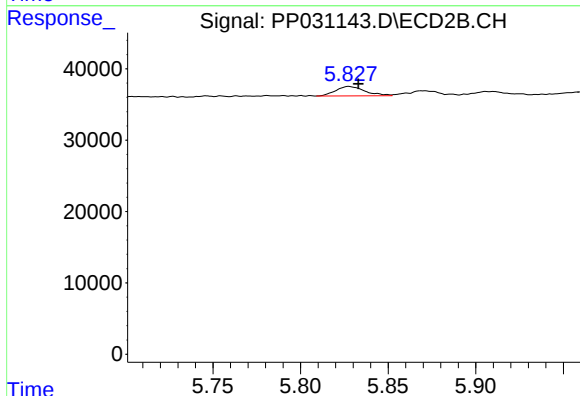


#15 AR-1232-5

R.T.: 5.827 min
Delta R.T.: -0.006 min
Response: 15609
Conc: 32.32 ng/ml

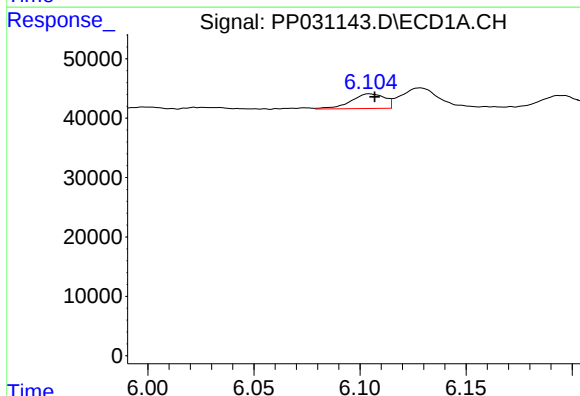


#16 AR-1242-1

R.T.: 6.105 min
Delta R.T.: -0.002 min
Response: 27400
Conc: 20.39 ng/ml

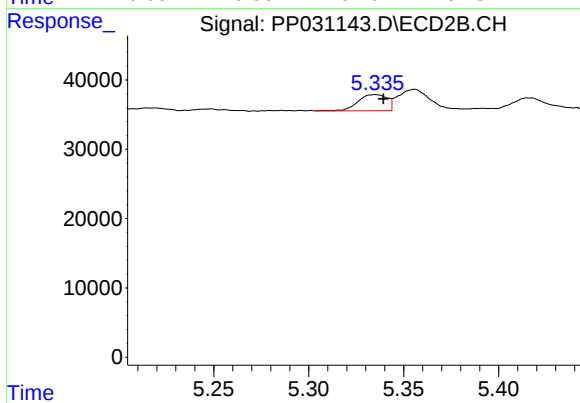

#16 AR-1242-1


R.T.: 5.335 min
Delta R.T.: -0.004 min
Response: 25031
Conc: 19.45 ng/ml

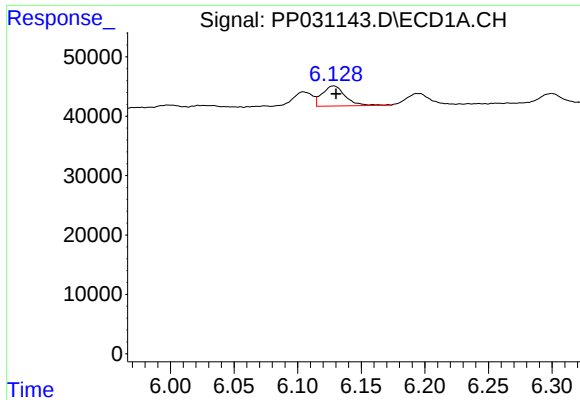

#17 AR-1242-2


R.T.: 6.128 min
Delta R.T.: -0.002 min
Response: 43201
Conc: 22.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

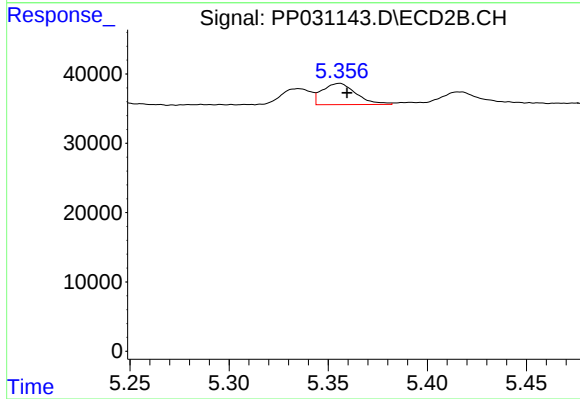


#17 AR-1242-2

R.T.: 5.356 min
Delta R.T.: -0.004 min
Response: 36268
Conc: 19.42 ng/ml

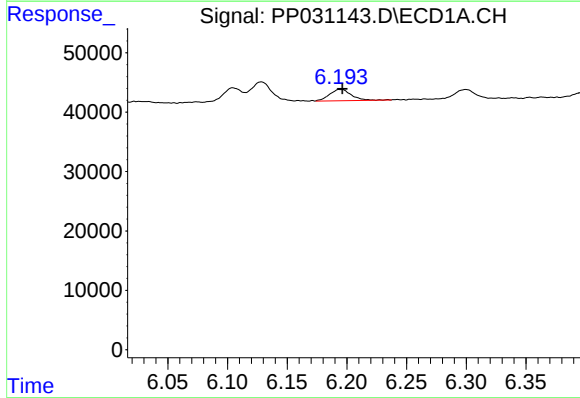


#18 AR-1242-3

R.T.: 6.195 min
Delta R.T.: -0.001 min
Response: 24420
Conc: 20.02 ng/ml

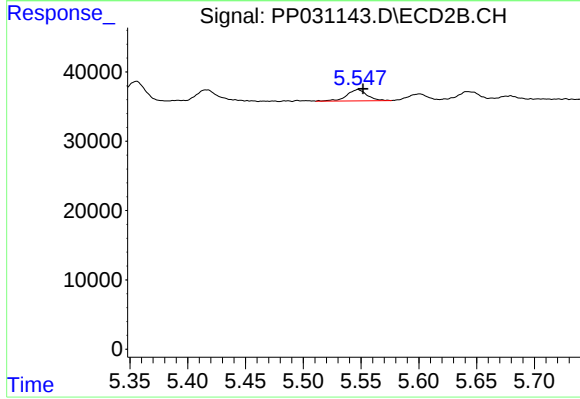

#18 AR-1242-3


R.T.: 5.547 min
Delta R.T.: -0.004 min
Response: 19590
Conc: 20.87 ng/ml

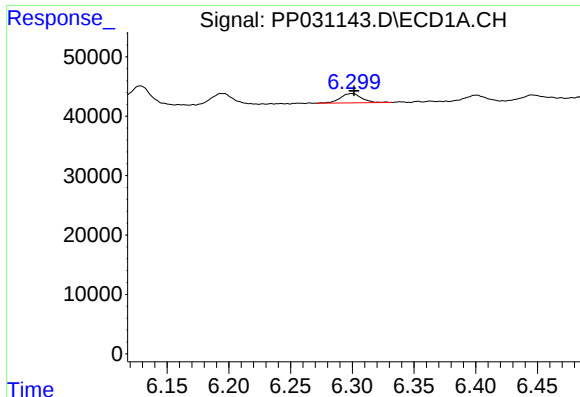

#19 AR-1242-4


R.T.: 6.300 min
Delta R.T.: -0.002 min
Response: 18853
Conc: 18.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

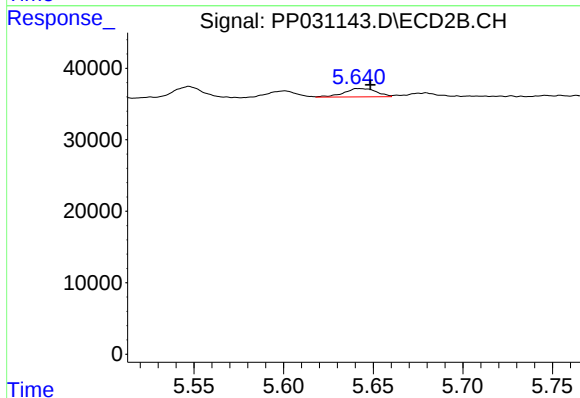


#19 AR-1242-4

R.T.: 5.642 min
Delta R.T.: -0.007 min
Response: 14876
Conc: 17.15 ng/ml

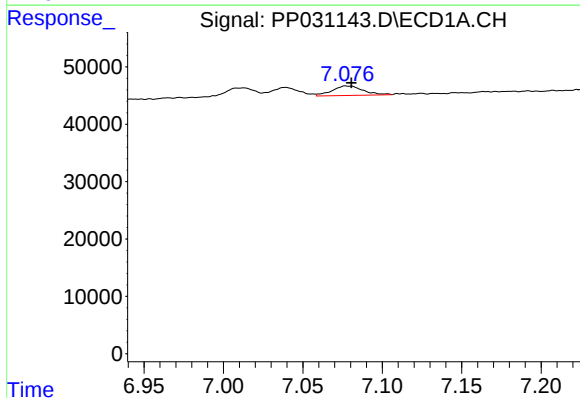


#20 AR-1242-5

R.T.: 7.078 min
Delta R.T.: -0.003 min
Response: 22466
Conc: 23.54 ng/ml

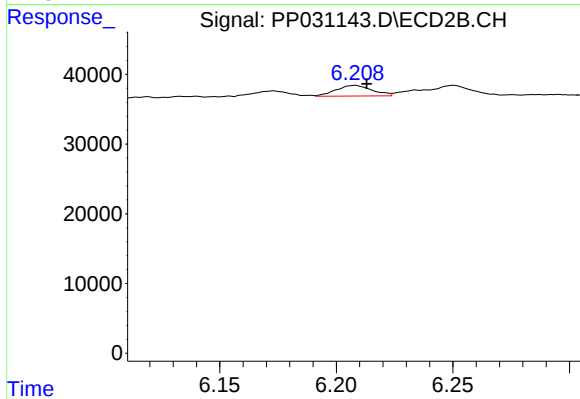

#20 AR-1242-5


R.T.: 6.208 min
Delta R.T.: -0.005 min
Response: 16536
Conc: 16.61 ng/ml

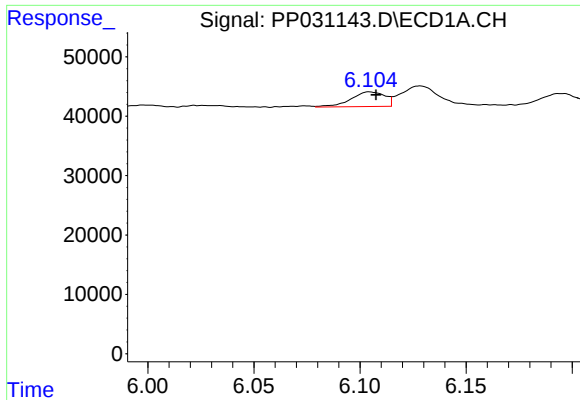

#21 AR-1248-1


R.T.: 6.105 min
Delta R.T.: -0.003 min
Response: 27400
Conc: 28.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

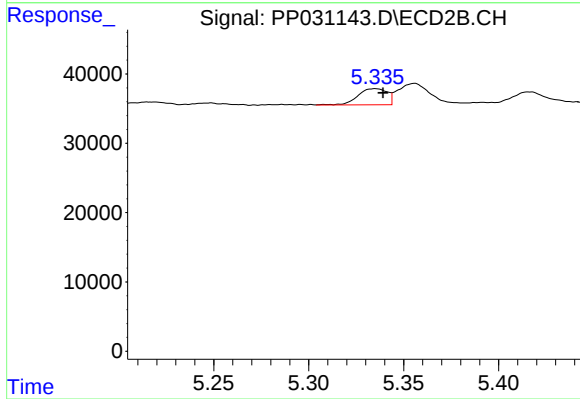


#21 AR-1248-1

R.T.: 5.335 min
Delta R.T.: -0.004 min
Response: 25031
Conc: 27.05 ng/ml

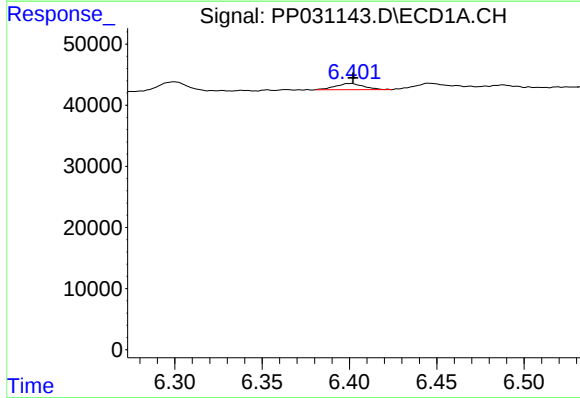


#22 AR-1248-2

R.T.: 6.400 min
Delta R.T.: -0.002 min
Response: 11203
Conc: 9.69 ng/ml

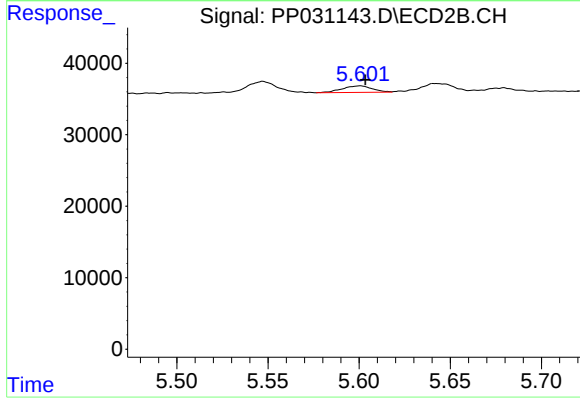

#22 AR-1248-2


R.T.: 5.601 min
Delta R.T.: -0.003 min
Response: 10536
Conc: 9.56 ng/ml

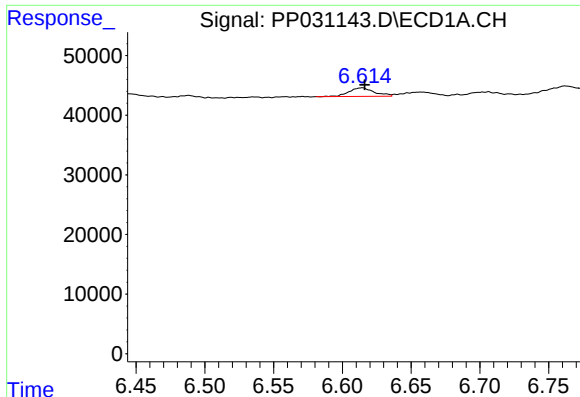

#23 AR-1248-3


R.T.: 6.614 min
Delta R.T.: -0.002 min
Response: 18059
Conc: 12.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

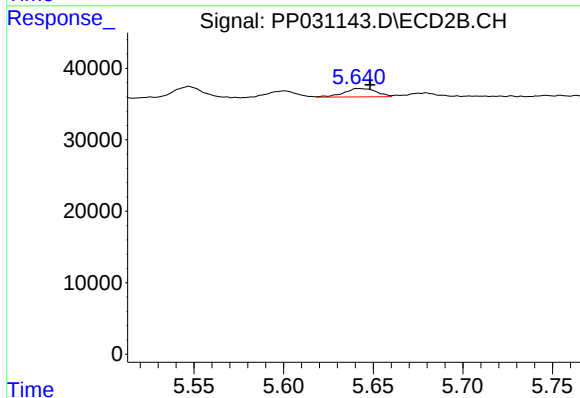


#23 AR-1248-3

R.T.: 5.642 min
Delta R.T.: -0.007 min
Response: 14876
Conc: 12.29 ng/ml

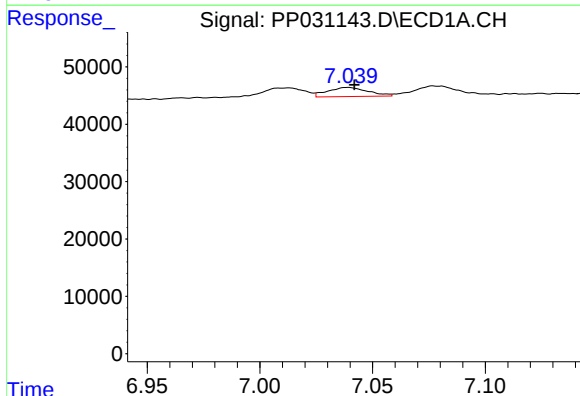


#24 AR-1248-4

R.T.: 7.039 min
Delta R.T.: -0.003 min
Response: 19666
Conc: 12.90 ng/ml

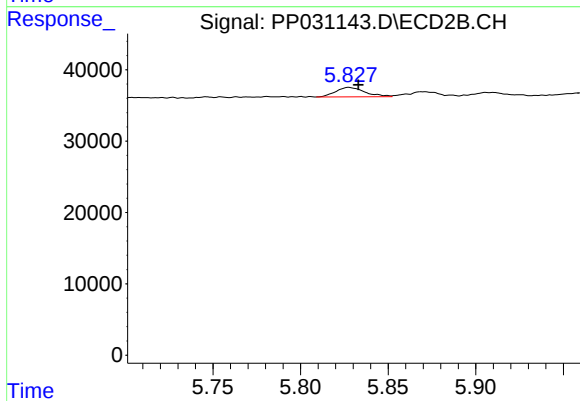

#24 AR-1248-4


R.T.: 5.827 min
Delta R.T.: -0.006 min
Response: 15609
Conc: 10.58 ng/ml

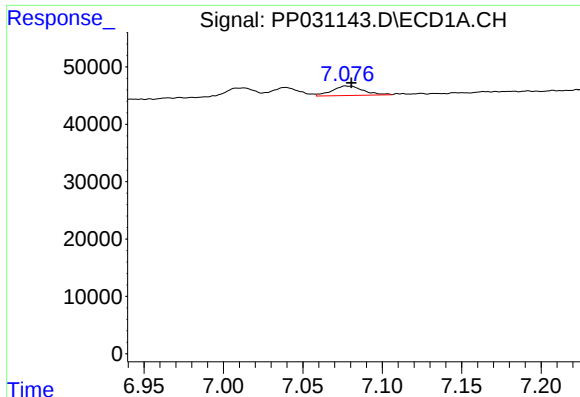

#25 AR-1248-5


R.T.: 7.078 min
Delta R.T.: -0.003 min
Response: 22466
Conc: 14.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

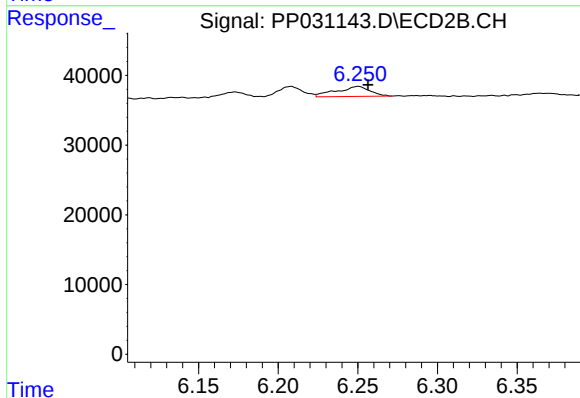


#25 AR-1248-5

R.T.: 6.250 min
Delta R.T.: -0.006 min
Response: 21085
Conc: 16.69 ng/ml

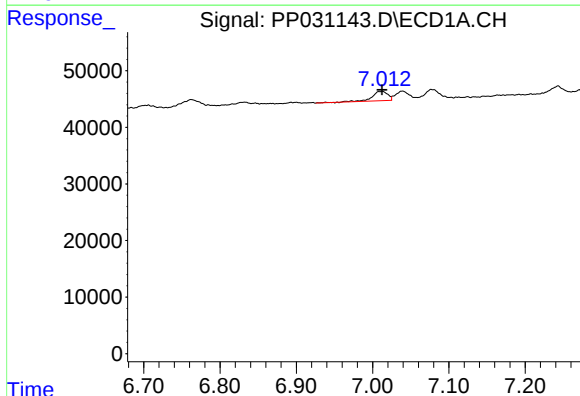


#26 AR-1254-1

R.T.: 7.012 min
Delta R.T.: 0.000 min
Response: 23342
Conc: 16.63 ng/ml

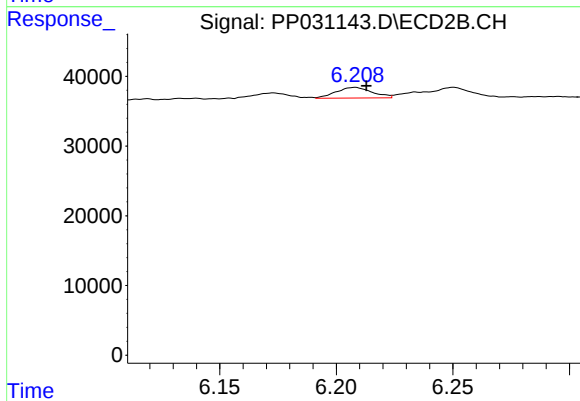

#26 AR-1254-1


R.T.: 6.208 min
Delta R.T.: -0.005 min
Response: 16536
Conc: 8.41 ng/ml

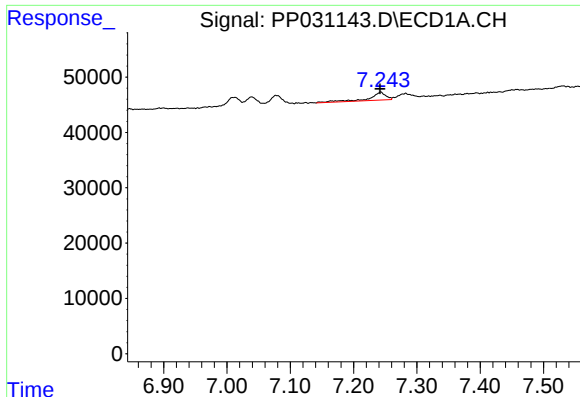

#27 AR-1254-2


R.T.: 7.243 min
Delta R.T.: 0.001 min
Response: 26224
Conc: 12.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

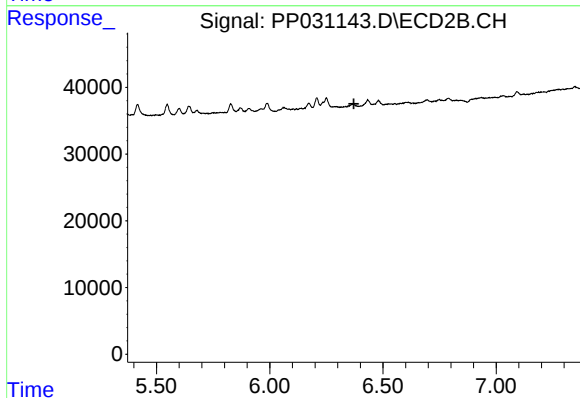


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 6.372 min
Response: 0
Conc: N.D.

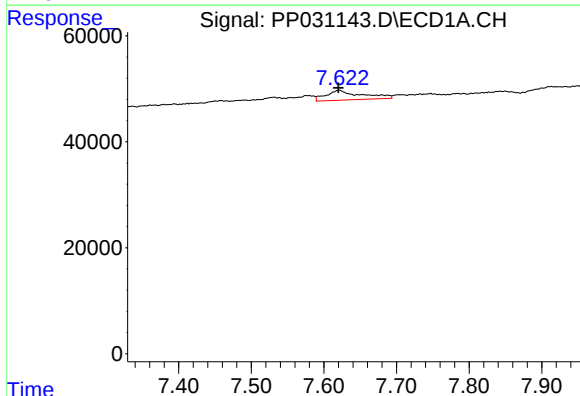


#28 AR-1254-3

R.T.: 7.621 min
Delta R.T.: 0.002 min
Response: 62951
Conc: 27.27 ng/ml

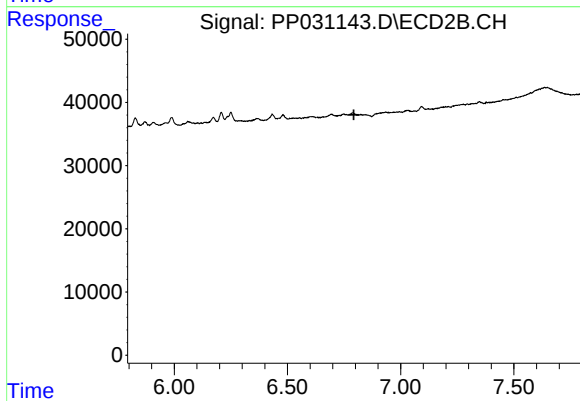

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.793 min
Response: 0
Conc: N.D.

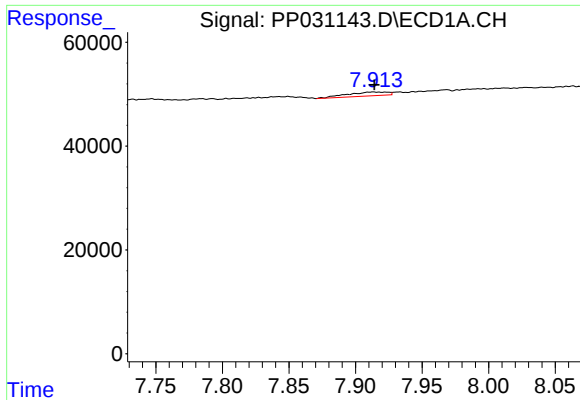

#29 AR-1254-4


R.T.: 7.913 min
Delta R.T.: 0.000 min
Response: 15857
Conc: 9.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

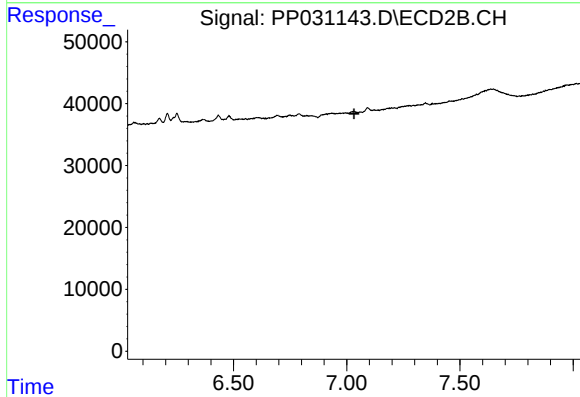


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 7.032 min
Response: 0
Conc: N.D.

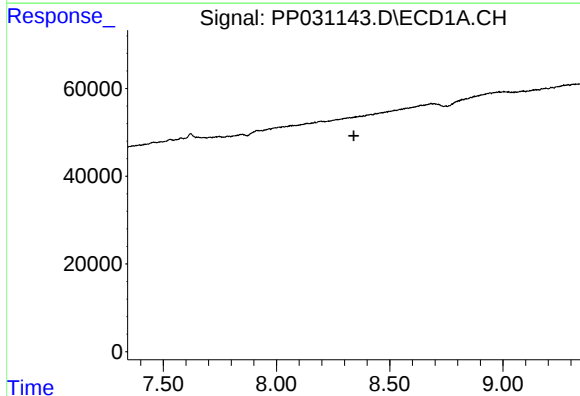


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 8.341 min
Response: 0
Conc: N.D.

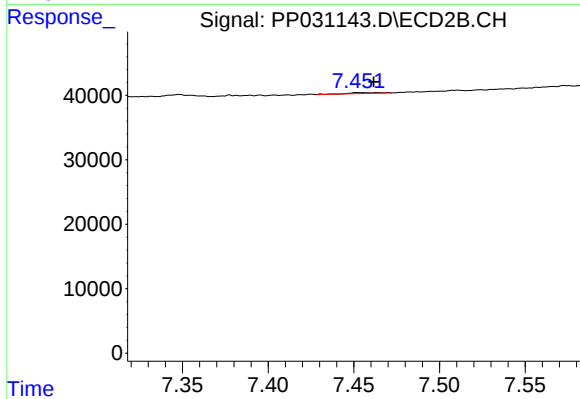

#30 AR-1254-5


R.T.: 7.452 min
Delta R.T.: -0.010 min
Response: 1514
Conc: 0.69 ng/ml

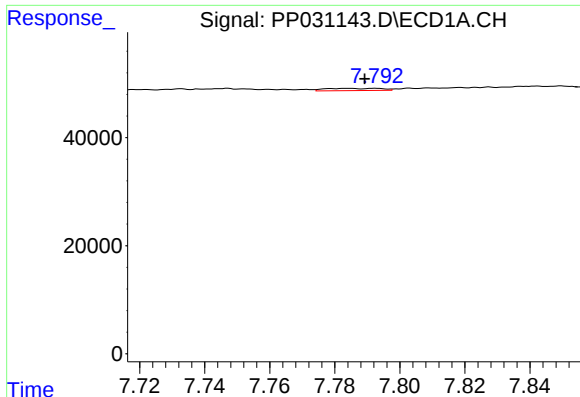

#31 AR-1260-1


R.T.: 7.784 min
Delta R.T.: -0.005 min
Response: 5195
Conc: 2.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

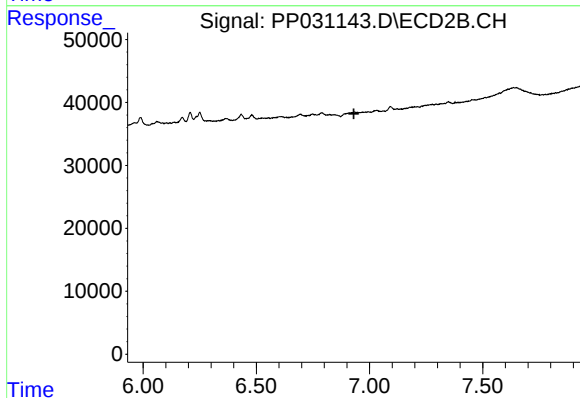


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 6.931 min
Response: 0
Conc: N.D.

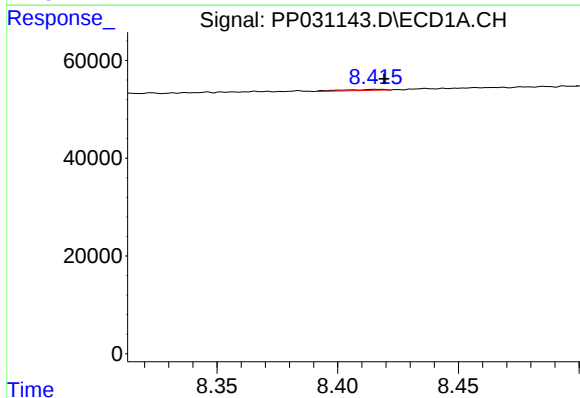


#33 AR-1260-3

R.T.: 8.416 min
Delta R.T.: -0.003 min
Response: 2746
Conc: 1.67 ng/ml

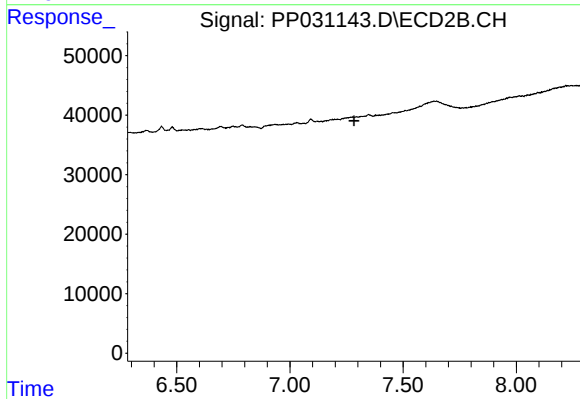

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 7.283 min
Response: 0
Conc: N.D.

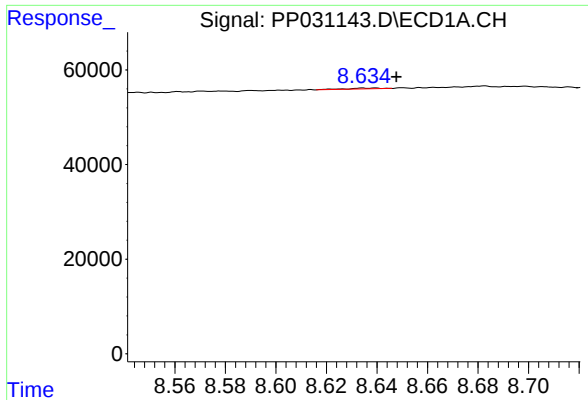

#34 AR-1260-4


R.T.: 8.634 min
Delta R.T.: -0.013 min
Response: 1683
Conc: 0.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

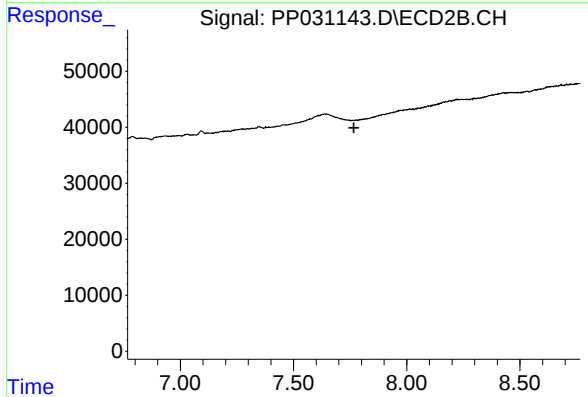


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.767 min
Response: 0
Conc: N.D.

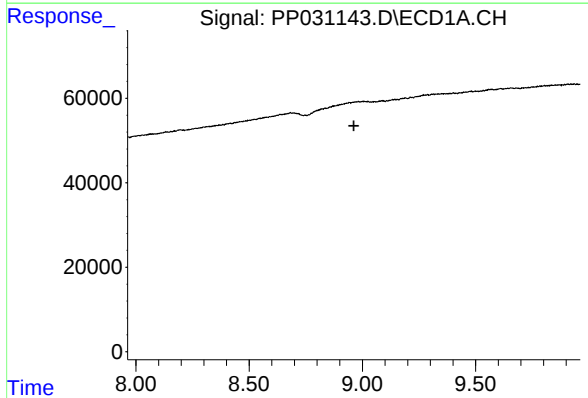


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 8.962 min
Response: 0
Conc: N.D.

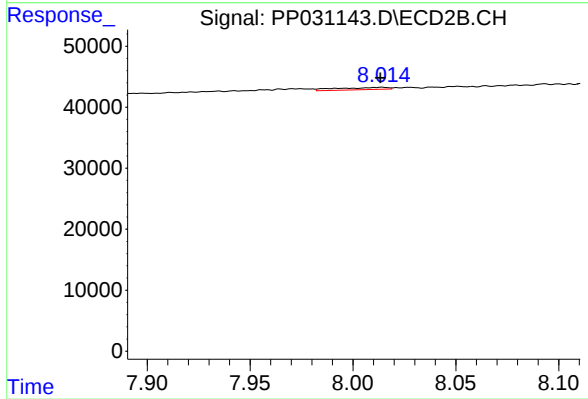

#35 AR-1260-5


R.T.: 8.014 min
Delta R.T.: 0.000 min
Response: 6104
Conc: 1.36 ng/ml

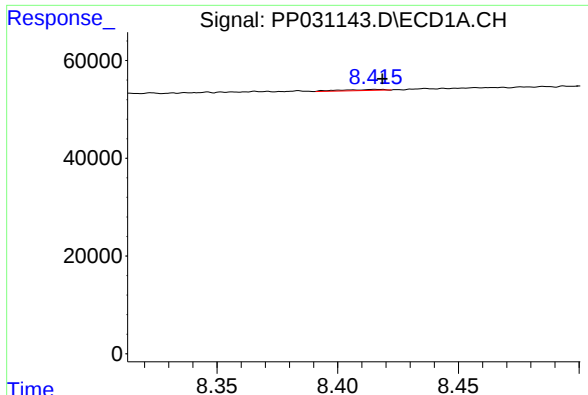

#36 AR-1262-1


R.T.: 8.416 min
Delta R.T.: -0.002 min
Response: 2746
Conc: 1.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

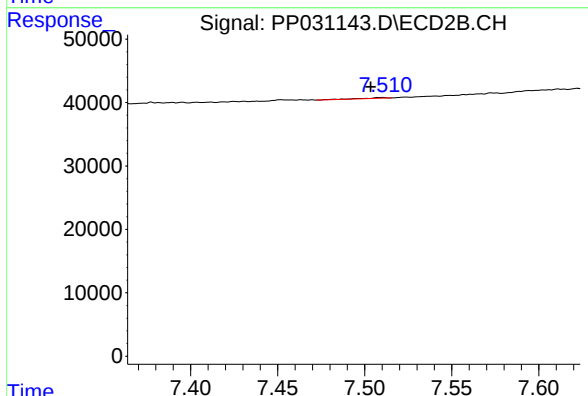


#36 AR-1262-1

R.T.: 7.511 min
Delta R.T.: 0.007 min
Response: 1137
Conc: 0.49 ng/ml

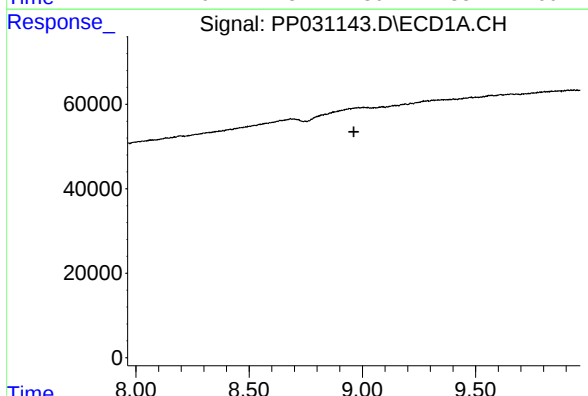


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 8.963 min
Response: 0
Conc: N.D.

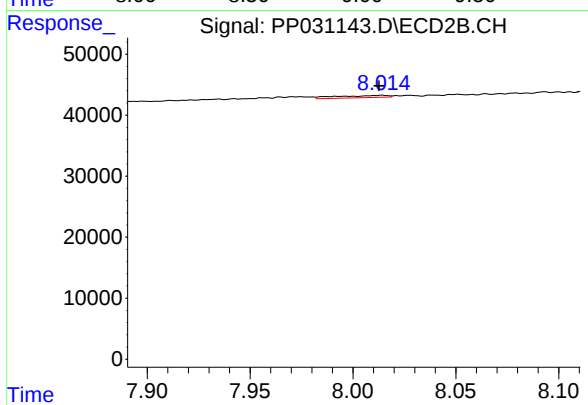

#37 AR-1262-2


R.T.: 8.014 min
Delta R.T.: 0.001 min
Response: 6104
Conc: 1.47 ng/ml

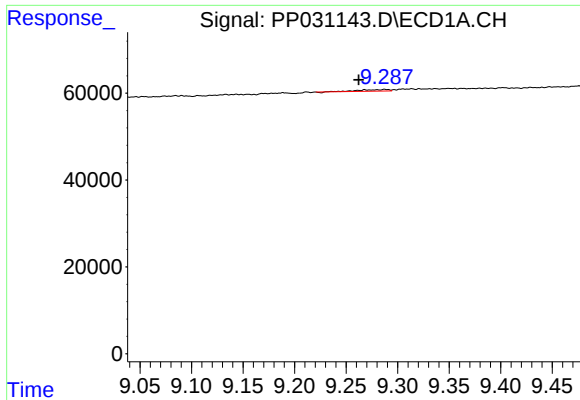

#38 AR-1262-3


R.T.: 9.288 min
Delta R.T.: 0.025 min
Response: 7107
Conc: 2.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

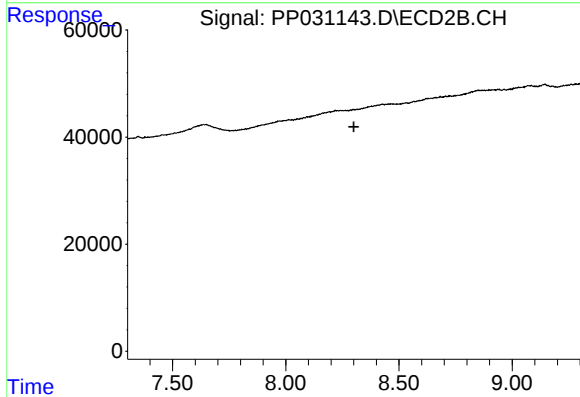


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 8.301 min
Response: 0
Conc: N.D.

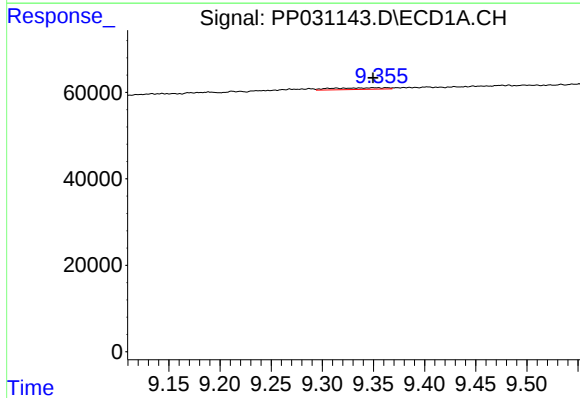


#39 AR-1262-4

R.T.: 9.349 min
Delta R.T.: 0.000 min
Response: 13640
Conc: 6.62 ng/ml

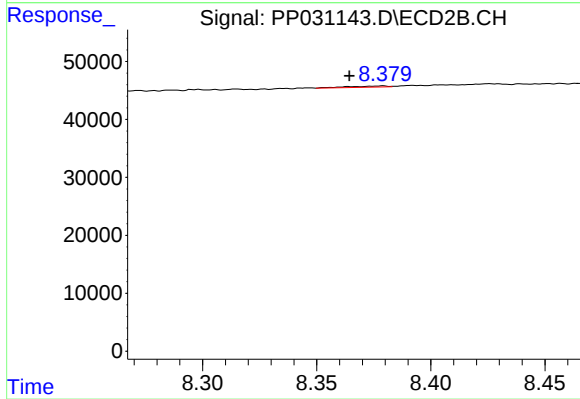

#39 AR-1262-4


R.T.: 8.379 min
Delta R.T.: 0.015 min
Response: 2390
Conc: 0.75 ng/ml

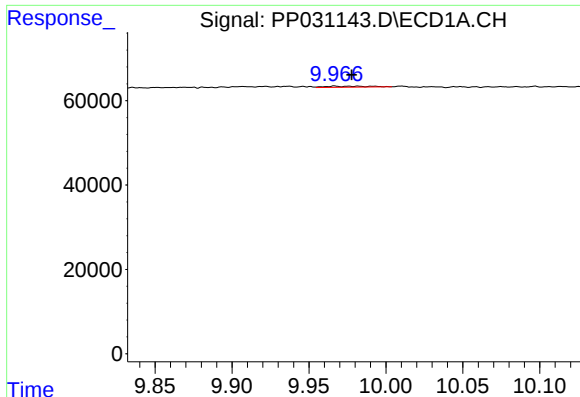

#40 AR-1262-5


R.T.: 9.967 min
Delta R.T.: -0.011 min
Response: 4722
Conc: 3.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

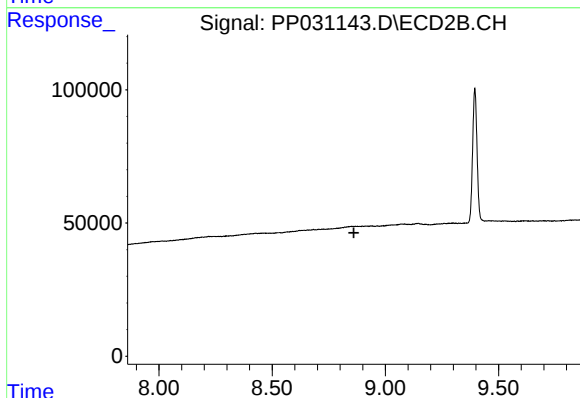


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 8.861 min
Response: 0
Conc: N.D.

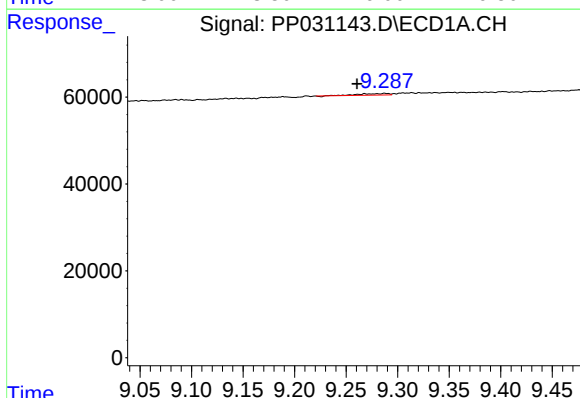


#41 AR-1268-1

R.T.: 9.288 min
Delta R.T.: 0.027 min
Response: 7107
Conc: 1.63 ng/ml

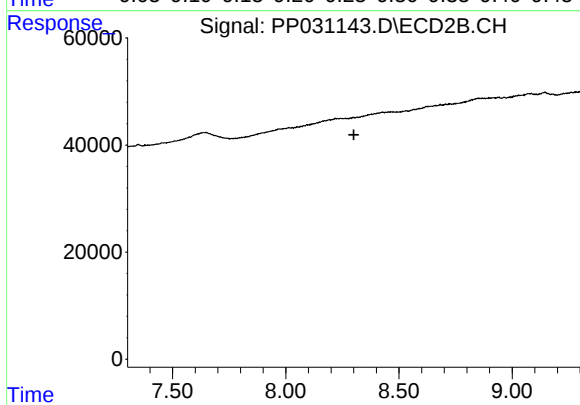

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 8.300 min
Response: 0
Conc: N.D.

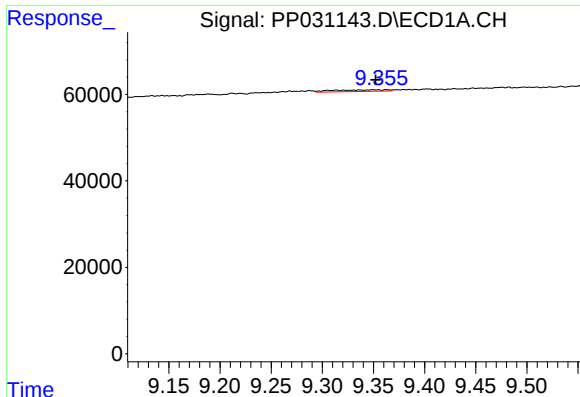

#42 AR-1268-2


R.T.: 9.349 min
Delta R.T.: -0.003 min
Response: 13640
Conc: 3.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

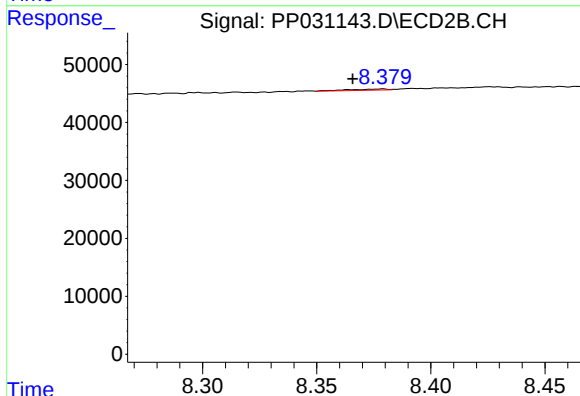


#42 AR-1268-2

R.T.: 8.379 min
Delta R.T.: 0.014 min
Response: 2390
Conc: 0.50 ng/ml

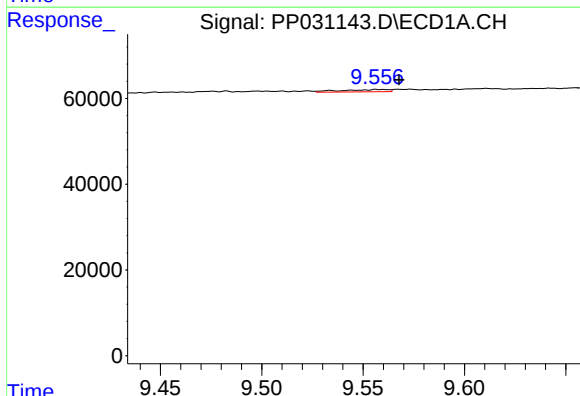


#43 AR-1268-3

R.T.: 9.557 min
Delta R.T.: -0.010 min
Response: 8674
Conc: 2.40 ng/ml

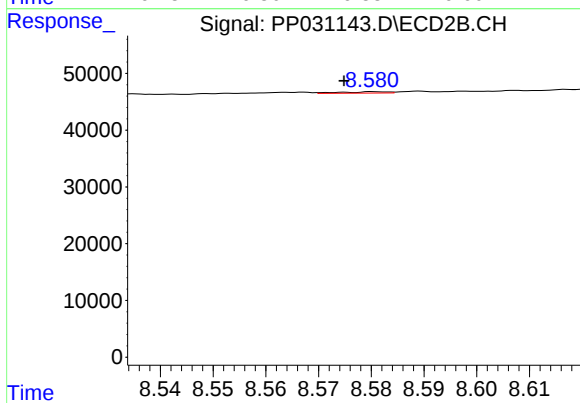

#43 AR-1268-3


R.T.: 8.580 min
Delta R.T.: 0.005 min
Response: 1532
Conc: 0.38 ng/ml

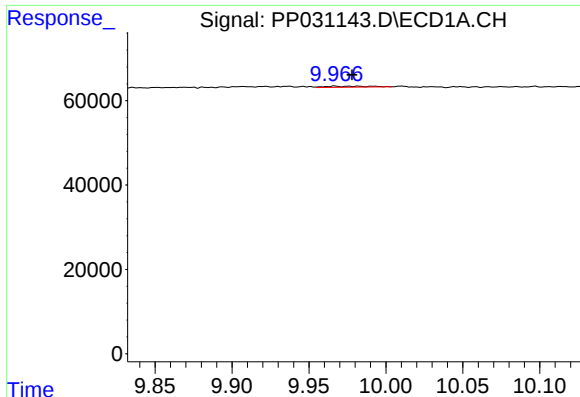

#44 AR-1268-4


R.T.: 9.967 min
Delta R.T.: -0.011 min
Response: 4722
Conc: 2.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

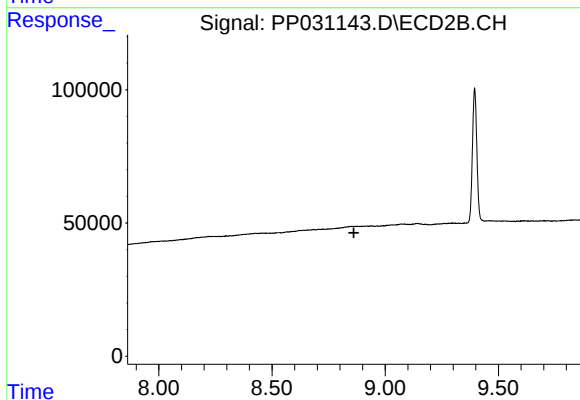


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 8.862 min
Response: 0
Conc: N.D.

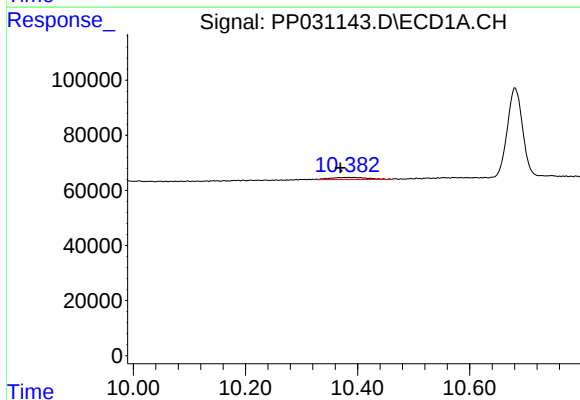

#45 AR-1268-5

R.T.: 10.383 min
Delta R.T.: 0.014 min
Response: 33968
Conc: 2.84 ng/ml

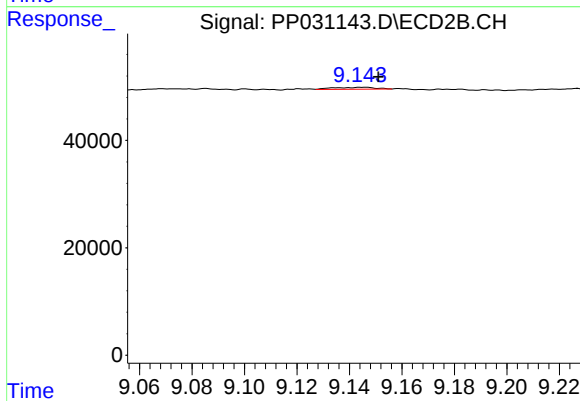

#45 AR-1268-5

R.T.: 9.146 min
Delta R.T.: -0.005 min
Response: 3912
Conc: 0.29 ng/ml