

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110420\
 Data File : PP031146.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Nov 2020 2:28
 Operator : DD\AJ
 Sample : L4214-07
 Misc : AR1254 LOD 40 PPB
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2020

Manual Integrations
 APPROVED

Ankita
 11/5/2020 11:16:39 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 05:14:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 04 08:24:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.799	4.073	988928	953097	14.806	14.339
2)	SA Decachlor...	10.680	9.394	637747	705236	15.950	16.889
Target Compounds							
26)	L6 AR-1254-1	7.009	6.207	75678	84135	53.902	42.780
27)	L6 AR-1254-2	7.238	6.366	103061	67867	49.442	41.301
28)	L6 AR-1254-3	7.616	6.787	109162	123801	47.296m	45.210
29)	L6 AR-1254-4	7.911	7.026	81709	63411	49.908	39.297
30)	L6 AR-1254-5	8.338	7.455	69873	91847	41.391	41.949

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110420\
Data File : PP031146.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Nov 2020 2:28
Operator : DD\AJ
Sample : L4214-07
Misc : AR1254 LOD 40 PPB
ALS Vial : 53 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020


Manual Integrations
APPROVED

Ankita
11/5/2020 11:16:39 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 05:14:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 04 08:24:38 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

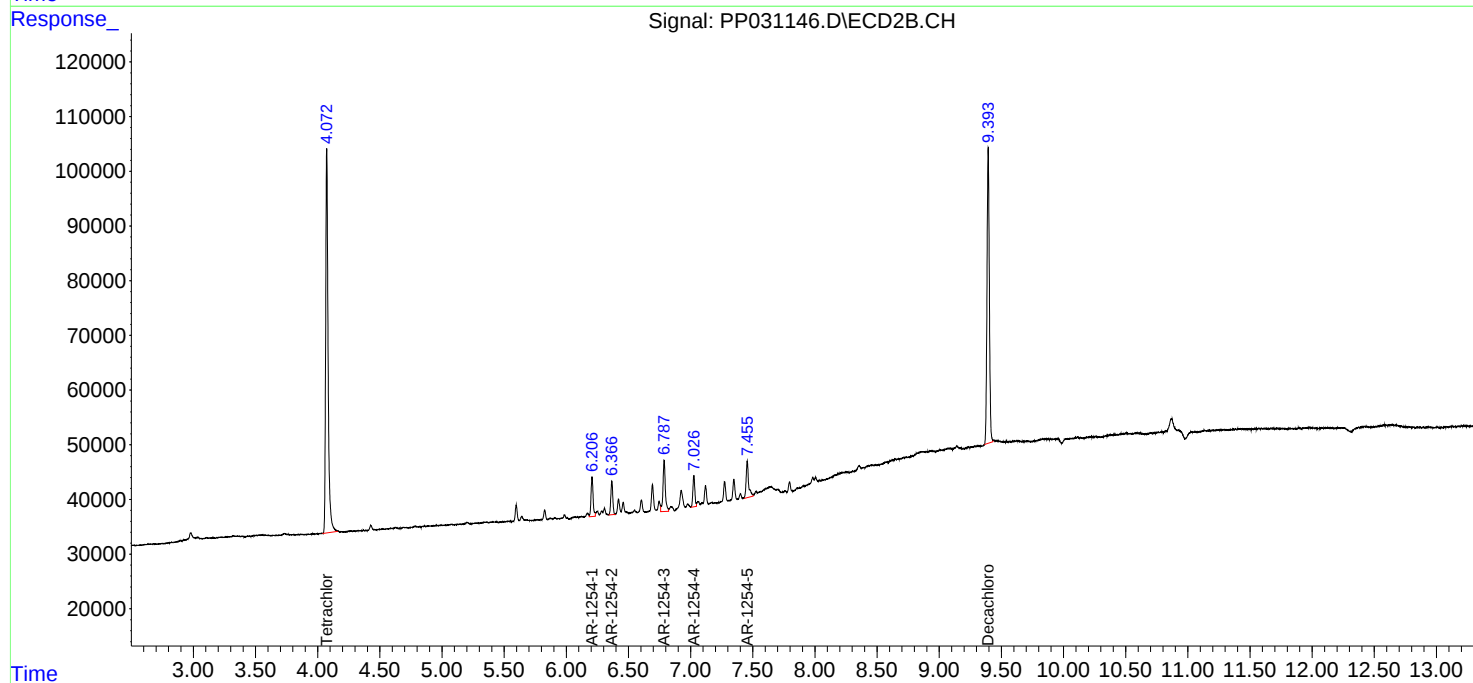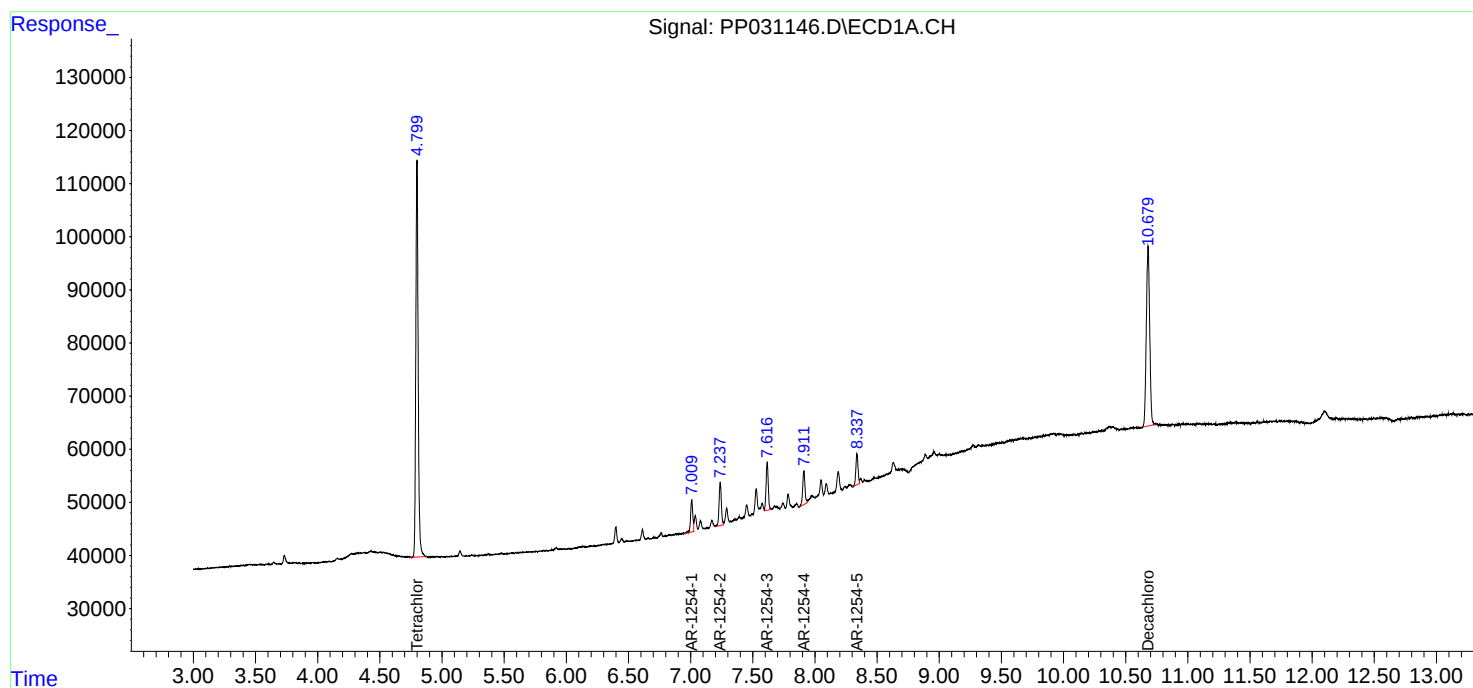

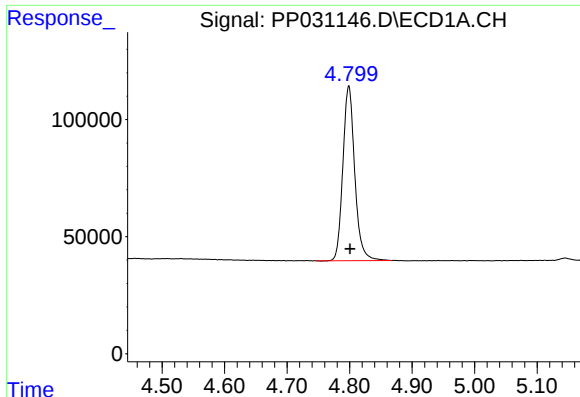


#1 Tetrachloro-m-xylene

R.T.: 4.799 min
Delta R.T.: -0.002 min
Response: 988928
Conc: 14.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020


Manual Integrations
APPROVED

Ankita
11/5/2020 11:16:39 AM

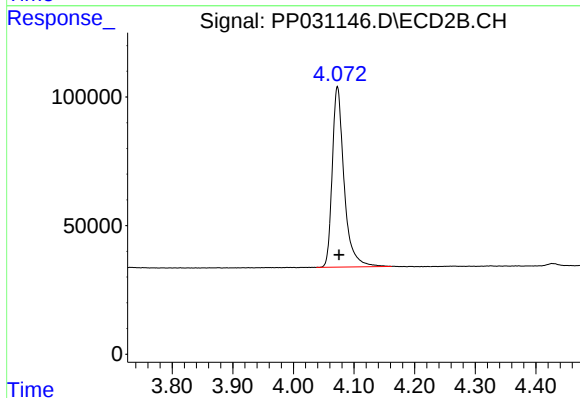


#1 Tetrachloro-m-xylene

R.T.: 4.073 min
Delta R.T.: -0.003 min
Response: 953097
Conc: 14.34 ng/ml

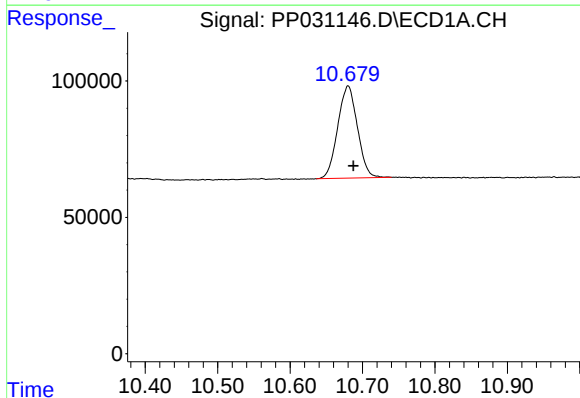


#2 Decachlorobiphenyl

R.T.: 10.680 min
Delta R.T.: -0.007 min
Response: 637747
Conc: 15.95 ng/ml

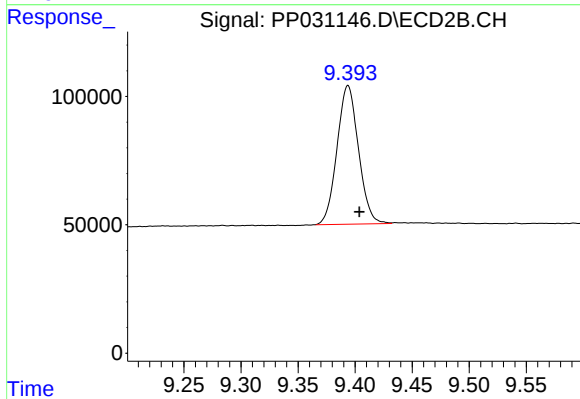

#2 Decachlorobiphenyl

R.T.: 9.394 min
Delta R.T.: -0.010 min
Response: 705236
Conc: 16.89 ng/ml

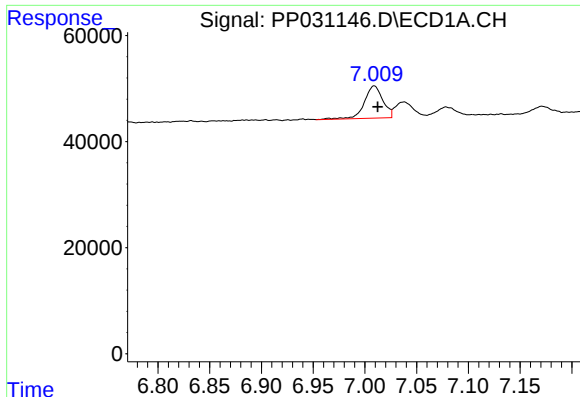


#26 AR-1254-1

R.T.: 7.009 min
Delta R.T.: -0.003 min
Response: 75678
Conc: 53.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020


Manual Integrations
APPROVED

Ankita
11/5/2020 11:16:39 AM

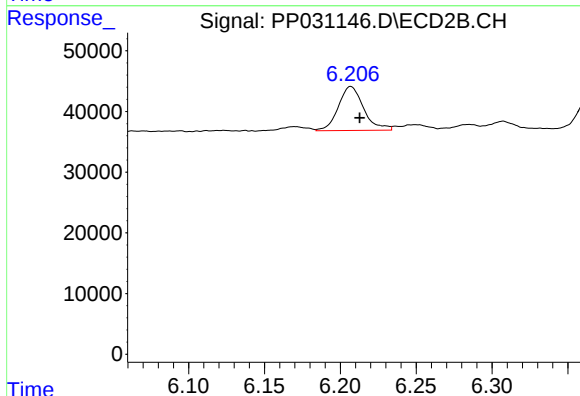


#26 AR-1254-1

R.T.: 6.207 min
Delta R.T.: -0.006 min
Response: 84135
Conc: 42.78 ng/ml

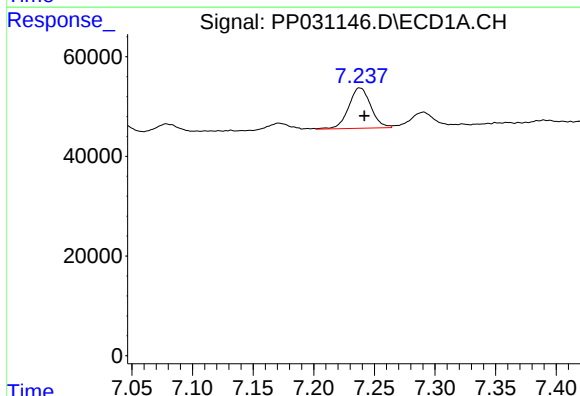


#27 AR-1254-2

R.T.: 7.238 min
Delta R.T.: -0.004 min
Response: 103061
Conc: 49.44 ng/ml

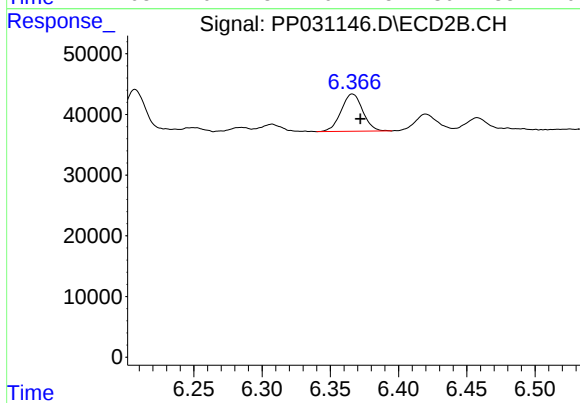

#27 AR-1254-2

R.T.: 6.366 min
Delta R.T.: -0.006 min
Response: 67867
Conc: 41.30 ng/ml

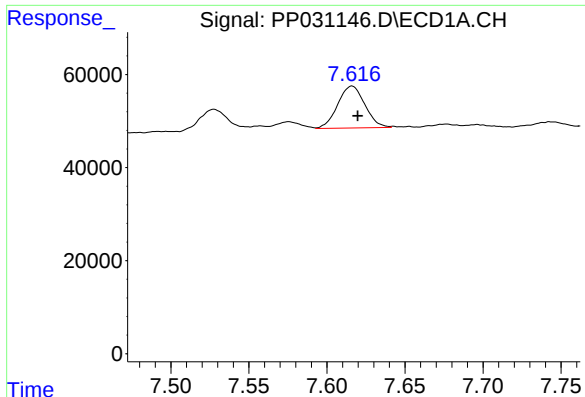


#28 AR-1254-3

R.T.: 7.616 min
Delta R.T.: -0.004 min
Response: 109162
Conc: 47.30 ng/ml m

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020


Manual Integrations
APPROVED

Ankita
11/5/2020 11:16:39 AM

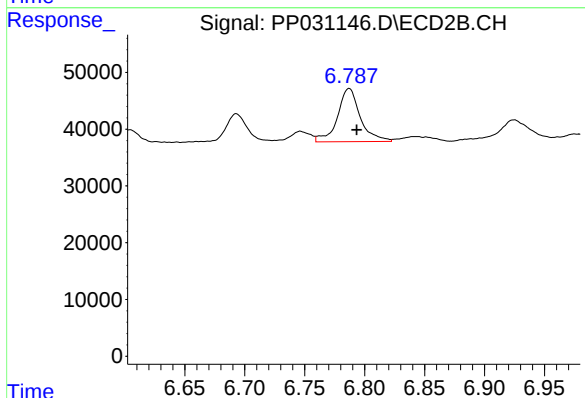


#28 AR-1254-3

R.T.: 6.787 min
Delta R.T.: -0.006 min
Response: 123801
Conc: 45.21 ng/ml

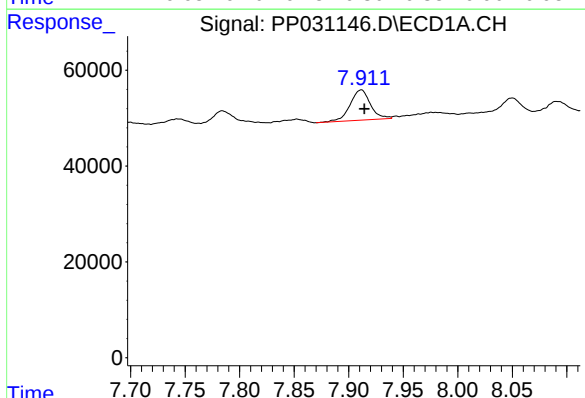


#29 AR-1254-4

R.T.: 7.911 min
Delta R.T.: -0.003 min
Response: 81709
Conc: 49.91 ng/ml

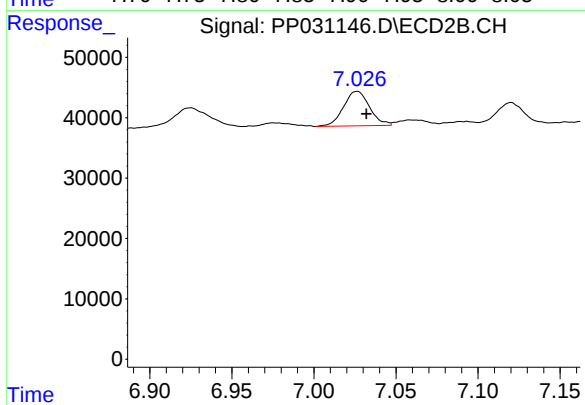

#29 AR-1254-4

R.T.: 7.026 min
Delta R.T.: -0.006 min
Response: 63411
Conc: 39.30 ng/ml

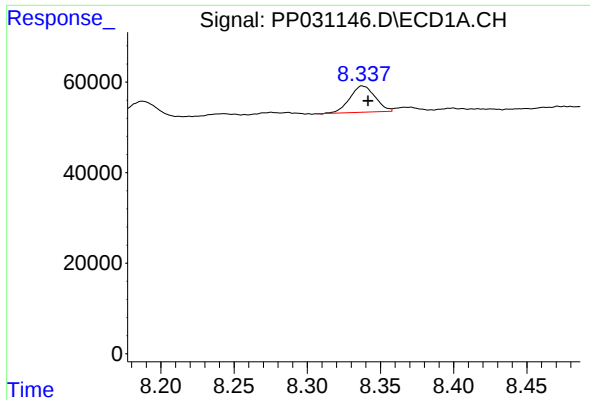


#30 AR-1254-5

R.T.: 8.338 min
Delta R.T.: -0.004 min
Response: 69873
Conc: 41.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

Manual Integrations
APPROVED

Ankita
11/5/2020 11:16:39 AM

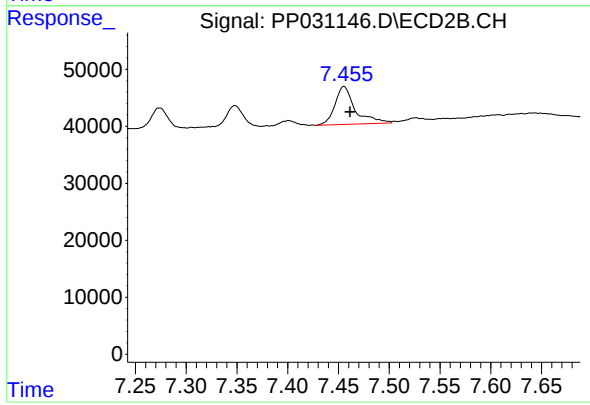

#30 AR-1254-5

R.T.: 7.455 min
Delta R.T.: -0.006 min
Response: 91847
Conc: 41.95 ng/ml