

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110420\
 Data File : PP031167.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Nov 2020 9:07
 Operator : DD\AJ
 Sample : L4214-09
 Misc : AR1248 MDL 25 PPB
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT4-2020

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 11:30:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 04 08:24:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.799	4.073	917538	879622	13.737	13.234
2) SA Decachlor...	10.679	9.394	646443	676268	16.168	16.196
Target Compounds						
21) L5 AR-1248-1	6.104	5.333	22750	19825	23.592	21.426
22) L5 AR-1248-2	6.398	5.597	32849	26221	28.401	23.792
23) L5 AR-1248-3	6.612	5.642	41475	27867	29.151	23.024
24) L5 AR-1248-4	7.038	5.827	40017	31391	26.256	21.270
25) L5 AR-1248-5	7.078	6.251	40235	31368	26.521	24.838



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110420\
Data File : PP031167.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Nov 2020 9:07
Operator : DD\AJ
Sample : L4214-09
Misc : AR1248 MDL 25 PPB
ALS Vial : 70 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2020

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 11:30:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 04 08:24:38 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

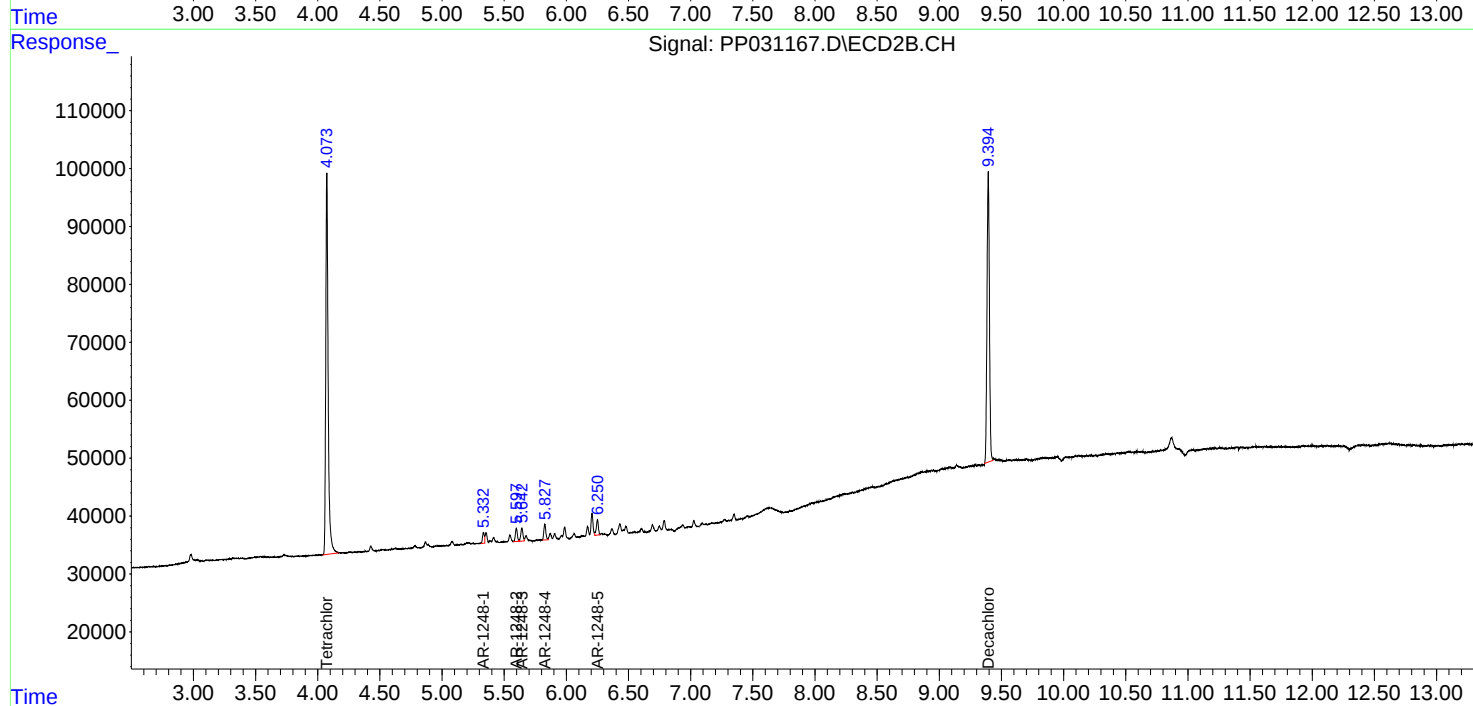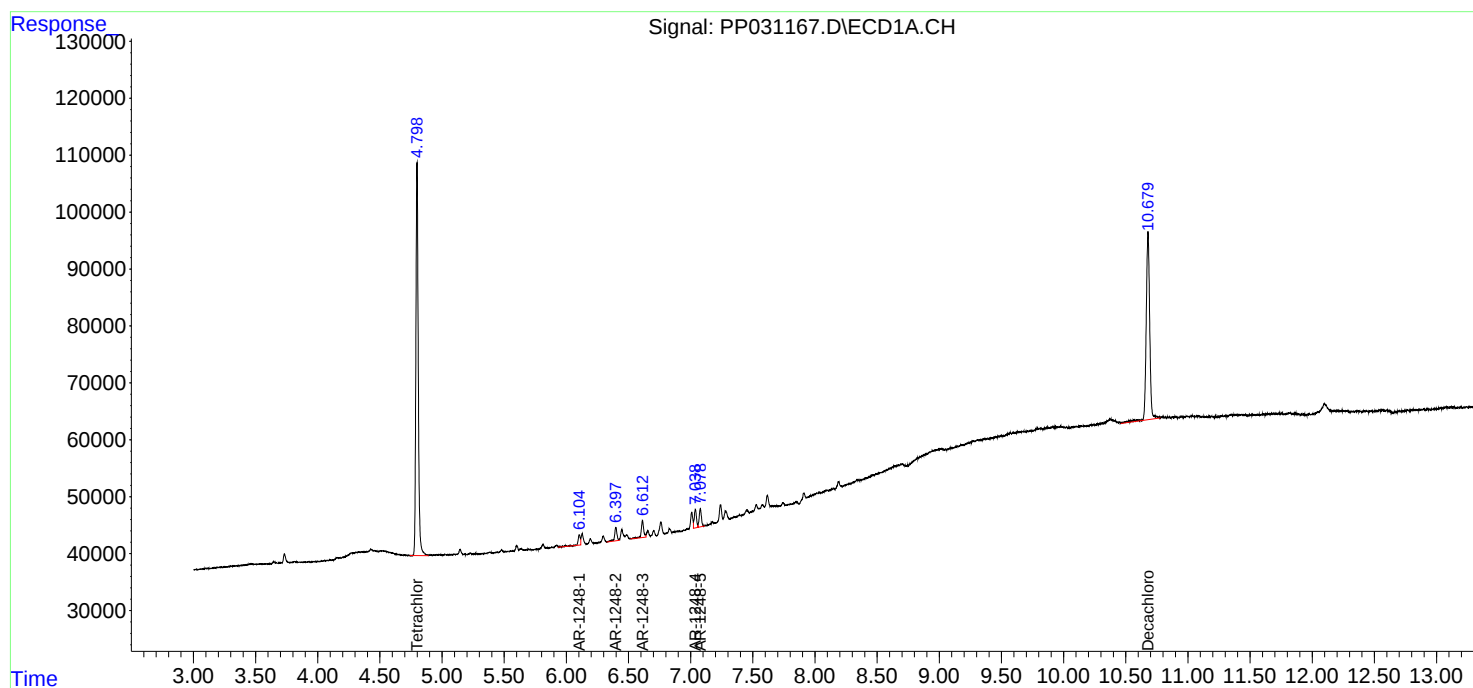


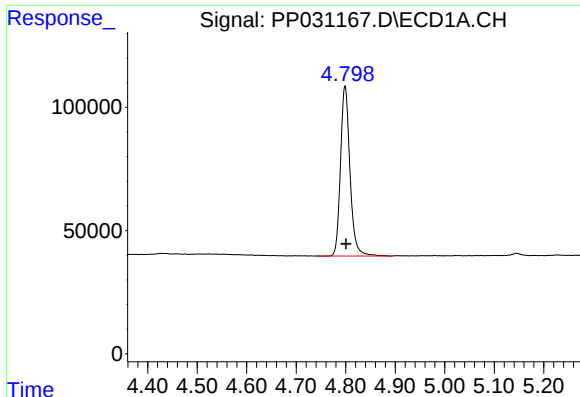

#1 Tetrachloro-m-xylene


R.T.: 4.799 min
Delta R.T.: -0.002 min
Response: 917538
Conc: 13.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2020

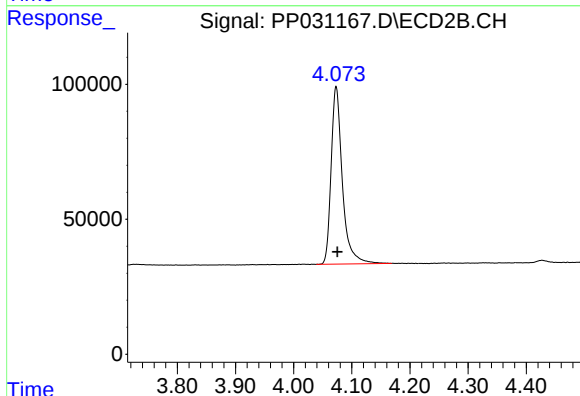


#1 Tetrachloro-m-xylene

R.T.: 4.073 min
Delta R.T.: -0.002 min
Response: 879622
Conc: 13.23 ng/ml

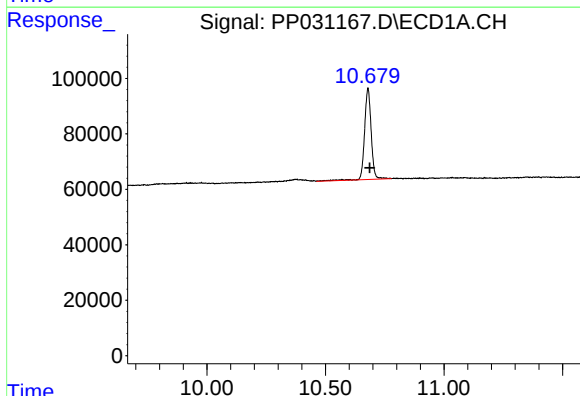


#2 Decachlorobiphenyl

R.T.: 10.679 min
Delta R.T.: -0.008 min
Response: 646443
Conc: 16.17 ng/ml

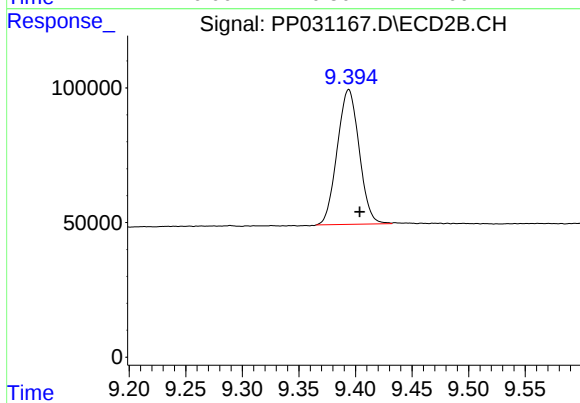

#2 Decachlorobiphenyl


R.T.: 9.394 min
Delta R.T.: -0.010 min
Response: 676268
Conc: 16.20 ng/ml

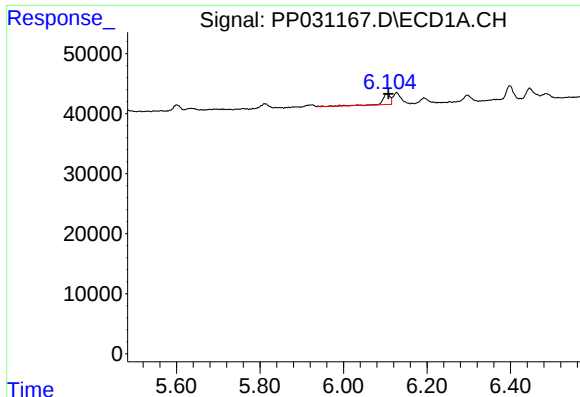

#21 AR-1248-1


R.T.: 6.104 min
Delta R.T.: -0.003 min
Response: 22750
Conc: 23.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2020

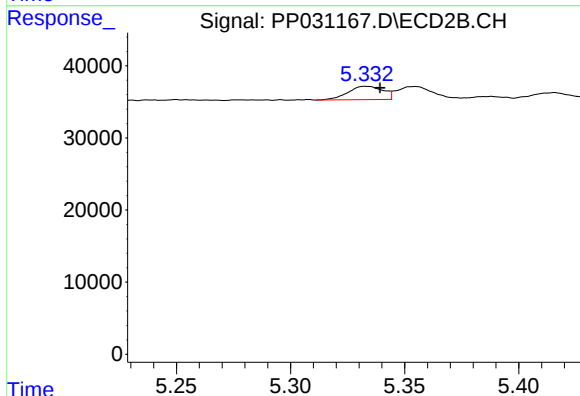


#21 AR-1248-1

R.T.: 5.333 min
Delta R.T.: -0.006 min
Response: 19825
Conc: 21.43 ng/ml

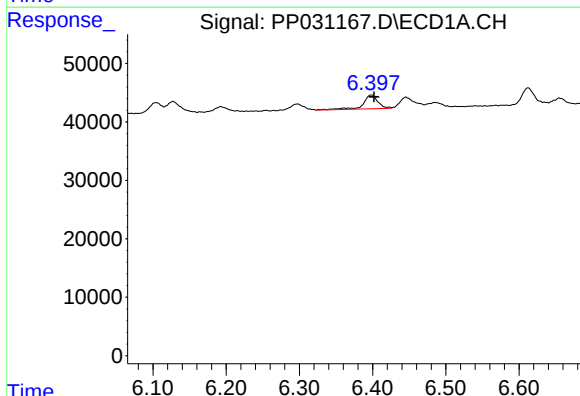


#22 AR-1248-2

R.T.: 6.398 min
Delta R.T.: -0.004 min
Response: 32849
Conc: 28.40 ng/ml

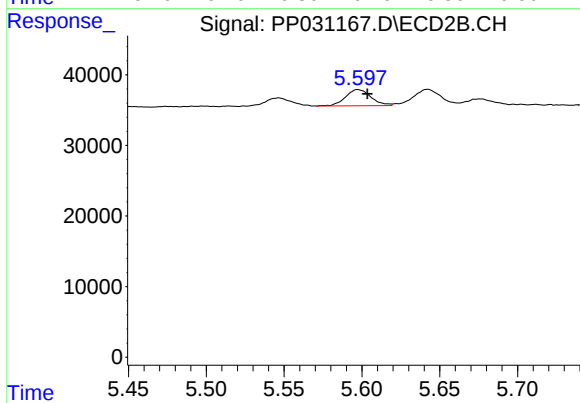

#22 AR-1248-2


R.T.: 5.597 min
Delta R.T.: -0.006 min
Response: 26221
Conc: 23.79 ng/ml

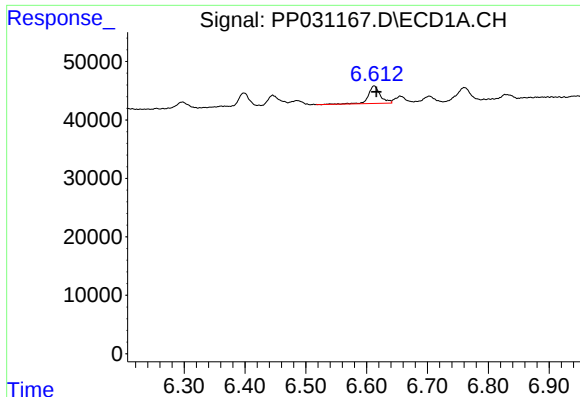

#23 AR-1248-3


R.T.: 6.612 min
Delta R.T.: -0.004 min
Response: 41475
Conc: 29.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2020

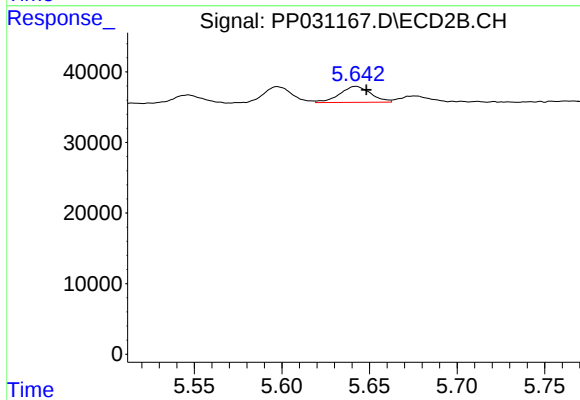


#23 AR-1248-3

R.T.: 5.642 min
Delta R.T.: -0.006 min
Response: 27867
Conc: 23.02 ng/ml

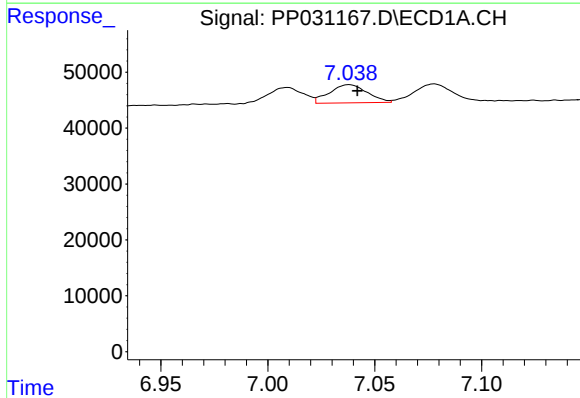


#24 AR-1248-4

R.T.: 7.038 min
Delta R.T.: -0.004 min
Response: 40017
Conc: 26.26 ng/ml

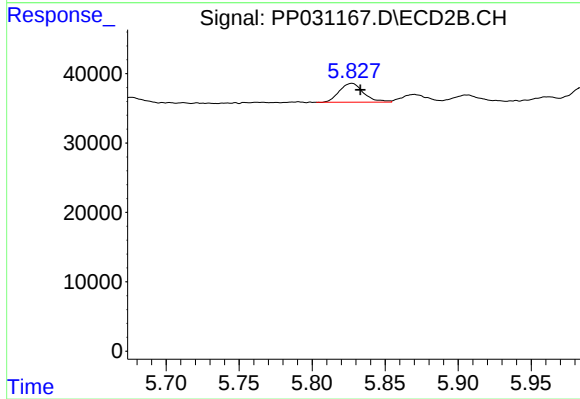

#24 AR-1248-4


R.T.: 5.827 min
Delta R.T.: -0.006 min
Response: 31391
Conc: 21.27 ng/ml

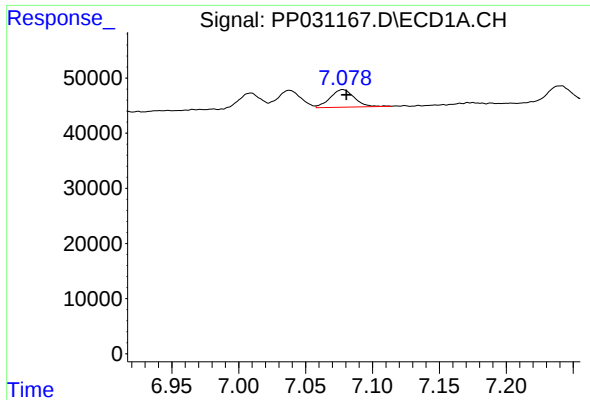

#25 AR-1248-5

R.T.: 7.078 min
Delta R.T.: -0.003 min
Response: 40235
Conc: 26.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2020

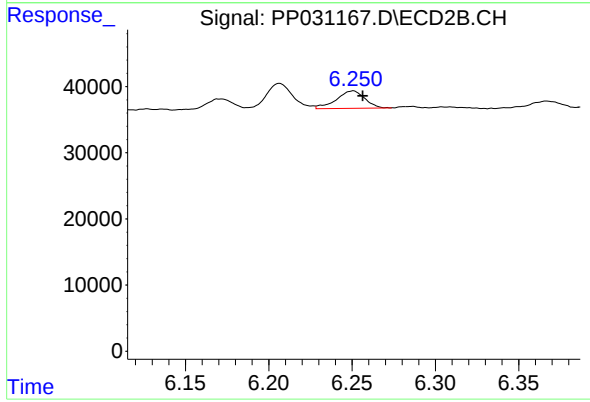

#25 AR-1248-5

R.T.: 6.251 min
Delta R.T.: -0.006 min
Response: 31368
Conc: 24.84 ng/ml