

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110420\
 Data File : PP031168.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Nov 2020 9:24
 Operator : DD\AJ
 Sample : L4214-09
 Misc : AR1254 MDL 25 PPB
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT4-2020

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 11:15:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 04 08:24:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.799	4.073	867166	844378	12.983	12.703
2) SA Decachlor...	10.680	9.394	576695	639110	14.423	15.306
Target Compounds						
26) L6 AR-1254-1	7.010	6.207	23619	44167	16.823	22.458 #
27) L6 AR-1254-2	7.239	6.365	52882	38856	25.370	23.646
28) L6 AR-1254-3	7.617	6.786	57819	60080	25.051	21.941
29) L6 AR-1254-4	7.912	7.026	37220	34839	22.734	21.591
30) L6 AR-1254-5	8.338	7.455	33307	66759	19.730	30.491 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110420\
Data File : PP031168.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Nov 2020 9:24
Operator : DD\AJ
Sample : L4214-09
Misc : AR1254 MDL 25 PPB
ALS Vial : 71 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2020

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 11:15:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 04 08:24:38 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

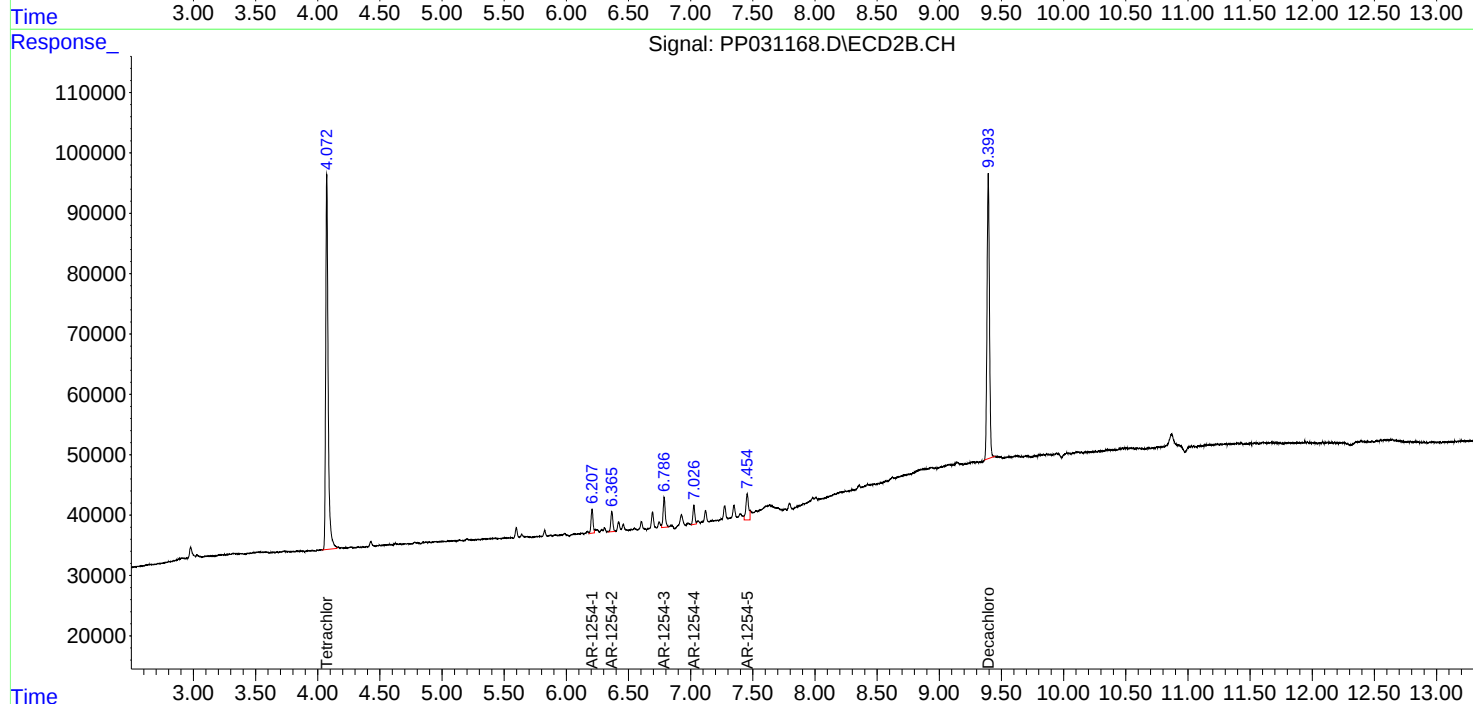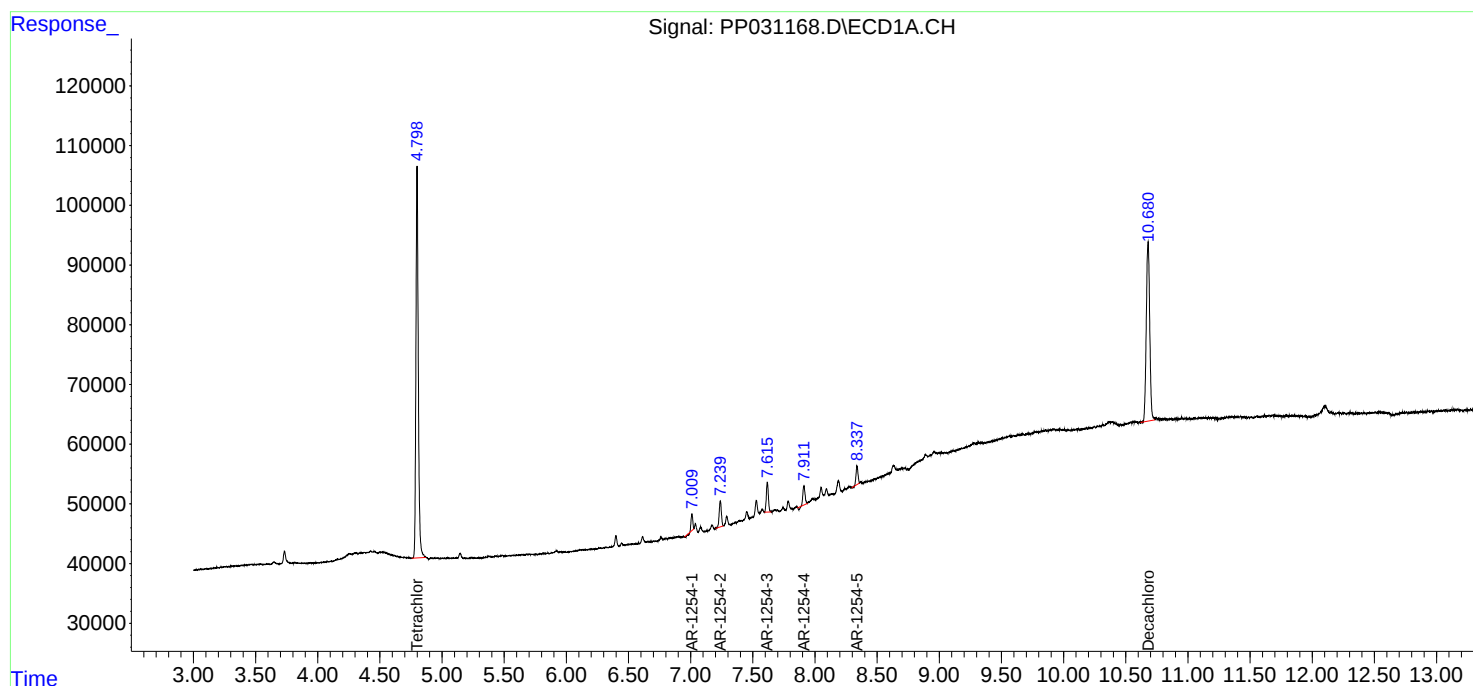


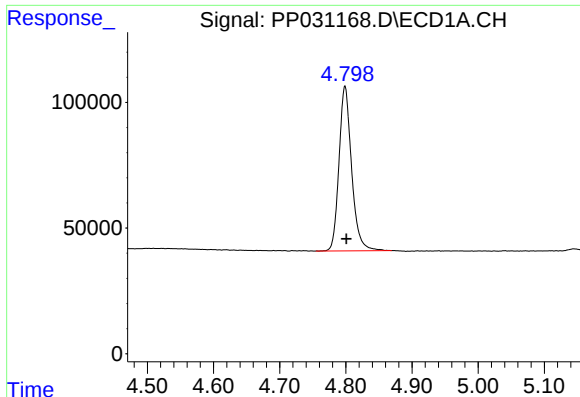

#1 Tetrachloro-m-xylene


R.T.: 4.799 min
Delta R.T.: -0.002 min
Response: 867166
Conc: 12.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2020

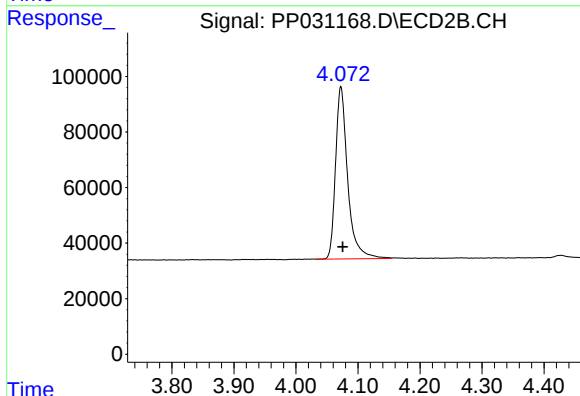


#1 Tetrachloro-m-xylene

R.T.: 4.073 min
Delta R.T.: -0.003 min
Response: 844378
Conc: 12.70 ng/ml

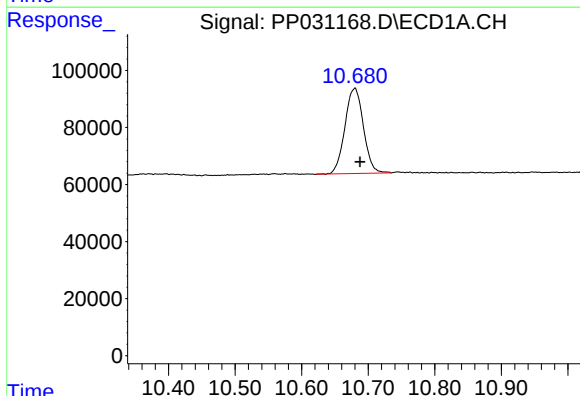


#2 Decachlorobiphenyl

R.T.: 10.680 min
Delta R.T.: -0.008 min
Response: 576695
Conc: 14.42 ng/ml

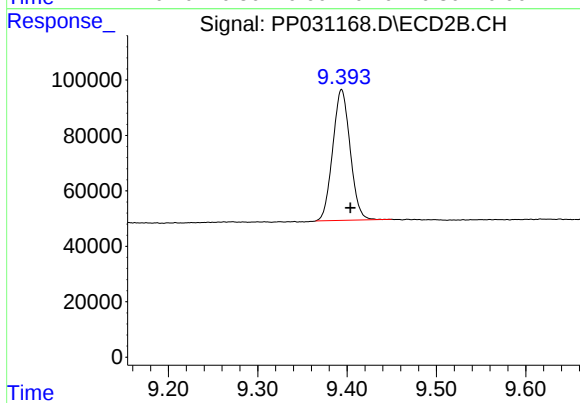

#2 Decachlorobiphenyl


R.T.: 9.394 min
Delta R.T.: -0.010 min
Response: 639110
Conc: 15.31 ng/ml

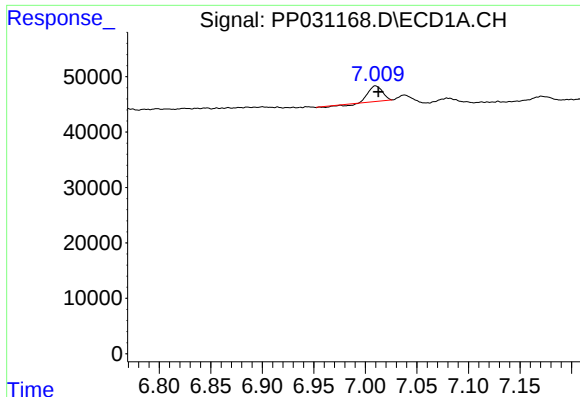

#26 AR-1254-1


R.T.: 7.010 min
Delta R.T.: -0.003 min
Response: 23619
Conc: 16.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2020

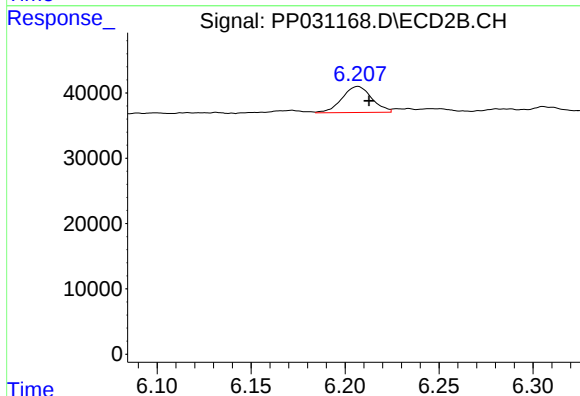


#26 AR-1254-1

R.T.: 6.207 min
Delta R.T.: -0.006 min
Response: 44167
Conc: 22.46 ng/ml

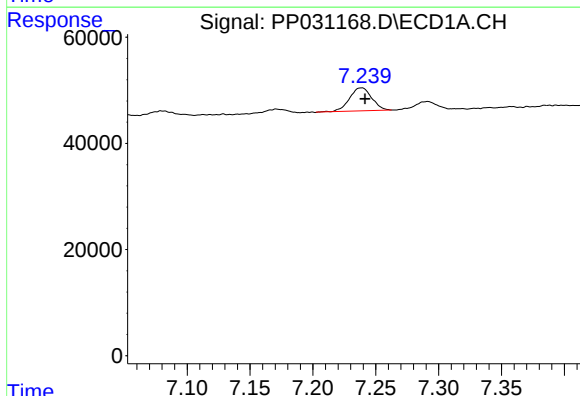


#27 AR-1254-2

R.T.: 7.239 min
Delta R.T.: -0.003 min
Response: 52882
Conc: 25.37 ng/ml

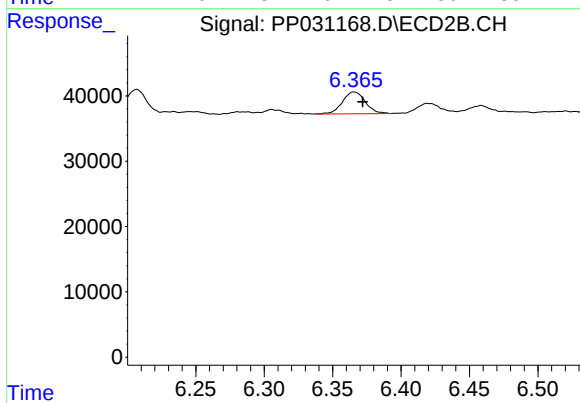

#27 AR-1254-2


R.T.: 6.365 min
Delta R.T.: -0.006 min
Response: 38856
Conc: 23.65 ng/ml

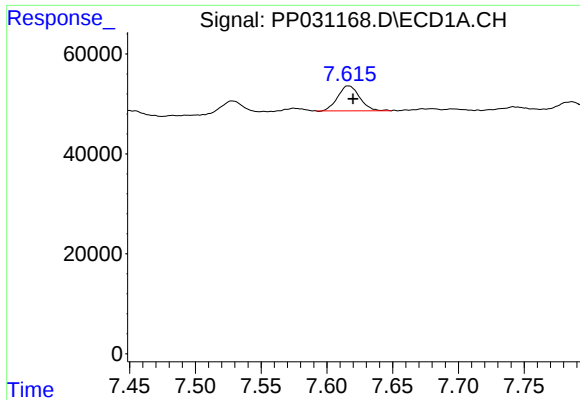

#28 AR-1254-3


R.T.: 7.617 min
Delta R.T.: -0.003 min
Response: 57819
Conc: 25.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2020

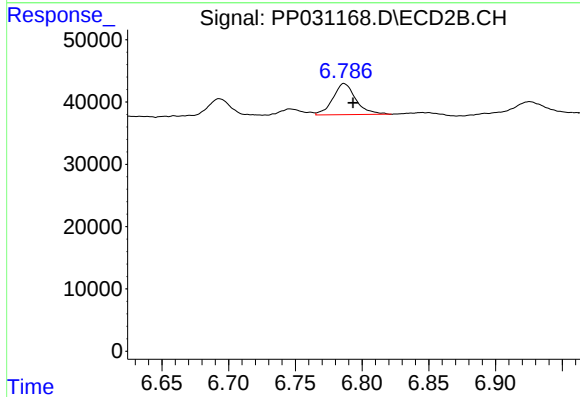


#28 AR-1254-3

R.T.: 6.786 min
Delta R.T.: -0.007 min
Response: 60080
Conc: 21.94 ng/ml

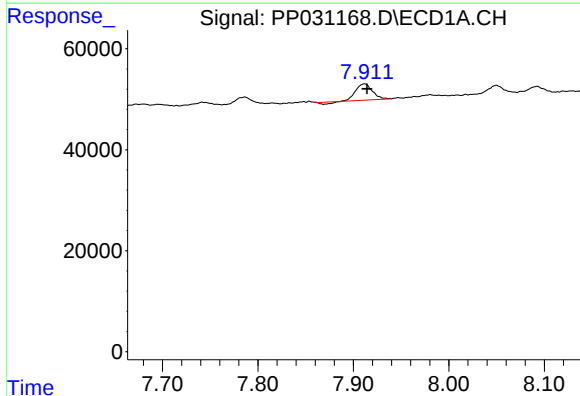


#29 AR-1254-4

R.T.: 7.912 min
Delta R.T.: -0.003 min
Response: 37220
Conc: 22.73 ng/ml

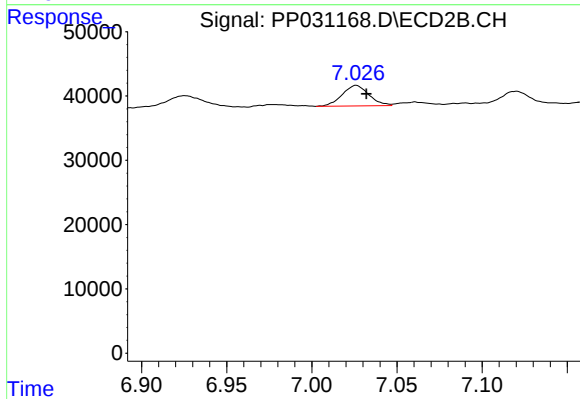

#29 AR-1254-4


R.T.: 7.026 min
Delta R.T.: -0.006 min
Response: 34839
Conc: 21.59 ng/ml

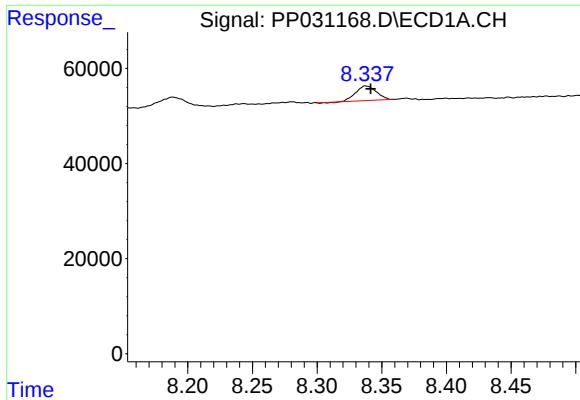

#30 AR-1254-5

R.T.: 8.338 min
Delta R.T.: -0.004 min
Response: 33307
Conc: 19.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2020

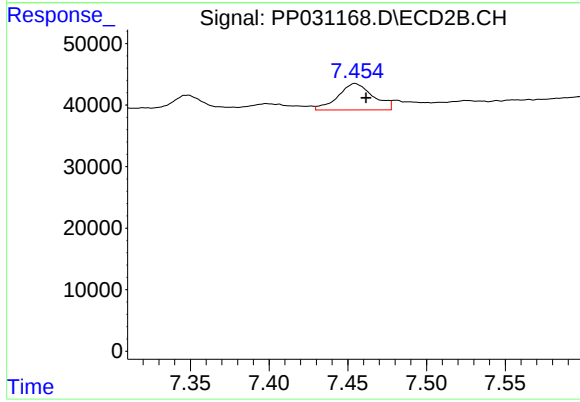

#30 AR-1254-5

R.T.: 7.455 min
Delta R.T.: -0.007 min
Response: 66759
Conc: 30.49 ng/ml