

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110422\
 Data File : PP053113.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Nov 2022 05:26
 Operator : YP\AJ
 Sample : N5450-01 10X
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC-279313-FRONT

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 08:01:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 27 04:46:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.403	3.649	3091223	2602891	1.399	1.385
2) SA Decachlor...	10.207	8.730	2490592	2766658	1.962	1.650

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110422\
Data File : PP053113.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Nov 2022 05:26
Operator : YP\AJ
Sample : N5450-01 10X
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
BC-279313-FRONT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 08:01:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 27 04:46:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

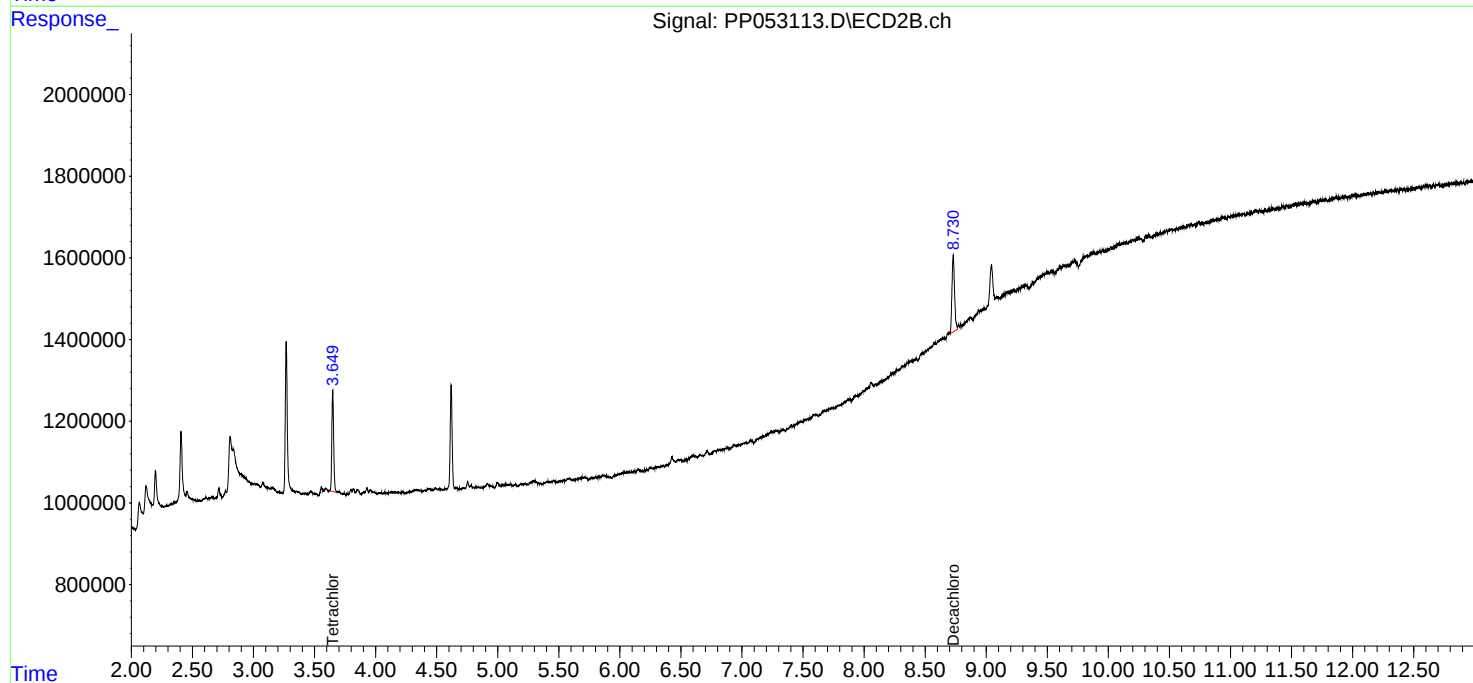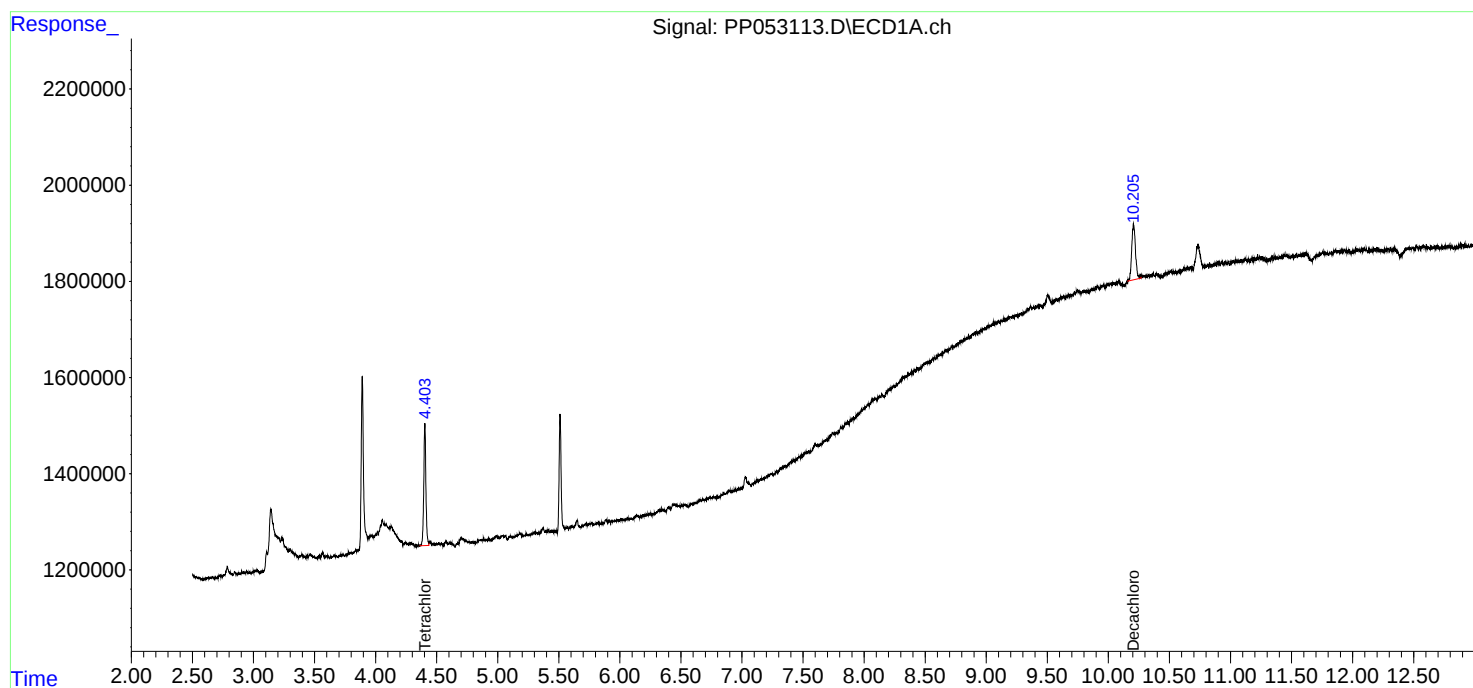


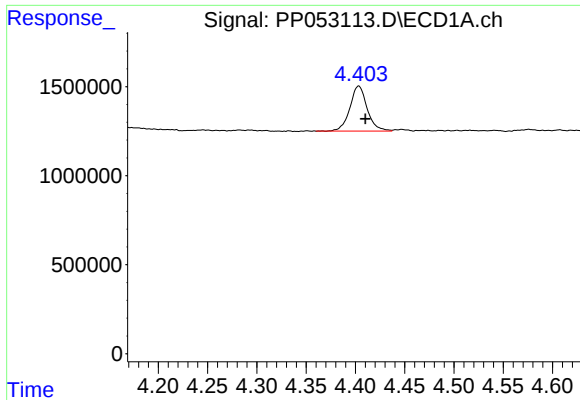

#1 Tetrachloro-m-xylene


R.T.: 4.403 min
Delta R.T.: -0.007 min
Response: 3091223
Conc: 1.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC-279313-FRONT

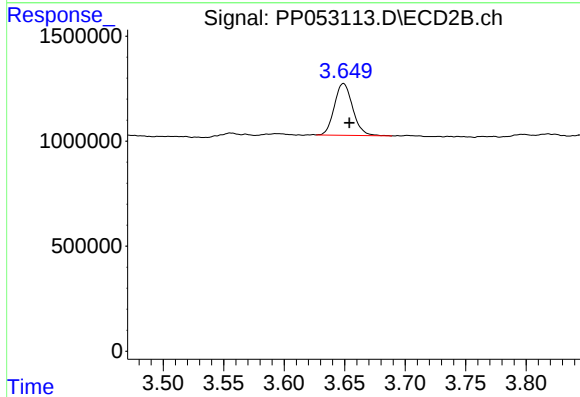


#1 Tetrachloro-m-xylene

R.T.: 3.649 min
Delta R.T.: -0.005 min
Response: 2602891
Conc: 1.39 ng/ml

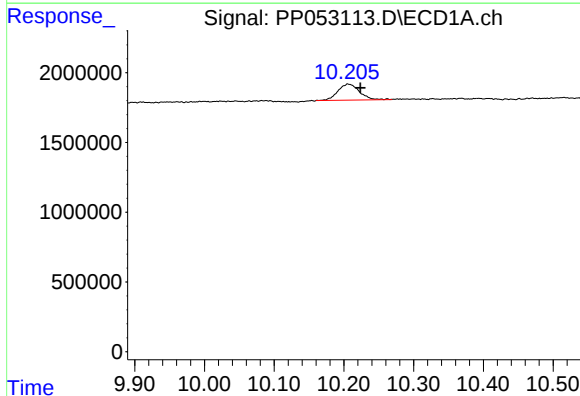

#2 Decachlorobiphenyl

R.T.: 10.207 min
Delta R.T.: -0.017 min
Response: 2490592
Conc: 1.96 ng/ml

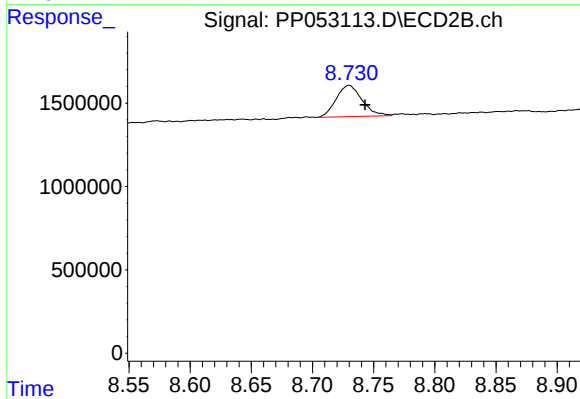

#2 Decachlorobiphenyl

R.T.: 8.730 min
Delta R.T.: -0.013 min
Response: 2766658
Conc: 1.65 ng/ml