

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110519\
 Data File : PP030526.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Nov 2019 13:14
 Operator : DD\AJ
 Sample : HSTDCC750
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HSTDCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 13:32:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110519.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 05 13:32:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.032	11.192	248.2E6	132.4E6	750.000	750.000
Target Compounds							
1) T	Dalapon	2.634	2.450	358.6E6	175.4E6	682.500	682.500
2) T	3,5-DICHL...	9.453	9.318	388.8E6	162.3E6	697.500	697.500
3) T	4-Nitroph...	10.601	10.348	263.2E6	68156669	682.500	682.500
5) T	DICAMBA	11.339	11.485	970.1E6	483.5E6	705.000	705.000
6) T	MCPD	11.686	11.692	56350161	23786883	70.500	70.500
7) T	MCPA	11.936	12.077	79139952	35622434	69.750	69.750
8) T	DICHLORPROP	12.531	12.601	236.8E6	115.9E6	705.000	705.000
9) T	2,4-D	12.888	13.085	273.5E6	137.2E6	705.000	705.000
10) T	Pentachlo...	13.244	13.640	3886.7E6	1933.2E6	712.500	712.500
11) T	2,4,5-TP ...	14.133	14.243	1358.7E6	704.3E6	712.500	712.500
12) T	2,4,5-T	14.529	14.785	1351.1E6	669.0E6	712.500	712.500
13) T	2,4-DB	15.272	15.467	182.5E6	92772214	712.500	712.500
14) T	DINOSEB	16.730	15.871	890.6E6	459.7E6	705.000	705.000
15) T	Picloram	16.510	17.188	1500.5E6	929.6E6	712.500	712.500
16) T	DCPA	17.084	17.084	1833.1E6	977.6E6	720.000	720.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110519\
Data File : PP030526.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Nov 2019 13:14
Operator : DD\AJ
Sample : HSTDCC750
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_P
Client Sampled :
HSTDCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 13:32:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110519.M
Quant Title : 8080.M
QLast Update : Tue Nov 05 13:32:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

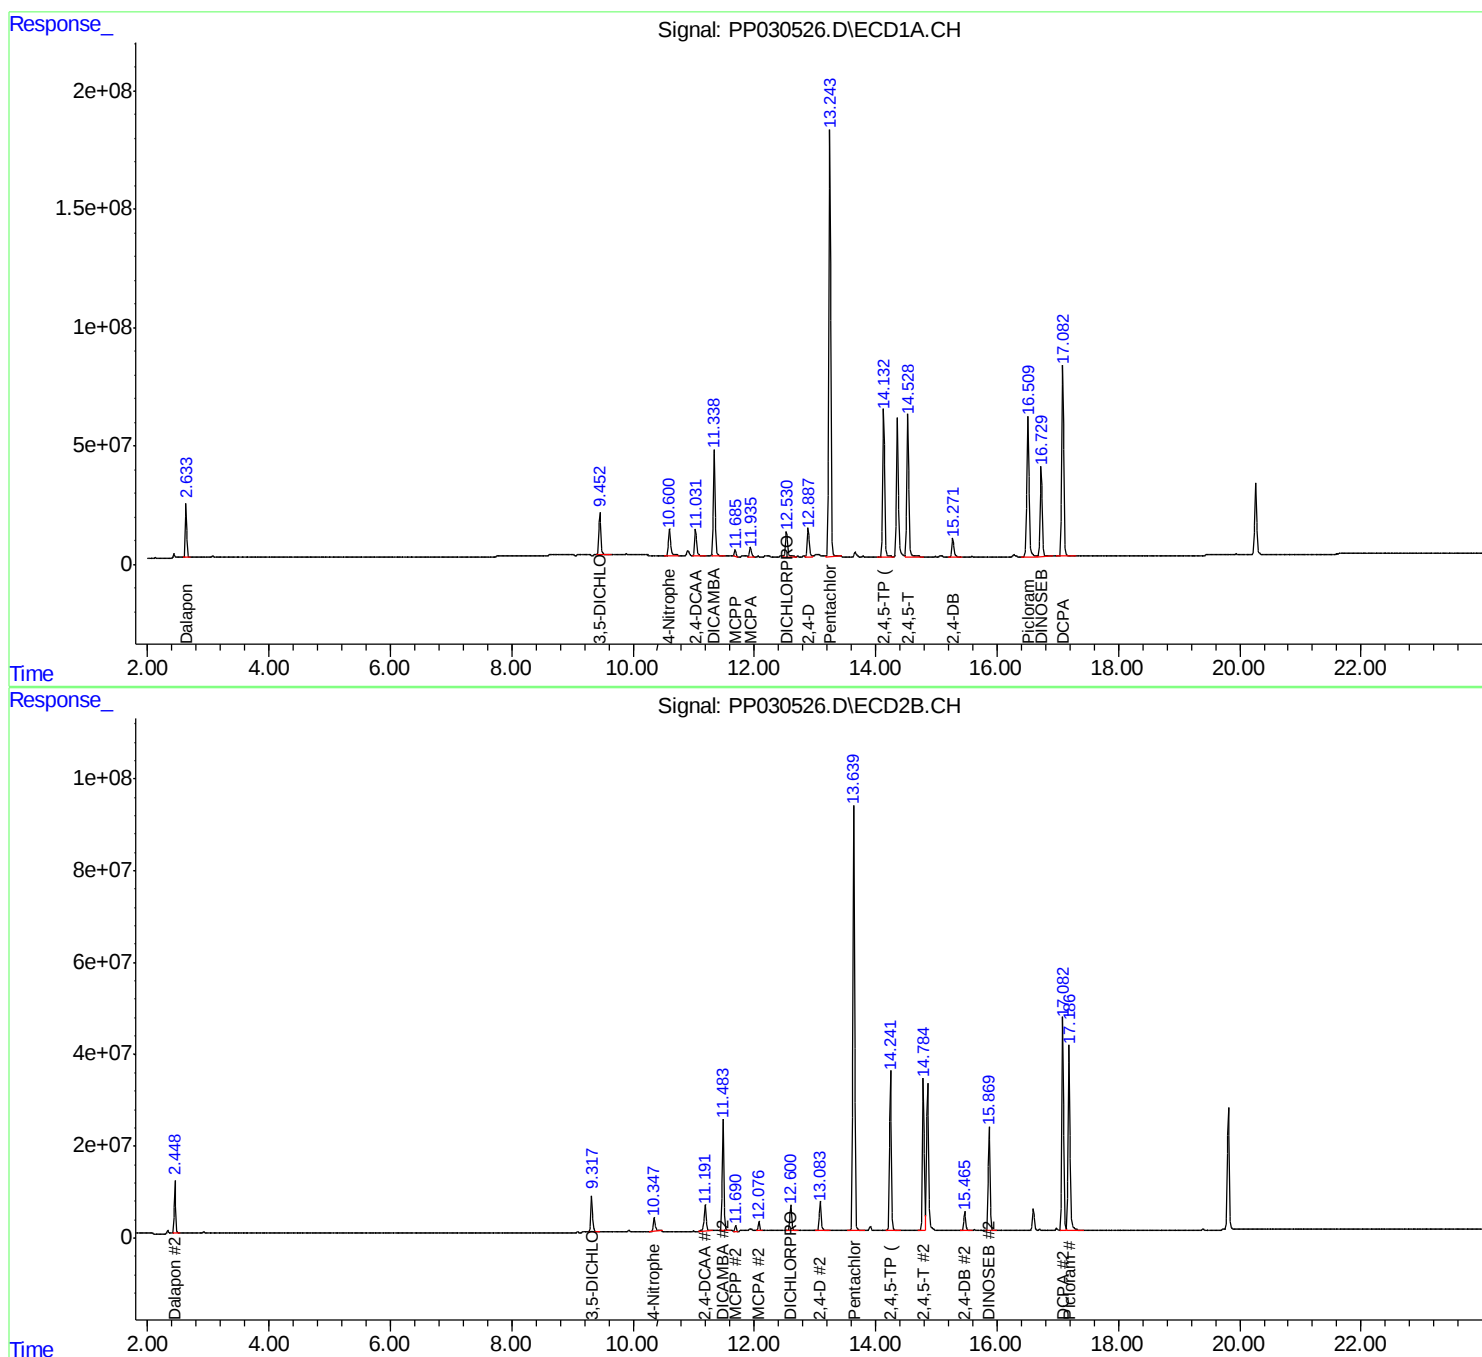


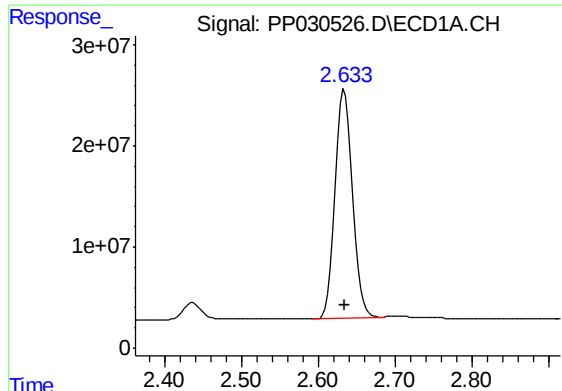

#1 Dalapon


R.T.: 2.634 min
Delta R.T.: 0.000 min
Response: 358570328
Conc: 682.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
HSTDCC750

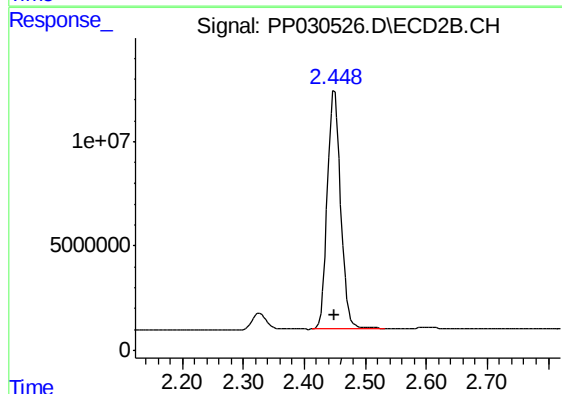


#1 Dalapon

R.T.: 2.450 min
Delta R.T.: 0.000 min
Response: 175376707
Conc: 682.50 ng/ml

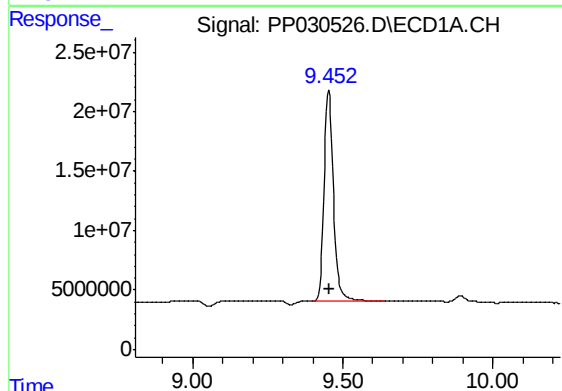


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.453 min
Delta R.T.: 0.000 min
Response: 388789258
Conc: 697.50 ng/ml

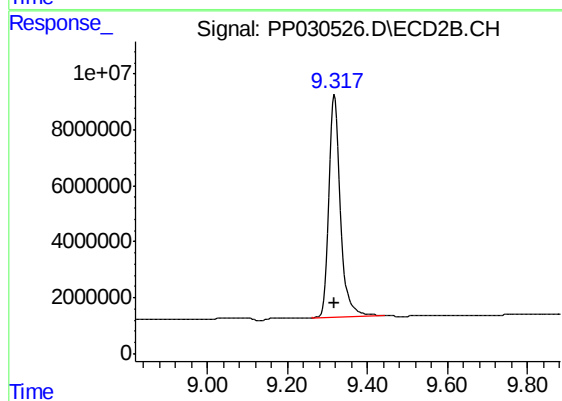

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.318 min
Delta R.T.: 0.000 min
Response: 162293838
Conc: 697.50 ng/ml

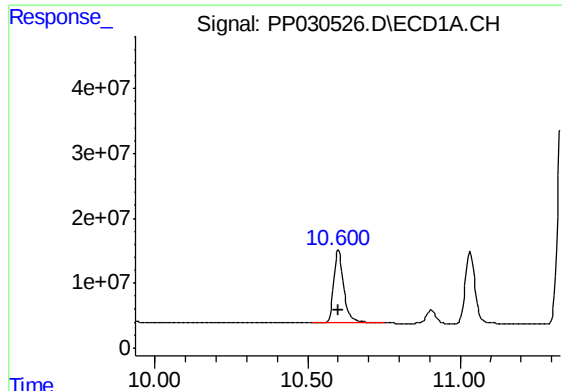

#3 4-Nitrophenol


R.T.: 10.601 min
Delta R.T.: 0.000 min
Response: 263181056
Conc: 682.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
HSTDCC750

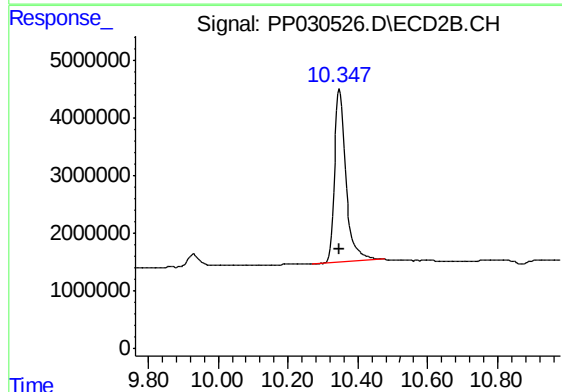


#3 4-Nitrophenol

R.T.: 10.348 min
Delta R.T.: 0.000 min
Response: 68156669
Conc: 682.50 ng/ml

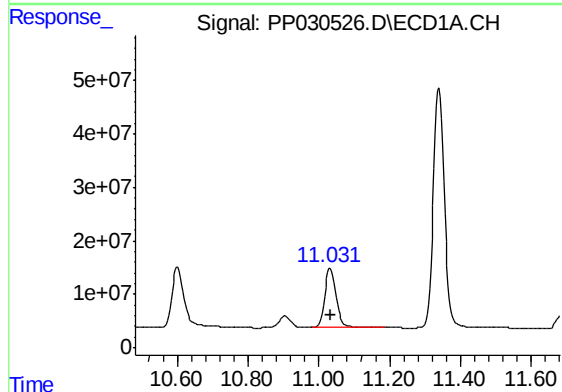


#4 2,4-DCAA

R.T.: 11.032 min
Delta R.T.: 0.000 min
Response: 248236824
Conc: 750.00 ng/ml

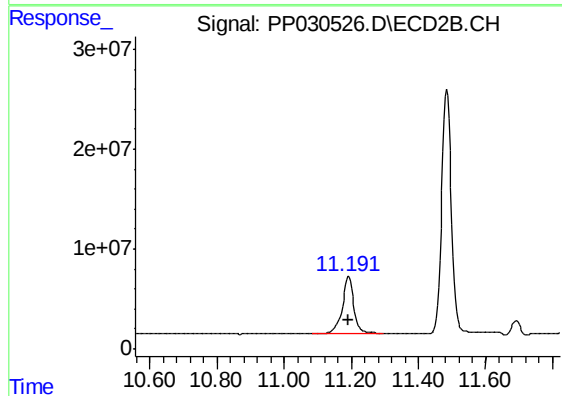

#4 2,4-DCAA


R.T.: 11.192 min
Delta R.T.: 0.000 min
Response: 132418272
Conc: 750.00 ng/ml

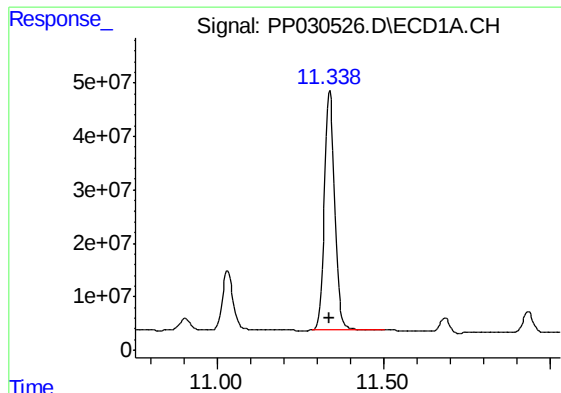

#5 DICAMBA


R.T.: 11.339 min
Delta R.T.: 0.000 min
Response: 970125587
Conc: 705.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
HSTDCC750

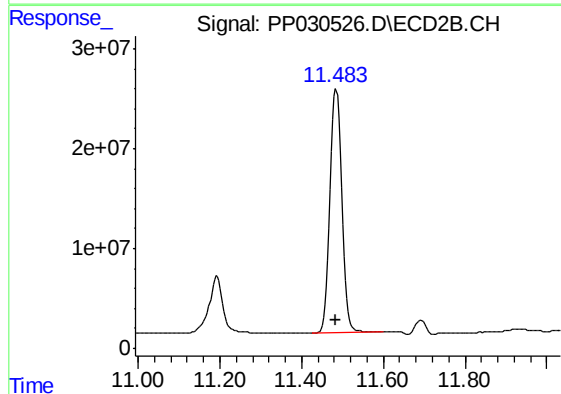


#5 DICAMBA

R.T.: 11.485 min
Delta R.T.: 0.000 min
Response: 483533048
Conc: 705.00 ng/ml

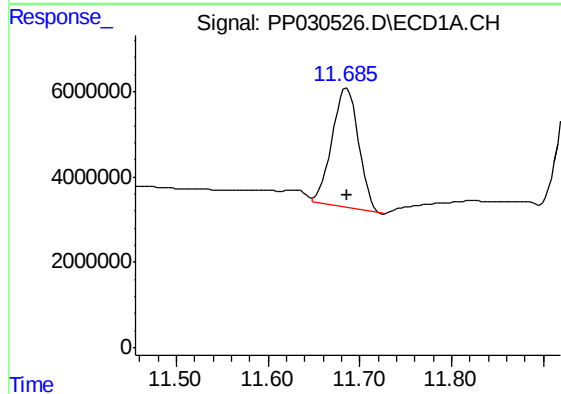


#6 MCPP

R.T.: 11.686 min
Delta R.T.: 0.000 min
Response: 56350161
Conc: 70.50 ug/ml

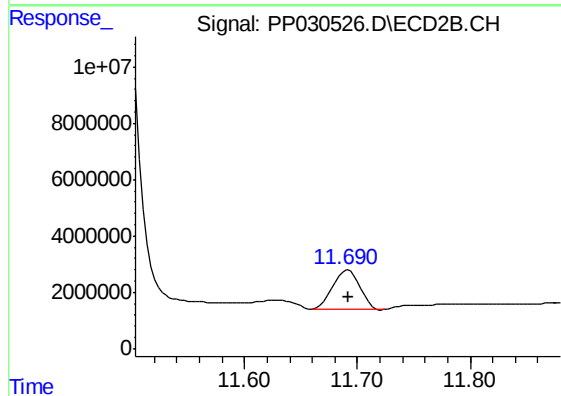

#6 MCPP


R.T.: 11.692 min
Delta R.T.: 0.000 min
Response: 23786883
Conc: 70.50 ug/ml

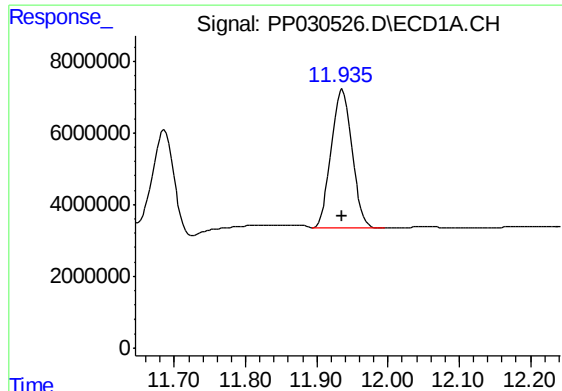

#7 MCPA


R.T.: 11.936 min
Delta R.T.: 0.000 min
Response: 79139952
Conc: 69.75 ug/ml

Instrument :
ECD_P
ClientSampleId :
HSTDCC750

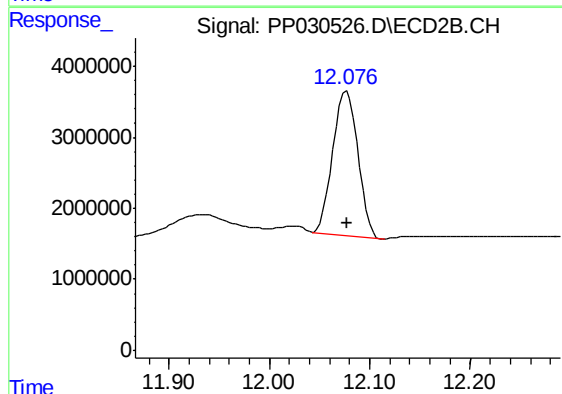


#7 MCPA

R.T.: 12.077 min
Delta R.T.: 0.000 min
Response: 35622434
Conc: 69.75 ug/ml

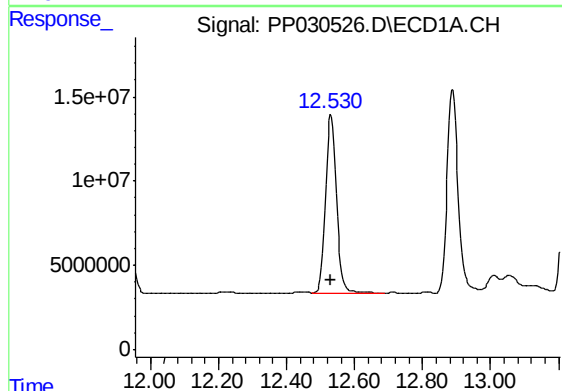


#8 DICHLORPROP

R.T.: 12.531 min
Delta R.T.: 0.000 min
Response: 236781003
Conc: 705.00 ng/ml

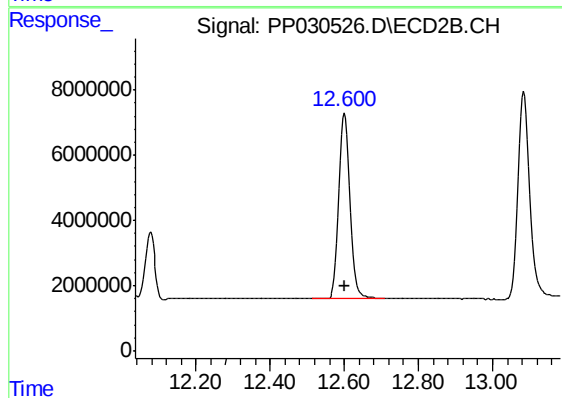

#8 DICHLORPROP


R.T.: 12.601 min
Delta R.T.: 0.000 min
Response: 115877353
Conc: 705.00 ng/ml

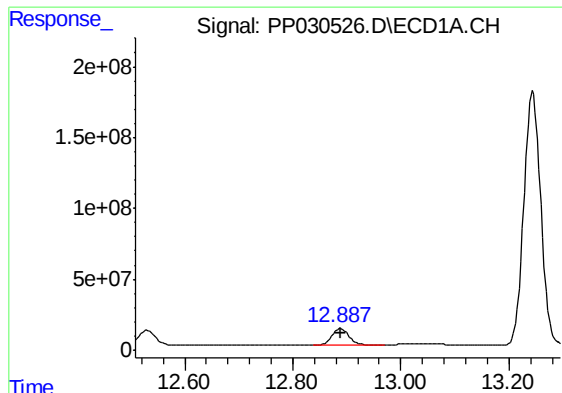

#9 2,4-D


R.T.: 12.888 min
Delta R.T.: 0.000 min
Response: 273514668
Conc: 705.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
HSTDCC750

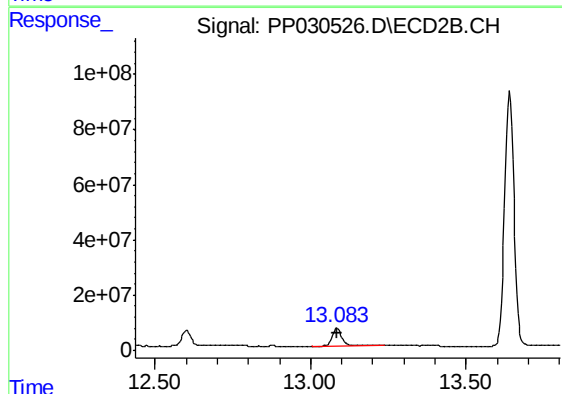


#9 2,4-D

R.T.: 13.085 min
Delta R.T.: 0.000 min
Response: 137240248
Conc: 705.00 ng/ml

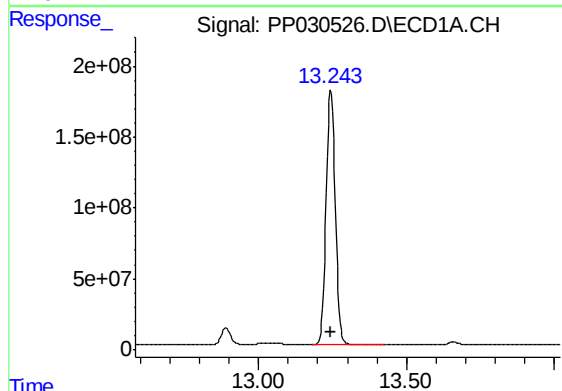


#10 Pentachlorophenol

R.T.: 13.244 min
Delta R.T.: 0.000 min
Response: 3886691491
Conc: 712.50 ng/ml

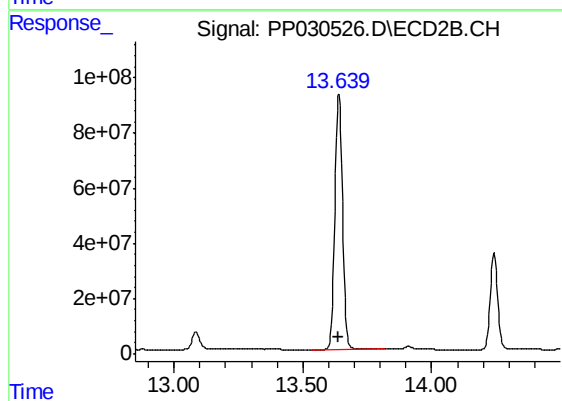

#10 Pentachlorophenol


R.T.: 13.640 min
Delta R.T.: 0.000 min
Response: 1933213820
Conc: 712.50 ng/ml

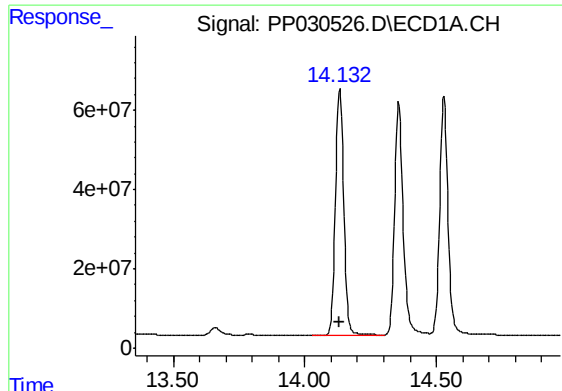

#11 2,4,5-TP (SILVEX)


R.T.: 14.133 min
Delta R.T.: 0.000 min
Response: 1358720649
Conc: 712.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
HSTDCC750

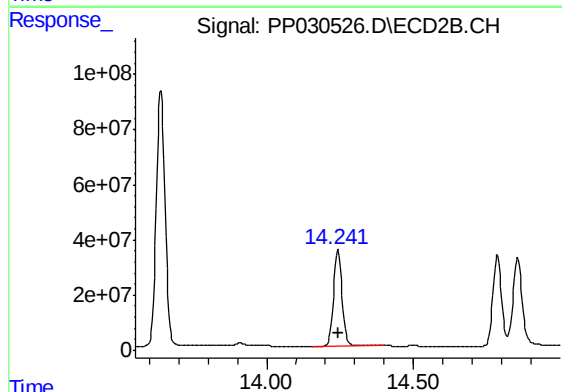


#11 2,4,5-TP (SILVEX)

R.T.: 14.243 min
Delta R.T.: 0.000 min
Response: 704340258
Conc: 712.50 ng/ml

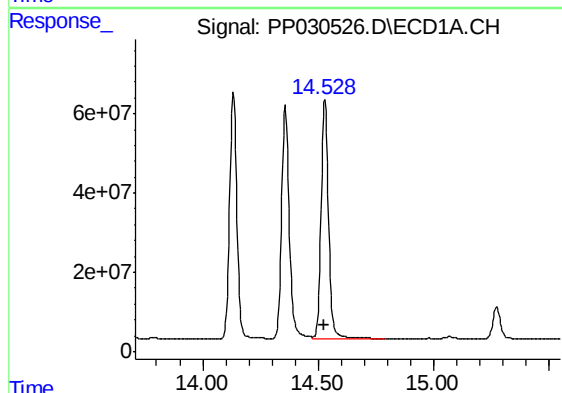


#12 2,4,5-T

R.T.: 14.529 min
Delta R.T.: 0.000 min
Response: 1351081294
Conc: 712.50 ng/ml

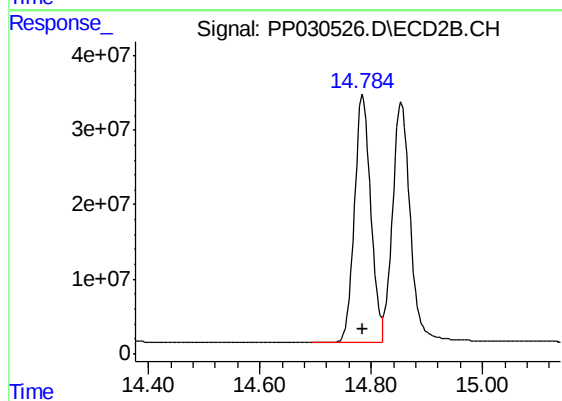

#12 2,4,5-T


R.T.: 14.785 min
Delta R.T.: 0.000 min
Response: 669011212
Conc: 712.50 ng/ml

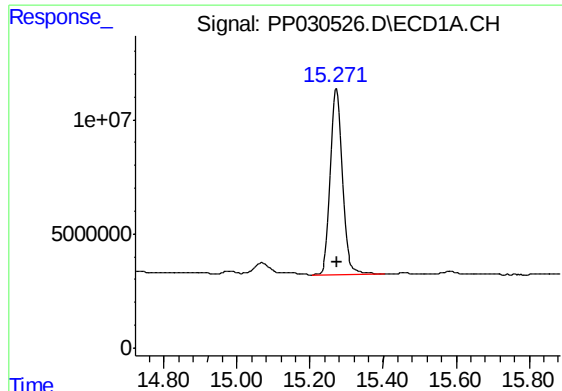

#13 2,4-DB


R.T.: 15.272 min
Delta R.T.: 0.000 min
Response: 182522722
Conc: 712.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
HSTDCC750

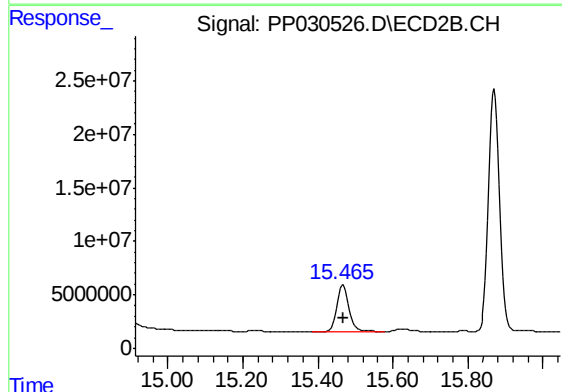


#13 2,4-DB

R.T.: 15.467 min
Delta R.T.: 0.000 min
Response: 92772214
Conc: 712.50 ng/ml

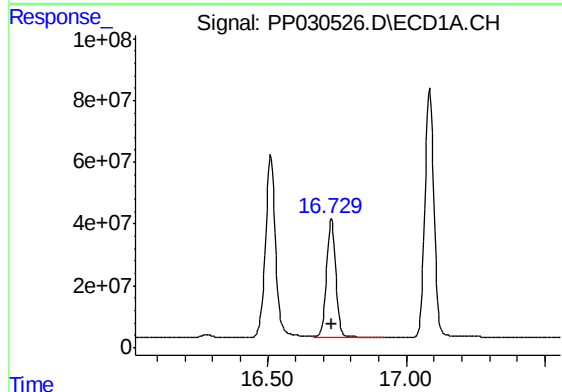


#14 DINOSEB

R.T.: 16.730 min
Delta R.T.: 0.000 min
Response: 890589987
Conc: 705.00 ng/ml

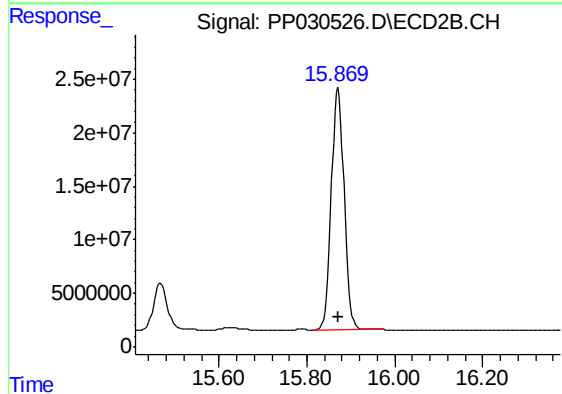

#14 DINOSEB


R.T.: 15.871 min
Delta R.T.: 0.000 min
Response: 459653945
Conc: 705.00 ng/ml

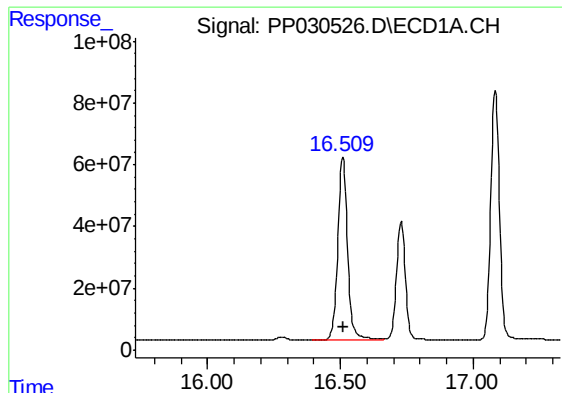

#15 Picloram


R.T.: 16.510 min
Delta R.T.: 0.000 min
Response: 1500498415
Conc: 712.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
HSTDCC750

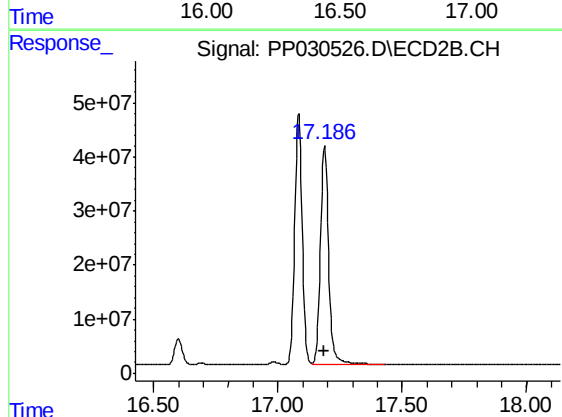


#15 Picloram

R.T.: 17.188 min
Delta R.T.: 0.000 min
Response: 929582466
Conc: 712.50 ng/ml

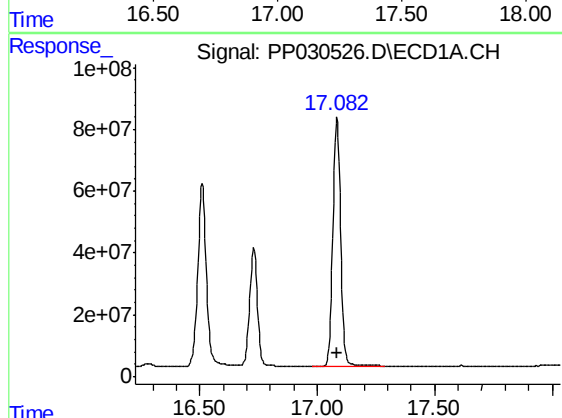

#16 DCPA

R.T.: 17.084 min
Delta R.T.: 0.000 min
Response: 1833062196
Conc: 720.00 ng/ml

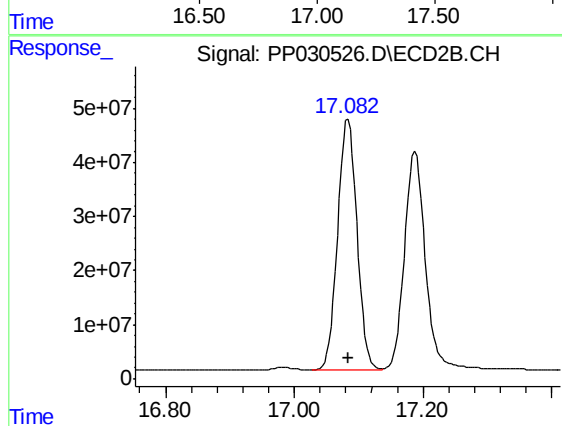

#16 DCPA

R.T.: 17.084 min
Delta R.T.: 0.000 min
Response: 977616979
Conc: 720.00 ng/ml