

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110521\
 Data File : PP040726.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Nov 2021 19:43
 Operator : AJ\MA
 Sample : PB140496BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 14:48:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 04 11:28:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.763	3.766	430446	539024	21.247	22.461
2)	SA Decachlor...	10.668	9.035	439218	354608	20.623	20.306
Target Compounds							
8)	L2 AR-1221-1	5.014f	0.000	11315	0	49.547	N.D. #
32)	L7 AR-1260-2	8.059f	0.000	12495	0	10.793	N.D. #
35)	L7 AR-1260-5	0.000	7.705f	0	12750	N.D.	7.177 #
37)	L8 AR-1262-2	0.000	7.705f	0	12750	N.D.	7.160 #
38)	L8 AR-1262-3	9.220	0.000	29258	0	27.519	N.D. #
39)	L8 AR-1262-4	9.274f	8.037	8225	14557	14.026	10.386 #
41)	L9 AR-1268-1	9.220	0.000	29258	0	10.733	N.D. #
42)	L9 AR-1268-2	0.000	8.037	0	14557	N.D.	7.303 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110521\
Data File : PP040726.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Nov 2021 19:43
Operator : AJ\MA
Sample : PB140496BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 14:48:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 04 11:28:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

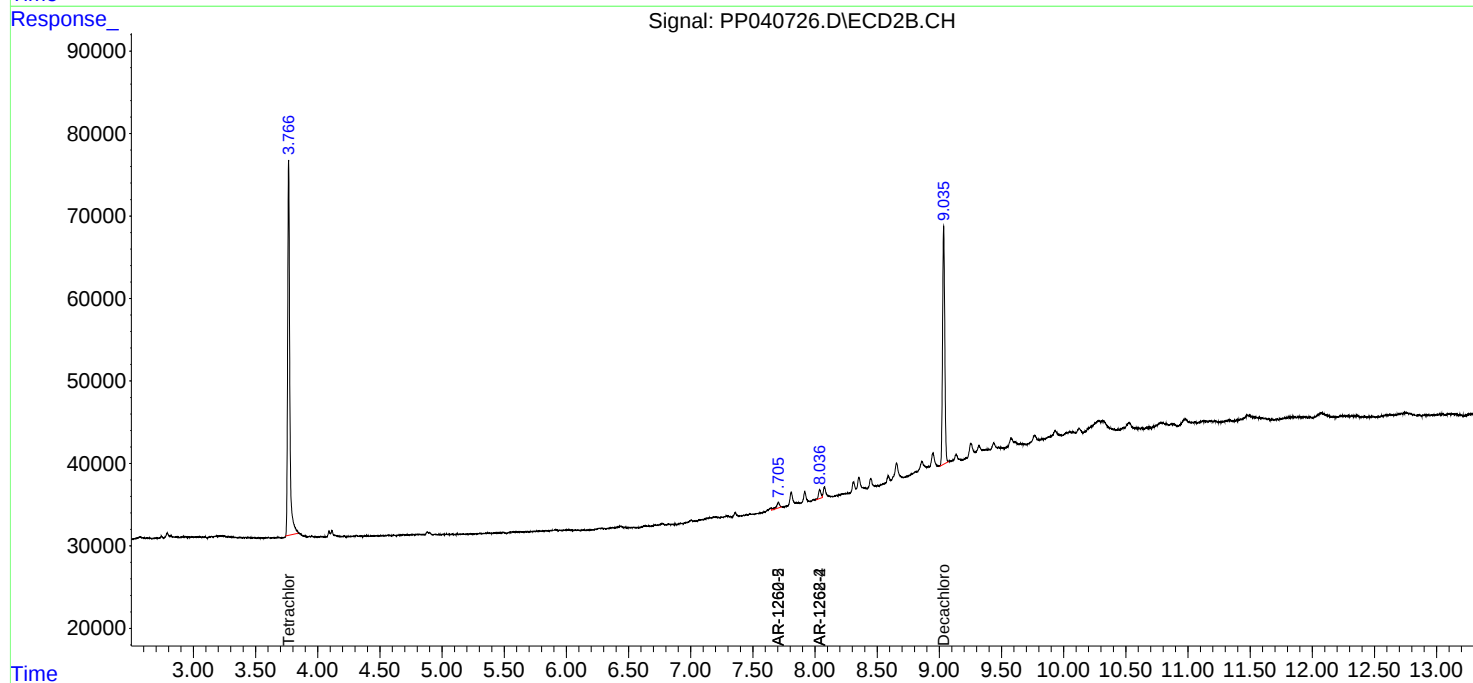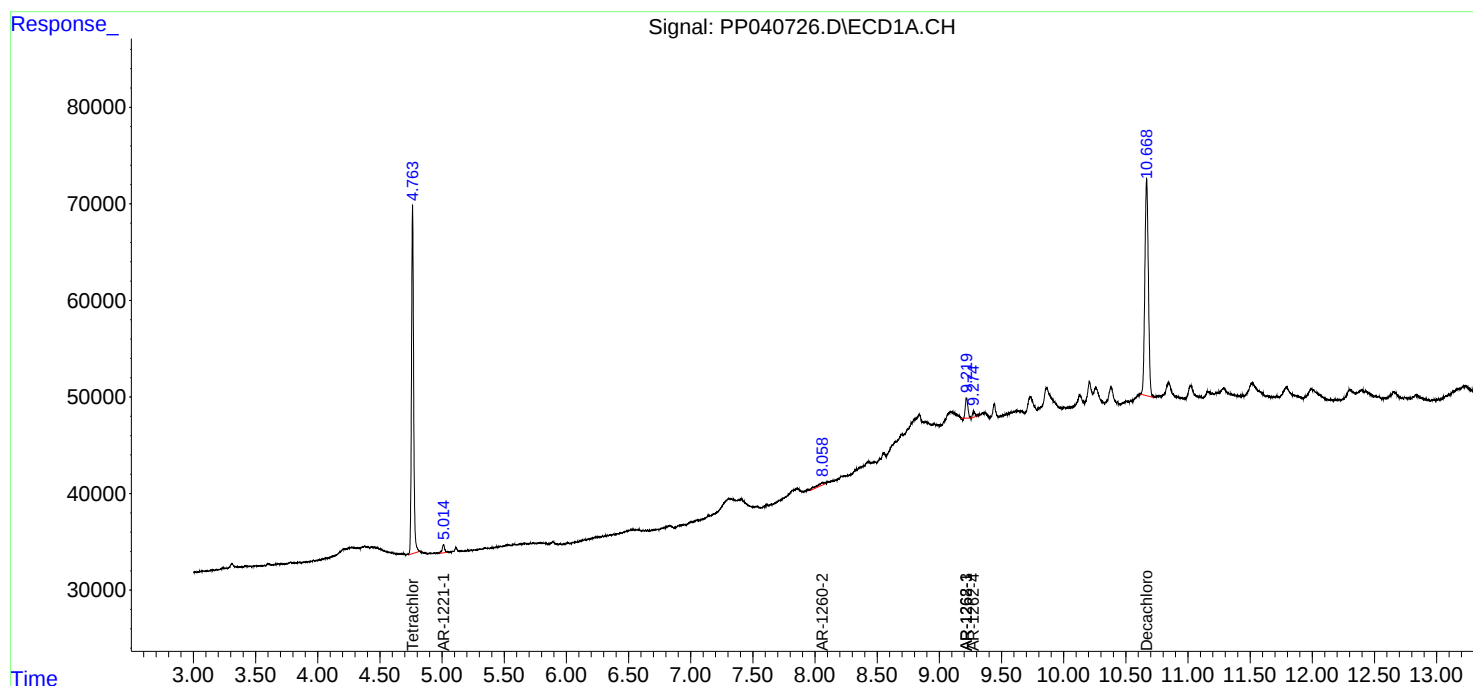


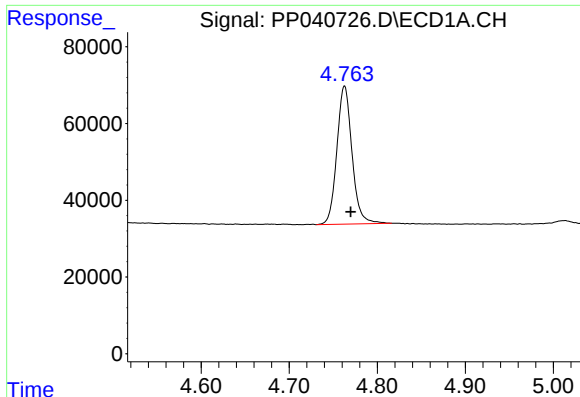

#1 Tetrachloro-m-xylene


R.T.: 4.763 min
Delta R.T.: -0.007 min
Response: 430446
Conc: 21.25 ng/ml

Instrument :
ECD_P
ClientSampleId :

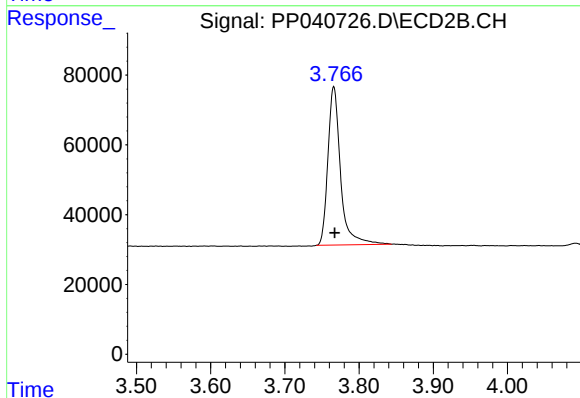


#1 Tetrachloro-m-xylene

R.T.: 3.766 min
Delta R.T.: -0.001 min
Response: 539024
Conc: 22.46 ng/ml

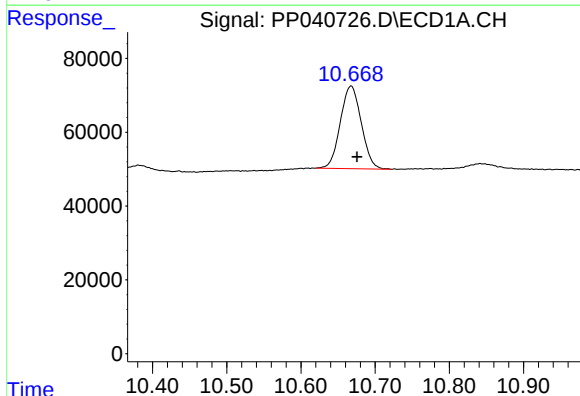


#2 Decachlorobiphenyl

R.T.: 10.668 min
Delta R.T.: -0.008 min
Response: 439218
Conc: 20.62 ng/ml

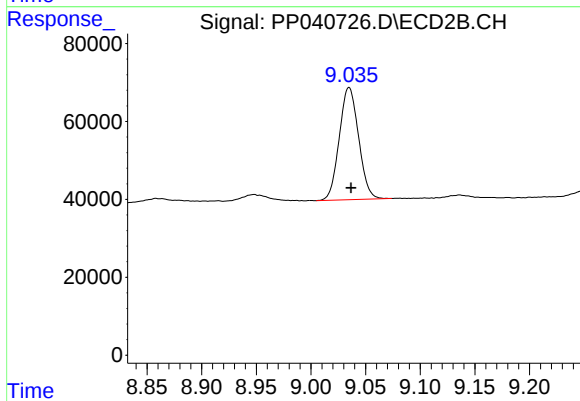

#2 Decachlorobiphenyl


R.T.: 9.035 min
Delta R.T.: -0.002 min
Response: 354608
Conc: 20.31 ng/ml

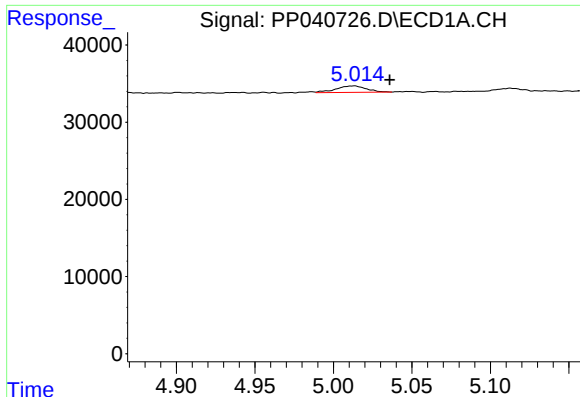

#8 AR-1221-1


R.T.: 5.014 min
Delta R.T.: -0.022 min
Response: 11315
Conc: 49.55 ng/ml

Instrument :
ECD_P
ClientSampleId :

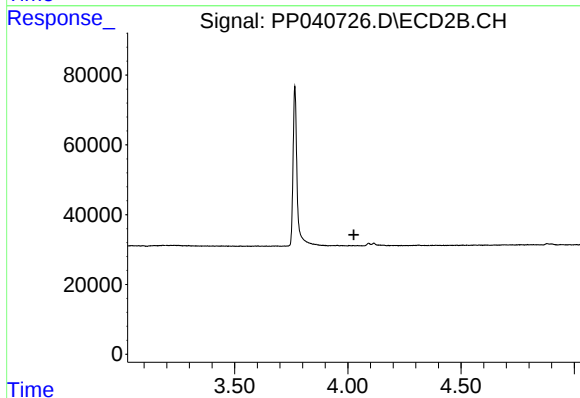


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.027 min
Response: 0
Conc: N.D.

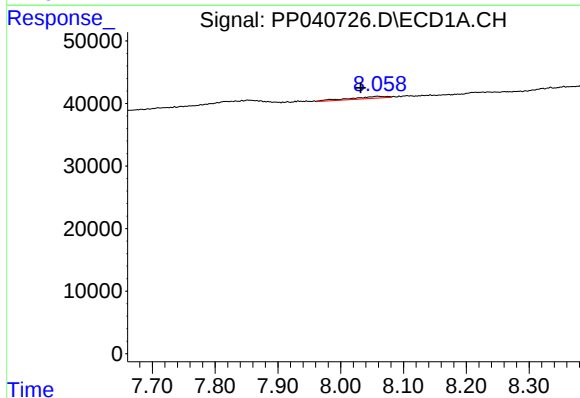


#32 AR-1260-2

R.T.: 8.059 min
Delta R.T.: 0.027 min
Response: 12495
Conc: 10.79 ng/ml

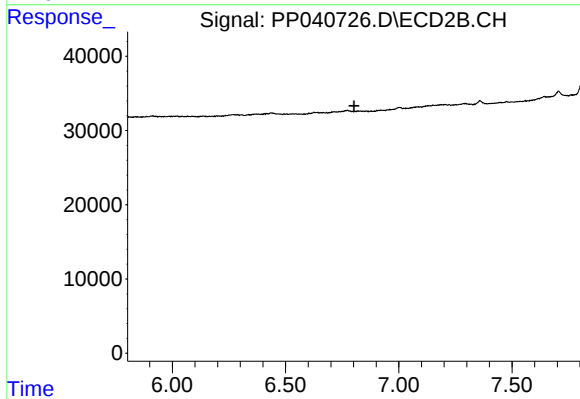

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.802 min
Response: 0
Conc: N.D.

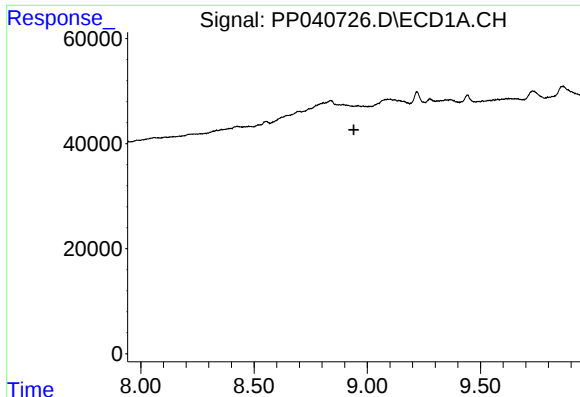

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.941 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

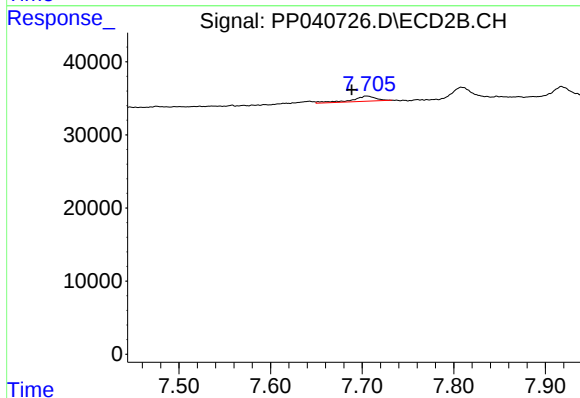


#35 AR-1260-5

R.T.: 7.705 min
Delta R.T.: 0.016 min
Response: 12750
Conc: 7.18 ng/ml

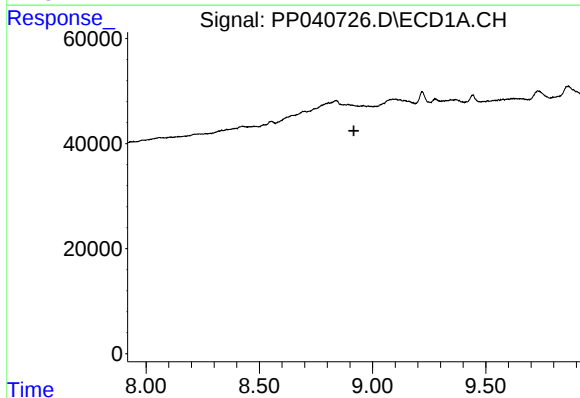


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T.: 8.918 min
Response: 0
Conc: N.D.

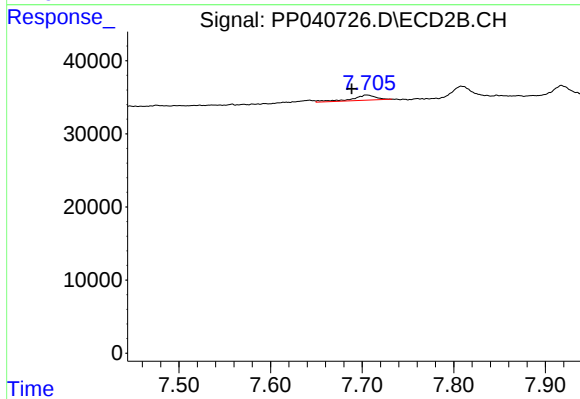

#37 AR-1262-2

R.T.: 7.705 min
Delta R.T.: 0.016 min
Response: 12750
Conc: 7.16 ng/ml

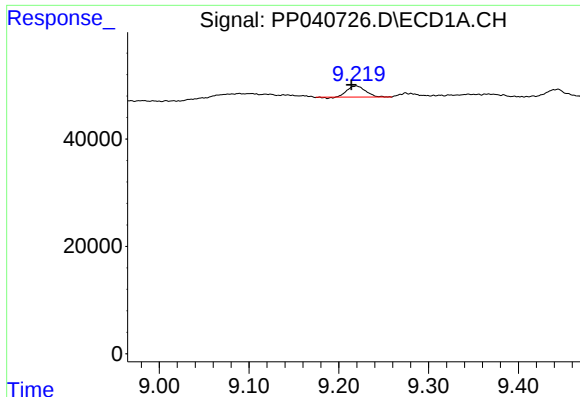

#38 AR-1262-3

R.T.: 9.220 min
Delta R.T.: 0.006 min
Response: 29258
Conc: 27.52 ng/ml

Instrument :
ECD_P
ClientSampleId :

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 7.974 min
Response: 0
Conc: N.D.

#39 AR-1262-4

R.T.: 9.274 min
Delta R.T.: -0.029 min
Response: 8225
Conc: 14.03 ng/ml

#39 AR-1262-4


R.T.: 8.037 min
Delta R.T.: -0.002 min
Response: 14557
Conc: 10.39 ng/ml

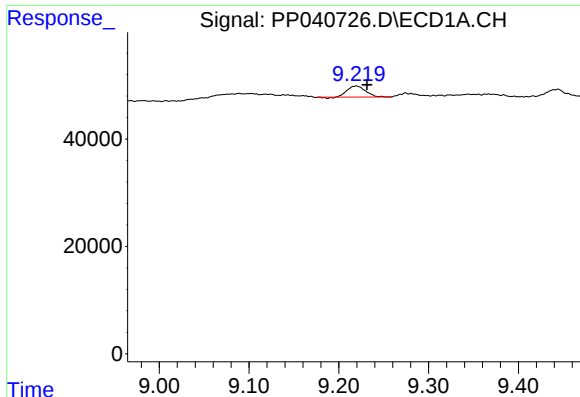

#41 AR-1268-1


R.T.: 9.220 min
Delta R.T.: -0.012 min
Response: 29258
Conc: 10.73 ng/ml

Instrument :
ECD_P
ClientSampleId :

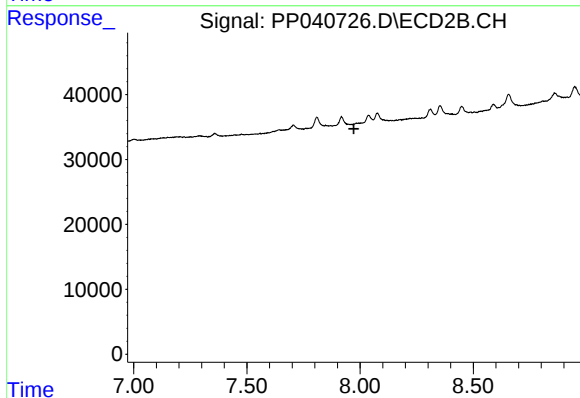


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 7.972 min
Response: 0
Conc: N.D.

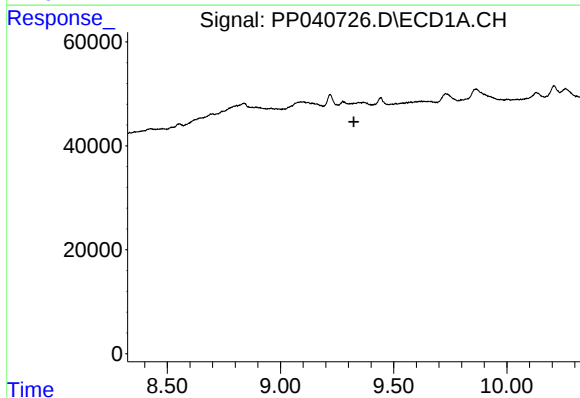

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 9.324 min
Response: 0
Conc: N.D.

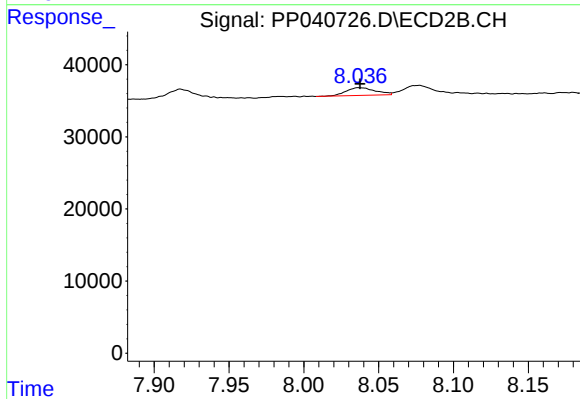

#42 AR-1268-2

R.T.: 8.037 min
Delta R.T.: -0.001 min
Response: 14557
Conc: 7.30 ng/ml