

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110521\
 Data File : PP040740.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Nov 2021 00:17
 Operator : AJ\MA
 Sample : M4491-08 10X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 14:51:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 04 11:28:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.763	3.766	32646	45910	1.611	1.913
2)	SA Decachlor...	10.664	9.035	53510	33295	2.513	1.907
Target Compounds							
4)	L1 AR-1016-2	6.129f	0.000	7232	0	6.781	N.D. #
13)	L3 AR-1232-3	6.129	0.000	7232	0	16.832	N.D. #
17)	L4 AR-1242-2	6.129f	0.000	7232	0	8.945	N.D. #
18)	L4 AR-1242-3	6.139f	0.000	1555	0	3.136	N.D. #
30)	L6 AR-1254-5	8.323	0.000	6894	0	6.355	N.D. #
36)	L8 AR-1262-1	8.349f	0.000	773	0	0.617	N.D. #
38)	L8 AR-1262-3	9.223	0.000	14090	0	13.253	N.D. #
41)	L9 AR-1268-1	9.223	0.000	14090	0	5.169	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110521\
Data File : PP040740.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Nov 2021 00:17
Operator : AJ\MA
Sample : M4491-08 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 14:51:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 04 11:28:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

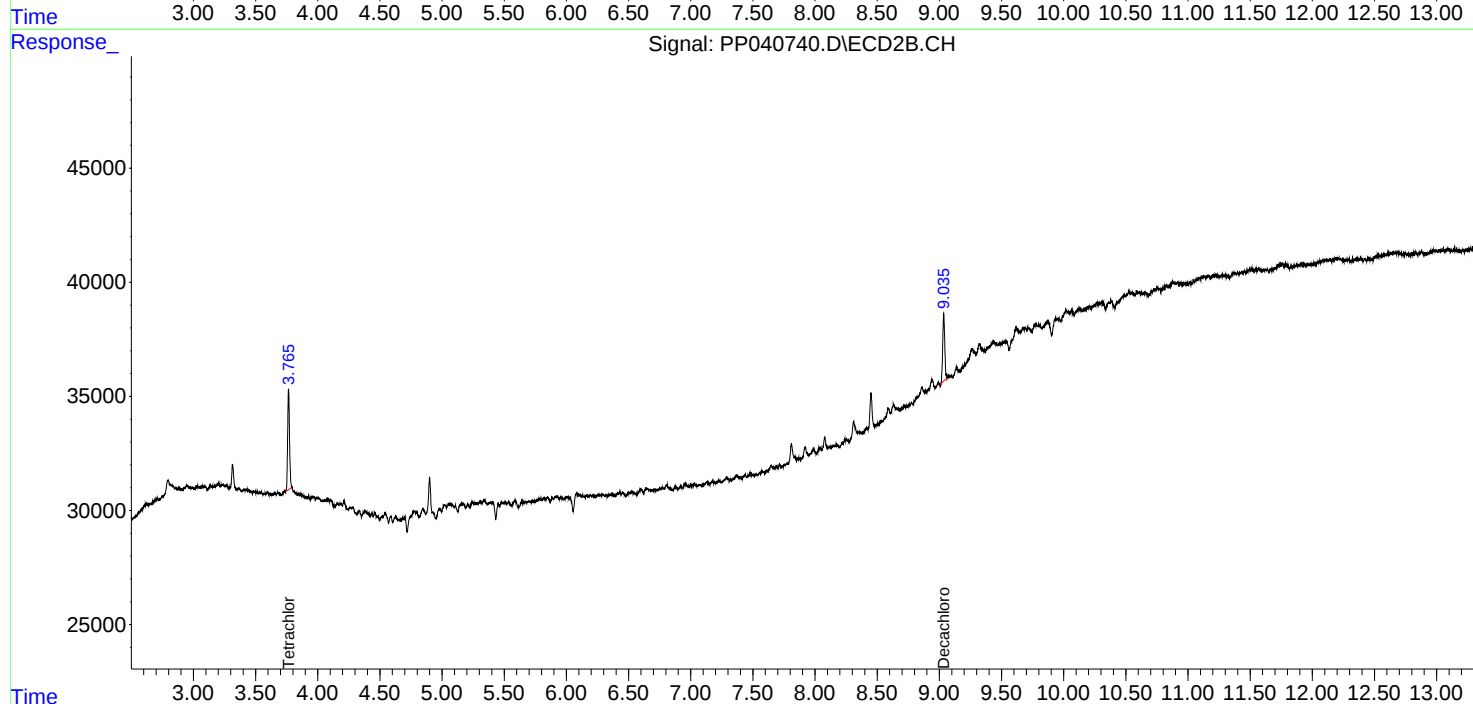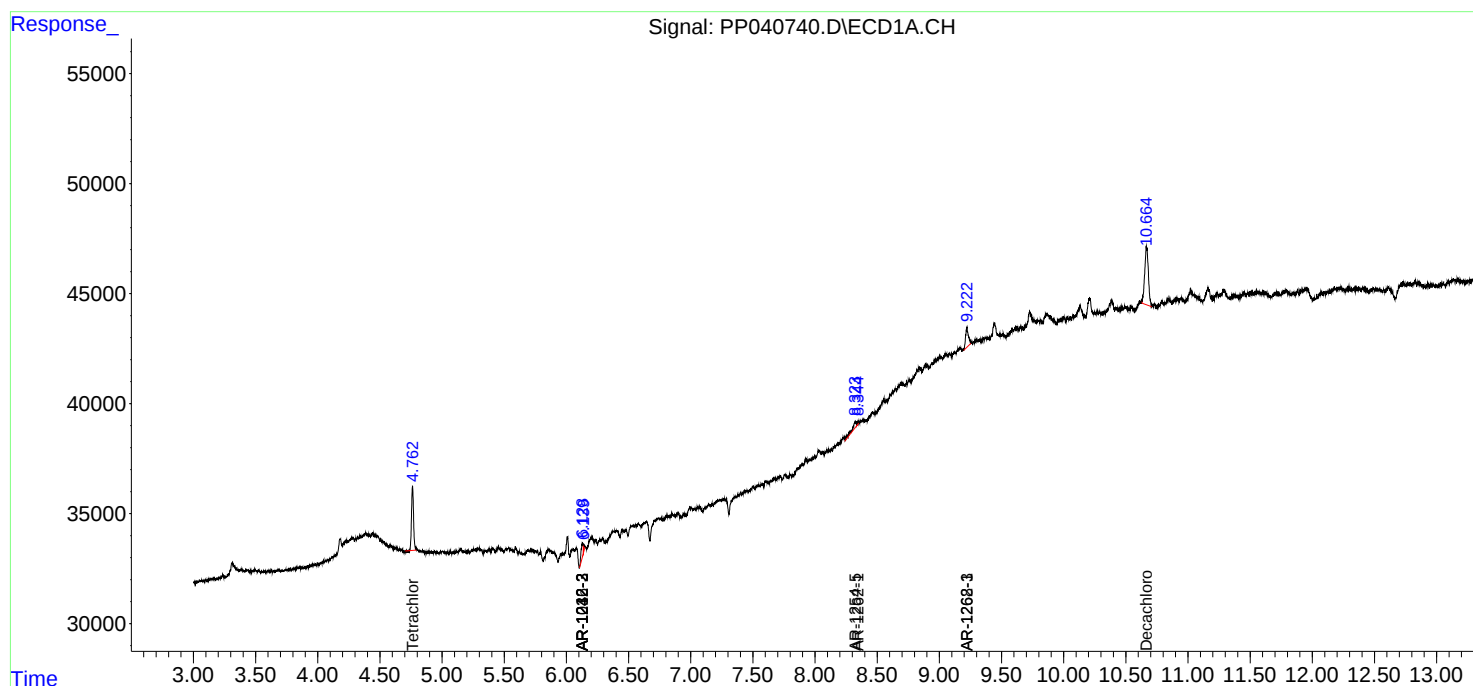


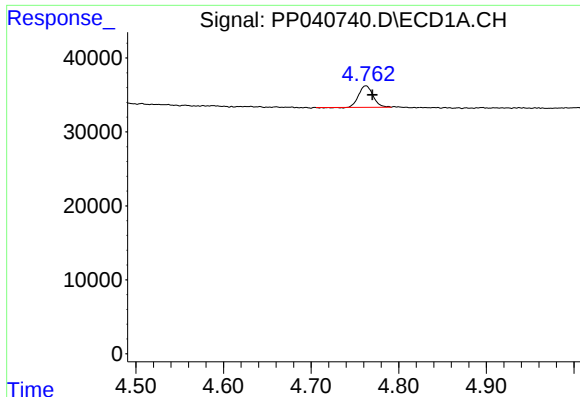

#1 Tetrachloro-m-xylene


R.T.: 4.763 min
Delta R.T.: -0.007 min
Response: 32646
Conc: 1.61 ng/ml

Instrument :
ECD_P
ClientSampleId :

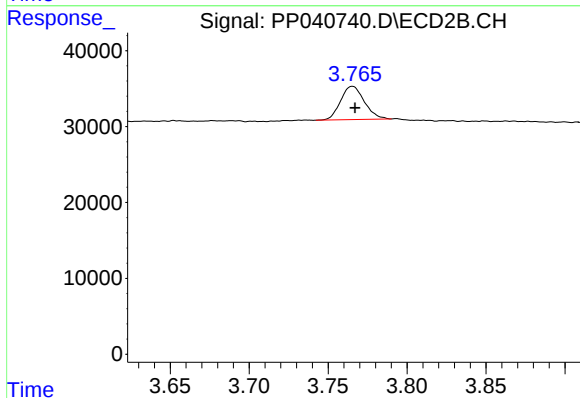


#1 Tetrachloro-m-xylene

R.T.: 3.766 min
Delta R.T.: -0.002 min
Response: 45910
Conc: 1.91 ng/ml

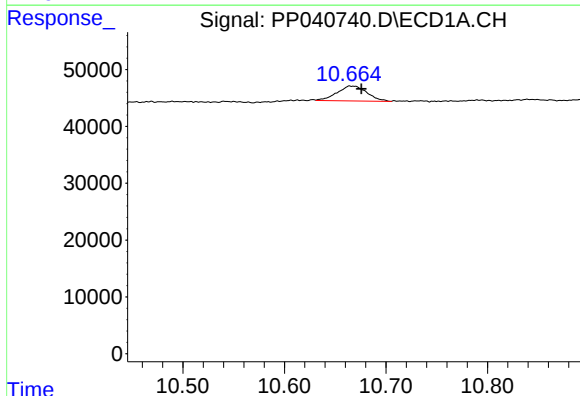


#2 Decachlorobiphenyl

R.T.: 10.664 min
Delta R.T.: -0.012 min
Response: 53510
Conc: 2.51 ng/ml

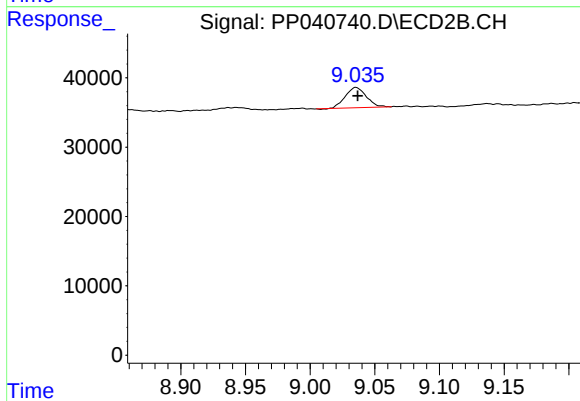

#2 Decachlorobiphenyl


R.T.: 9.035 min
Delta R.T.: -0.002 min
Response: 33295
Conc: 1.91 ng/ml

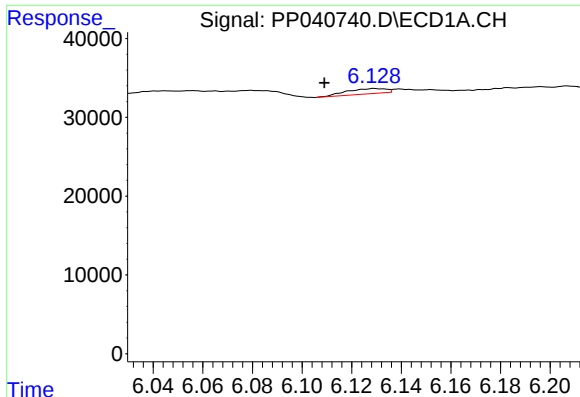

#4 AR-1016-2


R.T.: 6.129 min
Delta R.T.: 0.020 min
Response: 7232
Conc: 6.78 ng/ml

Instrument :
ECD_P
ClientSampleId :

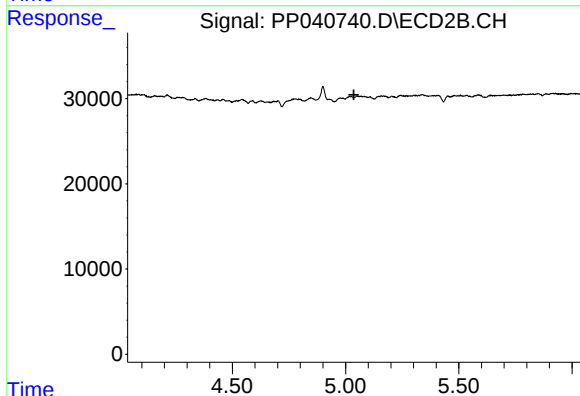


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T. : 5.037 min
Response: 0
Conc: N.D.

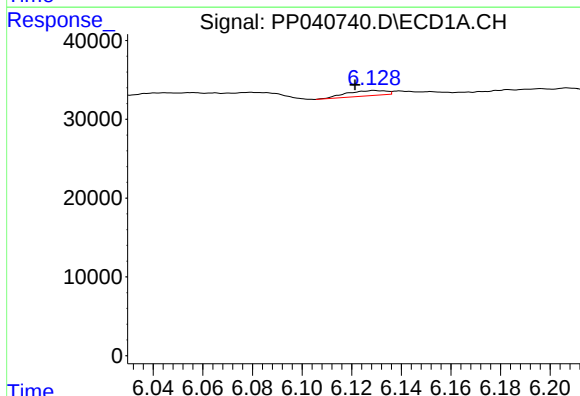


#13 AR-1232-3

R.T.: 6.129 min
Delta R.T.: 0.008 min
Response: 7232
Conc: 16.83 ng/ml

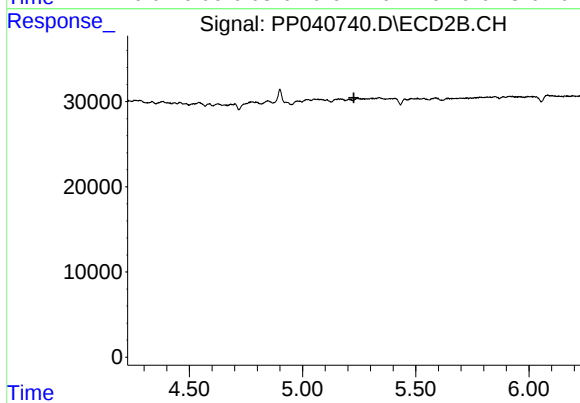

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T. : 5.227 min
Response: 0
Conc: N.D.

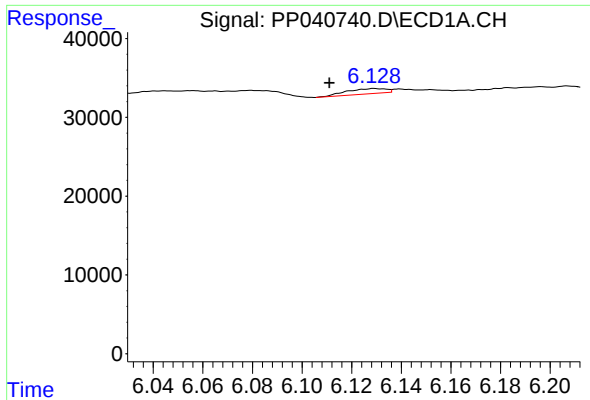

#17 AR-1242-2


R.T.: 6.129 min
Delta R.T.: 0.018 min
Response: 7232
Conc: 8.94 ng/ml

Instrument :
ECD_P
ClientSampleId :

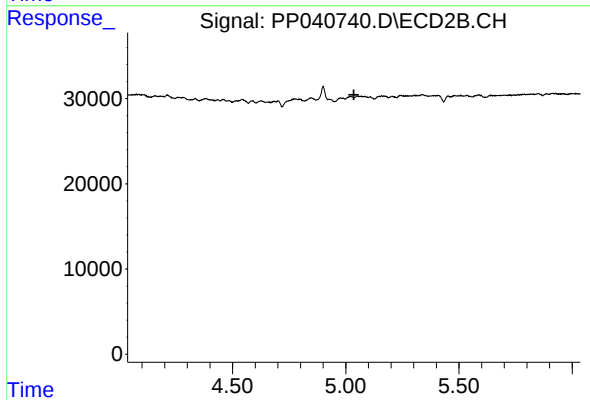


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T. : 5.036 min
Response: 0
Conc: N.D.

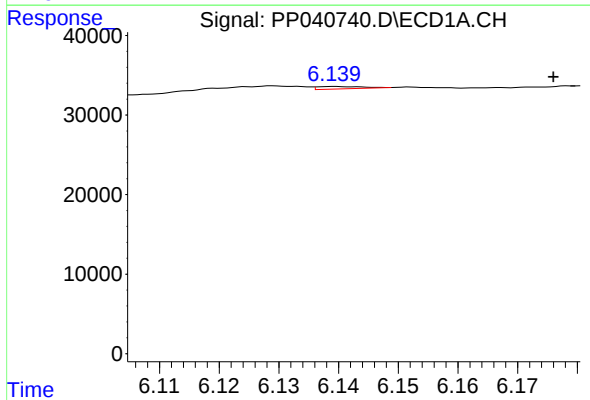


#18 AR-1242-3

R.T.: 6.139 min
Delta R.T.: -0.037 min
Response: 1555
Conc: 3.14 ng/ml

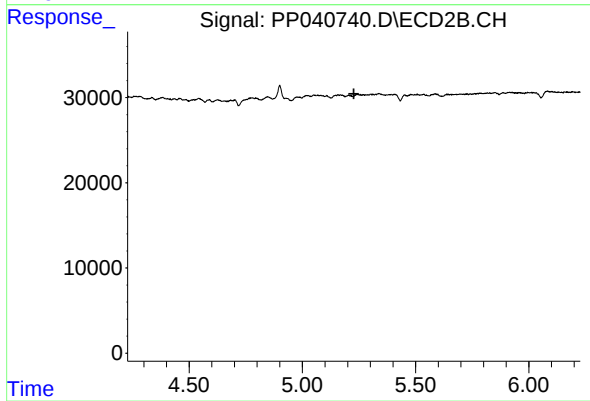

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T. : 5.227 min
Response: 0
Conc: N.D.

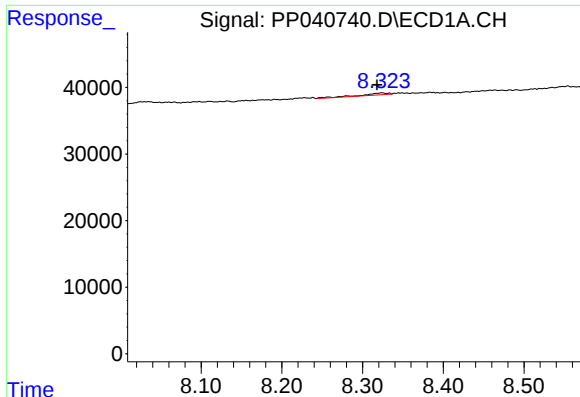

#30 AR-1254-5


R.T.: 8.323 min
Delta R.T.: 0.005 min
Response: 6894
Conc: 6.35 ng/ml

Instrument :
ECD_P
ClientSampleId :

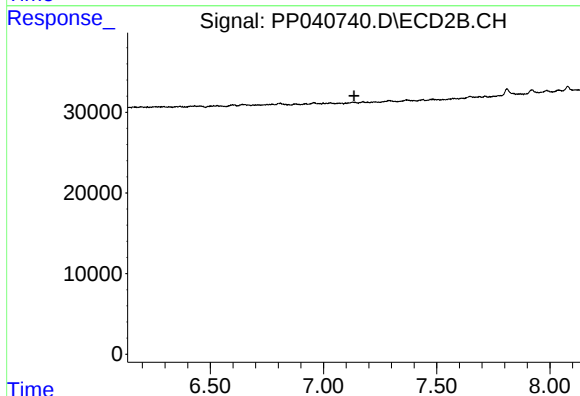


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.135 min
Response: 0
Conc: N.D.

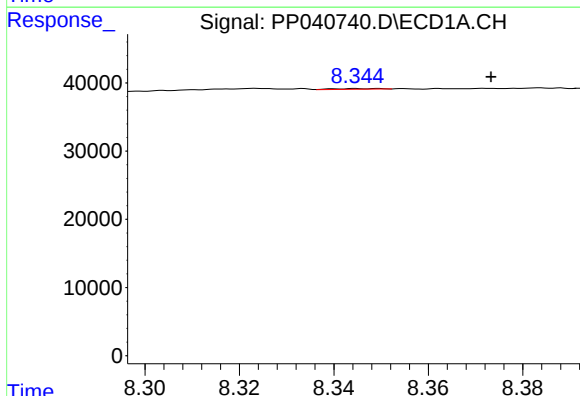


#36 AR-1262-1

R.T.: 8.349 min
Delta R.T.: -0.024 min
Response: 773
Conc: 0.62 ng/ml

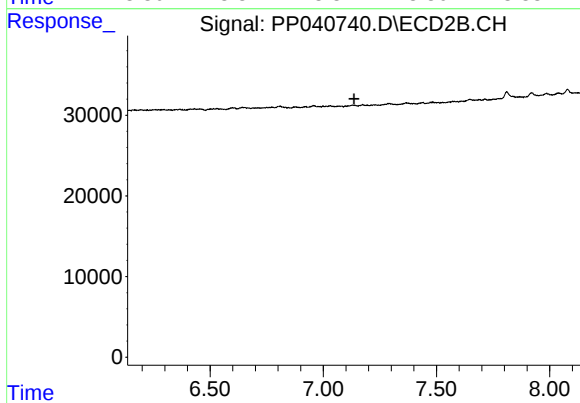

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 7.135 min
Response: 0
Conc: N.D.

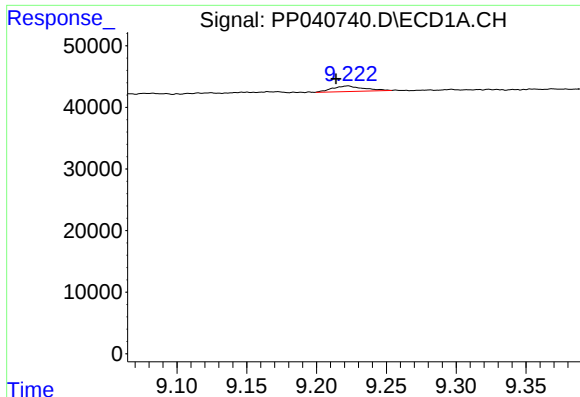

#38 AR-1262-3


R.T.: 9.223 min
Delta R.T.: 0.009 min
Response: 14090
Conc: 13.25 ng/ml

Instrument :
ECD_P
ClientSampleId :

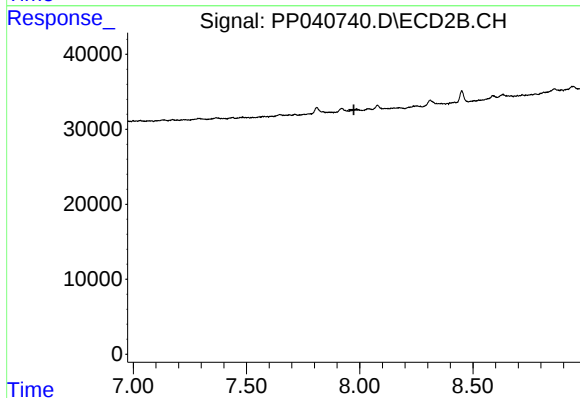


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 7.974 min
Response: 0
Conc: N.D.

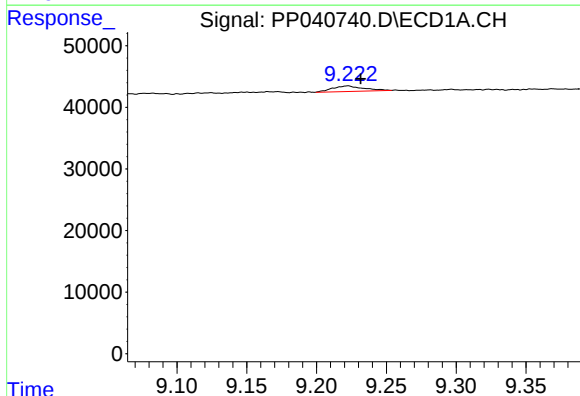

#41 AR-1268-1

R.T.: 9.223 min
Delta R.T.: -0.009 min
Response: 14090
Conc: 5.17 ng/ml

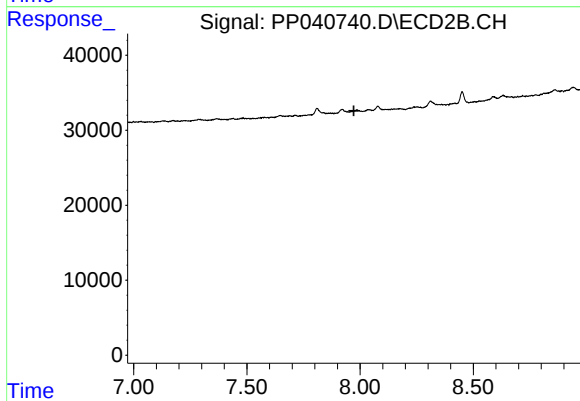

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 7.972 min
Response: 0
Conc: N.D.