

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110521\
 Data File : PP040709.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Nov 2021 14:15
 Operator : AJ\MA
 Sample : M4454-07 20X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 30860

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 11/08/2021
 Supervised By :mohammad ahmed 11/08/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 14:57:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 04 11:28:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.761	3.766	12235	9157	0.604m	0.382 #
2) SA Decachlor...	10.674	9.036	17629	5528	0.828	0.317m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110521\
Data File : PP040709.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Nov 2021 14:15
Operator : AJ\MA
Sample : M4454-07 20X
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
ECD_P
ClientSampleId :
30860


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/08/2021
Supervised By :mohammad ahmed 11/08/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 14:57:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 04 11:28:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

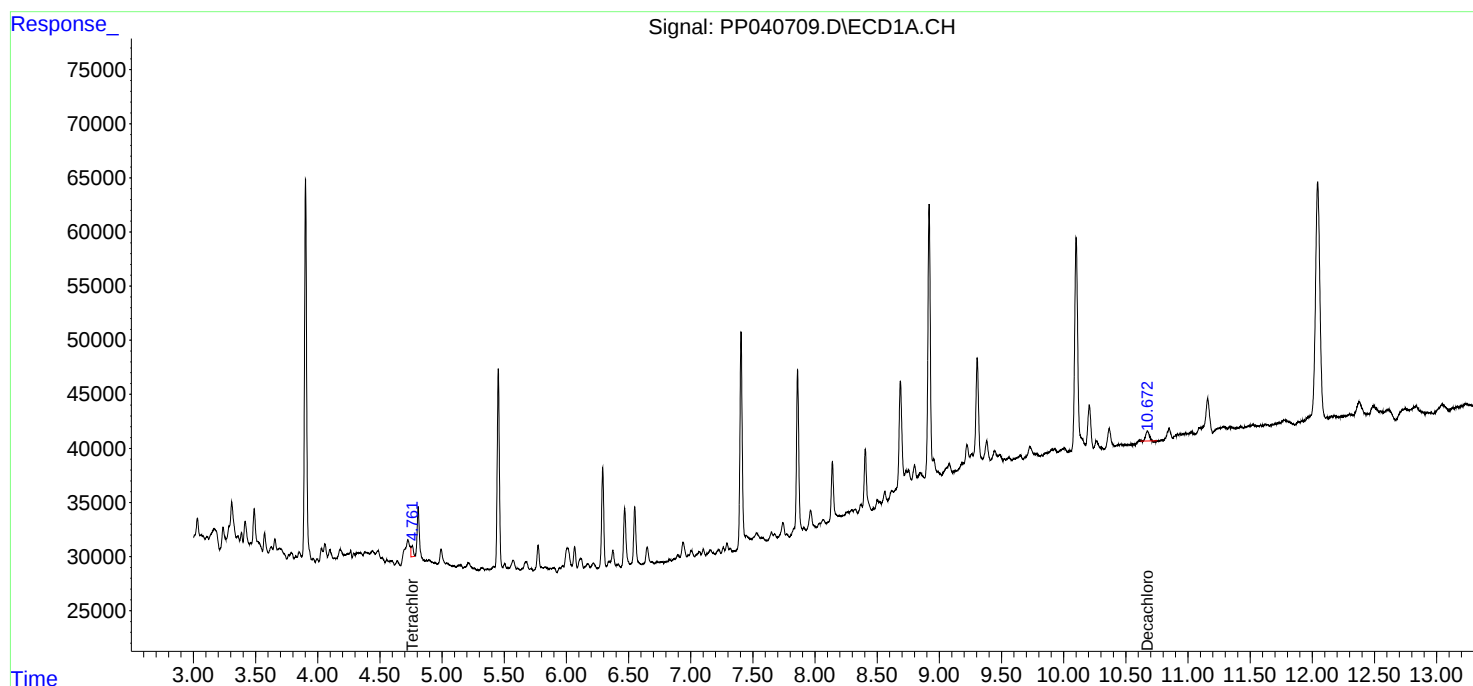

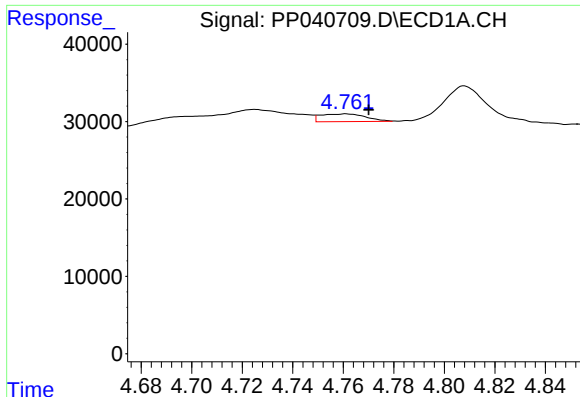


#1 Tetrachloro-m-xylene

R.T.: 4.761 min
Delta R.T.: -0.009 min
Response: 12235
Conc: 0.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
30860


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/08/2021
Supervised By :mohammad ahmed 11/08/2021

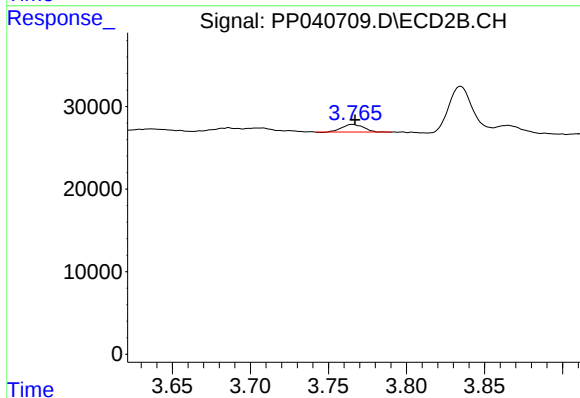


#1 Tetrachloro-m-xylene

R.T.: 3.766 min
Delta R.T.: -0.002 min
Response: 9157
Conc: 0.38 ng/ml

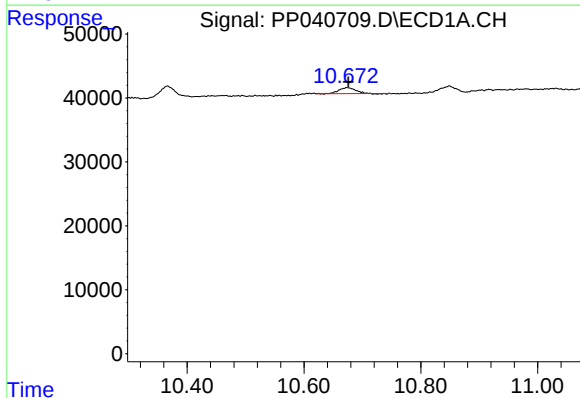

#2 Decachlorobiphenyl

R.T.: 10.674 min
Delta R.T.: -0.002 min
Response: 17629
Conc: 0.83 ng/ml

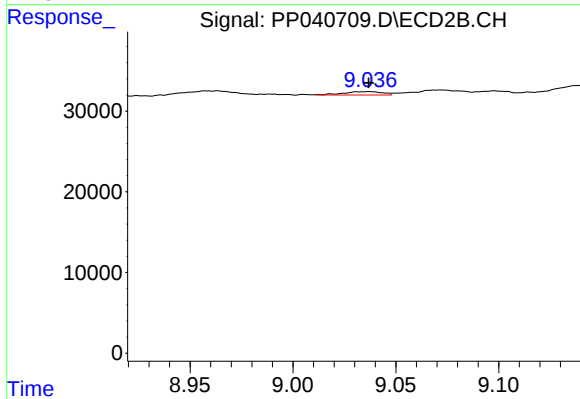

#2 Decachlorobiphenyl

R.T.: 9.036 min
Delta R.T.: 0.000 min
Response: 5528
Conc: 0.32 ng/ml m