

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110525\
 Data File : PP076332.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Nov 2025 13:37
 Operator : YP\AJ
 Sample : Q3522-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 102825-A

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 11/06/2025
 Supervised By :Yogesh Patel 11/06/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 01:17:39 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 24 15:40:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.640	3.780	21664565	110.3E6	15.160m	16.670
2) SA Decachlor...	10.416	8.778	20308408	112.9E6	18.865	13.736 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110525\
Data File : PP076332.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Nov 2025 13:37
Operator : YP\AJ
Sample : Q3522-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
102825-A


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/06/2025
Supervised By :Yogesh Patel 11/06/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 01:17:39 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 24 15:40:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

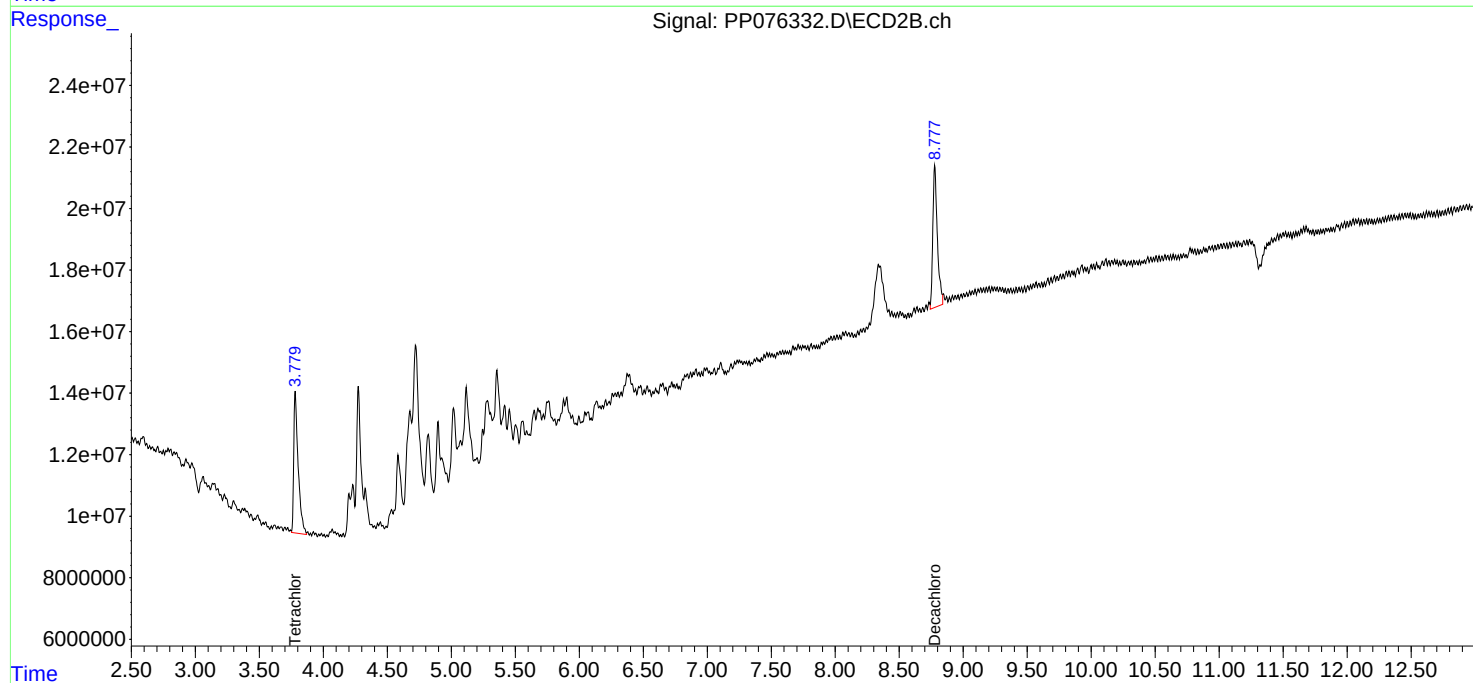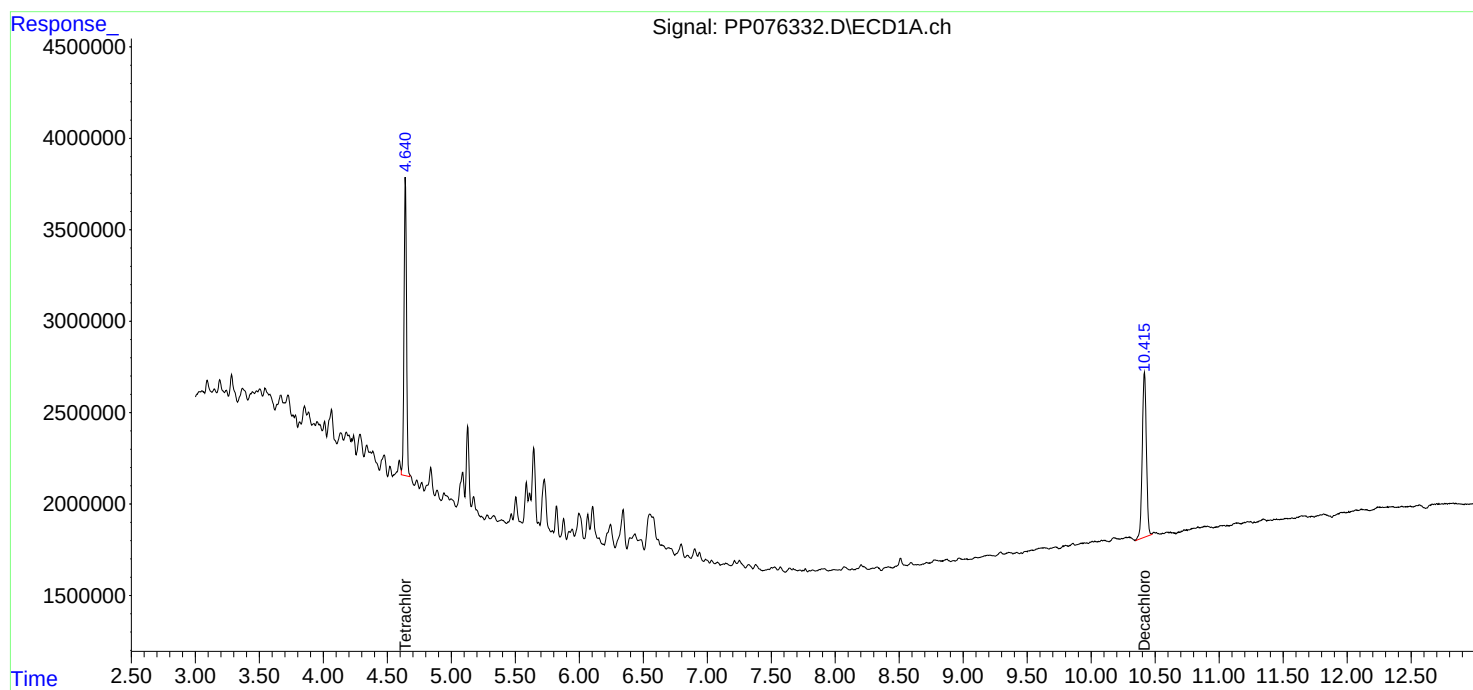

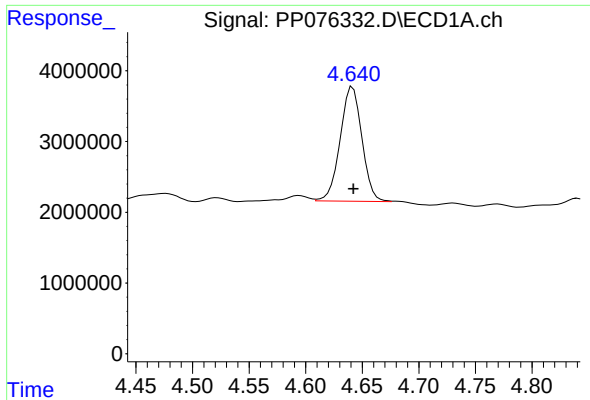


#1 Tetrachloro-m-xylene

R.T.: 4.640 min
Delta R.T.: -0.002 min
Response: 21664565
Conc: 15.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
102825-A


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/06/2025
Supervised By :Yogesh Patel 11/06/2025

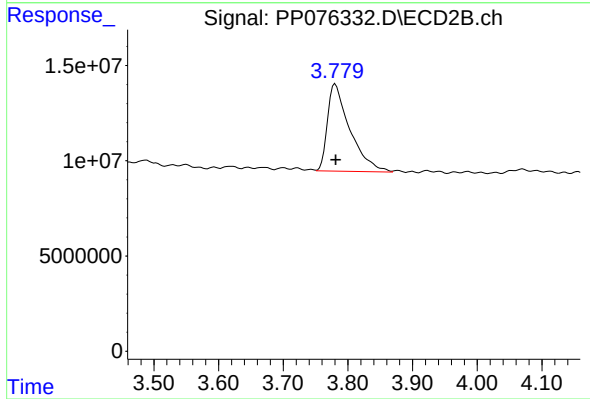


#1 Tetrachloro-m-xylene

R.T.: 3.780 min
Delta R.T.: 0.000 min
Response: 110326567
Conc: 16.67 ng/ml

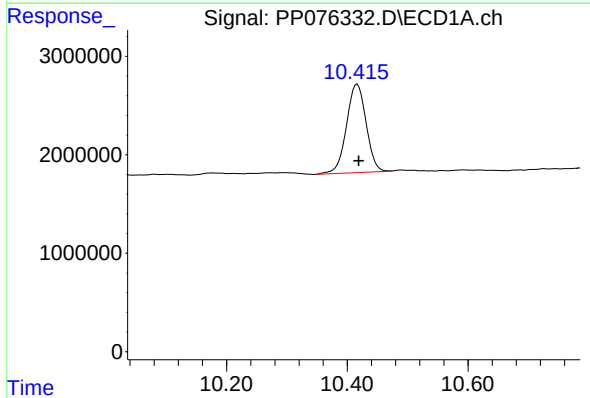

#2 Decachlorobiphenyl

R.T.: 10.416 min
Delta R.T.: -0.002 min
Response: 20308408
Conc: 18.86 ng/ml

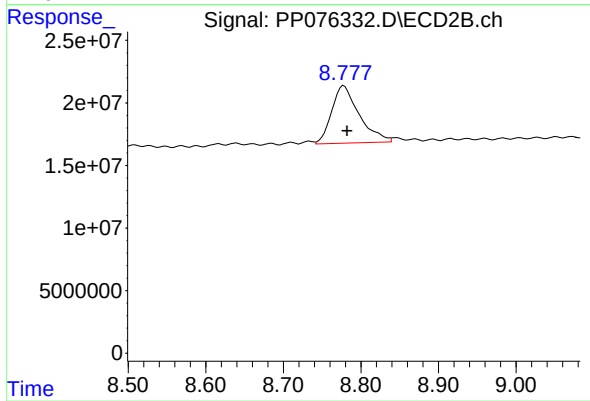

#2 Decachlorobiphenyl

R.T.: 8.778 min
Delta R.T.: -0.004 min
Response: 112949693
Conc: 13.74 ng/ml