

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110525\
 Data File : PP076334.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Nov 2025 14:10
 Operator : YP\AJ
 Sample : Q3522-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 VENT-1

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 11/06/2025
 Supervised By :Yogesh Patel 11/06/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 01:18:04 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 24 15:40:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.641	3.786	20690752	47343856	14.478m	7.153m#
2) SA Decachlor...	10.419	8.782	18487869	110.0E6	17.174	13.382

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110525\
Data File : PP076334.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Nov 2025 14:10
Operator : YP\AJ
Sample : Q3522-03
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
VENT-1


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/06/2025
Supervised By :Yogesh Patel 11/06/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 01:18:04 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 24 15:40:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

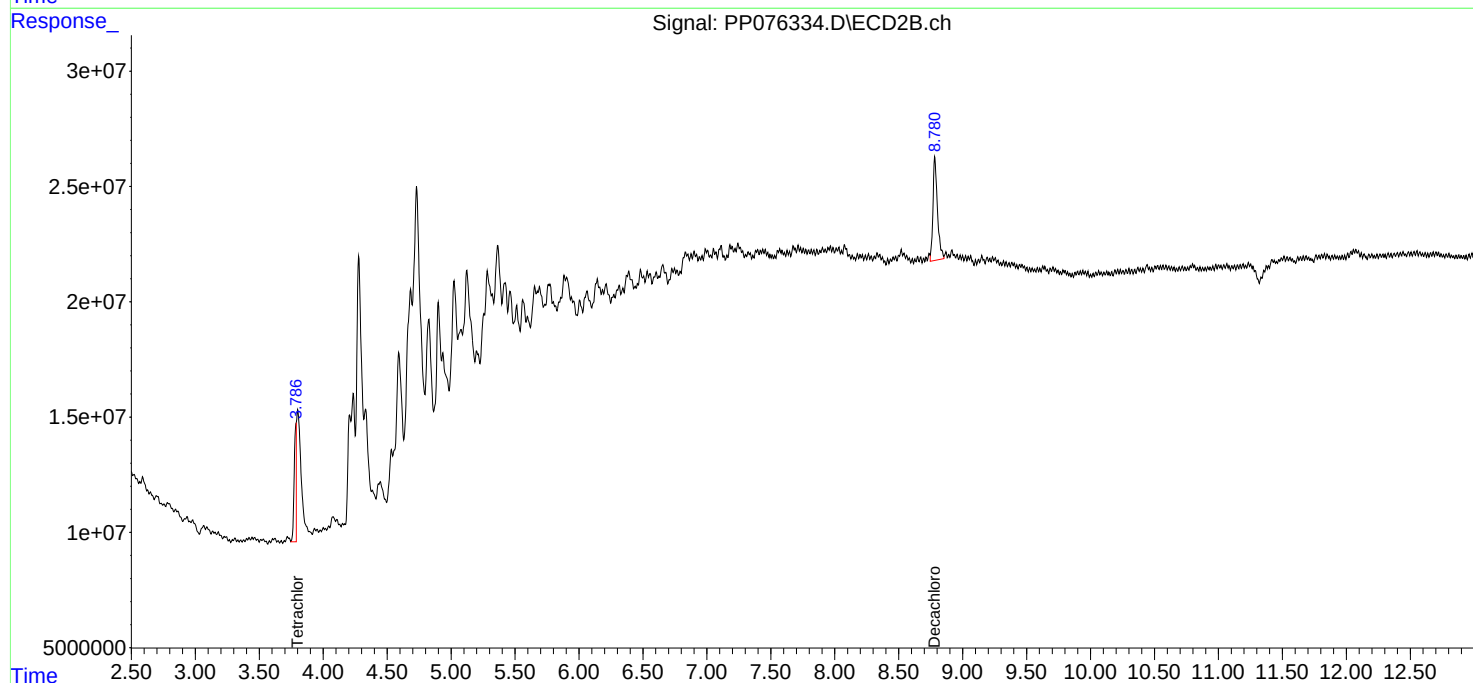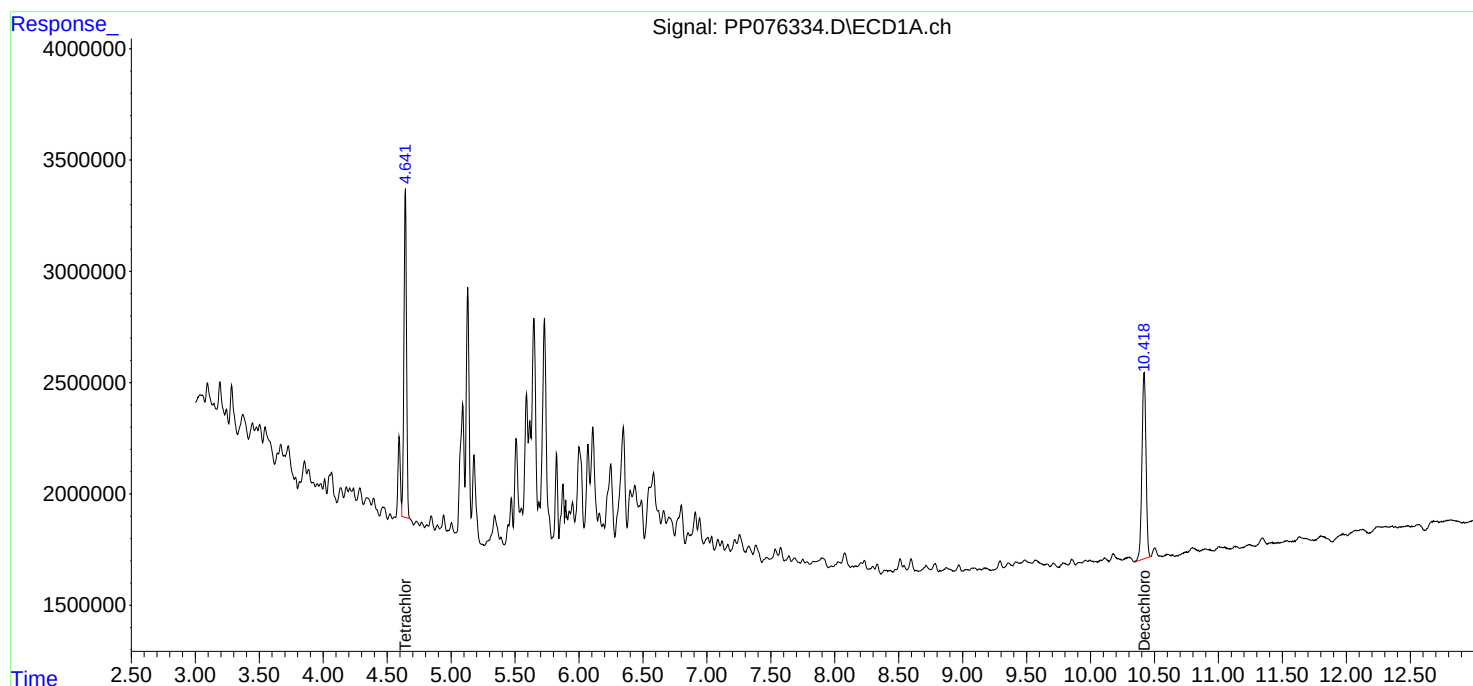

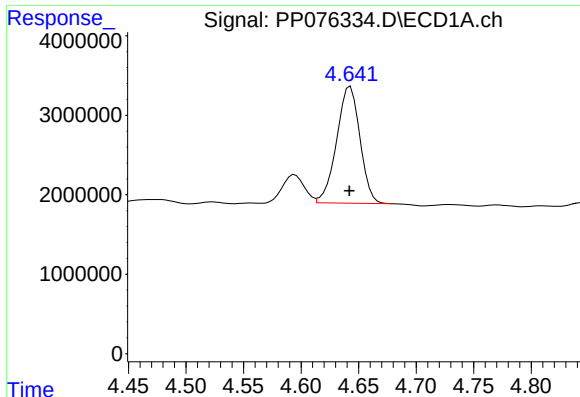


#1 Tetrachloro-m-xylene

R.T.: 4.641 min
Delta R.T.: 0.000 min
Response: 20690752
Conc: 14.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
VENT-1


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/06/2025
Supervised By :Yogesh Patel 11/06/2025

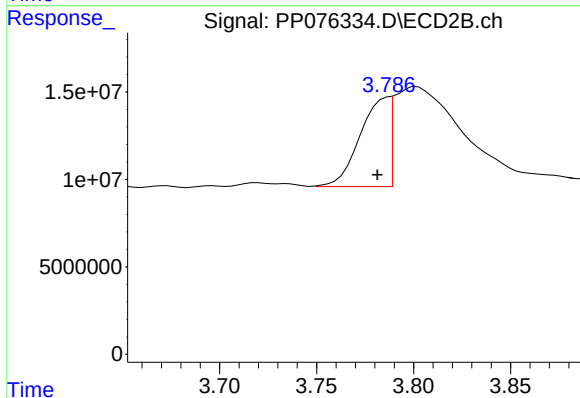


#1 Tetrachloro-m-xylene

R.T.: 3.786 min
Delta R.T.: 0.005 min
Response: 47343856
Conc: 7.15 ng/ml m

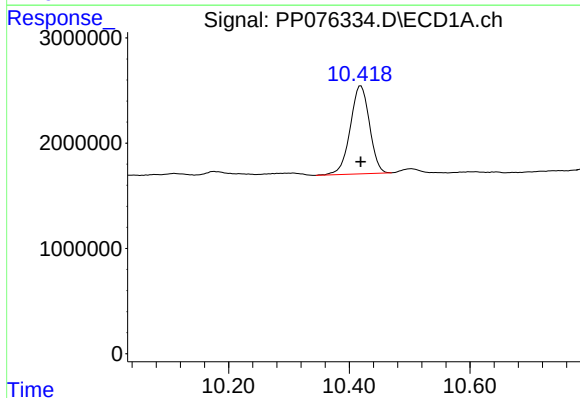

#2 Decachlorobiphenyl

R.T.: 10.419 min
Delta R.T.: 0.000 min
Response: 18487869
Conc: 17.17 ng/ml

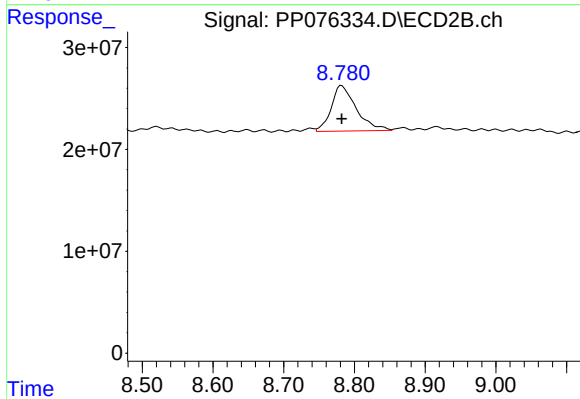

#2 Decachlorobiphenyl

R.T.: 8.782 min
Delta R.T.: 0.000 min
Response: 110041183
Conc: 13.38 ng/ml