

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110620\
 Data File : PP031189.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Nov 2020 12:48
 Operator : DD\AJ
 Sample : L4547-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TT-033-IDWSO-20201027

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 01:36:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 05 13:03:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.802	4.073	992807	953223	14.864	14.341
2) SA Decachlor...	10.683	9.396	460167	506554	11.509	12.131

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110620\
Data File : PP031189.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Nov 2020 12:48
Operator : DD\AJ
Sample : L4547-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
TT-033-IDWSO-20201027

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 01:36:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110420.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 05 13:03:18 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

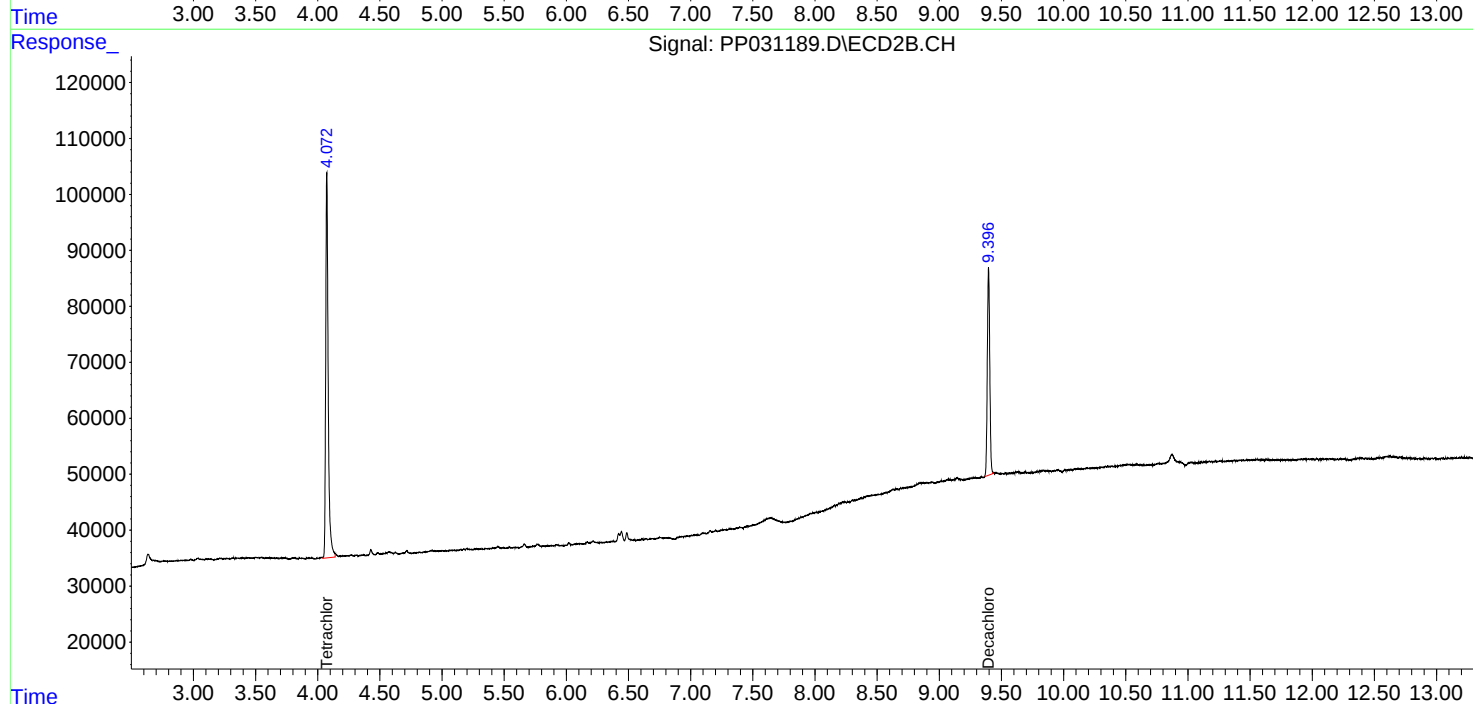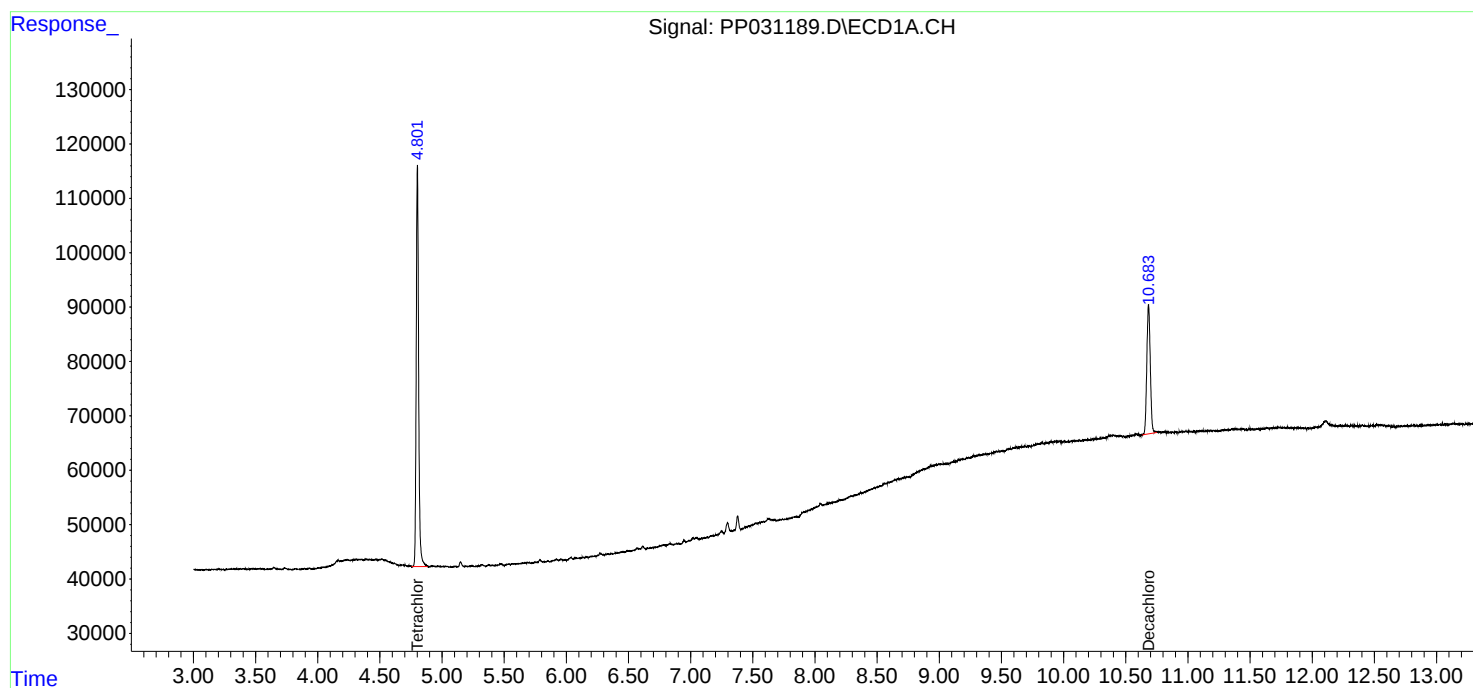


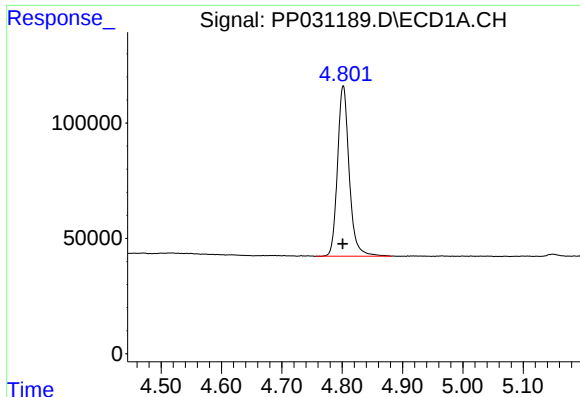

#1 Tetrachloro-m-xylene


R.T.: 4.802 min
Delta R.T.: 0.000 min
Response: 992807
Conc: 14.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
TT-033-IDWSO-20201027

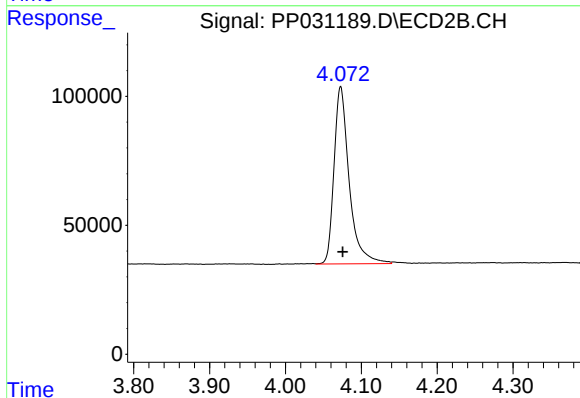


#1 Tetrachloro-m-xylene

R.T.: 4.073 min
Delta R.T.: -0.003 min
Response: 953223
Conc: 14.34 ng/ml

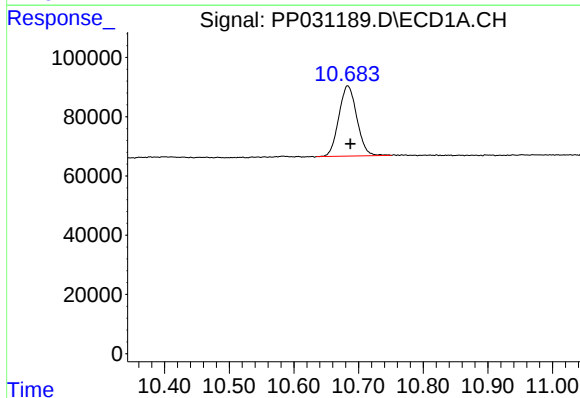

#2 Decachlorobiphenyl

R.T.: 10.683 min
Delta R.T.: -0.004 min
Response: 460167
Conc: 11.51 ng/ml

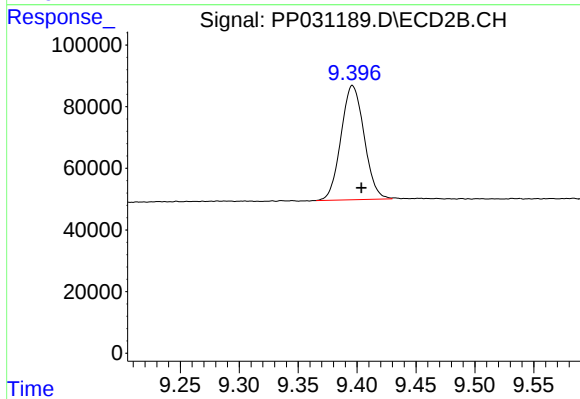

#2 Decachlorobiphenyl

R.T.: 9.396 min
Delta R.T.: -0.008 min
Response: 506554
Conc: 12.13 ng/ml