

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110623\
 Data File : PP061464.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2023 18:39
 Operator : YP\AJ
 Sample : 05257-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 WC-6

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/07/2023
 Supervised By :Ankita Jodhani 11/07/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 23:16:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 27 18:44:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.569	3.701	37604292	27282333	15.223	18.255
2) SA Decachlor...	10.556	8.774	16151904	15196315	8.565	9.895m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110623\
Data File : PP061464.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2023 18:39
Operator : YP\AJ
Sample : 05257-01
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
WC-6


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/07/2023
Supervised By :Ankita Jodhani 11/07/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 23:16:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102723.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 27 18:44:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

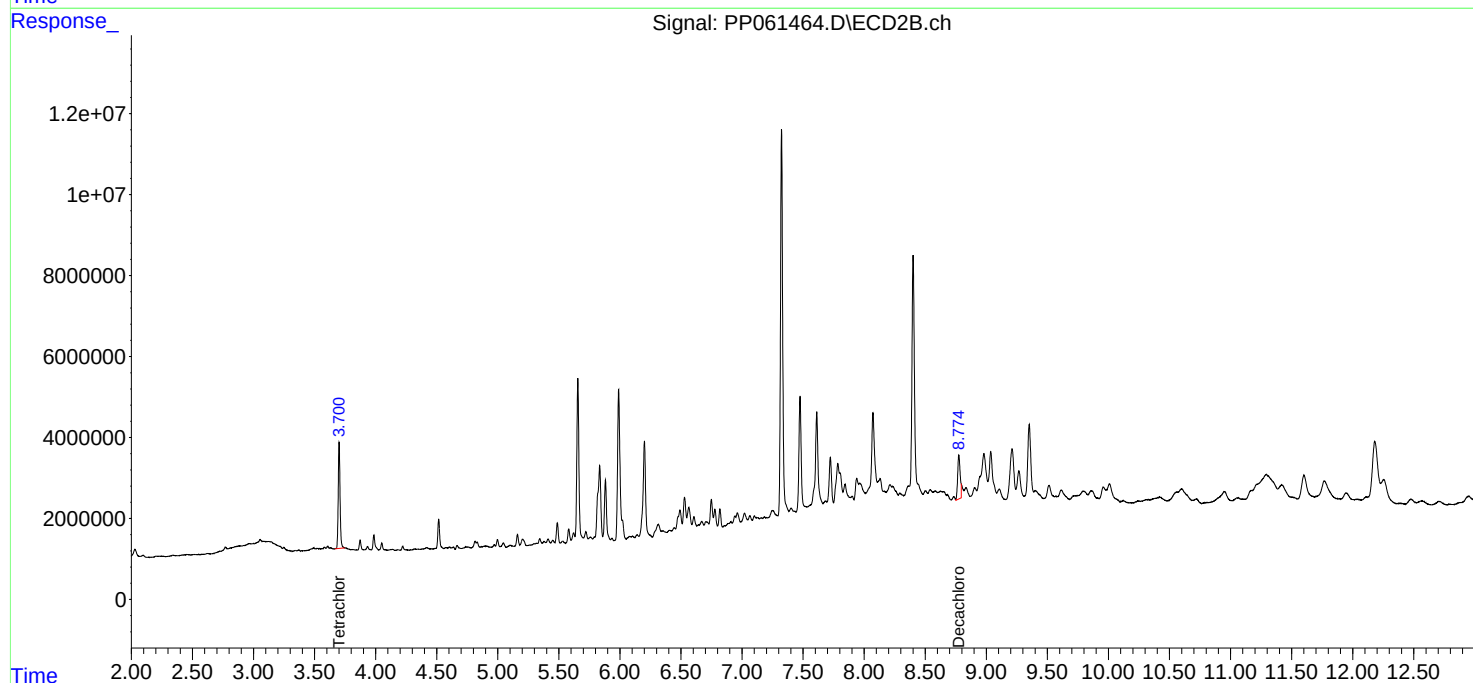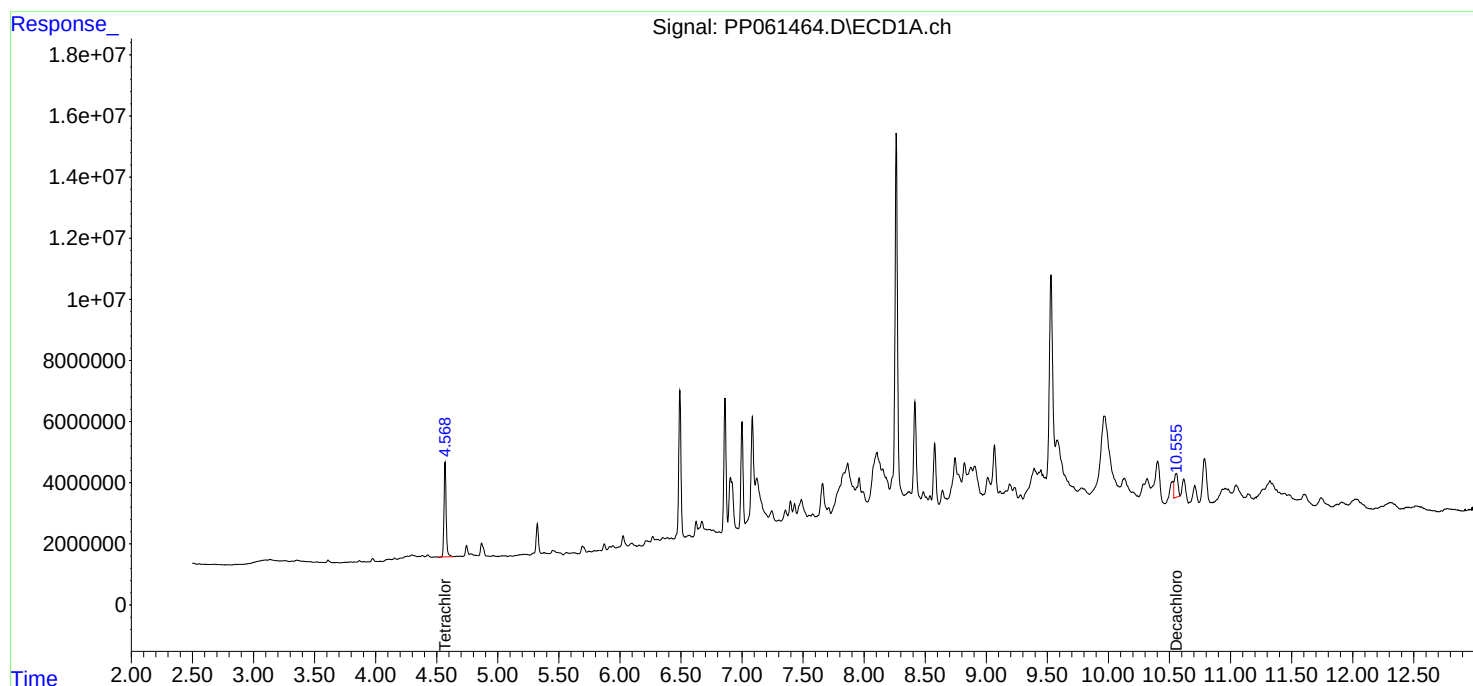

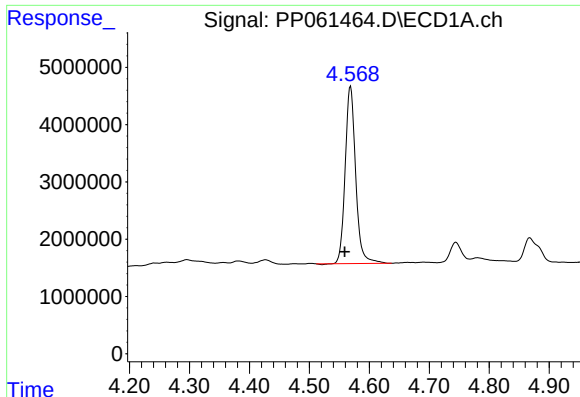


#1 Tetrachloro-m-xylene

R.T.: 4.569 min
Delta R.T.: 0.010 min
Response: 37604292
Conc: 15.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
WC-6


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/07/2023
Supervised By :Ankita Jodhani 11/07/2023

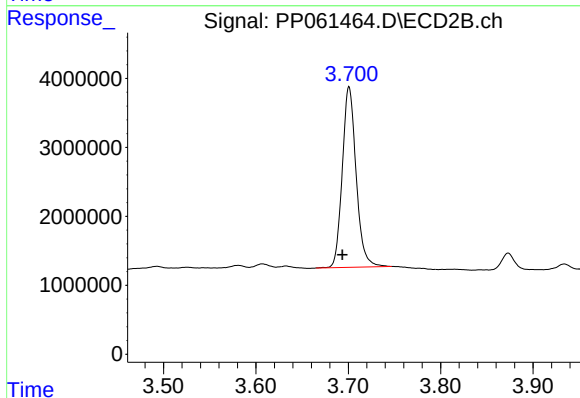


#1 Tetrachloro-m-xylene

R.T.: 3.701 min
Delta R.T.: 0.007 min
Response: 27282333
Conc: 18.26 ng/ml

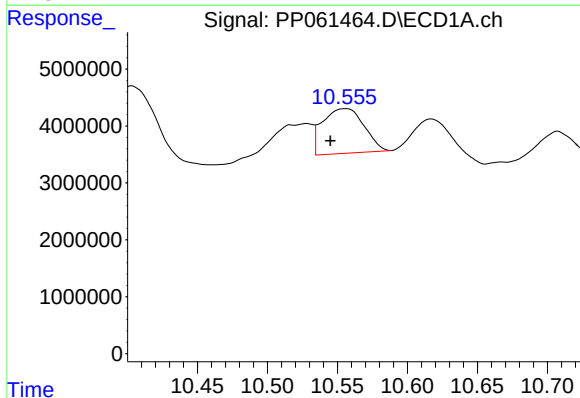

#2 Decachlorobiphenyl

R.T.: 10.556 min
Delta R.T.: 0.011 min
Response: 16151904
Conc: 8.57 ng/ml

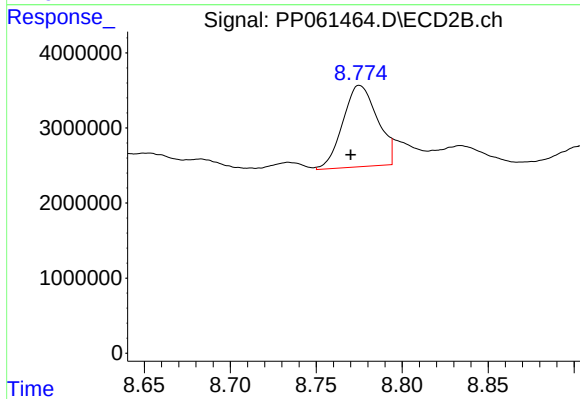

#2 Decachlorobiphenyl

R.T.: 8.774 min
Delta R.T.: 0.004 min
Response: 15196315
Conc: 9.90 ng/ml m