

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110623\
 Data File : PP061492.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2023 02:37
 Operator : YP\AJ
 Sample : 05258-19
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 19-A-19-B-19-C

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/07/2023
 Supervised By :Ankita Jodhani 11/07/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 06:29:05 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 27 18:44:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.569	3.701	50653675	33024457	20.506	22.097
2) SA Decachlor...	10.560	8.777	35483856	24320302	18.817m	15.837

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110623\
Data File : PP061492.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2023 02:37
Operator : YP\AJ
Sample : 05258-19
Misc :
ALS Vial : 44 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
19-A-19-B-19-C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/07/2023
Supervised By :Ankita Jodhani 11/07/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 06:29:05 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102723.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 27 18:44:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

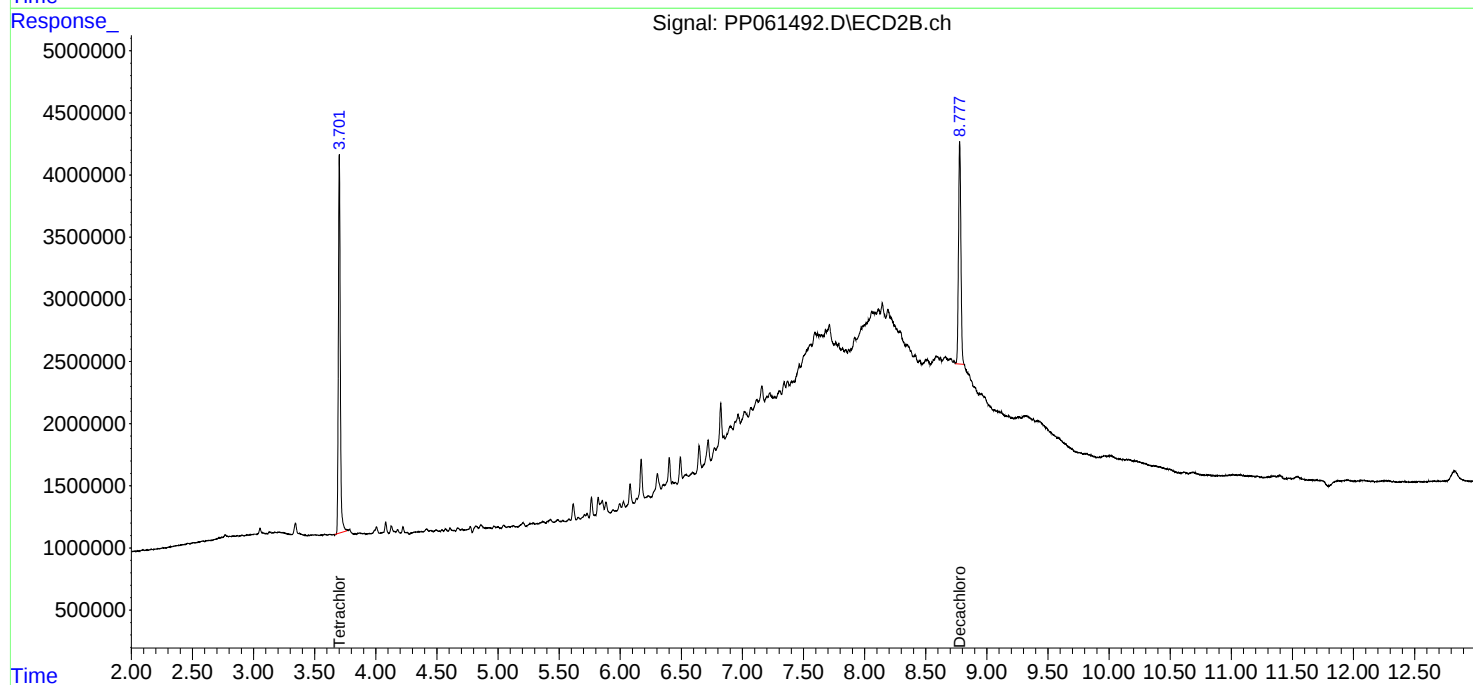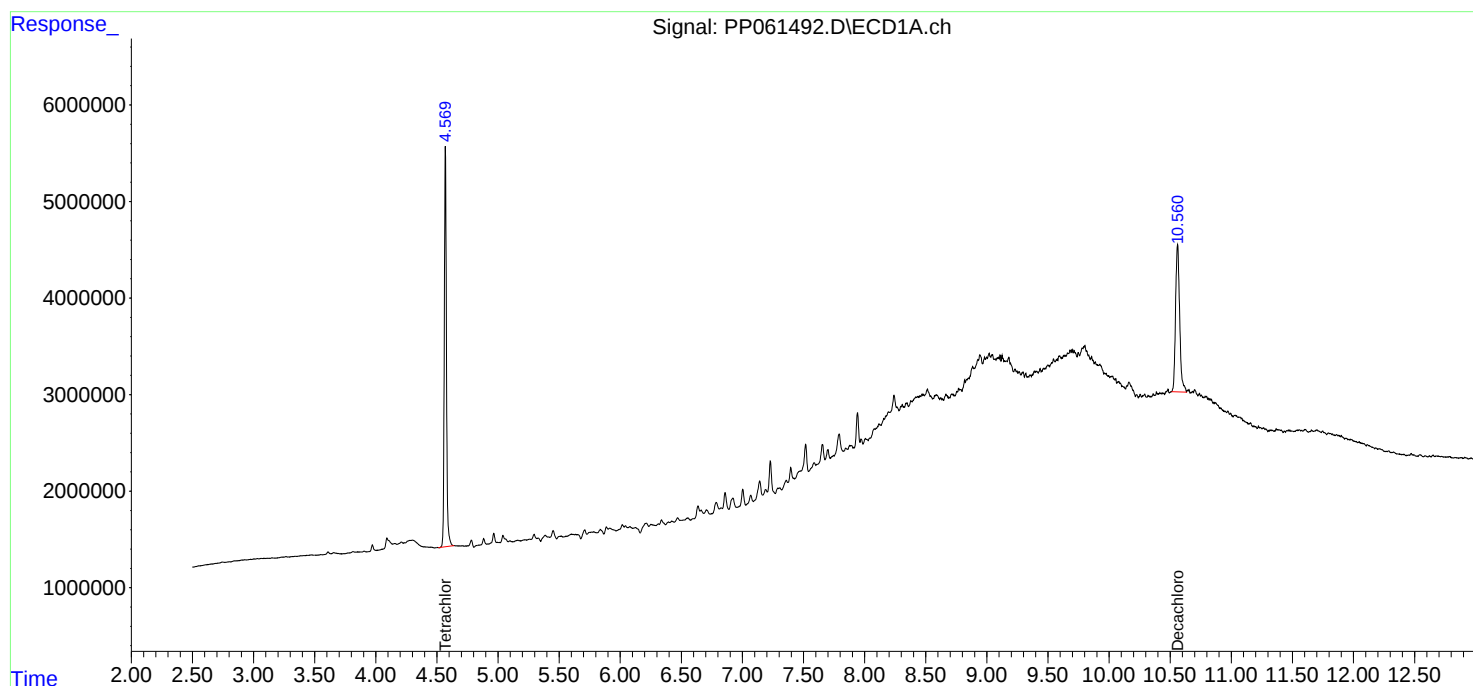

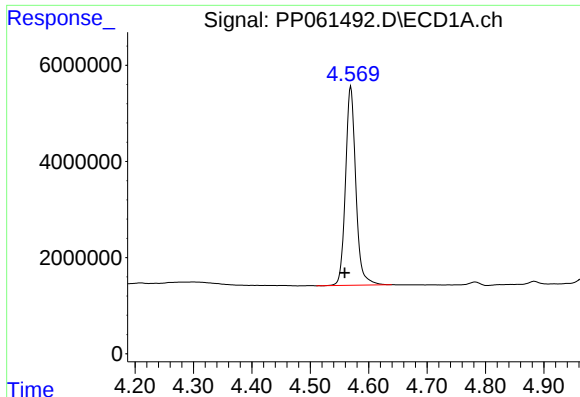


#1 Tetrachloro-m-xylene

R.T.: 4.569 min
Delta R.T.: 0.010 min
Response: 50653675
Conc: 20.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
19-A-19-B-19-C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/07/2023
Supervised By :Ankita Jodhani 11/07/2023

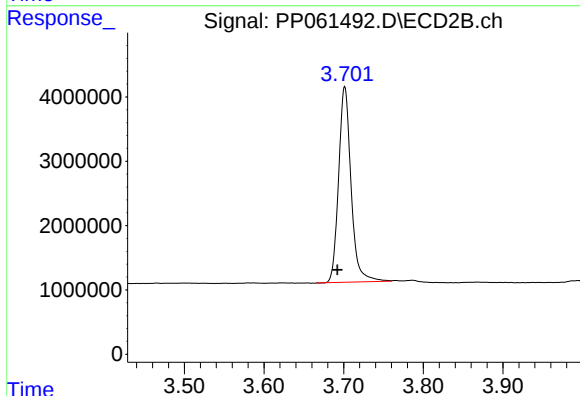


#1 Tetrachloro-m-xylene

R.T.: 3.701 min
Delta R.T.: 0.009 min
Response: 33024457
Conc: 22.10 ng/ml

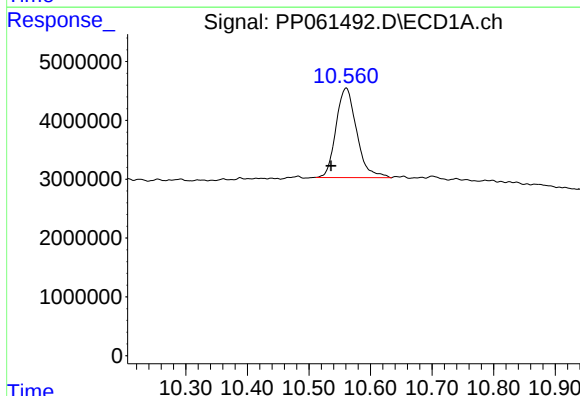

#2 Decachlorobiphenyl

R.T.: 10.560 min
Delta R.T.: 0.024 min
Response: 35483856
Conc: 18.82 ng/ml m

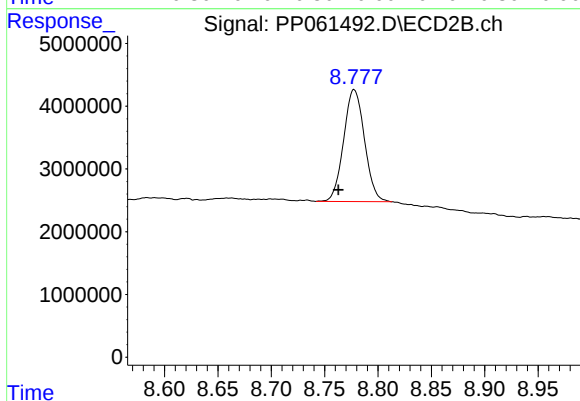

#2 Decachlorobiphenyl

R.T.: 8.777 min
Delta R.T.: 0.014 min
Response: 24320302
Conc: 15.84 ng/ml