

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110625\
 Data File : PP076358.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2025 15:39
 Operator : YP\AJ
 Sample : Q3534-10
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 EB-1

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 11/07/2025
 Supervised By :Yogesh Patel 11/07/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 00:26:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 24 15:40:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.639	3.777	46611336	194.5E6	32.616	29.389m
2) SA Decachlor...	10.407	8.774	28325713	192.2E6	26.312	23.372

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110625\
Data File : PP076358.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2025 15:39
Operator : YP\AJ
Sample : Q3534-10
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
EB-1


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/07/2025
Supervised By :Yogesh Patel 11/07/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 00:26:11 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 24 15:40:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

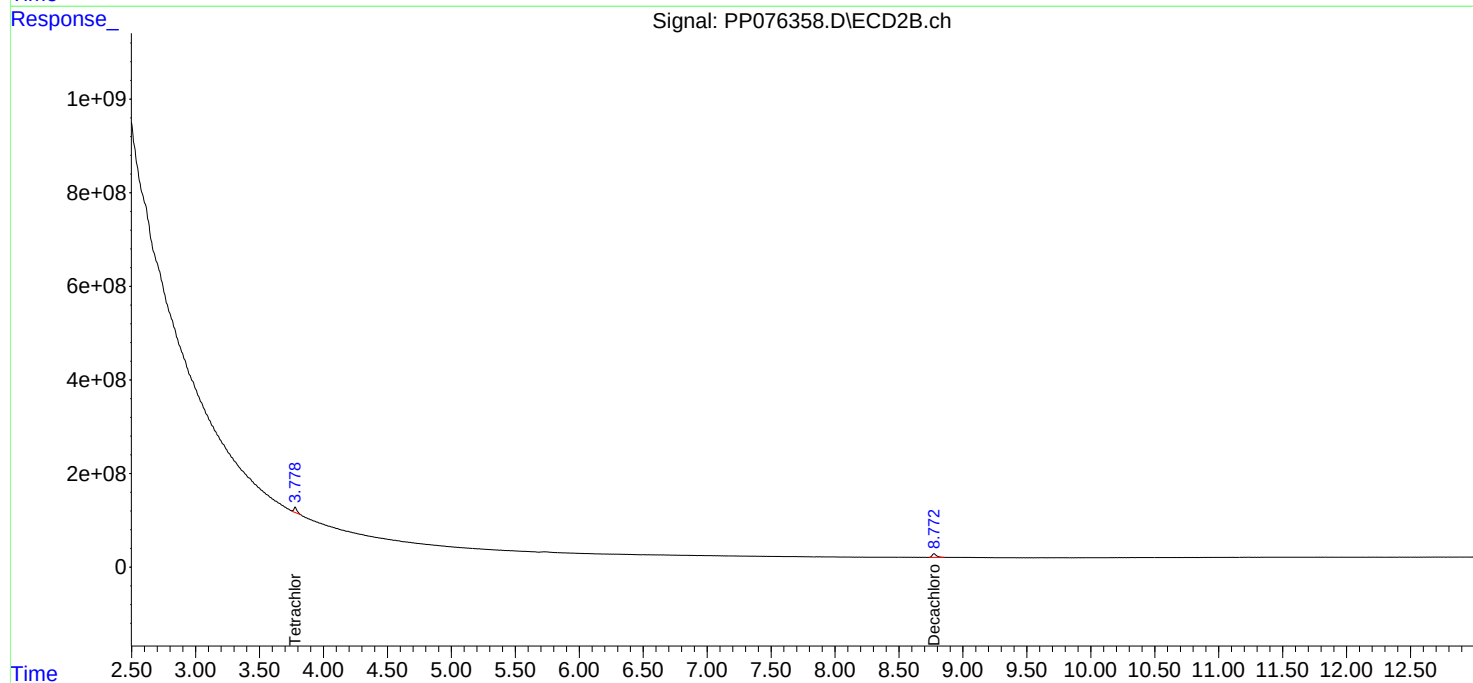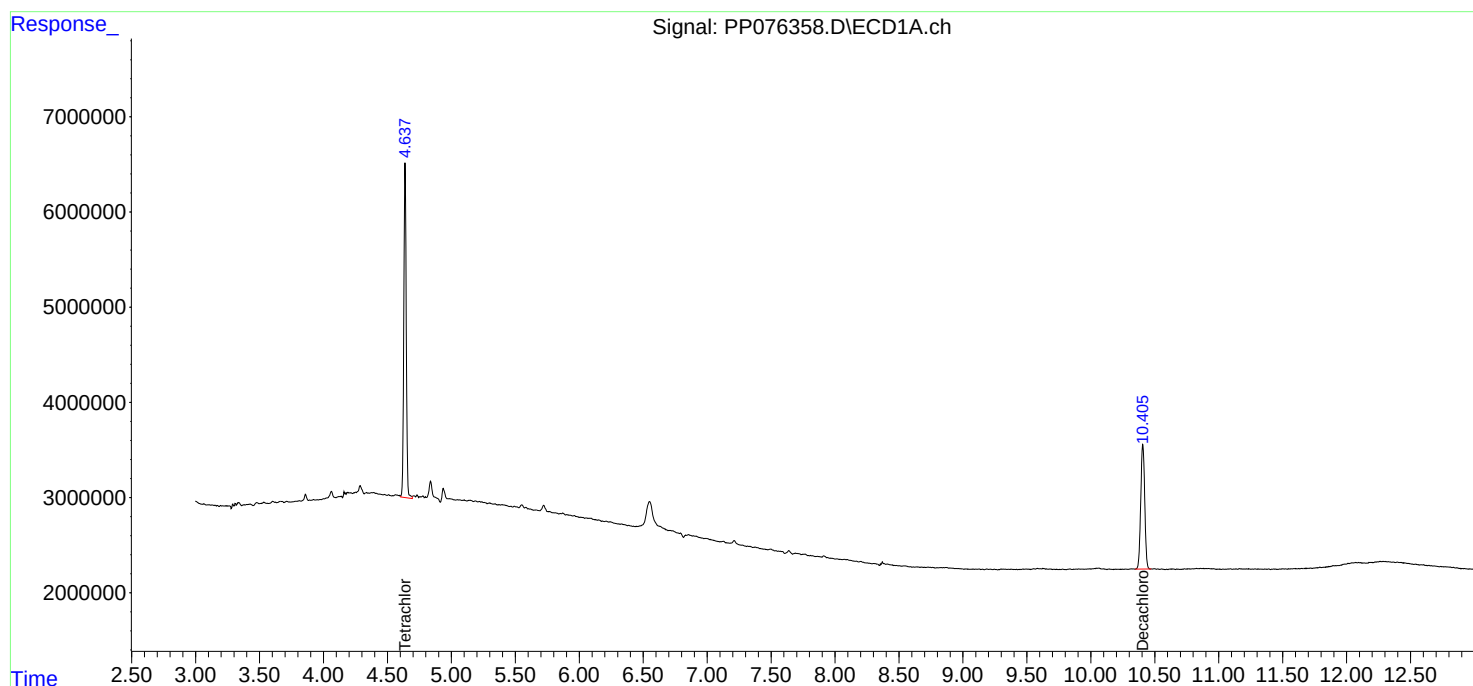

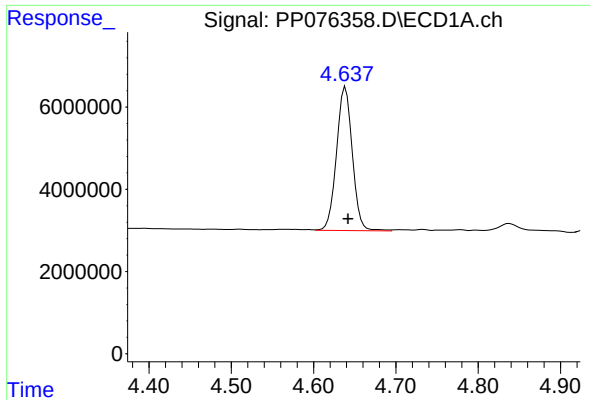


#1 Tetrachloro-m-xylene

R.T.: 4.639 min
Delta R.T.: -0.003 min
Response: 46611336
Conc: 32.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
EB-1


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/07/2025
Supervised By :Yogesh Patel 11/07/2025

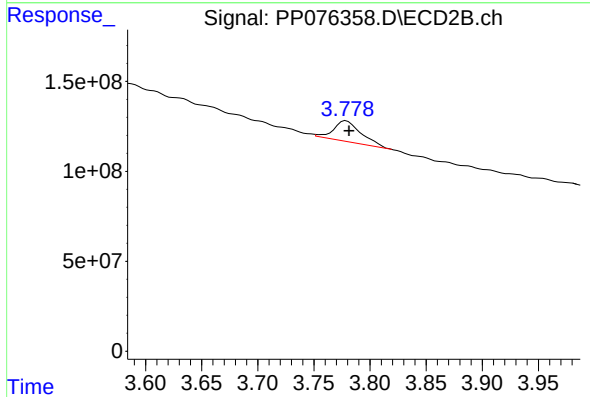


#1 Tetrachloro-m-xylene

R.T.: 3.777 min
Delta R.T.: -0.004 min
Response: 194503954
Conc: 29.39 ng/ml m

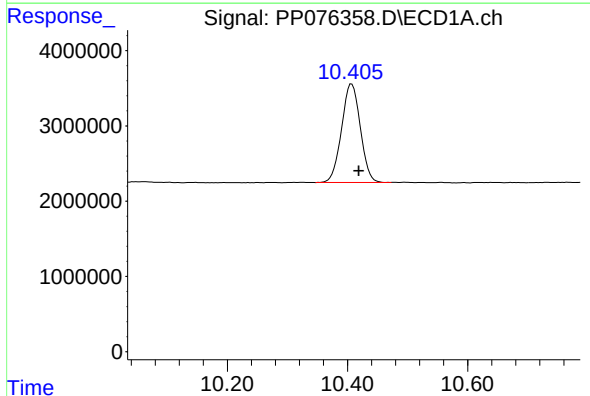

#2 Decachlorobiphenyl

R.T.: 10.407 min
Delta R.T.: -0.012 min
Response: 28325713
Conc: 26.31 ng/ml

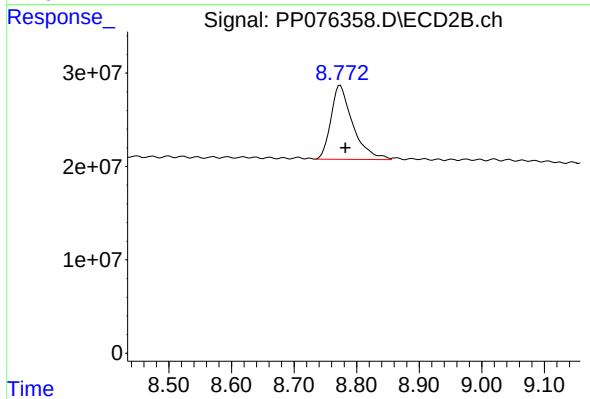

#2 Decachlorobiphenyl

R.T.: 8.774 min
Delta R.T.: -0.008 min
Response: 192188491
Conc: 23.37 ng/ml