

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110723\
 Data File : PP061523.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2023 21:26
 Operator : YP\AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1254ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/09/2023
 Supervised By :Ankita Jodhani 11/09/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 04:48:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 08 04:44:44 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.576	3.706	11288422	8064051	4.355	5.010m
2)	SA Decachlor...	10.579	8.789	9371963	7554456	4.713	5.008
Target Compounds							
26)	L6 AR-1254-1	6.645	5.624	4521249	4017642	52.151	51.275
27)	L6 AR-1254-2	6.867	5.773	7022905	3551334	51.701	51.436
28)	L6 AR-1254-3	7.239	6.180	7598278	5586468	54.068	49.203
29)	L6 AR-1254-4	7.528	6.411	5585404	3354820	55.184	48.250
30)	L6 AR-1254-5	7.952	6.831	5209746	4889390	46.379	45.797

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110723\
Data File : PP061523.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2023 21:26
Operator : YP\AJ
Sample : AR1254ICC050
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/09/2023
Supervised By :Ankita Jodhani 11/09/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 04:48:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110723.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 08 04:44:44 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

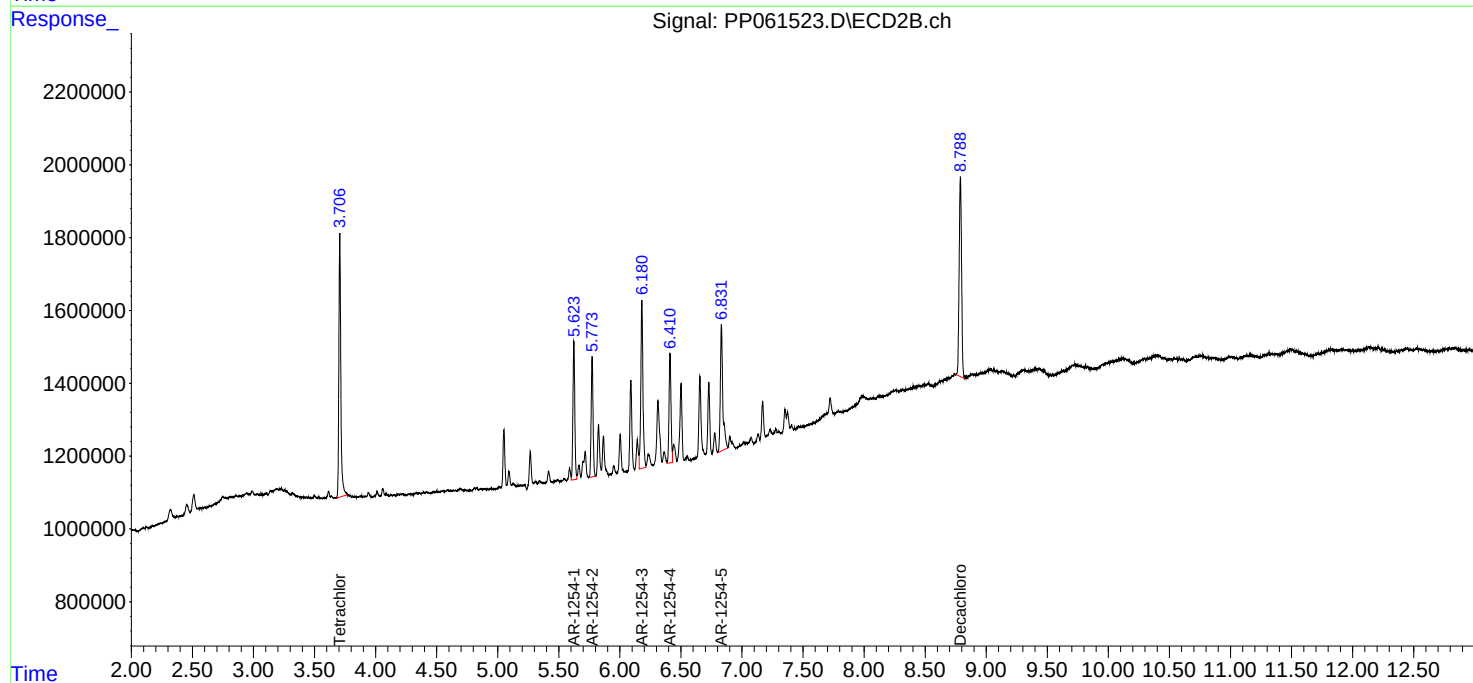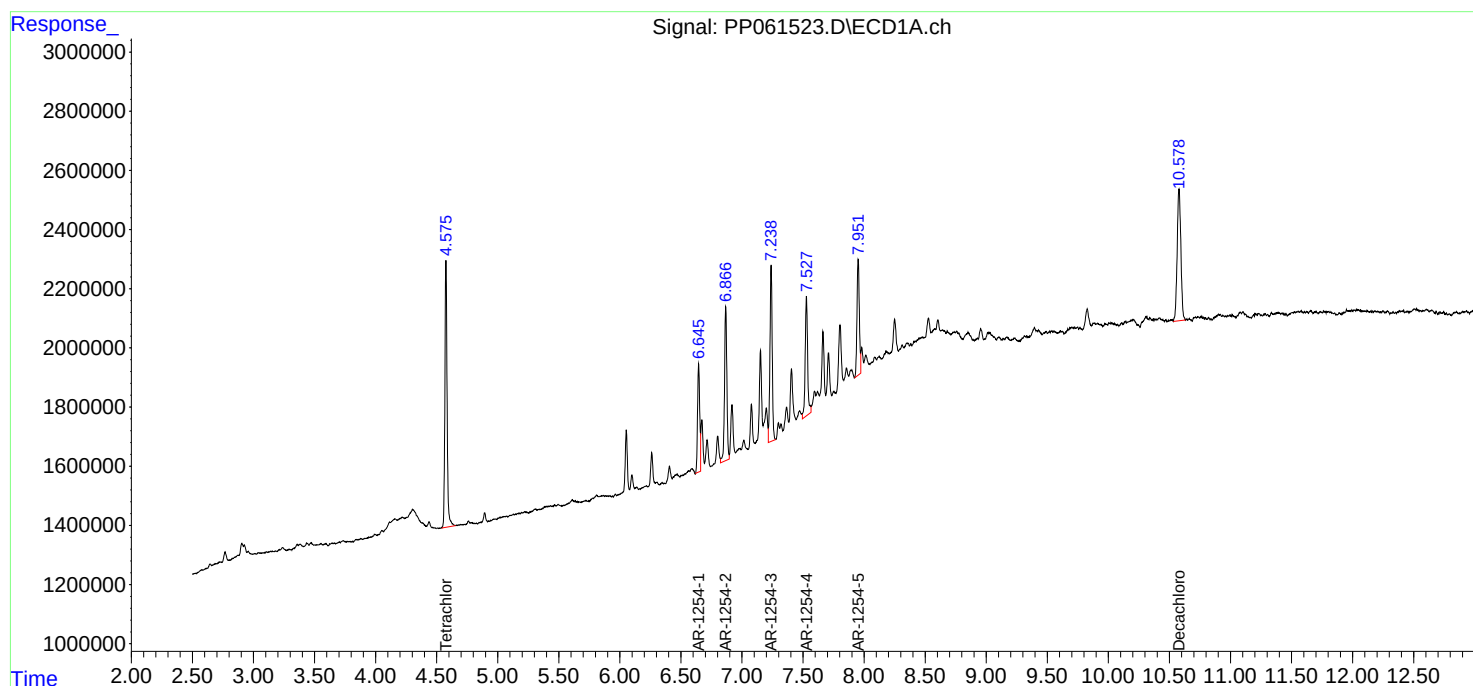

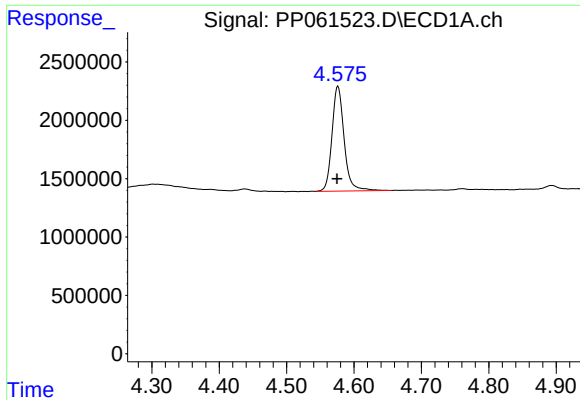


#1 Tetrachloro-m-xylene

R.T.: 4.576 min
Delta R.T.: 0.001 min
Response: 11288422
Conc: 4.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/09/2023
Supervised By :Ankita Jodhani 11/09/2023

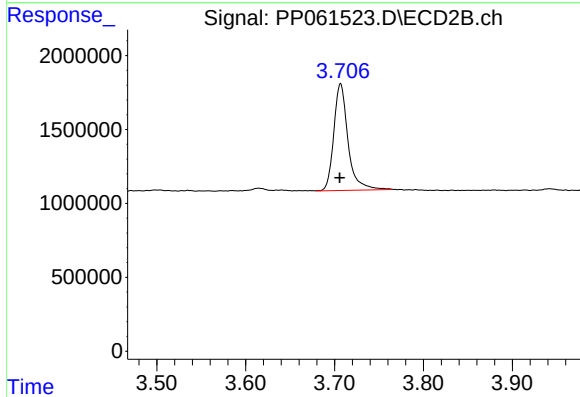


#1 Tetrachloro-m-xylene

R.T.: 3.706 min
Delta R.T.: 0.000 min
Response: 8064051
Conc: 5.01 ng/ml m

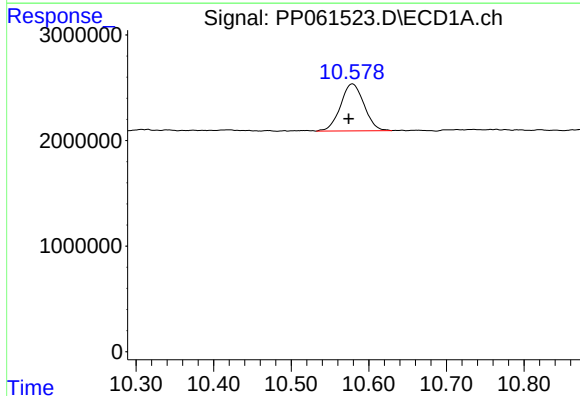


#2 Decachlorobiphenyl

R.T.: 10.579 min
Delta R.T.: 0.005 min
Response: 9371963
Conc: 4.71 ng/ml

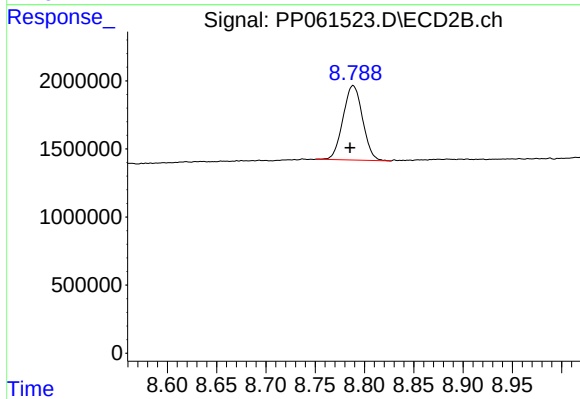

#2 Decachlorobiphenyl

R.T.: 8.789 min
Delta R.T.: 0.003 min
Response: 7554456
Conc: 5.01 ng/ml

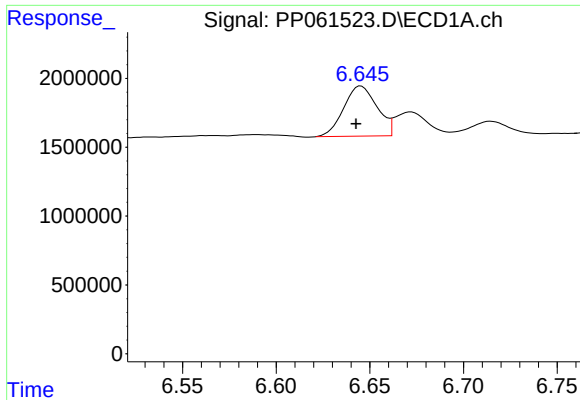


#26 AR-1254-1

R.T.: 6.645 min
Delta R.T.: 0.003 min
Response: 4521249
Conc: 52.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/09/2023
Supervised By :Ankita Jodhani 11/09/2023

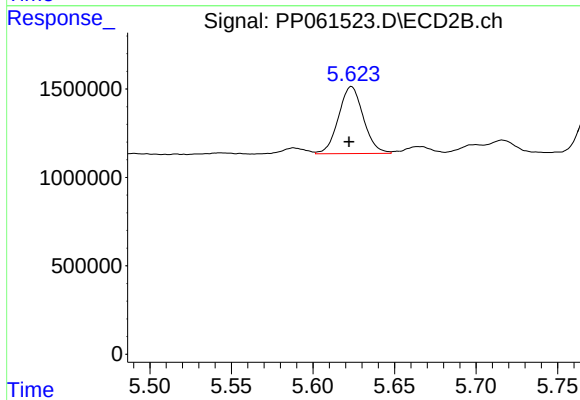


#26 AR-1254-1

R.T.: 5.624 min
Delta R.T.: 0.002 min
Response: 4017642
Conc: 51.28 ng/ml

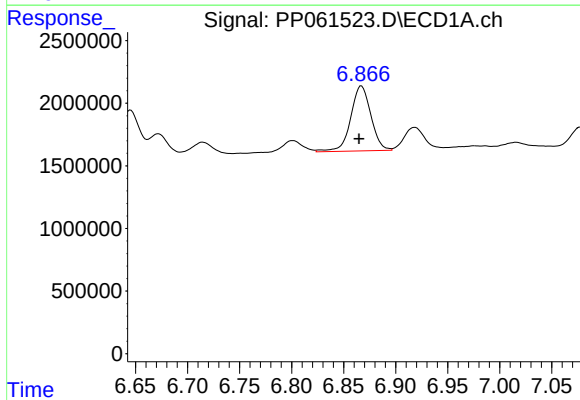


#27 AR-1254-2

R.T.: 6.867 min
Delta R.T.: 0.002 min
Response: 7022905
Conc: 51.70 ng/ml

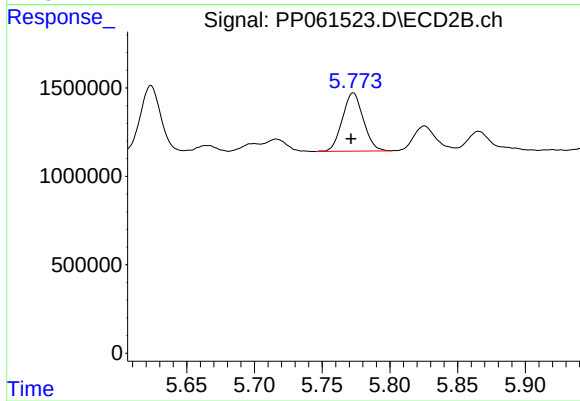

#27 AR-1254-2

R.T.: 5.773 min
Delta R.T.: 0.002 min
Response: 3551334
Conc: 51.44 ng/ml

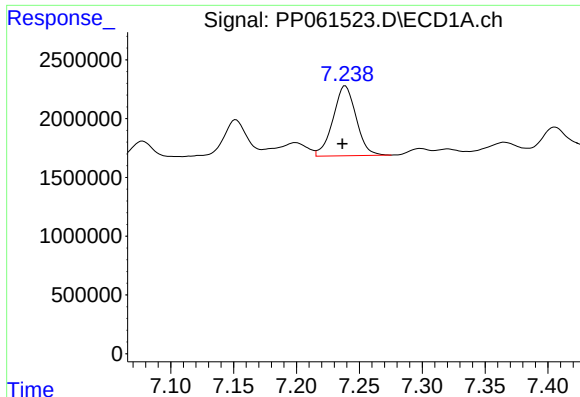


#28 AR-1254-3

R.T.: 7.239 min
Delta R.T.: 0.002 min
Response: 7598278
Conc: 54.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/09/2023
Supervised By :Ankita Jodhani 11/09/2023

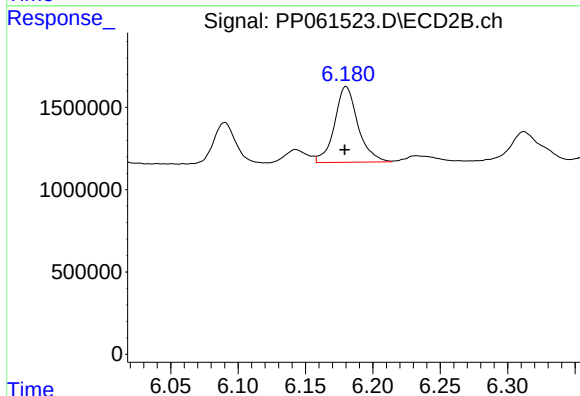


#28 AR-1254-3

R.T.: 6.180 min
Delta R.T.: 0.000 min
Response: 5586468
Conc: 49.20 ng/ml

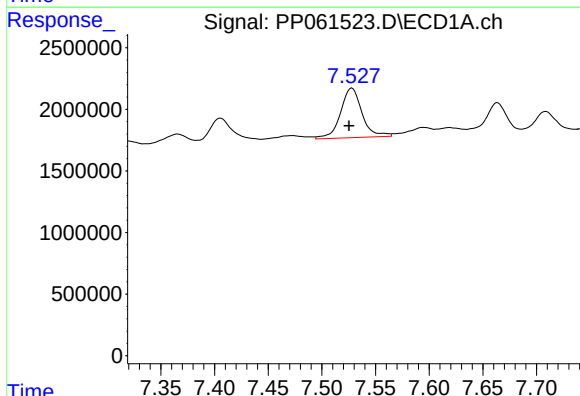


#29 AR-1254-4

R.T.: 7.528 min
Delta R.T.: 0.003 min
Response: 5585404
Conc: 55.18 ng/ml

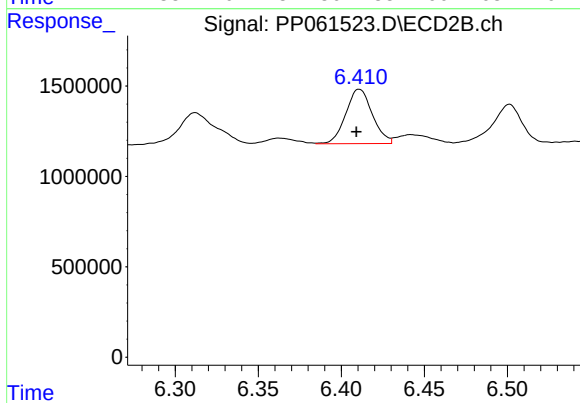

#29 AR-1254-4

R.T.: 6.411 min
Delta R.T.: 0.002 min
Response: 3354820
Conc: 48.25 ng/ml

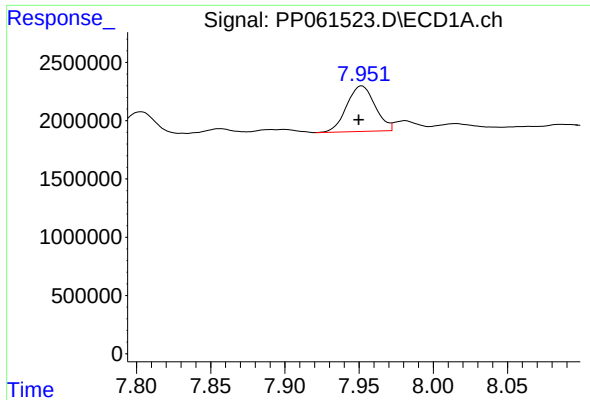


#30 AR-1254-5

R.T.: 7.952 min
Delta R.T.: 0.002 min
Response: 5209746
Conc: 46.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/09/2023
Supervised By :Ankita Jodhani 11/09/2023

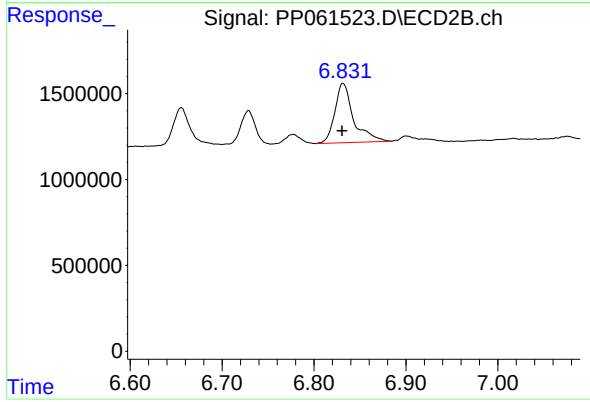

#30 AR-1254-5

R.T.: 6.831 min
Delta R.T.: 0.000 min
Response: 4889390
Conc: 45.80 ng/ml