

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110725\
 Data File : PP076378.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2025 11:09
 Operator : YP\AJ
 Sample : Q3307-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 S-38(6.0-6.5)

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 11/10/2025
 Supervised By :Yogesh Patel 11/10/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 02:56:41 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 24 15:40:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.640	3.781	23131473	64875724	16.186	9.802m#
2) SA Decachlor...	10.408	8.772	22020959	158.0E6	20.456	19.218

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110725\
Data File : PP076378.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2025 11:09
Operator : YP\AJ
Sample : Q3307-07
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
S-38(6.0-6.5)


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/10/2025
Supervised By :Yogesh Patel 11/10/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 02:56:41 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 24 15:40:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

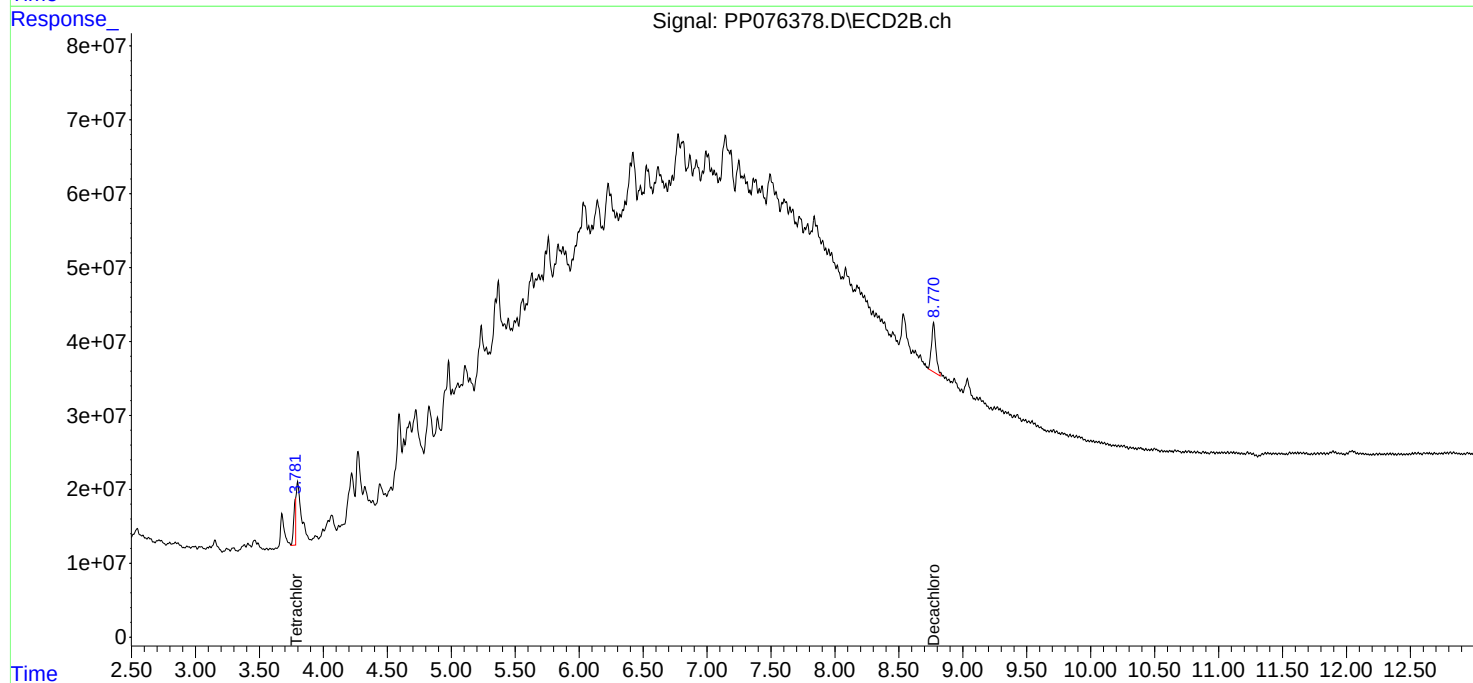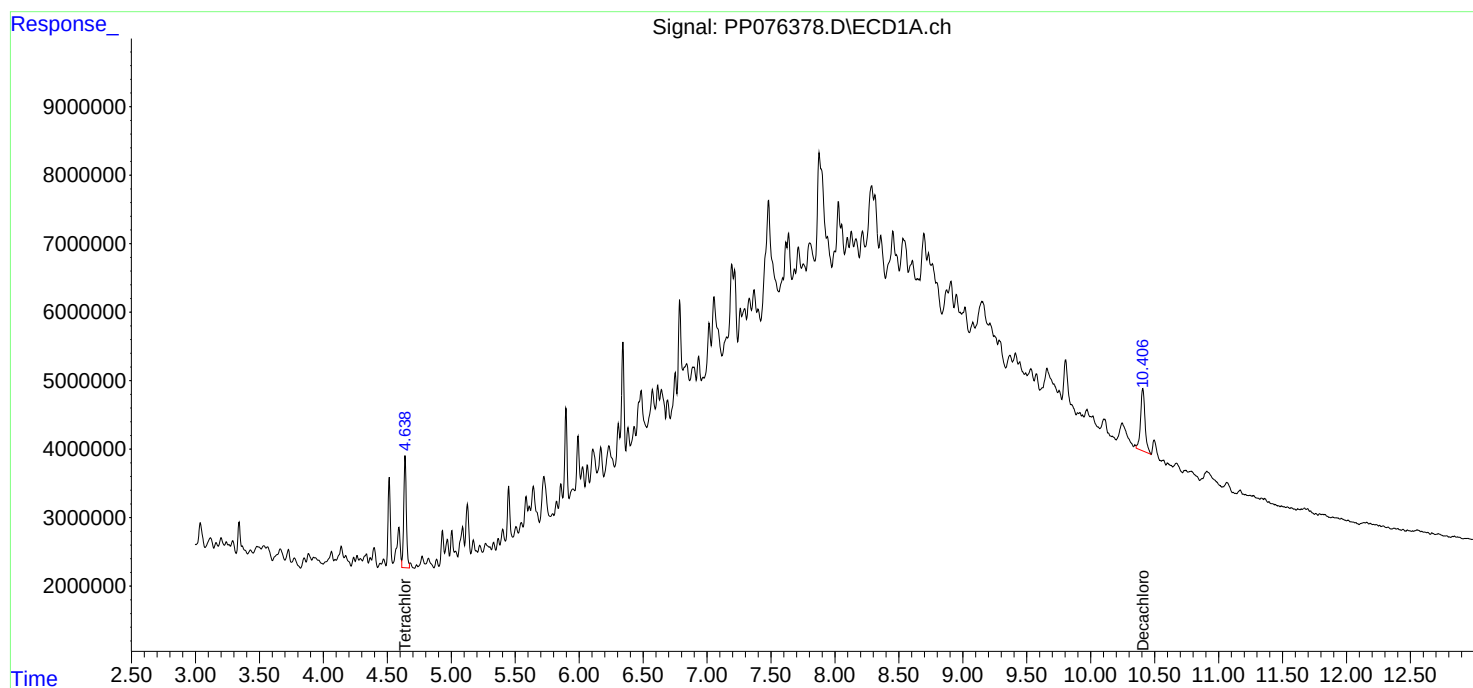

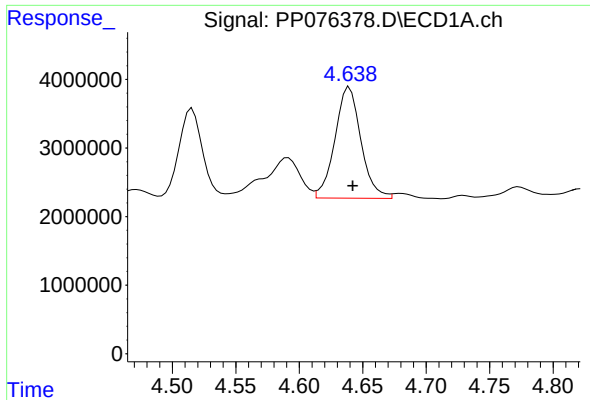


#1 Tetrachloro-m-xylene

R.T.: 4.640 min
Delta R.T.: -0.002 min
Response: 23131473
Conc: 16.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
S-38(6.0-6.5)


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/10/2025
Supervised By :Yogesh Patel 11/10/2025

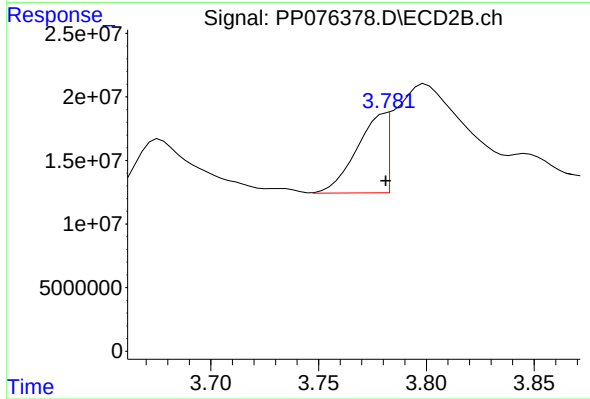


#1 Tetrachloro-m-xylene

R.T.: 3.781 min
Delta R.T.: 0.000 min
Response: 64875724
Conc: 9.80 ng/ml m

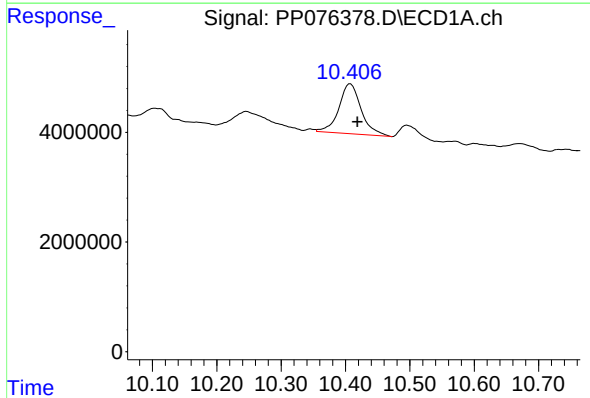

#2 Decachlorobiphenyl

R.T.: 10.408 min
Delta R.T.: -0.011 min
Response: 22020959
Conc: 20.46 ng/ml

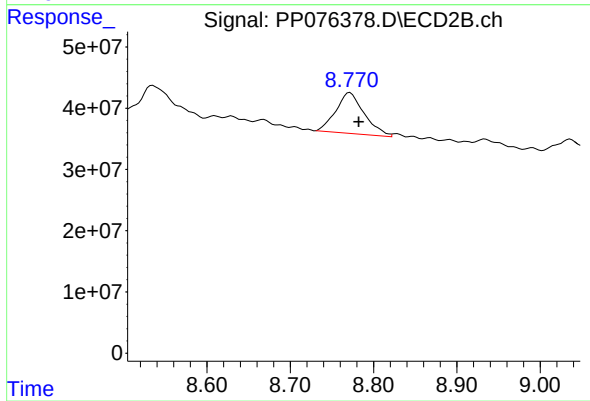

#2 Decachlorobiphenyl

R.T.: 8.772 min
Delta R.T.: -0.010 min
Response: 158026760
Conc: 19.22 ng/ml