

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110725\
 Data File : PP076386.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2025 13:54
 Operator : YP\AJ
 Sample : Q3545-01RE 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PCB-110325KC-01 Hard Doorframe Caulk

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 11/10/2025
 Supervised By :Yogesh Patel 11/10/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 02:59:56 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 24 15:40:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.639	3.774	2564991	6456794	1.795m	0.976m#
2) SA Decachlor...	10.412	8.770	4971422	30710095	4.618	3.735m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110725\
Data File : PP076386.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2025 13:54
Operator : YP\AJ
Sample : Q3545-01RE 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PCB-110325KC-01 Hard Doorframe Caulk


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/10/2025
Supervised By :Yogesh Patel 11/10/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 02:59:56 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 24 15:40:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

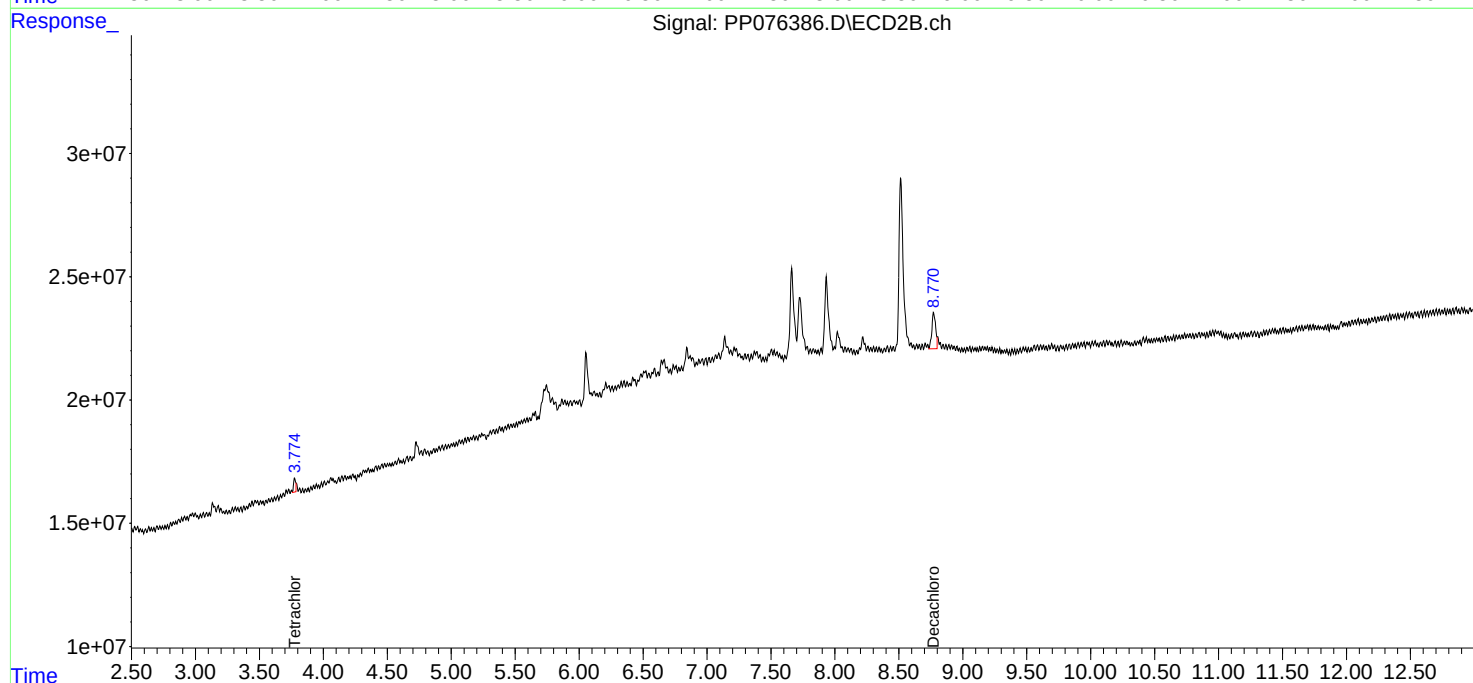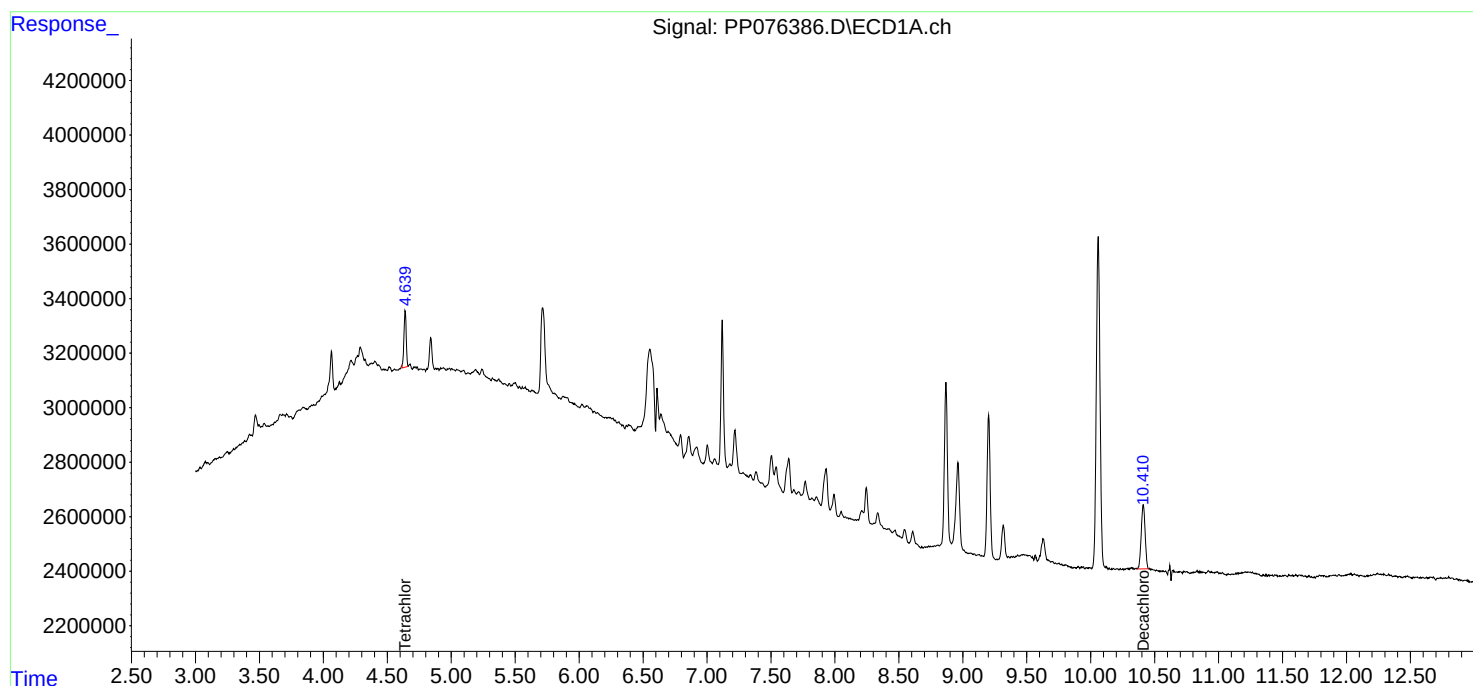

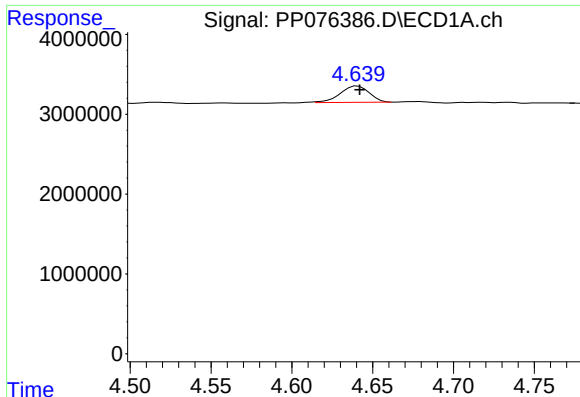


#1 Tetrachloro-m-xylene

R.T.: 4.639 min
Delta R.T.: -0.003 min
Response: 2564991
Conc: 1.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-110325KC-01 Hard Doorframe Caulk


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/10/2025
Supervised By :Yogesh Patel 11/10/2025

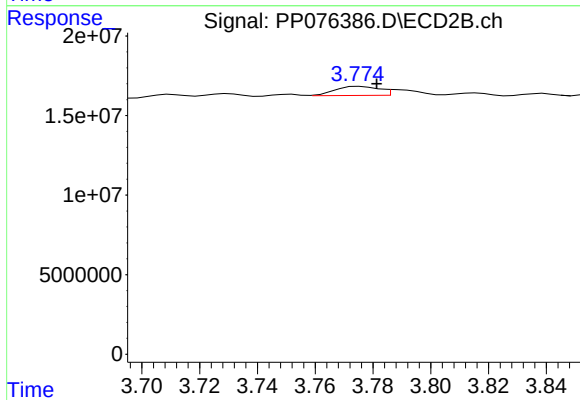


#1 Tetrachloro-m-xylene

R.T.: 3.774 min
Delta R.T.: -0.007 min
Response: 6456794
Conc: 0.98 ng/ml m

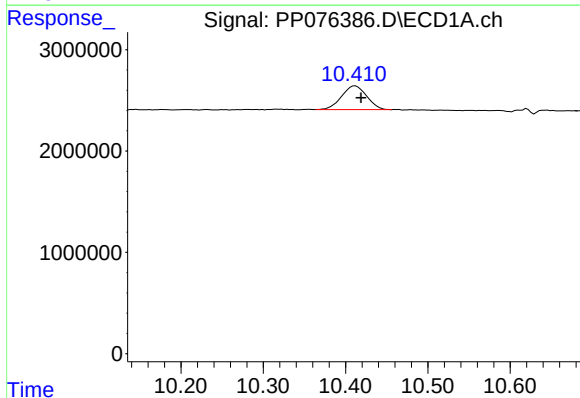

#2 Decachlorobiphenyl

R.T.: 10.412 min
Delta R.T.: -0.007 min
Response: 4971422
Conc: 4.62 ng/ml

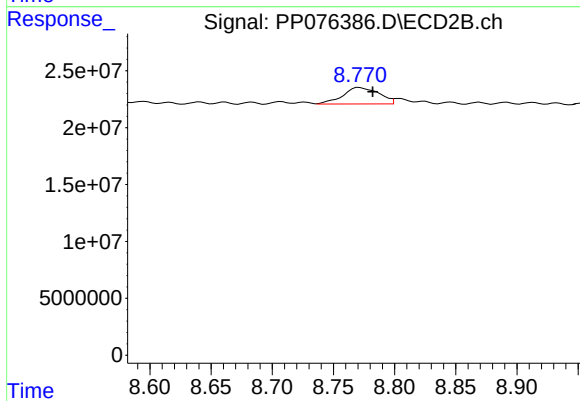

#2 Decachlorobiphenyl

R.T.: 8.770 min
Delta R.T.: -0.012 min
Response: 30710095
Conc: 3.73 ng/ml m