

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110821\
 Data File : PP040770.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Nov 2021 13:40
 Operator : AJ\MA
 Sample : PB140552BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 00:34:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 04 11:28:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.764	3.768	433822	538742	21.414	22.449
2)	SA Decachlor...	10.671	9.037	427638	351809	20.079	20.146
Target Compounds							
28)	L6 AR-1254-3	7.612f	0.000	50314	0	37.373	N.D. #
30)	L6 AR-1254-5	8.329	0.000	5012	0	4.620	N.D. #
31)	L7 AR-1260-1	7.740f	0.000	21258	0	21.892	N.D. #
32)	L7 AR-1260-2	8.052f	0.000	9591	0	8.284	N.D. #
33)	L7 AR-1260-3	8.374f	0.000	2180	0	2.469	N.D. #
35)	L7 AR-1260-5	8.958f	0.000	22023	0	10.547	N.D. #
36)	L8 AR-1262-1	8.374	0.000	2180	0	1.740	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110821\
Data File : PP040770.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Nov 2021 13:40
Operator : AJ\MA
Sample : PB140552BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 00:34:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 04 11:28:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

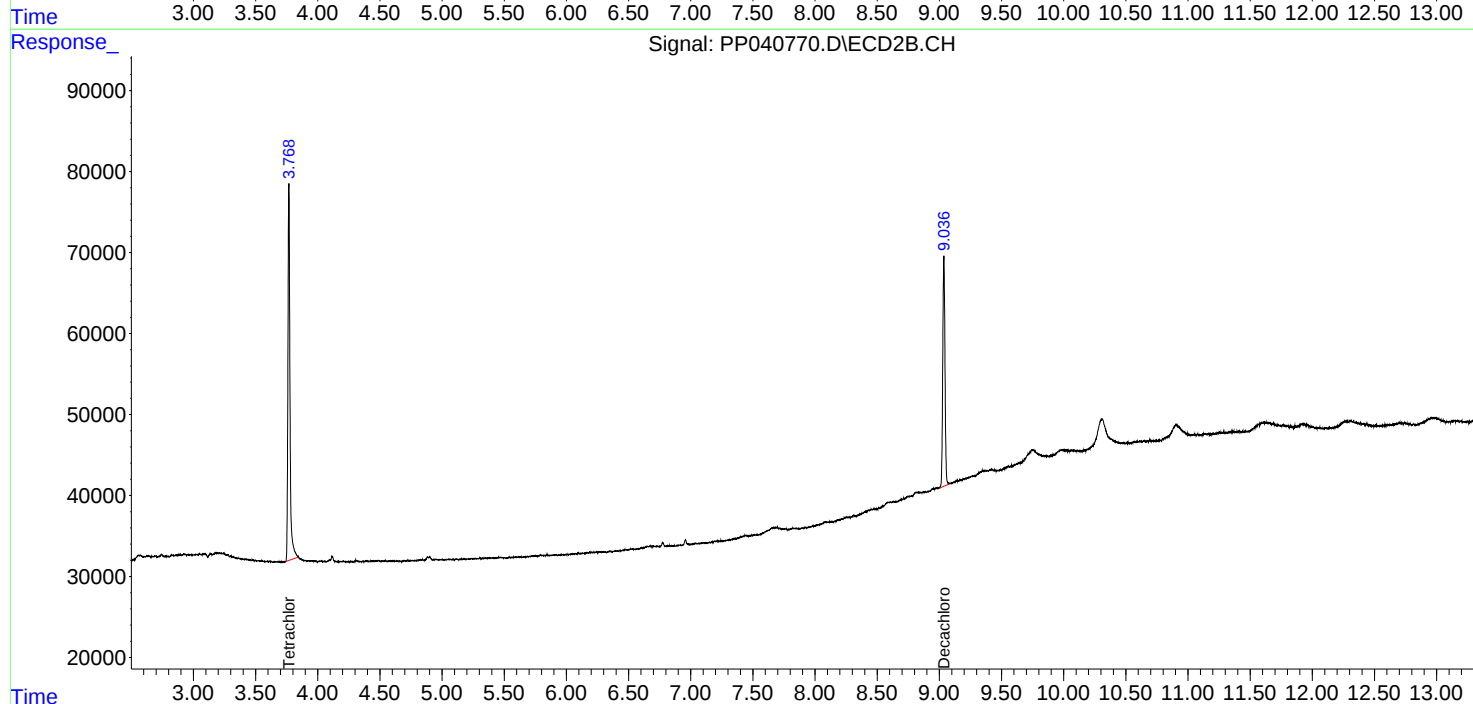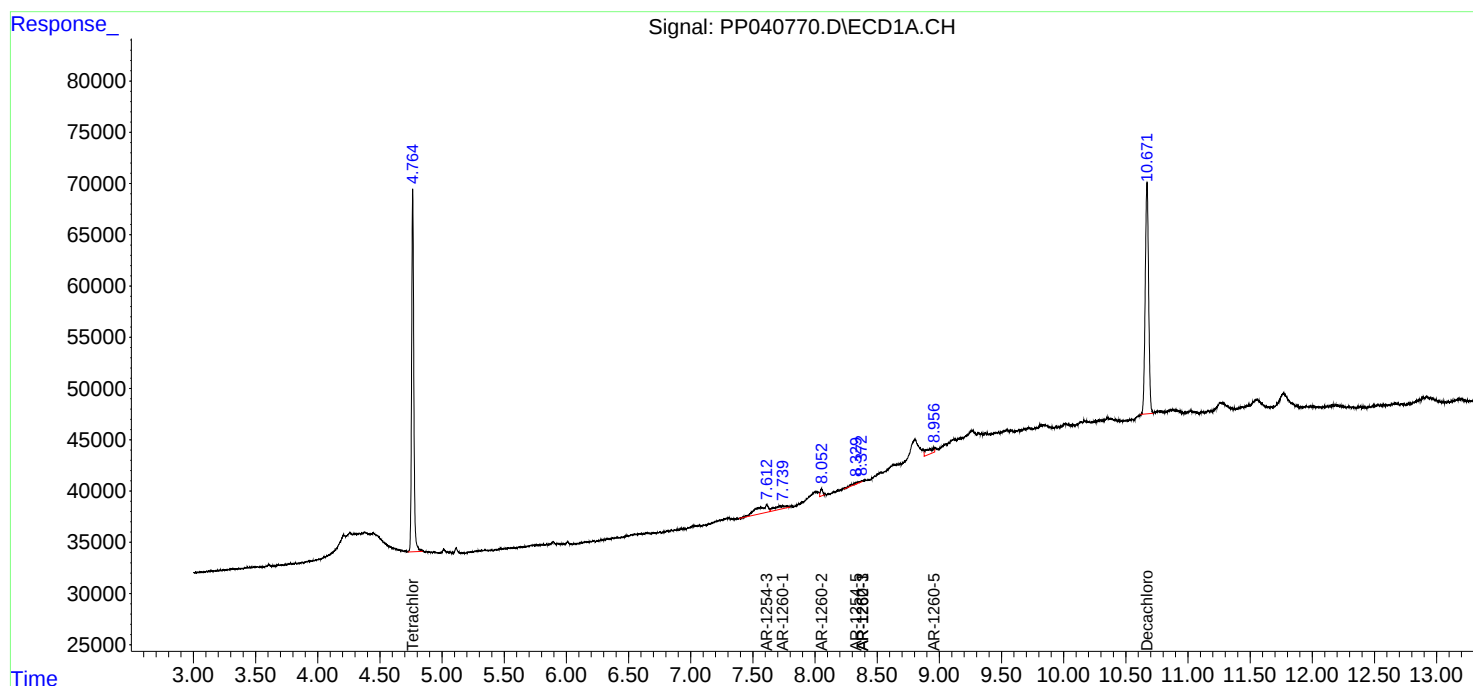


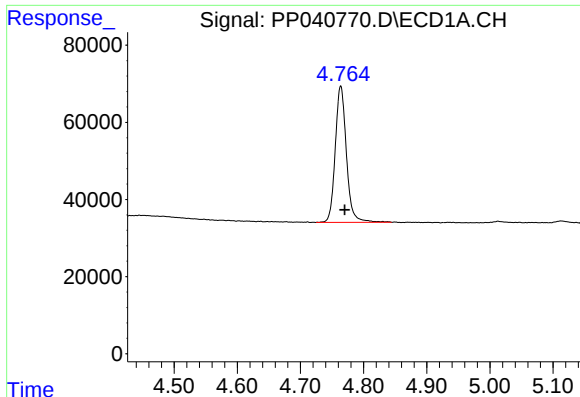

#1 Tetrachloro-m-xylene


R.T.: 4.764 min
Delta R.T.: -0.006 min
Response: 433822
Conc: 21.41 ng/ml

Instrument :
ECD_P
ClientSampleId :

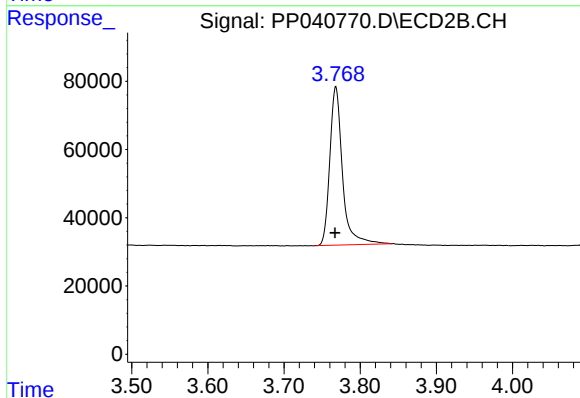


#1 Tetrachloro-m-xylene

R.T.: 3.768 min
Delta R.T.: 0.000 min
Response: 538742
Conc: 22.45 ng/ml

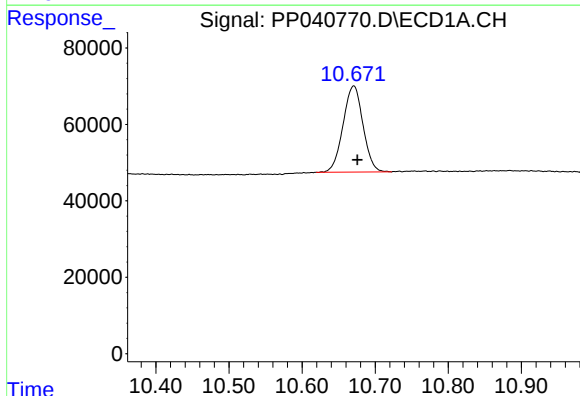


#2 Decachlorobiphenyl

R.T.: 10.671 min
Delta R.T.: -0.005 min
Response: 427638
Conc: 20.08 ng/ml

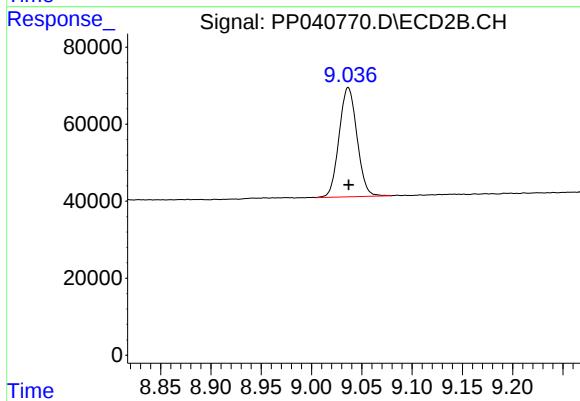

#2 Decachlorobiphenyl


R.T.: 9.037 min
Delta R.T.: 0.000 min
Response: 351809
Conc: 20.15 ng/ml

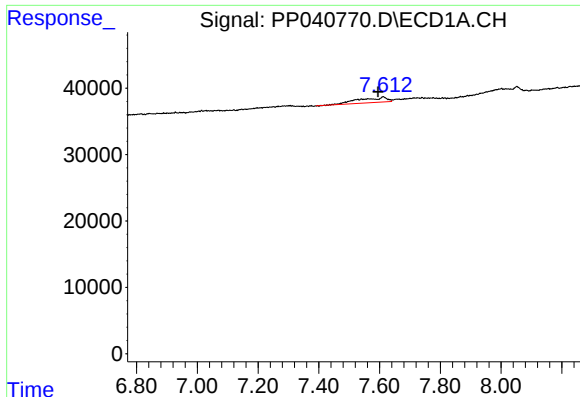

#28 AR-1254-3


R.T.: 7.612 min
Delta R.T.: 0.017 min
Response: 50314
Conc: 37.37 ng/ml

Instrument :
ECD_P
ClientSampleId :

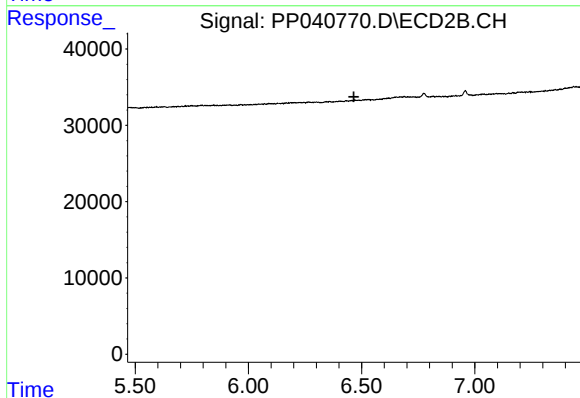


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.466 min
Response: 0
Conc: N.D.

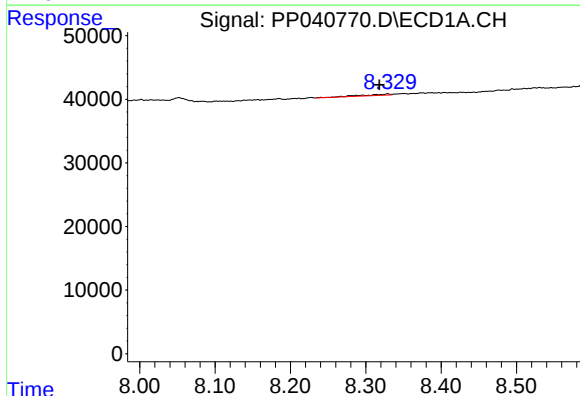


#30 AR-1254-5

R.T.: 8.329 min
Delta R.T.: 0.011 min
Response: 5012
Conc: 4.62 ng/ml

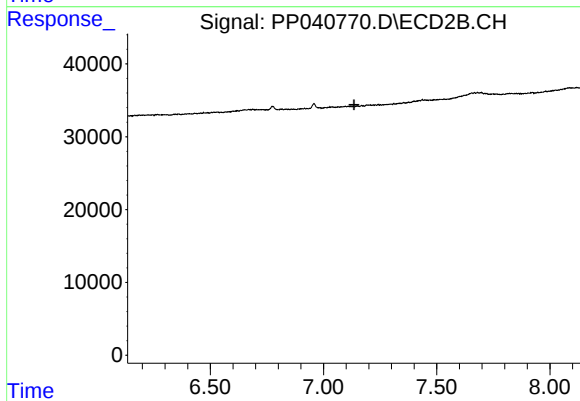

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.135 min
Response: 0
Conc: N.D.

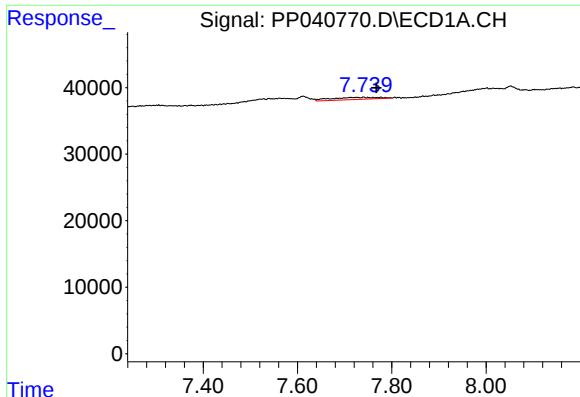

#31 AR-1260-1


R.T.: 7.740 min
Delta R.T.: -0.027 min
Response: 21258
Conc: 21.89 ng/ml

Instrument :
ECD_P
ClientSampleId :

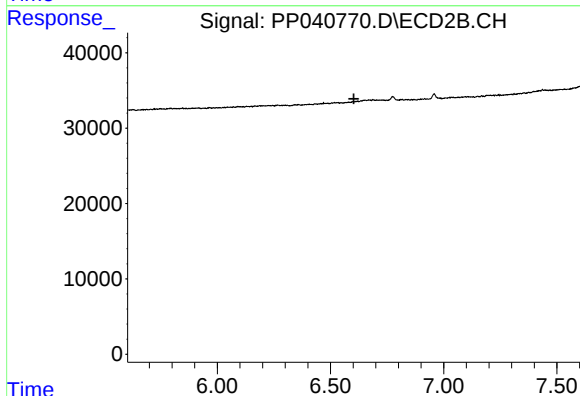


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 6.603 min
Response: 0
Conc: N.D.

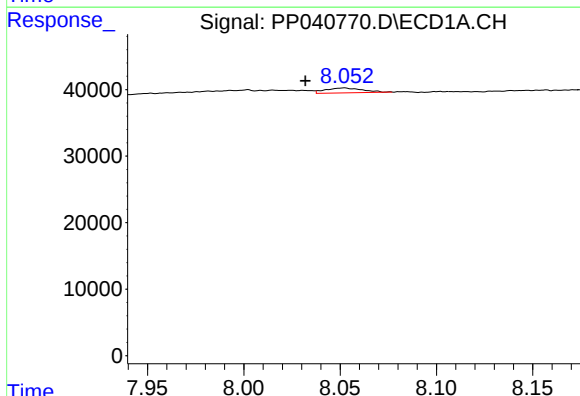


#32 AR-1260-2

R.T.: 8.052 min
Delta R.T.: 0.020 min
Response: 9591
Conc: 8.28 ng/ml

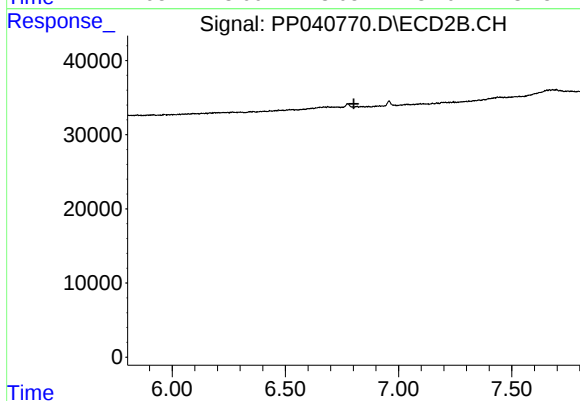

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.802 min
Response: 0
Conc: N.D.

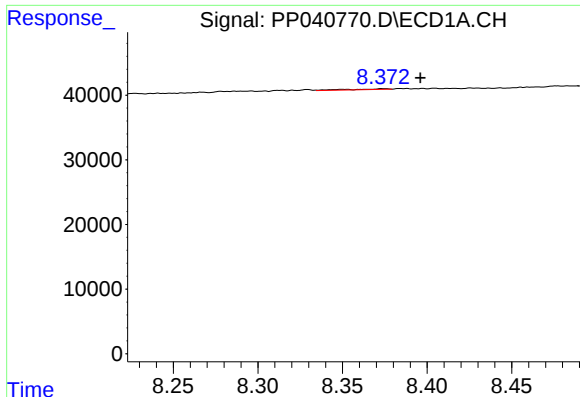

#33 AR-1260-3


R.T.: 8.374 min
Delta R.T.: -0.022 min
Response: 2180
Conc: 2.47 ng/ml

Instrument :
ECD_P
ClientSampleId :

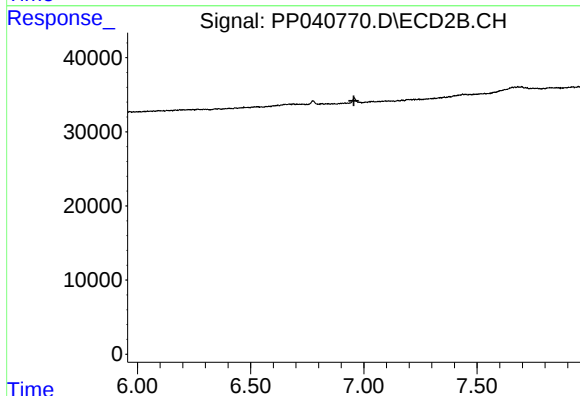


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 6.956 min
Response: 0
Conc: N.D.

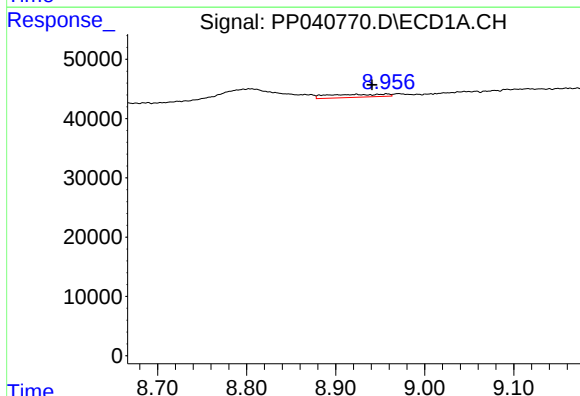


#35 AR-1260-5

R.T.: 8.958 min
Delta R.T.: 0.017 min
Response: 22023
Conc: 10.55 ng/ml

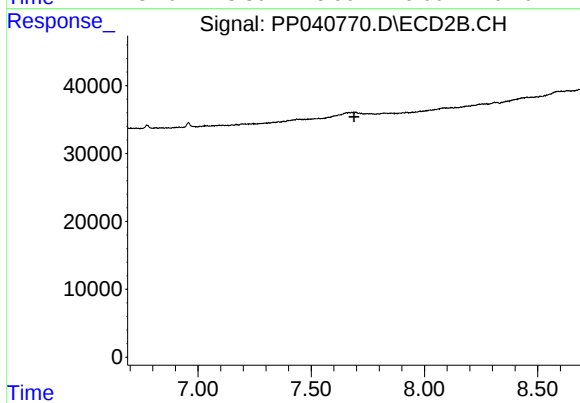

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.689 min
Response: 0
Conc: N.D.

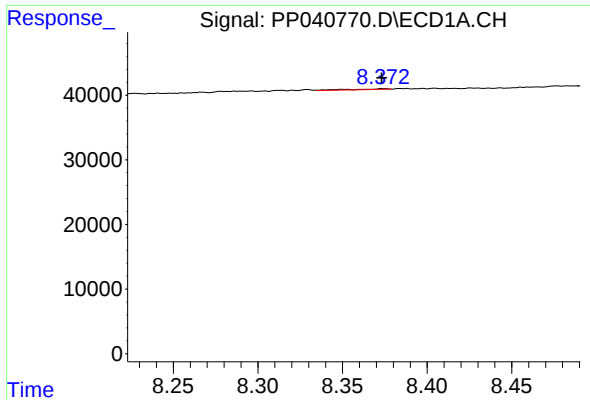

#36 AR-1262-1

R.T.: 8.374 min
Delta R.T.: 0.000 min
Response: 2180
Conc: 1.74 ng/ml

Instrument :
ECD_P
ClientSampleId :

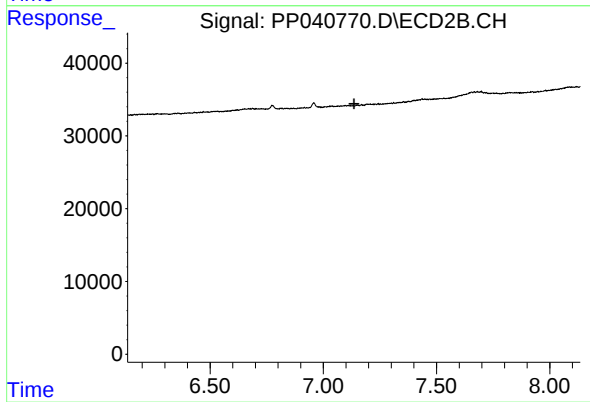

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.135 min
Response: 0
Conc: N.D.