

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110821\
 Data File : PP040772.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Nov 2021 14:13
 Operator : AJ\MA
 Sample : M4507-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 00:34:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 04 11:28:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.762	3.767	487291	601370	24.053	25.059
2)	SA Decachlor...	10.666	9.035	462315	376241	21.708	21.545
Target Compounds							
8)	L2 AR-1221-1	5.012f	0.000	19834	0	86.852	N.D. #
9)	L2 AR-1221-2	0.000	4.096f	0	1024	N.D.	4.869 #
20)	L4 AR-1242-5	0.000	5.888	0	10586	N.D.	22.984 #
24)	L5 AR-1248-4	6.996f	0.000	14849	0	18.797	N.D. #
26)	L6 AR-1254-1	6.996	5.888	14849	10586	19.234	10.883 #
27)	L6 AR-1254-2	7.221	0.000	8081	0	6.510	N.D. #
28)	L6 AR-1254-3	7.621f	0.000	21608	0	16.050	N.D. #
33)	L7 AR-1260-3	0.000	6.969	0	14951	N.D.	15.840 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110821\
Data File : PP040772.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Nov 2021 14:13
Operator : AJ\MA
Sample : M4507-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 00:34:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 04 11:28:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

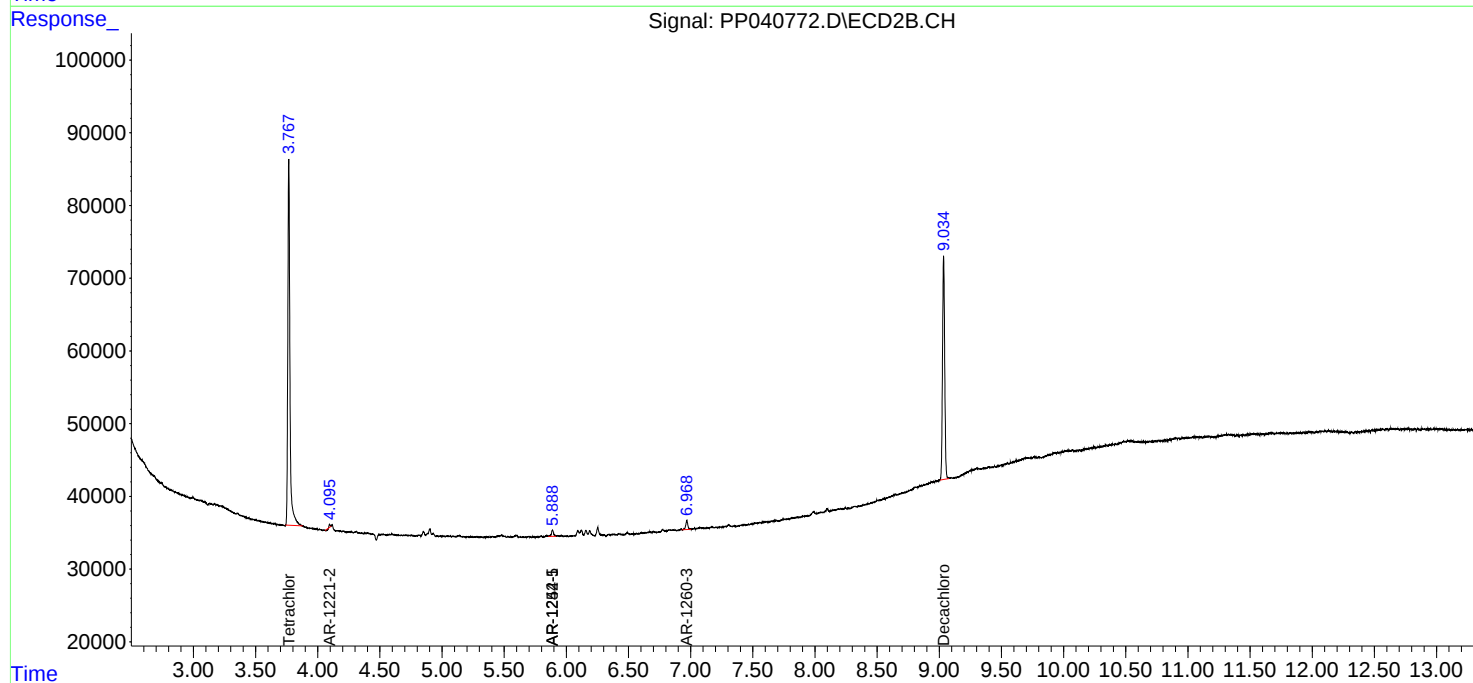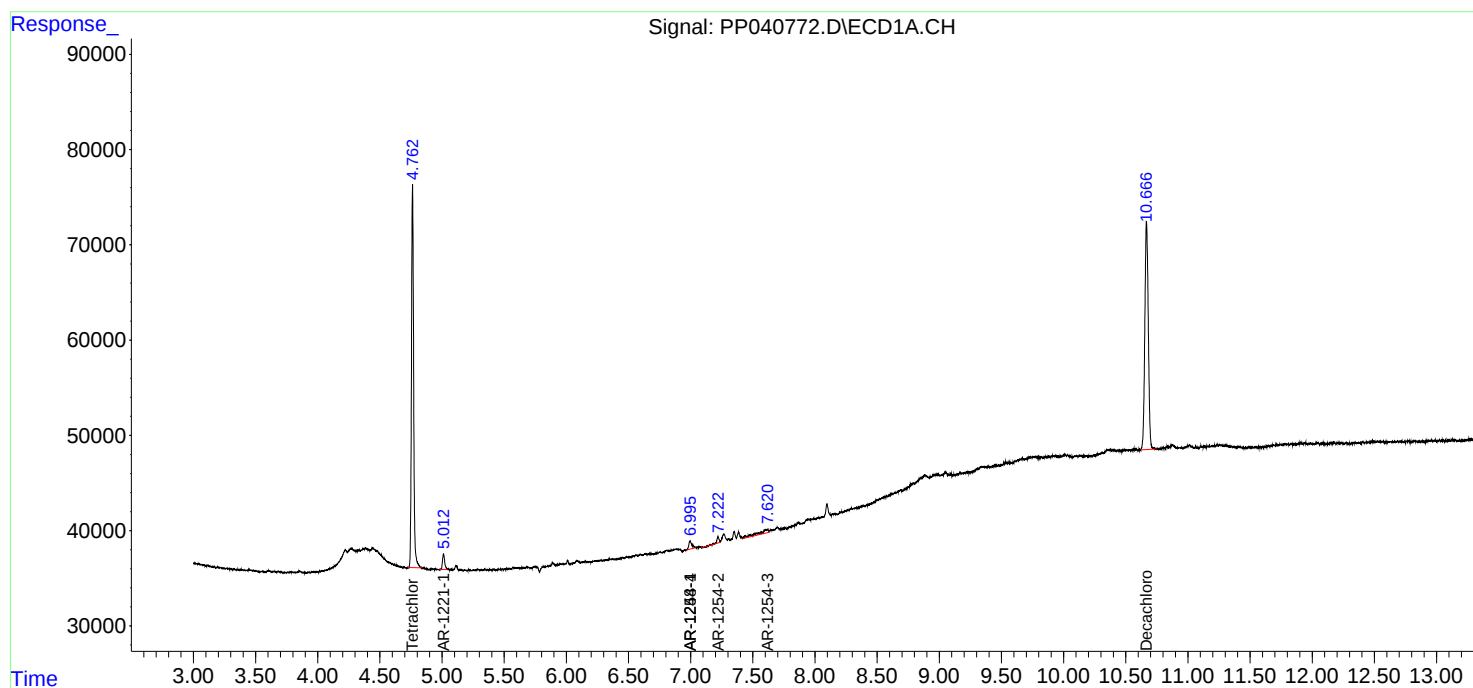


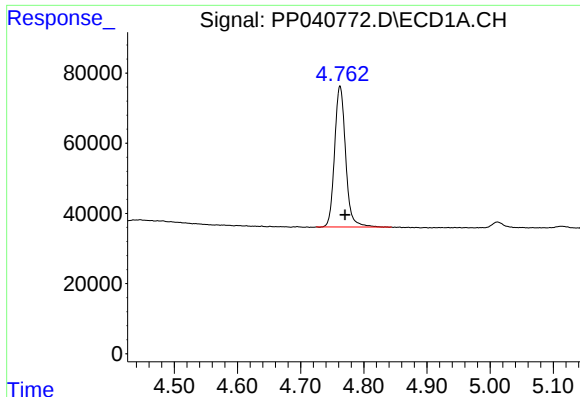

#1 Tetrachloro-m-xylene


R.T.: 4.762 min
Delta R.T.: -0.008 min
Response: 487291
Conc: 24.05 ng/ml

Instrument :
ECD_P
ClientSampleId :

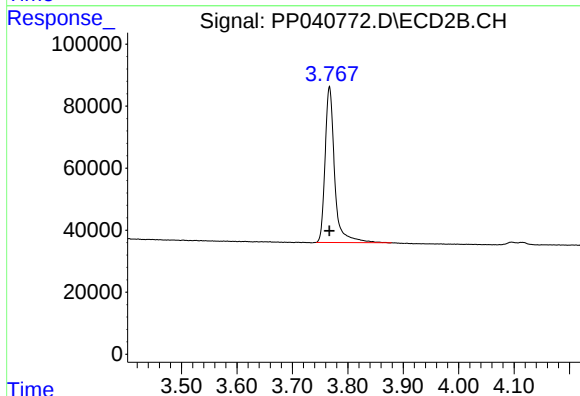


#1 Tetrachloro-m-xylene

R.T.: 3.767 min
Delta R.T.: 0.000 min
Response: 601370
Conc: 25.06 ng/ml

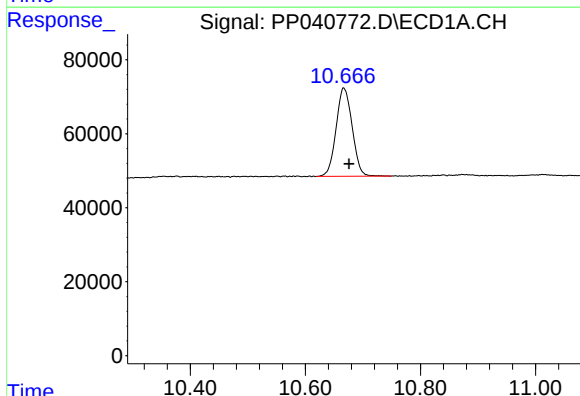


#2 Decachlorobiphenyl

R.T.: 10.666 min
Delta R.T.: -0.010 min
Response: 462315
Conc: 21.71 ng/ml

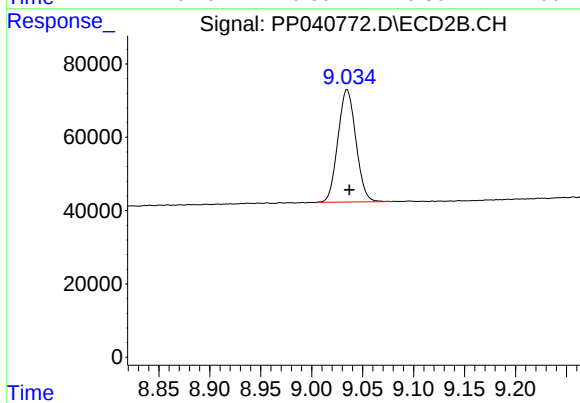

#2 Decachlorobiphenyl


R.T.: 9.035 min
Delta R.T.: -0.002 min
Response: 376241
Conc: 21.54 ng/ml

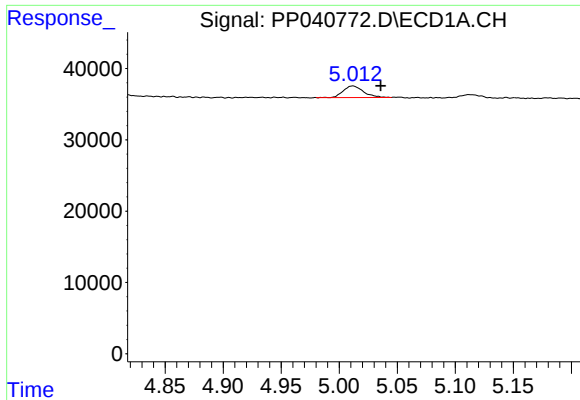

#8 AR-1221-1


R.T.: 5.012 min
Delta R.T.: -0.024 min
Response: 19834
Conc: 86.85 ng/ml

Instrument :
ECD_P
ClientSampleId :

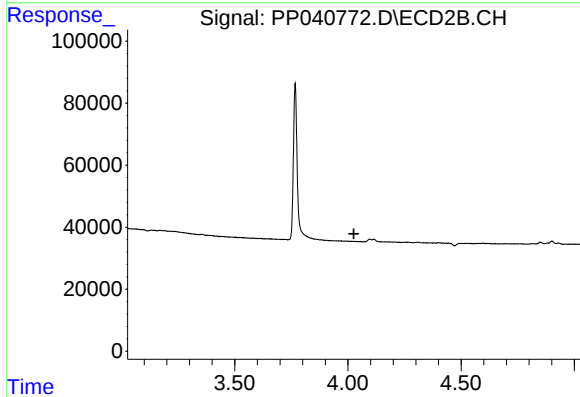


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.027 min
Response: 0
Conc: N.D.

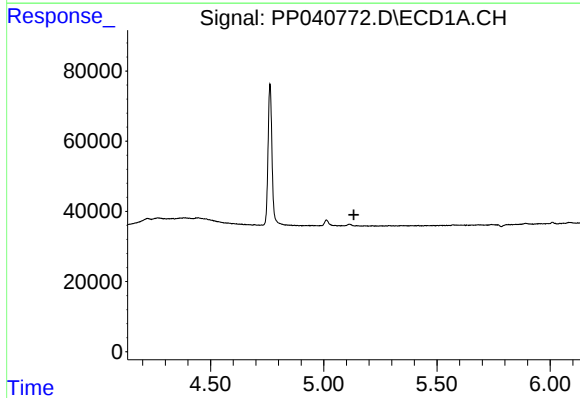


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 5.133 min
Response: 0
Conc: N.D.

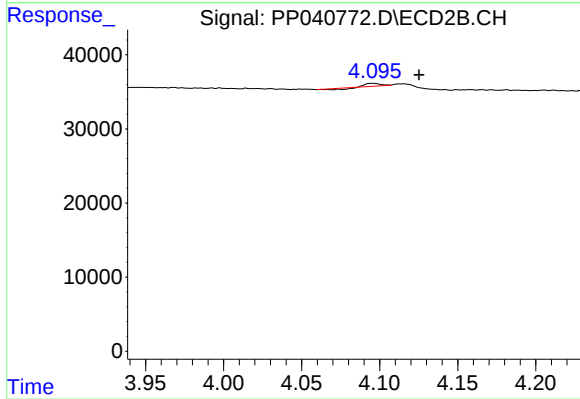

#9 AR-1221-2


R.T.: 4.096 min
Delta R.T.: -0.030 min
Response: 1024
Conc: 4.87 ng/ml

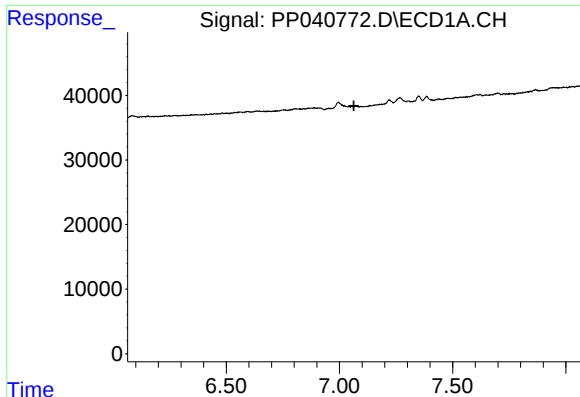

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 7.064 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

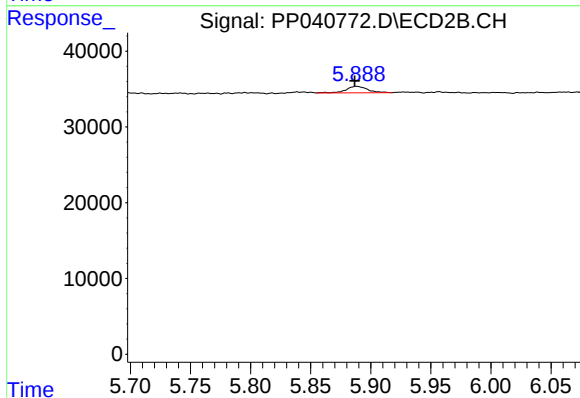


#20 AR-1242-5

R.T.: 5.888 min
Delta R.T.: 0.002 min
Response: 10586
Conc: 22.98 ng/ml

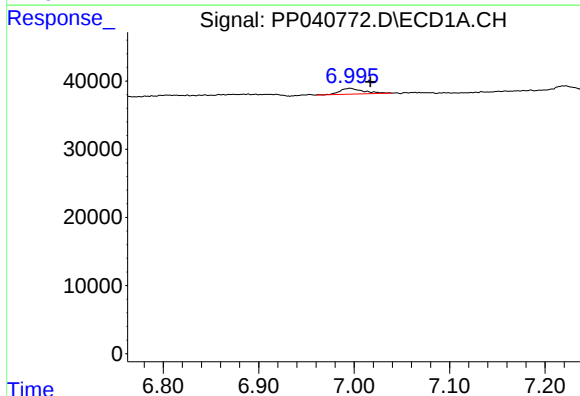


#24 AR-1248-4

R.T.: 6.996 min
Delta R.T.: -0.021 min
Response: 14849
Conc: 18.80 ng/ml

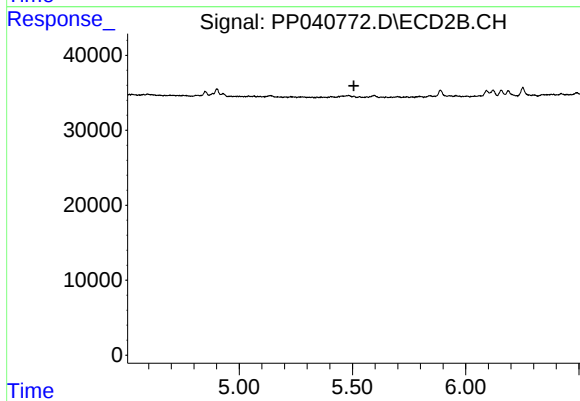

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.507 min
Response: 0
Conc: N.D.

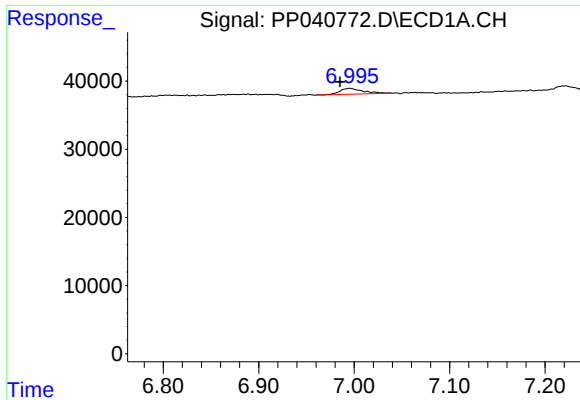

#26 AR-1254-1


R.T.: 6.996 min
Delta R.T.: 0.011 min
Response: 14849
Conc: 19.23 ng/ml

Instrument :
ECD_P
ClientSampleId :

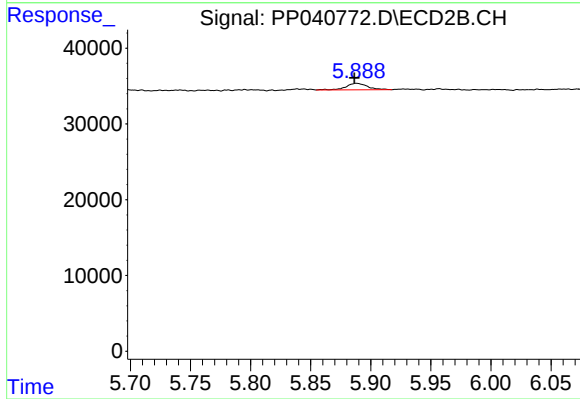


#26 AR-1254-1

R.T.: 5.888 min
Delta R.T.: 0.002 min
Response: 10586
Conc: 10.88 ng/ml

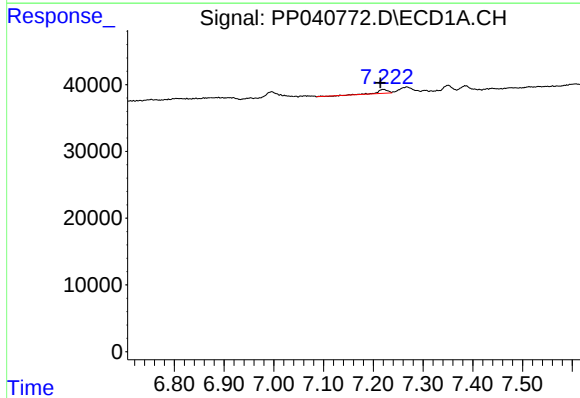


#27 AR-1254-2

R.T.: 7.221 min
Delta R.T.: 0.007 min
Response: 8081
Conc: 6.51 ng/ml

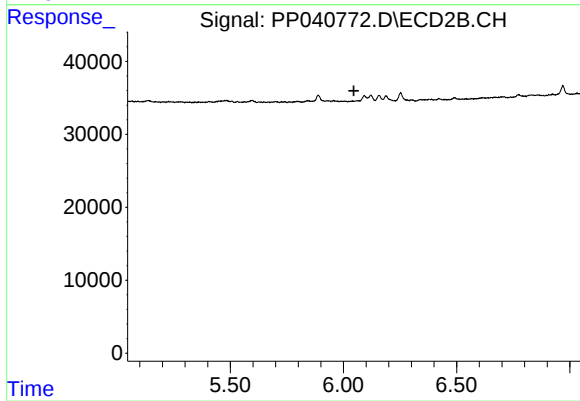

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T. : 6.046 min
Response: 0
Conc: N.D.

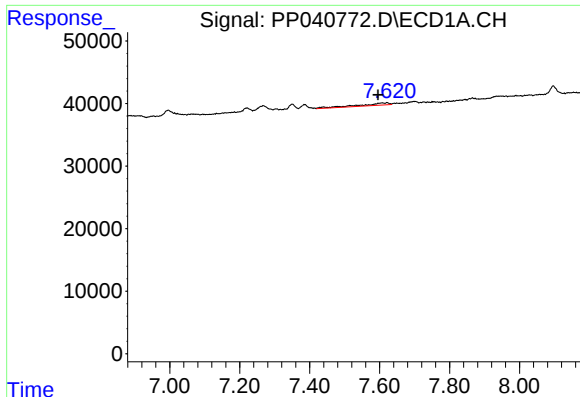

#28 AR-1254-3


R.T.: 7.621 min
Delta R.T.: 0.026 min
Response: 21608
Conc: 16.05 ng/ml

Instrument :
ECD_P
ClientSampleId :

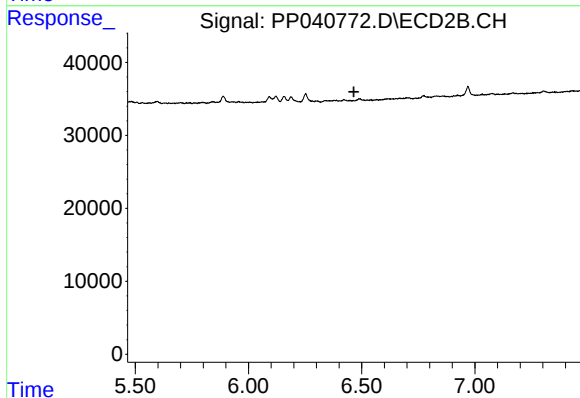


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.466 min
Response: 0
Conc: N.D.

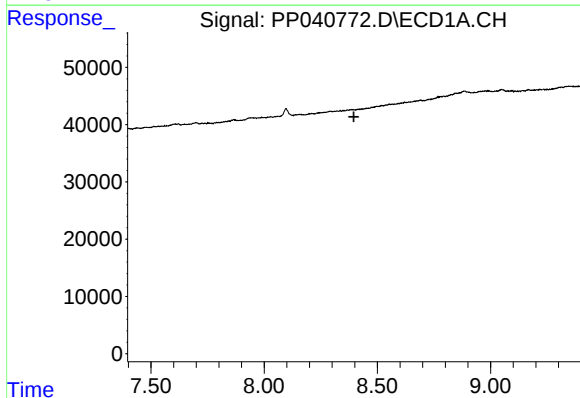

#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 8.396 min
Response: 0
Conc: N.D.

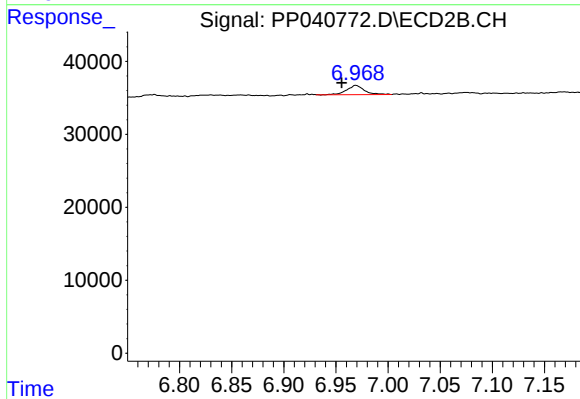

#33 AR-1260-3

R.T.: 6.969 min
Delta R.T.: 0.013 min
Response: 14951
Conc: 15.84 ng/ml