

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110821\
 Data File : PP040775.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Nov 2021 15:03
 Operator : AJ\MA
 Sample : M4507-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 00:35:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 04 11:28:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.763	3.767	466097	571776	23.007	23.826
2) SA Decachlor...	10.667	9.035	322887	273071	15.161	15.637
Target Compounds						
32) L7 AR-1260-2	8.009f	0.000	9834	0	8.495	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110821\
Data File : PP040775.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Nov 2021 15:03
Operator : AJ\MA
Sample : M4507-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 00:35:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 04 11:28:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

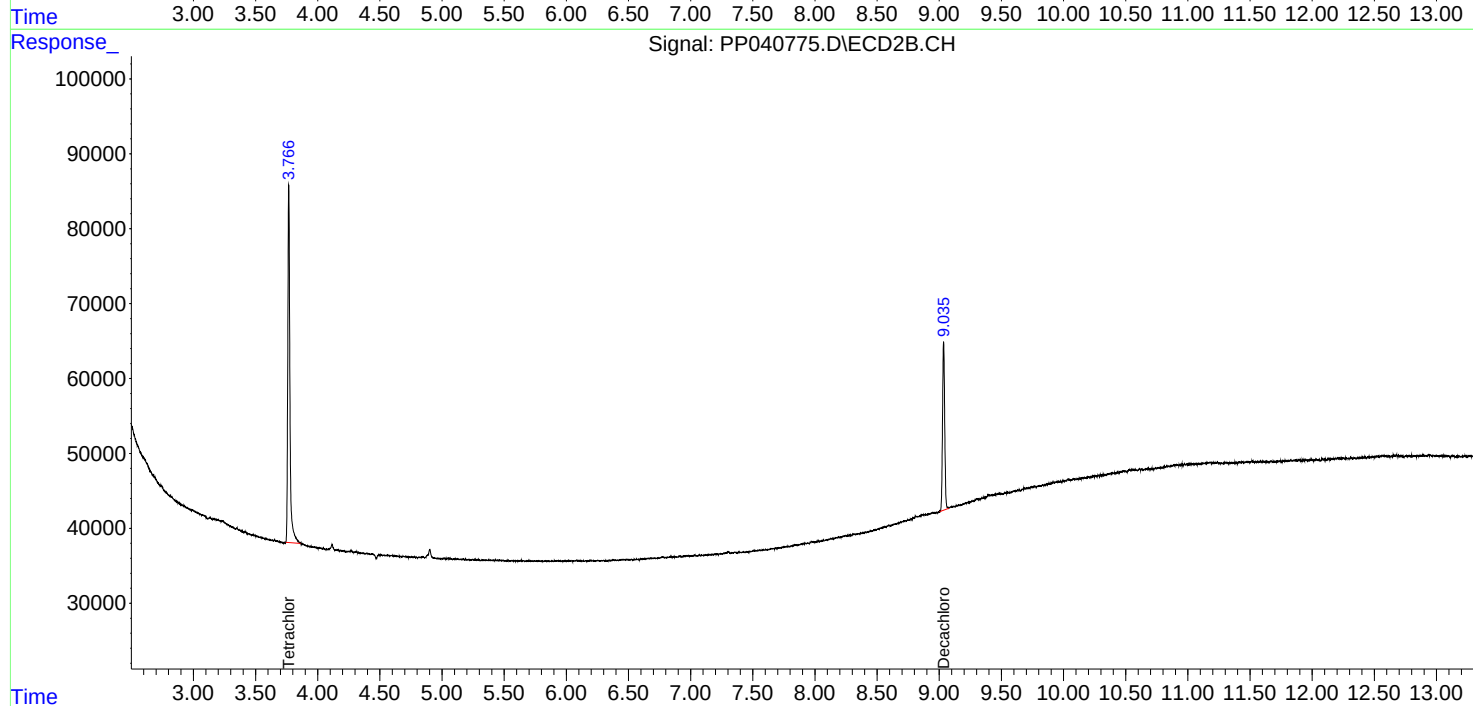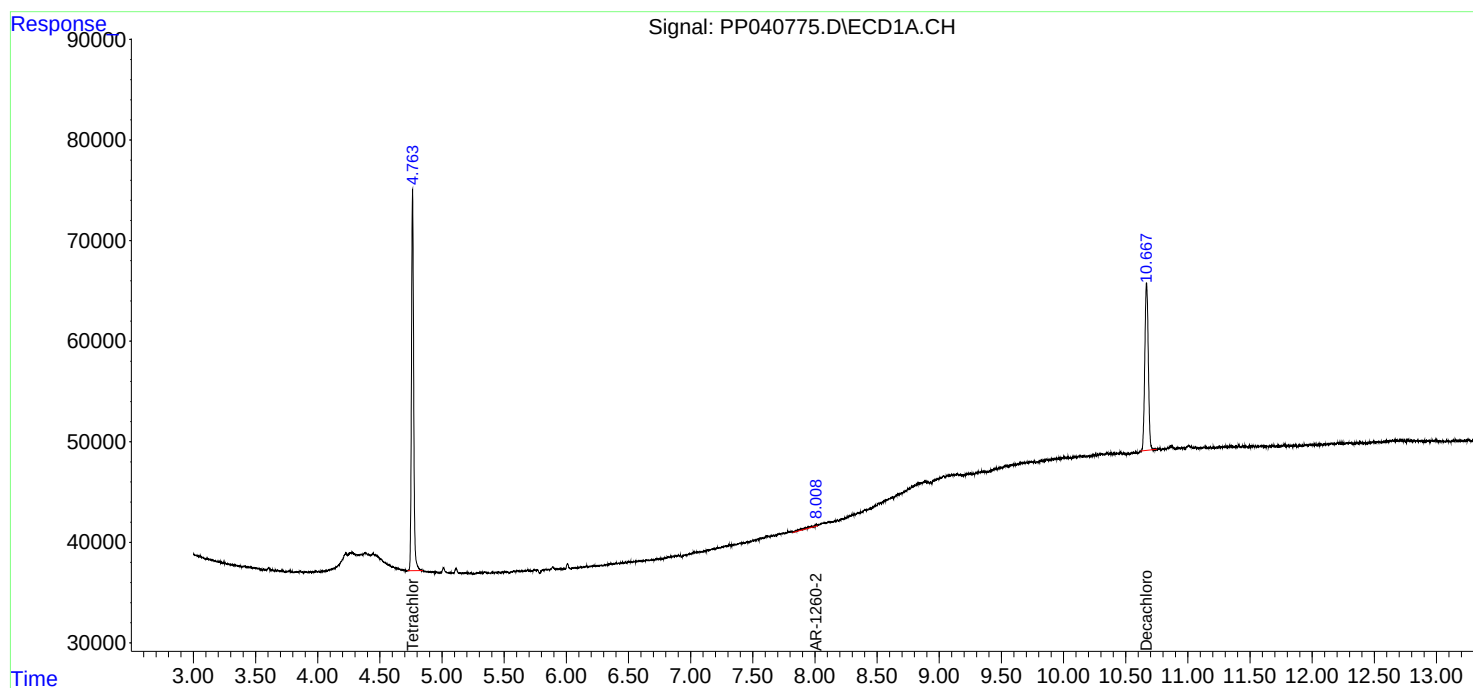


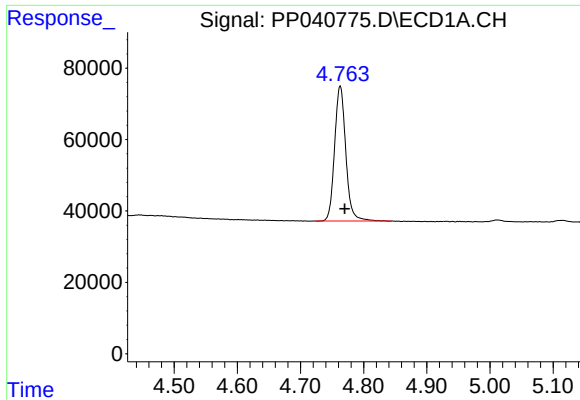

#1 Tetrachloro-m-xylene


R.T.: 4.763 min
Delta R.T.: -0.007 min
Response: 466097
Conc: 23.01 ng/ml

Instrument :
ECD_P
ClientSampleId :

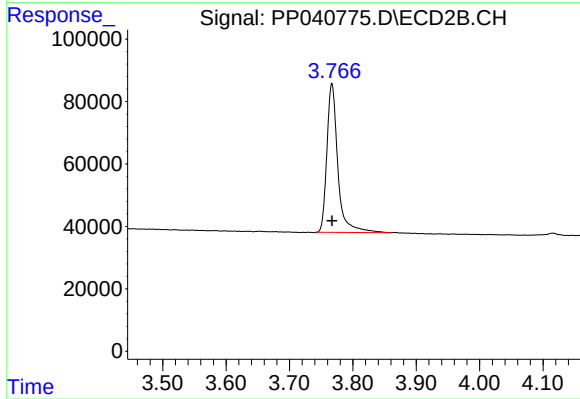


#1 Tetrachloro-m-xylene

R.T.: 3.767 min
Delta R.T.: 0.000 min
Response: 571776
Conc: 23.83 ng/ml

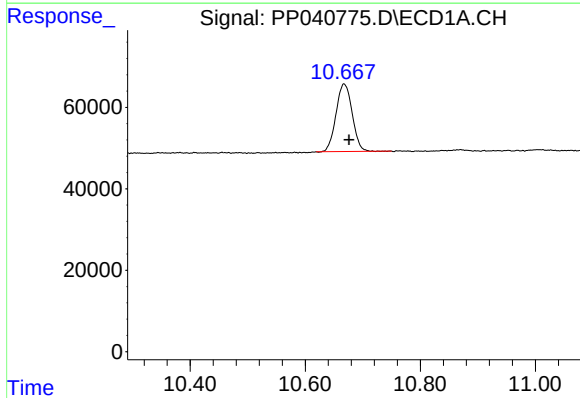


#2 Decachlorobiphenyl

R.T.: 10.667 min
Delta R.T.: -0.009 min
Response: 322887
Conc: 15.16 ng/ml

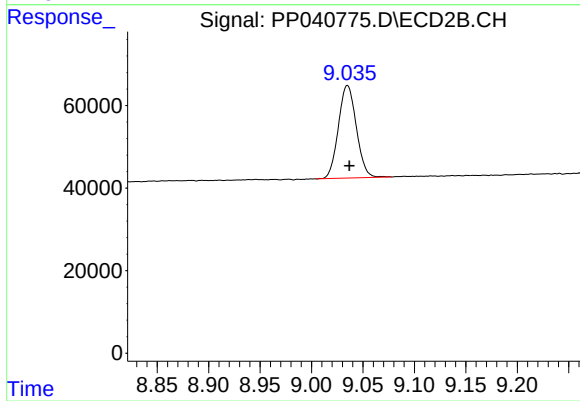

#2 Decachlorobiphenyl


R.T.: 9.035 min
Delta R.T.: -0.002 min
Response: 273071
Conc: 15.64 ng/ml

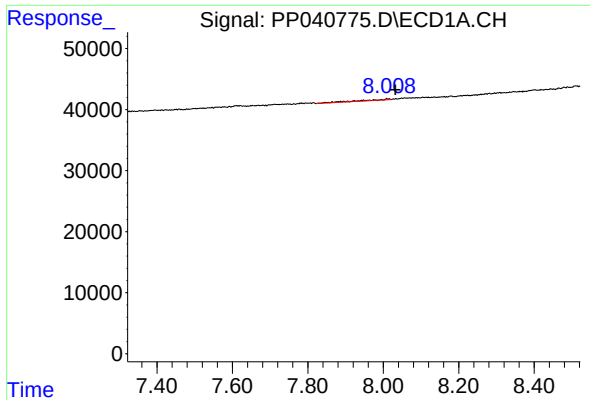

#32 AR-1260-2

R.T.: 8.009 min
Delta R.T.: -0.023 min
Response: 9834
Conc: 8.49 ng/ml

Instrument :
ECD_P
ClientSampleId :

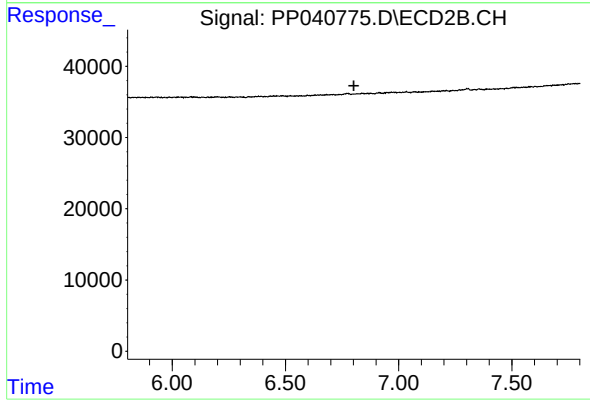

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.802 min
Response: 0
Conc: N.D.