

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110821\
 Data File : PP040811.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Nov 2021 1:45
 Operator : AJ\MA
 Sample : M4506-17 10X
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 03:11:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 04 11:28:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.762	3.766	28080	32607	1.386	1.359
2)	SA Decachlor...	10.672	9.035	47770	39083	2.243	2.238
Target Compounds							
31)	L7 AR-1260-1	0.000	6.630f	0	10485	N.D.	12.084 #
33)	L7 AR-1260-3	8.381	0.000	798	0	0.904	N.D. #
34)	L7 AR-1260-4	8.630	0.000	14217	0	13.455	N.D. #
35)	L7 AR-1260-5	8.963f	0.000	18241	0	8.736	N.D. #
36)	L8 AR-1262-1	8.381	0.000	798	0	0.637	N.D. #
37)	L8 AR-1262-2	8.893f	0.000	57043	0	25.102	N.D. #
38)	L8 AR-1262-3	9.221	0.000	33975	0	31.955	N.D. #
41)	L9 AR-1268-1	9.221	0.000	33975	0	12.463	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110821\
Data File : PP040811.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Nov 2021 1:45
Operator : AJ\MA
Sample : M4506-17 10X
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 03:11:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 04 11:28:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

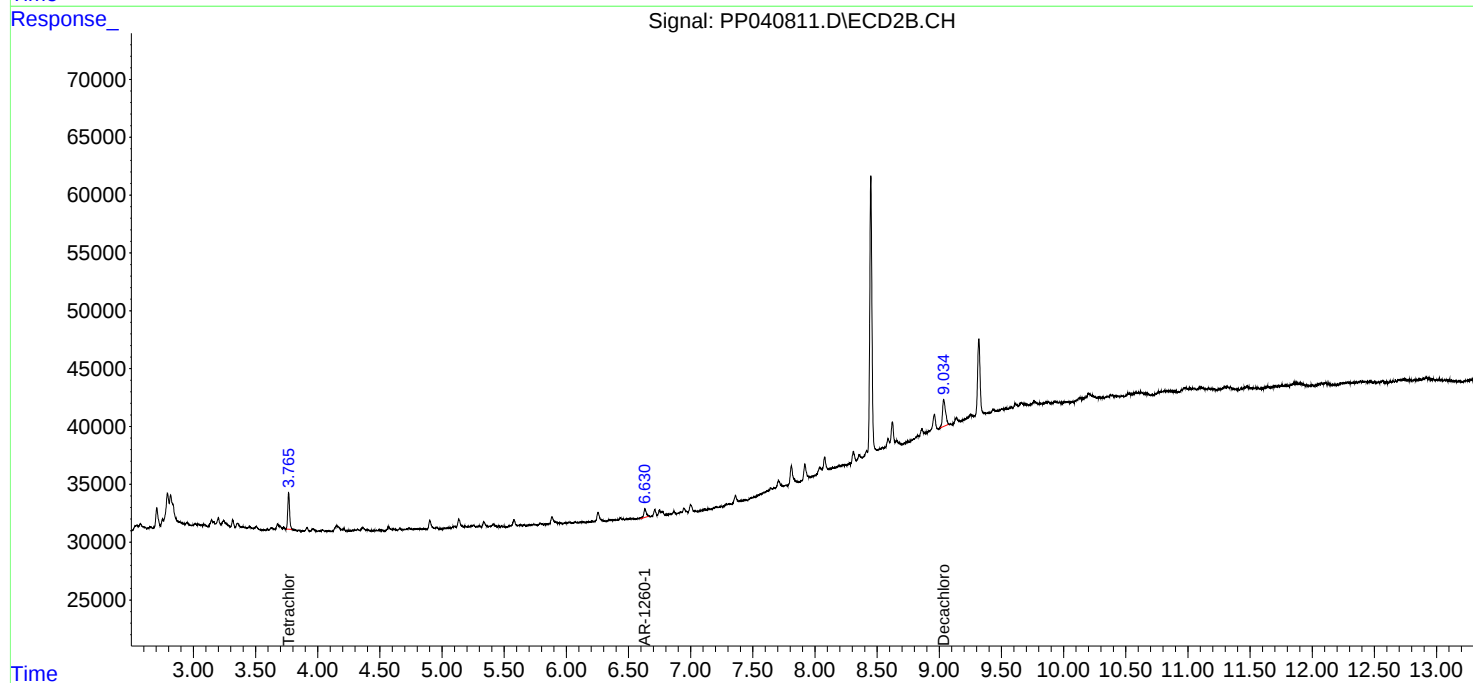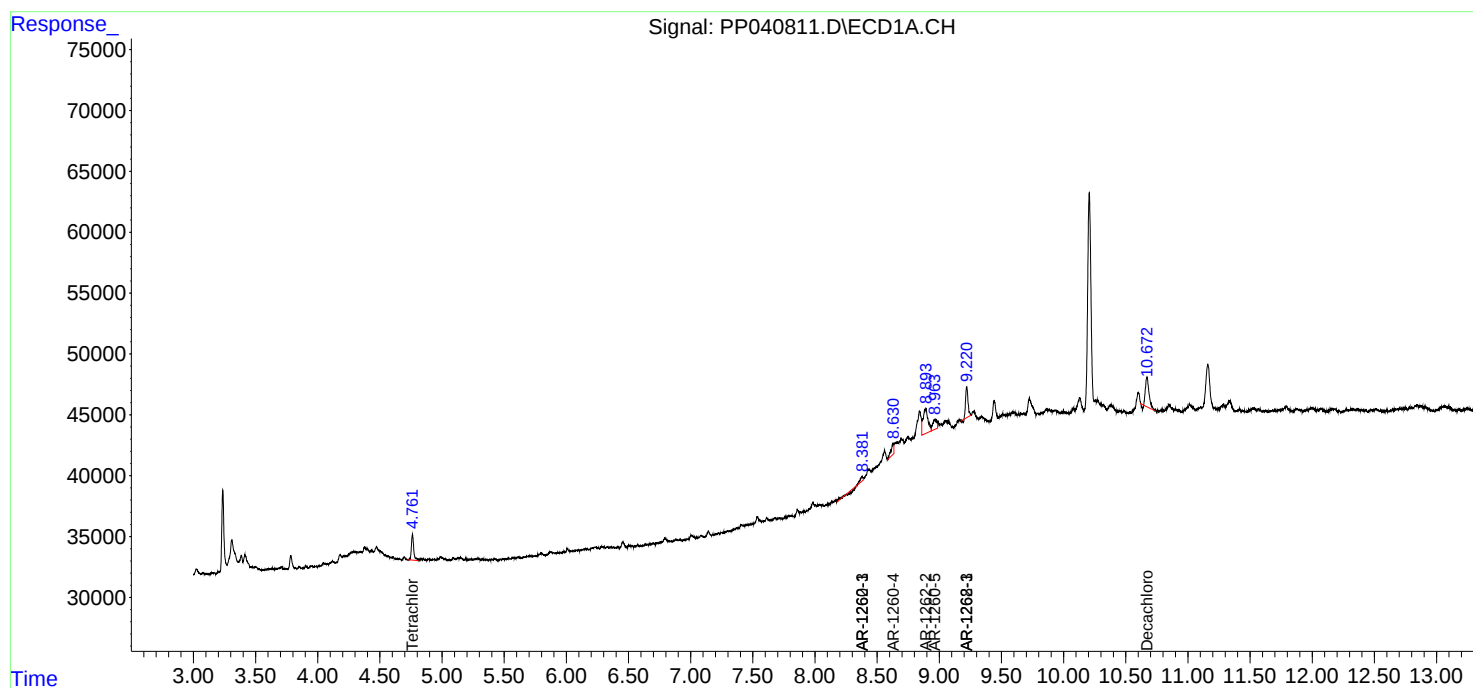


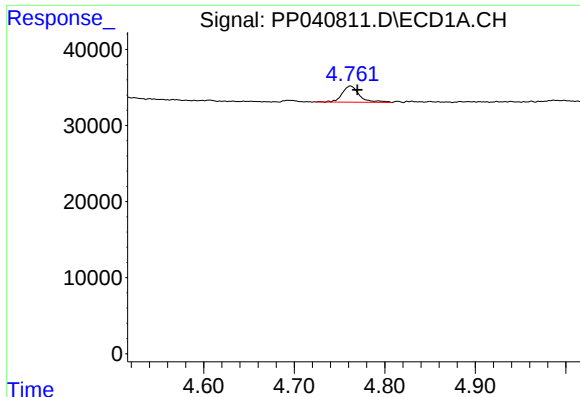

#1 Tetrachloro-m-xylene


R.T.: 4.762 min
Delta R.T.: -0.008 min
Response: 28080
Conc: 1.39 ng/ml

Instrument :
ECD_P
ClientSampleId :

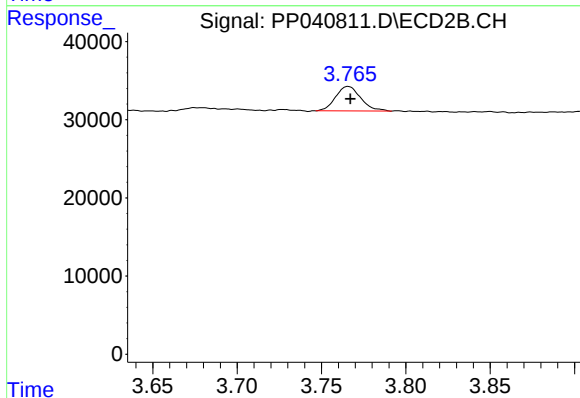


#1 Tetrachloro-m-xylene

R.T.: 3.766 min
Delta R.T.: -0.001 min
Response: 32607
Conc: 1.36 ng/ml

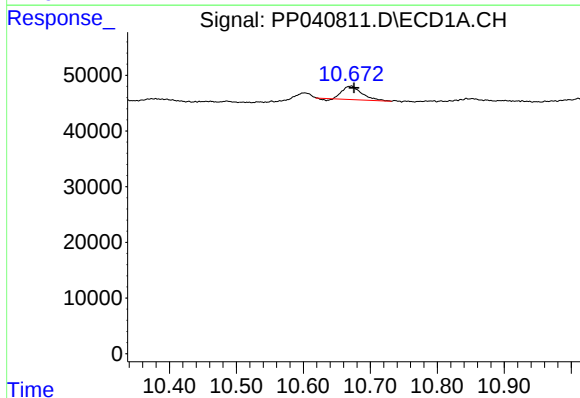


#2 Decachlorobiphenyl

R.T.: 10.672 min
Delta R.T.: -0.004 min
Response: 47770
Conc: 2.24 ng/ml

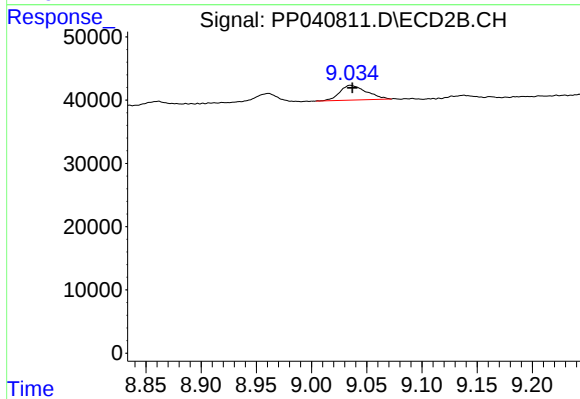

#2 Decachlorobiphenyl


R.T.: 9.035 min
Delta R.T.: -0.002 min
Response: 39083
Conc: 2.24 ng/ml

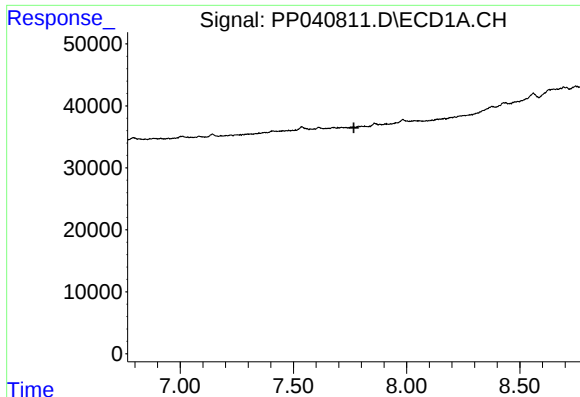

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.767 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

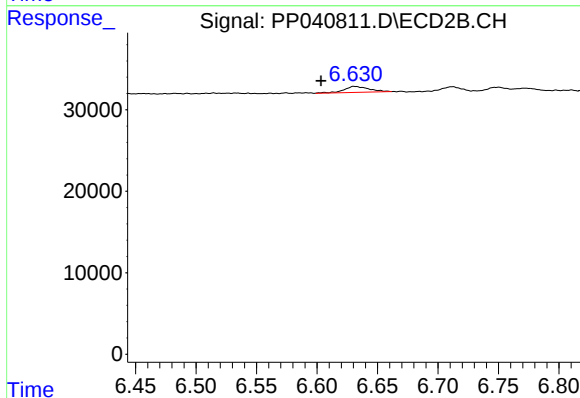


#31 AR-1260-1

R.T.: 6.630 min
Delta R.T.: 0.027 min
Response: 10485
Conc: 12.08 ng/ml

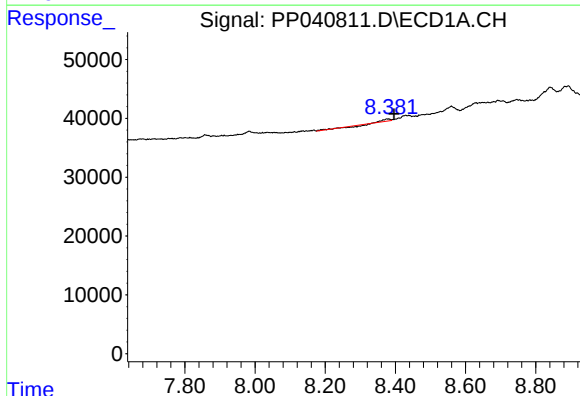


#33 AR-1260-3

R.T.: 8.381 min
Delta R.T.: -0.015 min
Response: 798
Conc: 0.90 ng/ml

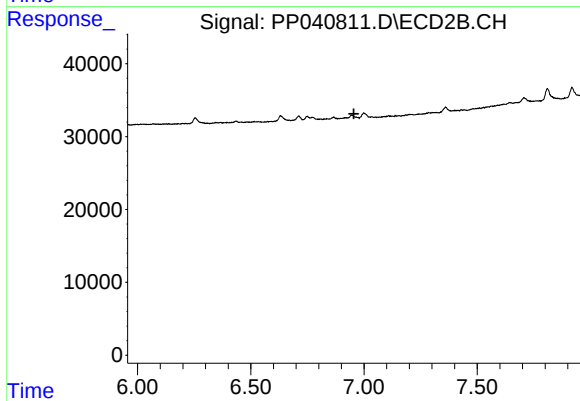

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 6.956 min
Response: 0
Conc: N.D.

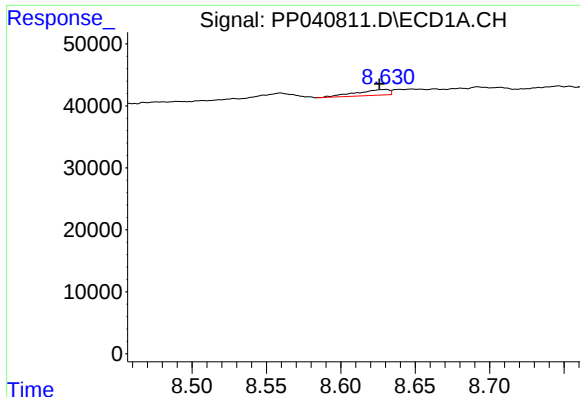

#34 AR-1260-4


R.T.: 8.630 min
Delta R.T.: 0.004 min
Response: 14217
Conc: 13.46 ng/ml

Instrument :
ECD_P
ClientSampleId :

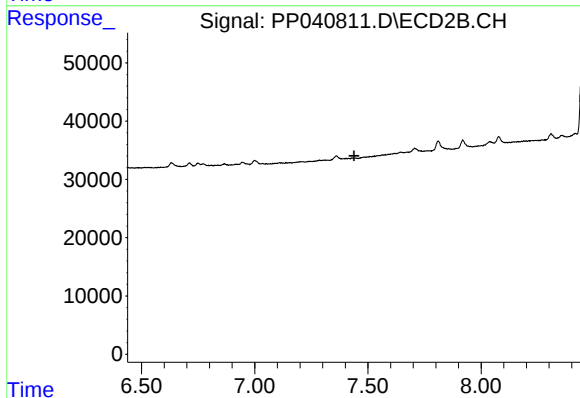


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.438 min
Response: 0
Conc: N.D.

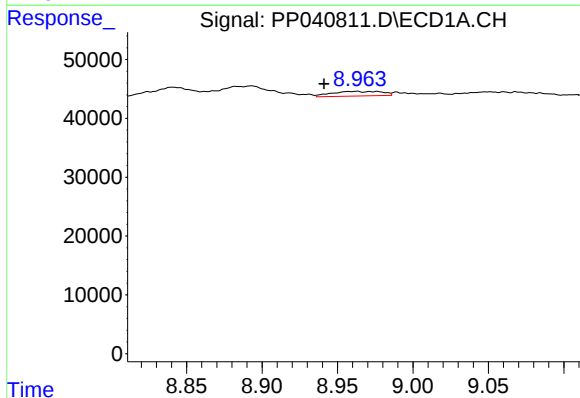


#35 AR-1260-5

R.T.: 8.963 min
Delta R.T.: 0.022 min
Response: 18241
Conc: 8.74 ng/ml

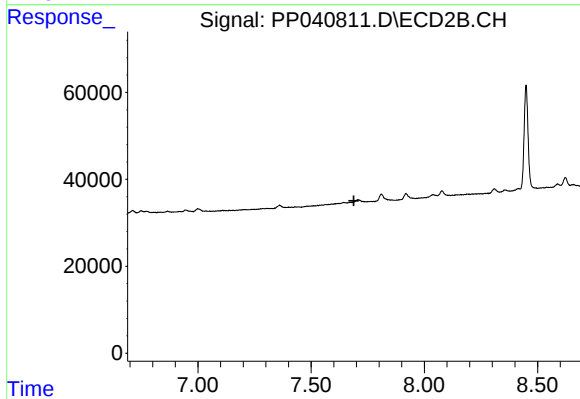

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.689 min
Response: 0
Conc: N.D.

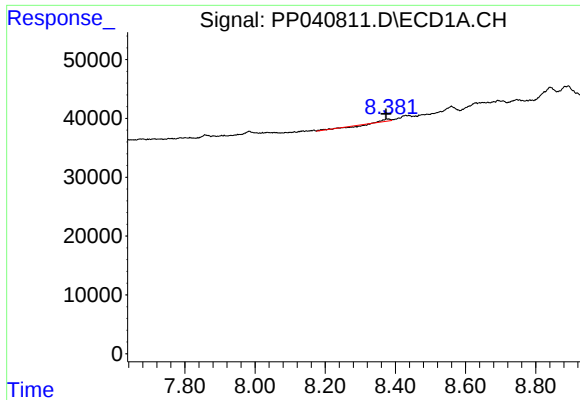

#36 AR-1262-1


R.T.: 8.381 min
Delta R.T.: 0.008 min
Response: 798
Conc: 0.64 ng/ml

Instrument :
ECD_P
ClientSampleId :

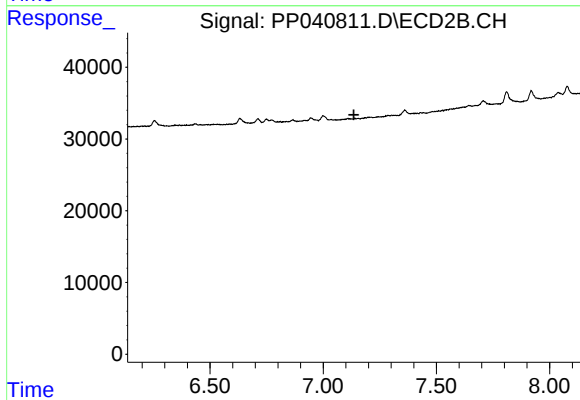


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.135 min
Response: 0
Conc: N.D.

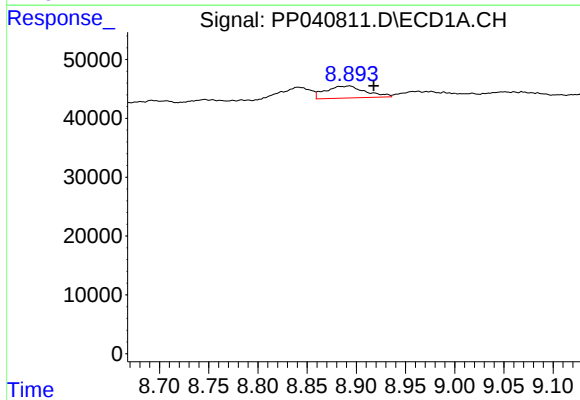


#37 AR-1262-2

R.T.: 8.893 min
Delta R.T.: -0.025 min
Response: 57043
Conc: 25.10 ng/ml

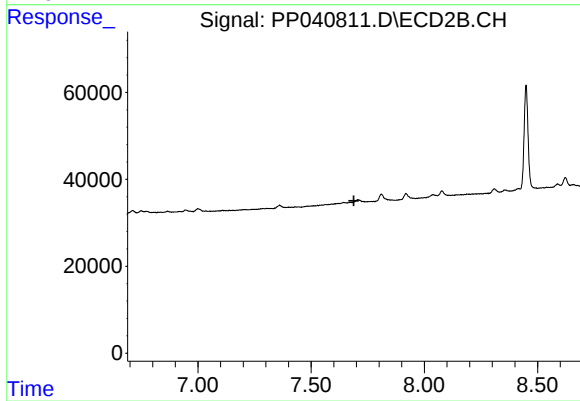

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 7.689 min
Response: 0
Conc: N.D.

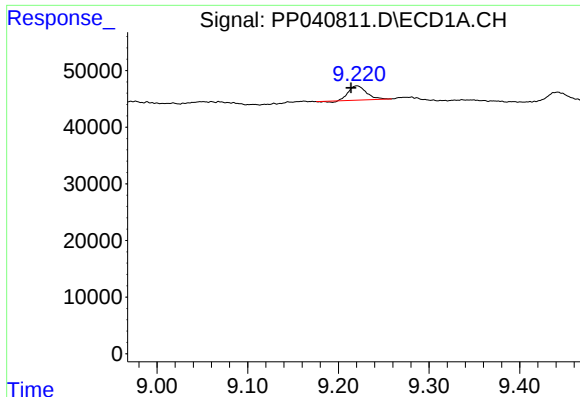

#38 AR-1262-3


R.T.: 9.221 min
Delta R.T.: 0.006 min
Response: 33975
Conc: 31.96 ng/ml

Instrument :
ECD_P
ClientSampleId :

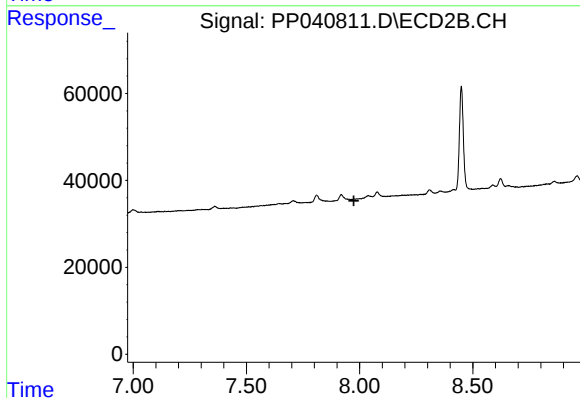


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 7.974 min
Response: 0
Conc: N.D.

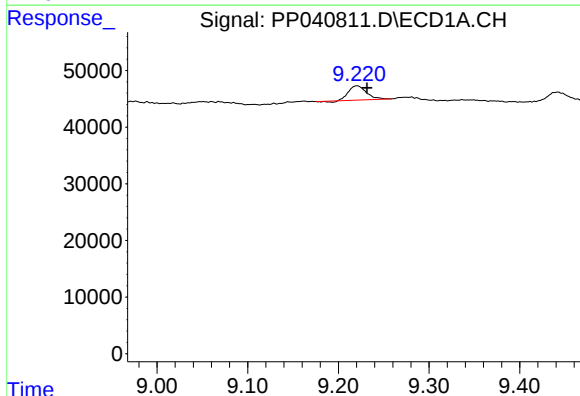

#41 AR-1268-1

R.T.: 9.221 min
Delta R.T.: -0.011 min
Response: 33975
Conc: 12.46 ng/ml

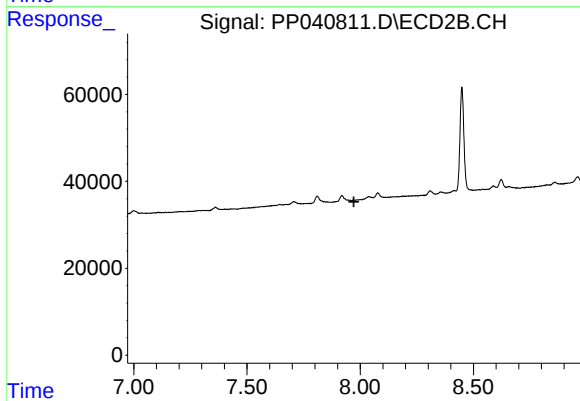

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 7.972 min
Response: 0
Conc: N.D.