

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110821\
 Data File : PP040816.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Nov 2021 3:36
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 04:42:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 04 11:28:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.762	3.766	461651	586165	22.788	24.425
2)	SA Decachlor...	10.669	9.034	450410	362962	21.149	20.784
Target Compounds							
9)	L2 AR-1221-2	5.149f	0.000	18963	0	125.640	N.D. #
10)	L2 AR-1221-3	0.000	4.209	0	28714	N.D.	43.742 #
11)	L3 AR-1232-1	0.000	4.209	0	28714	N.D.	53.203 #
24)	L5 AR-1248-4	6.994f	0.000	8982	0	11.370	N.D. #
26)	L6 AR-1254-1	6.994	0.000	8982	0	11.634	N.D. #
32)	L7 AR-1260-2	8.054f	0.000	18293	0	15.801	N.D. #
35)	L7 AR-1260-5	8.938	0.000	104046	0	49.831	N.D. #
37)	L8 AR-1262-2	8.938f	0.000	104046	0	45.786	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110821\
Data File : PP040816.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Nov 2021 3:36
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 04:42:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 04 11:28:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

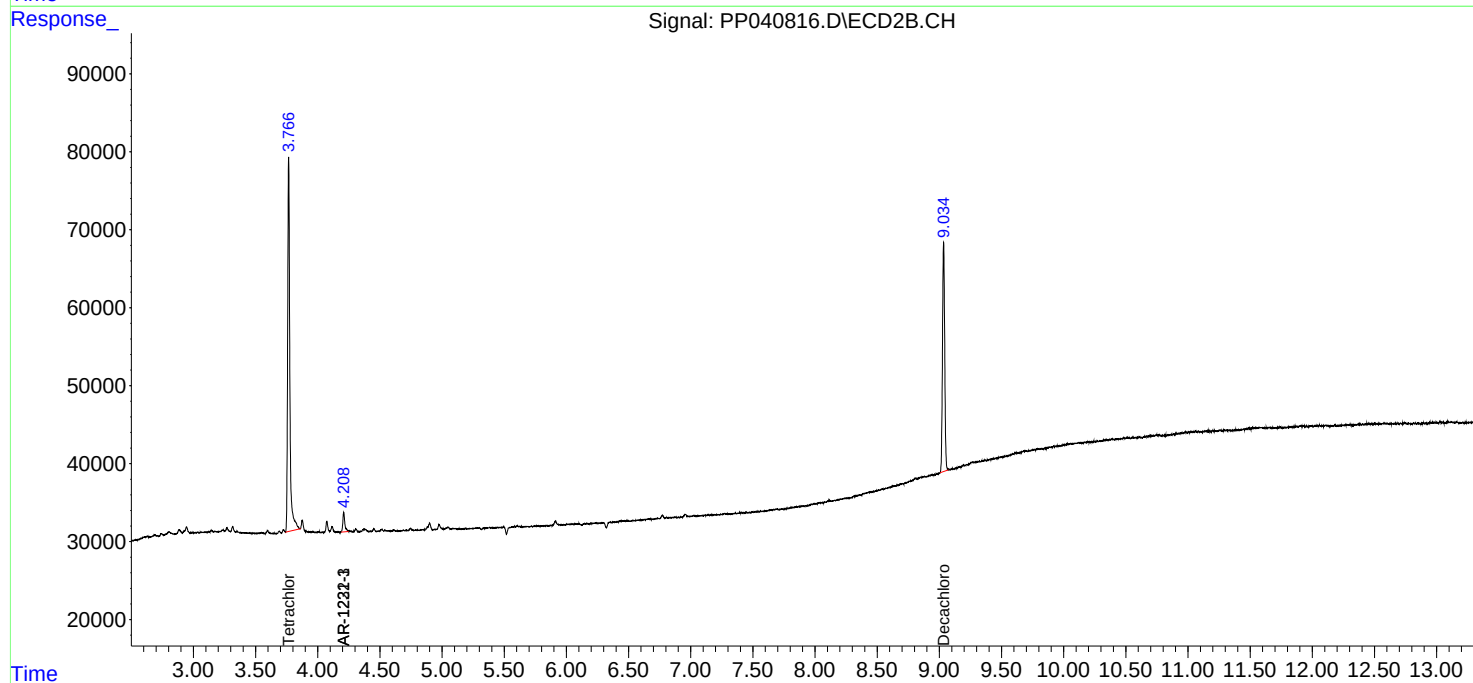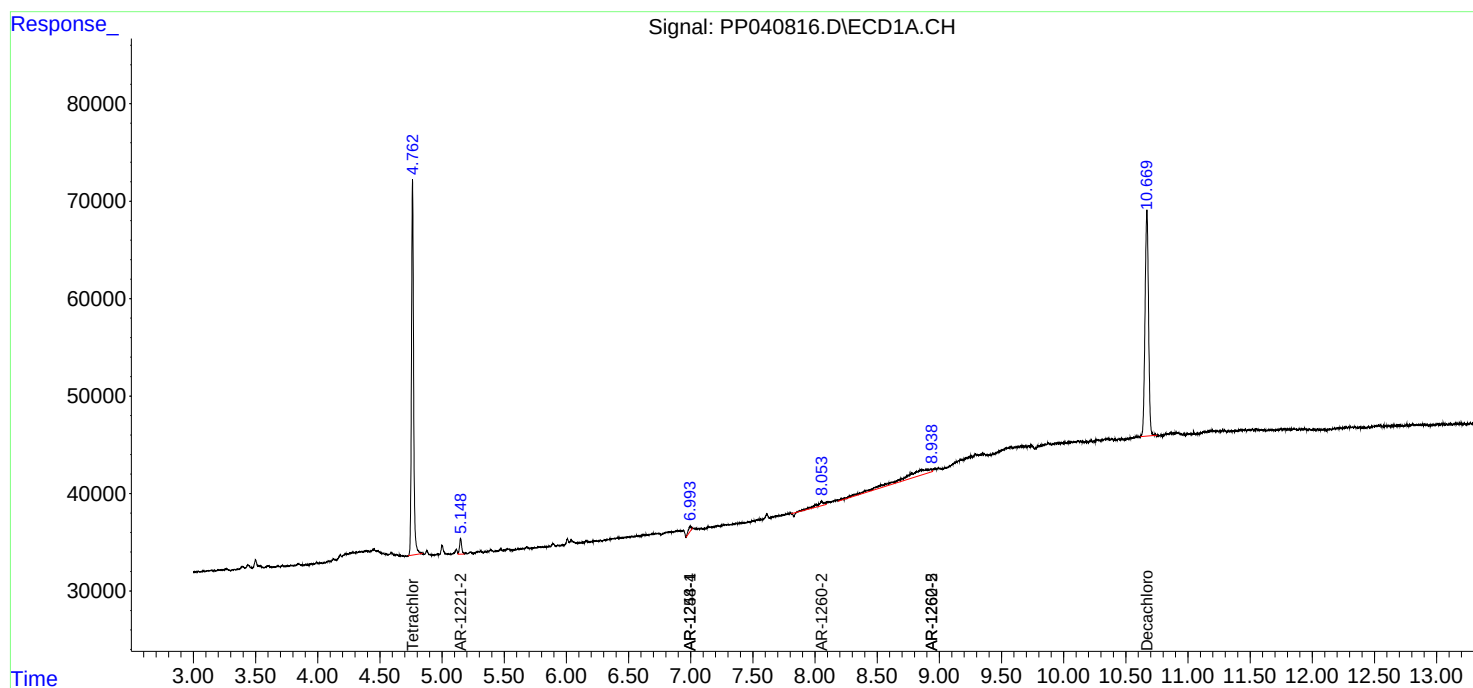


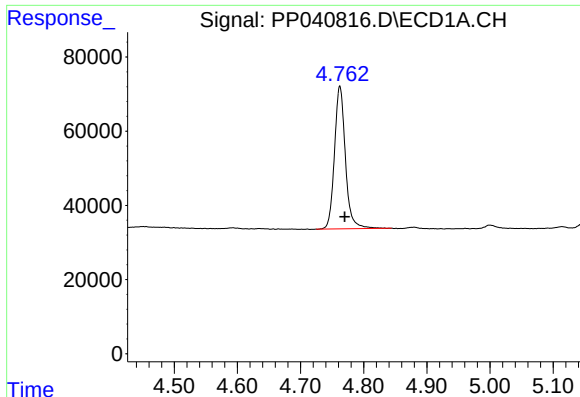

#1 Tetrachloro-m-xylene


R.T.: 4.762 min
Delta R.T.: -0.008 min
Response: 461651
Conc: 22.79 ng/ml

Instrument :
ECD_P
ClientSampleId :

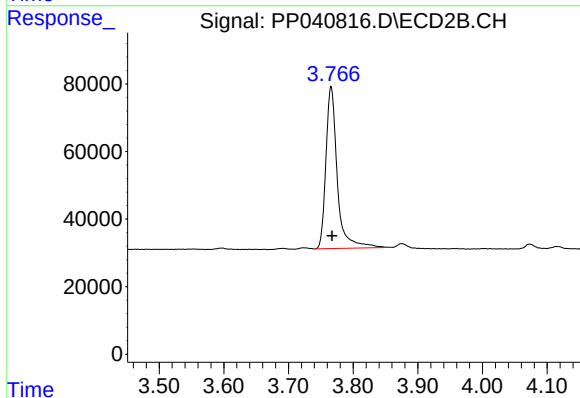


#1 Tetrachloro-m-xylene

R.T.: 3.766 min
Delta R.T.: -0.001 min
Response: 586165
Conc: 24.43 ng/ml

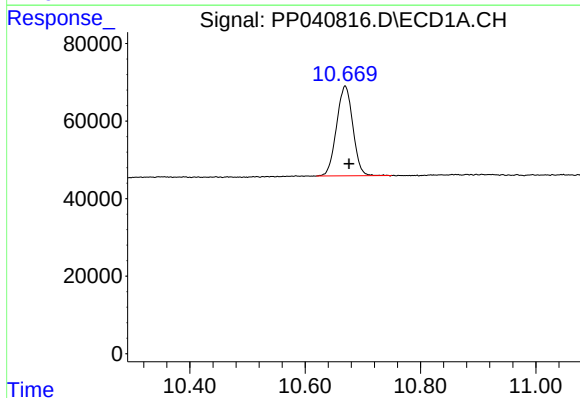


#2 Decachlorobiphenyl

R.T.: 10.669 min
Delta R.T.: -0.007 min
Response: 450410
Conc: 21.15 ng/ml

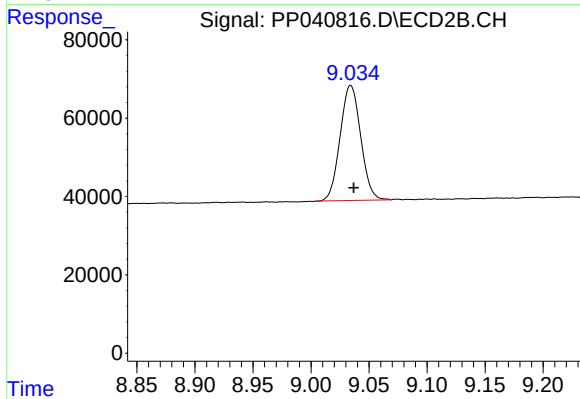

#2 Decachlorobiphenyl


R.T.: 9.034 min
Delta R.T.: -0.003 min
Response: 362962
Conc: 20.78 ng/ml

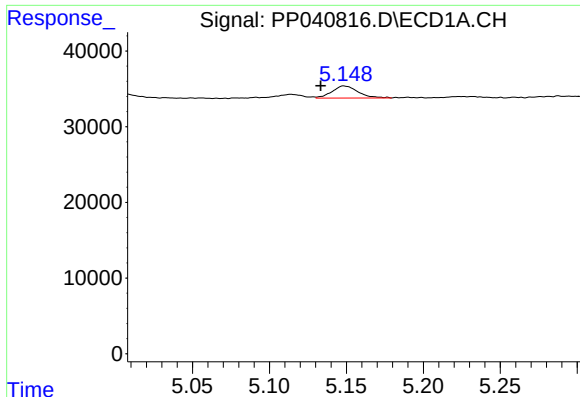

#9 AR-1221-2


R.T.: 5.149 min
Delta R.T.: 0.015 min
Response: 18963
Conc: 125.64 ng/ml

Instrument :
ECD_P
ClientSampleId :

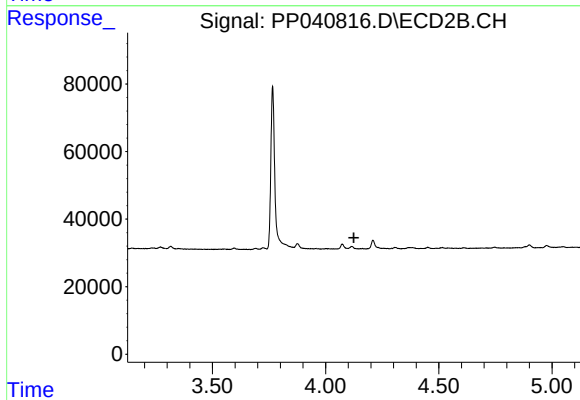


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.125 min
Response: 0
Conc: N.D.

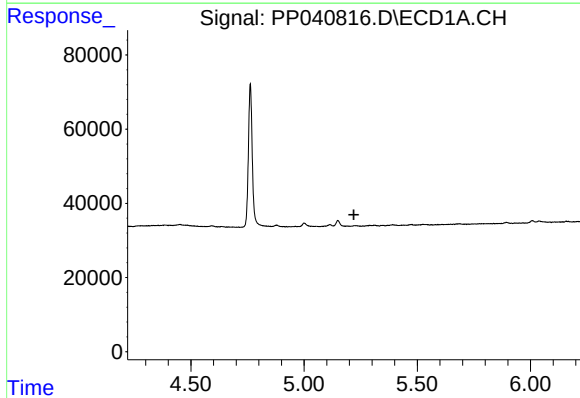


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 5.220 min
Response: 0
Conc: N.D.

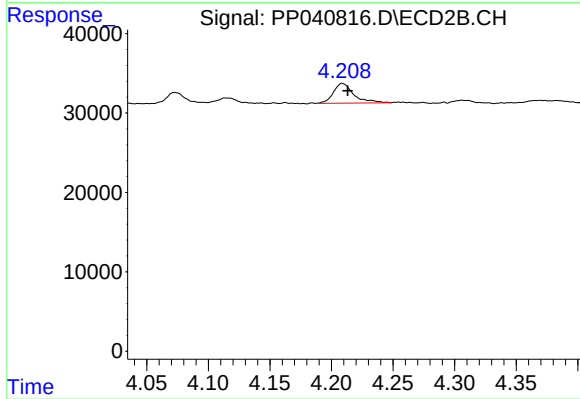

#10 AR-1221-3


R.T.: 4.209 min
Delta R.T.: -0.004 min
Response: 28714
Conc: 43.74 ng/ml

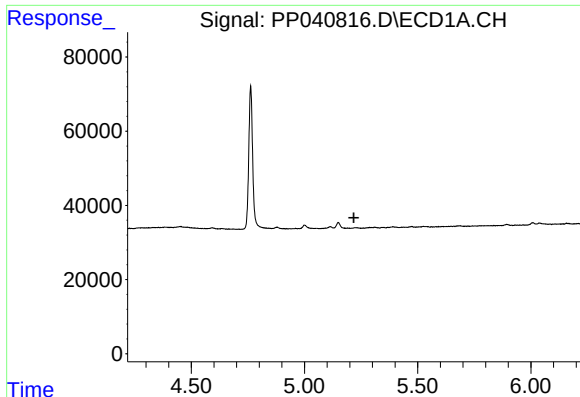

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T.: 5.218 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

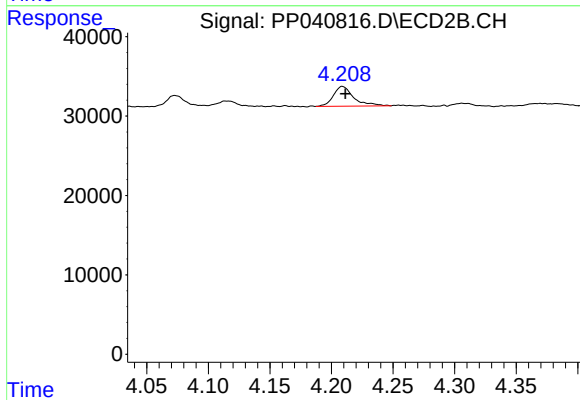


#11 AR-1232-1

R.T.: 4.209 min
Delta R.T.: -0.002 min
Response: 28714
Conc: 53.20 ng/ml

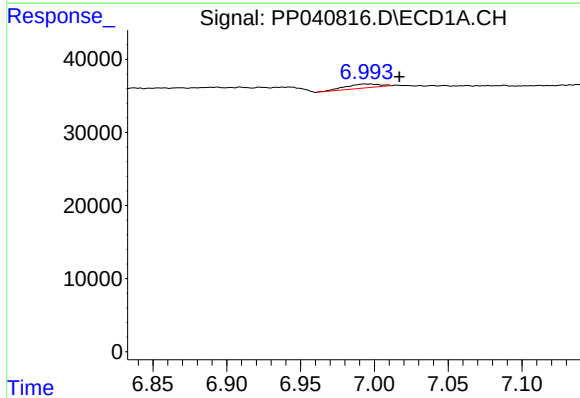


#24 AR-1248-4

R.T.: 6.994 min
Delta R.T.: -0.023 min
Response: 8982
Conc: 11.37 ng/ml

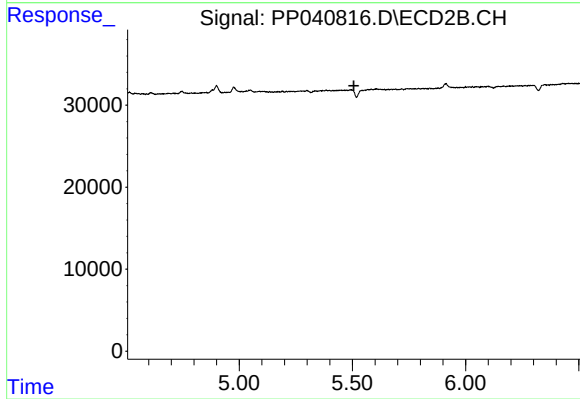

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.507 min
Response: 0
Conc: N.D.

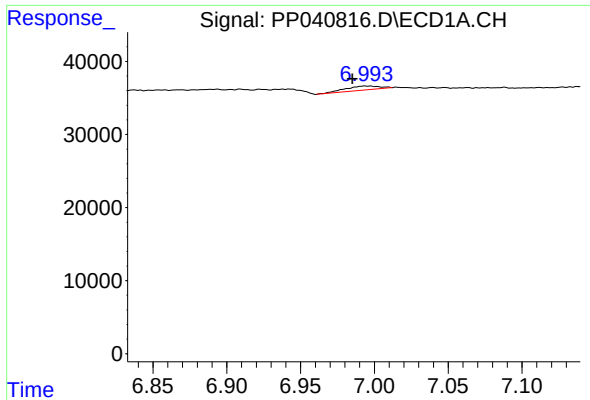

#26 AR-1254-1


R.T.: 6.994 min
Delta R.T.: 0.009 min
Response: 8982
Conc: 11.63 ng/ml

Instrument :
ECD_P
ClientSampleId :

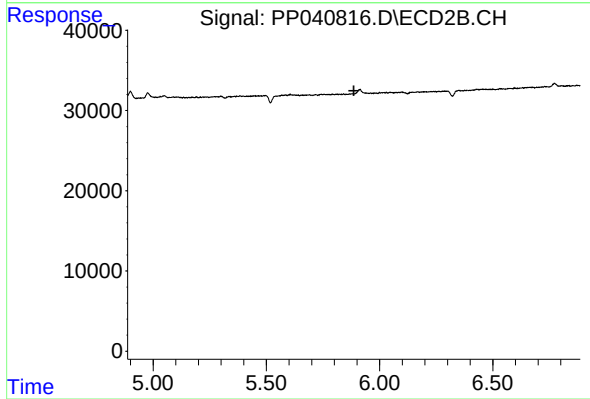


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 5.886 min
Response: 0
Conc: N.D.

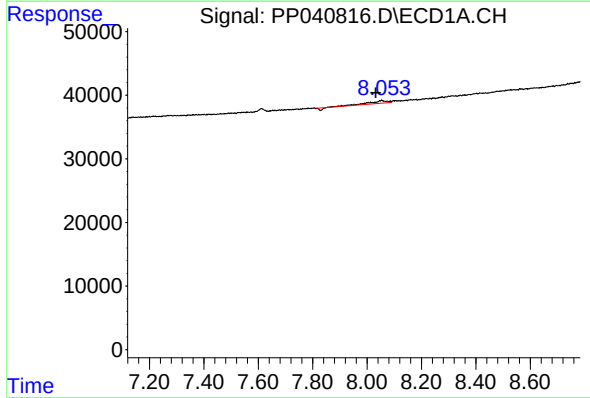


#32 AR-1260-2

R.T.: 8.054 min
Delta R.T.: 0.022 min
Response: 18293
Conc: 15.80 ng/ml

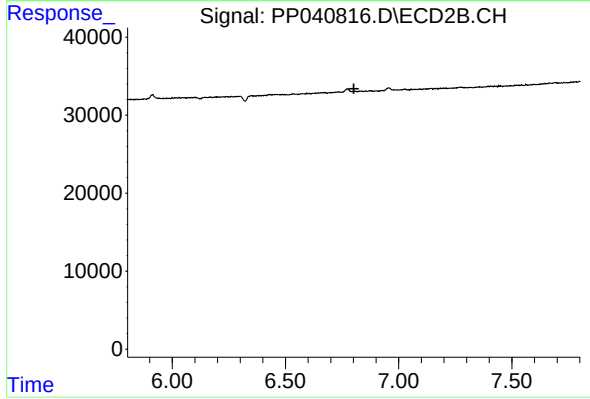

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.802 min
Response: 0
Conc: N.D.

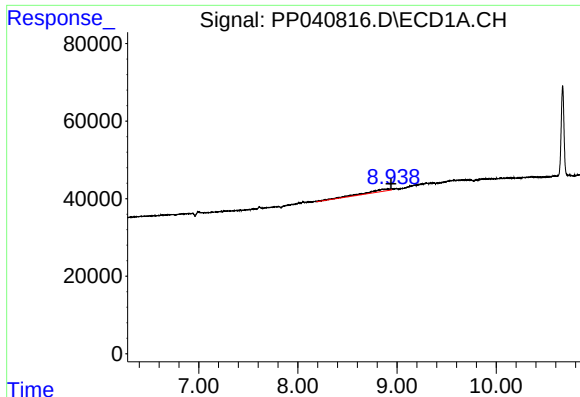

#35 AR-1260-5


R.T.: 8.938 min
Delta R.T.: -0.003 min
Response: 104046
Conc: 49.83 ng/ml

Instrument :
ECD_P
ClientSampleId :

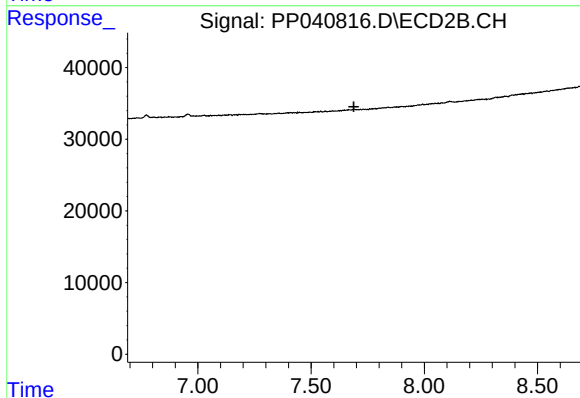


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.689 min
Response: 0
Conc: N.D.

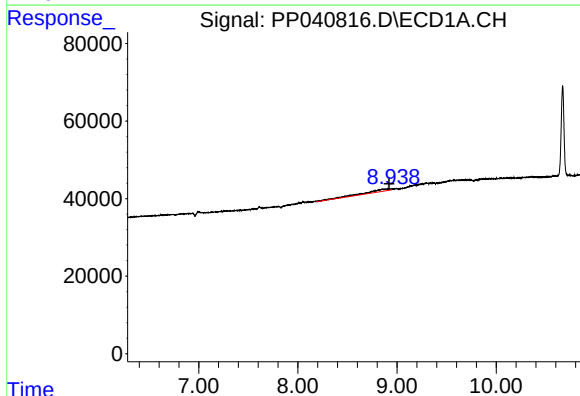

#37 AR-1262-2

R.T.: 8.938 min
Delta R.T.: 0.021 min
Response: 104046
Conc: 45.79 ng/ml

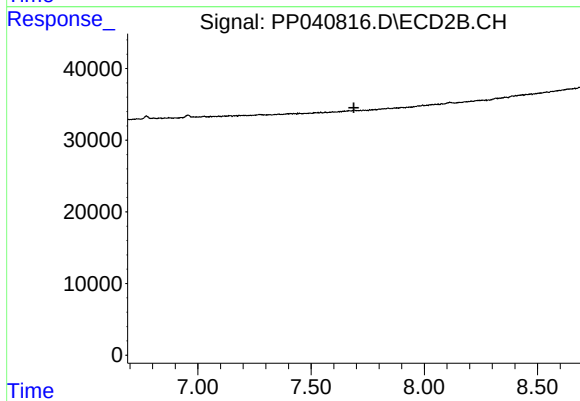

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.689 min
Response: 0
Conc: N.D.