

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP110821\  
 Data File : PP040769.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 08 Nov 2021 13:23  
 Operator : AJ\MA  
 Sample : M4407-02  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 FDR-BH-7-20211028-7.5-8

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Nov 09 00:34:08 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP110421.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Nov 04 11:28:51 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2  | Resp#1 | Resp#2 | ng/ml  | ng/ml  |
|-----------------------------|--------|-------|--------|--------|--------|--------|
| -----                       |        |       |        |        |        |        |
| System Monitoring Compounds |        |       |        |        |        |        |
| 1) SA Tetrachlo...          | 4.763  | 3.768 | 285621 | 391651 | 14.099 | 16.320 |
| 2) SA Decachlor...          | 10.669 | 9.036 | 308986 | 231704 | 14.508 | 13.268 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP110821\  
Data File : PP040769.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 08 Nov 2021 13:23  
Operator : AJ\MA  
Sample : M4407-02  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
ECD\_P  
ClientSampleId :  
FDR-BH-7-20211028-7.5-8

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Nov 09 00:34:08 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP110421.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Thu Nov 04 11:28:51 2021  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

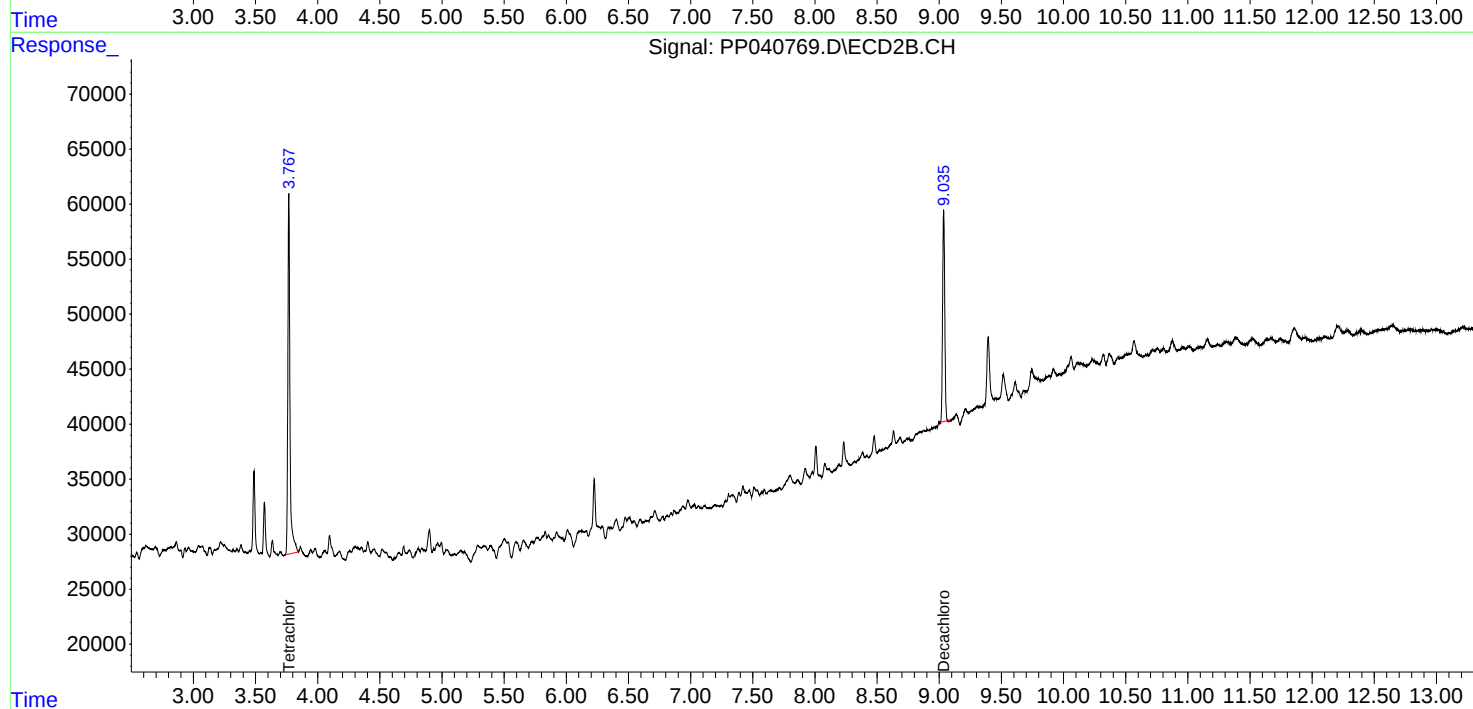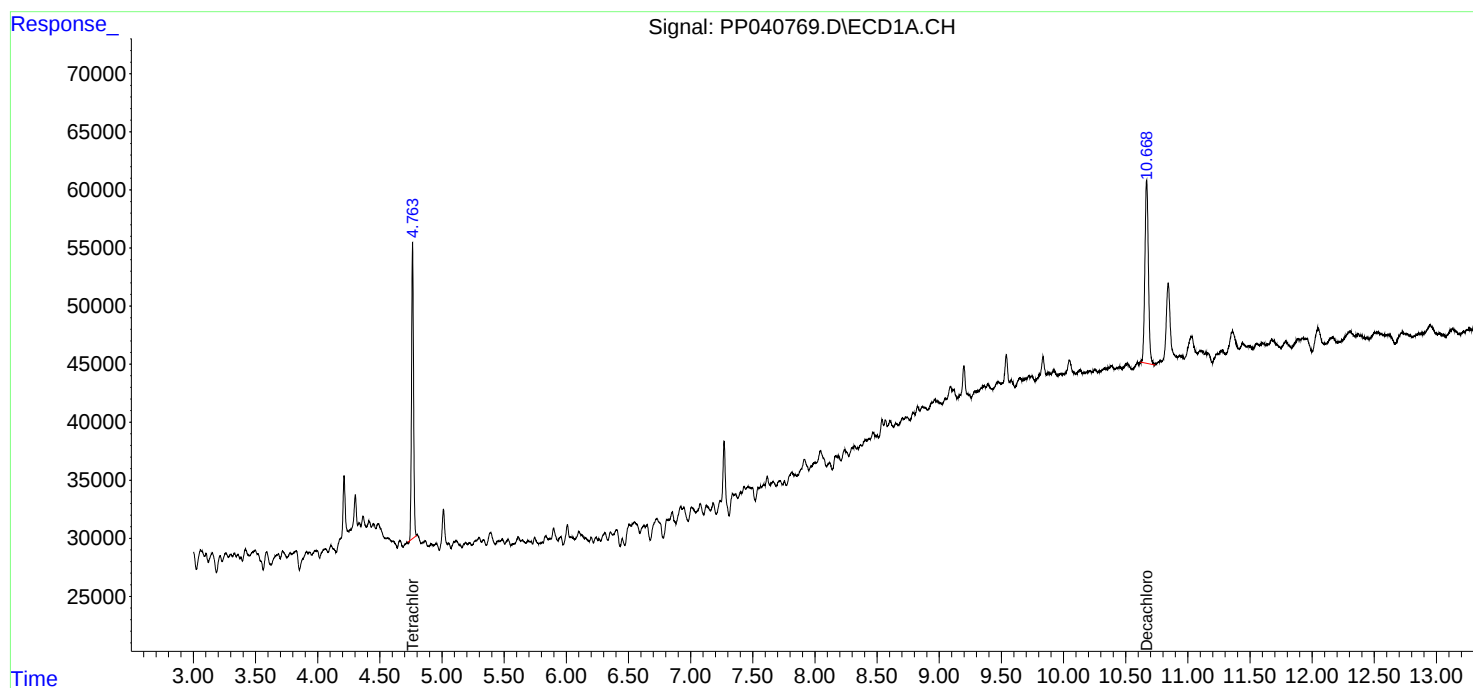


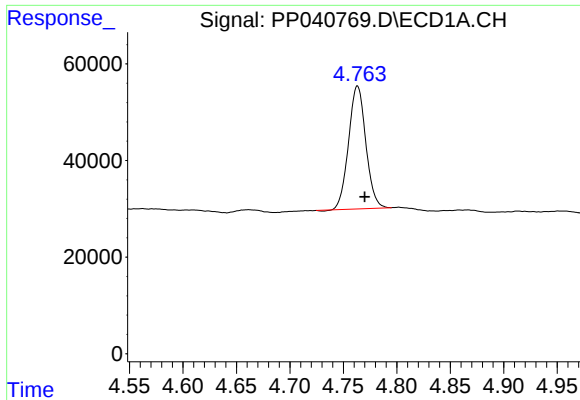

#1 Tetrachloro-m-xylene


R.T.: 4.763 min  
Delta R.T.: -0.007 min  
Response: 285621  
Conc: 14.10 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
FDR-BH-7-20211028-7.5-8

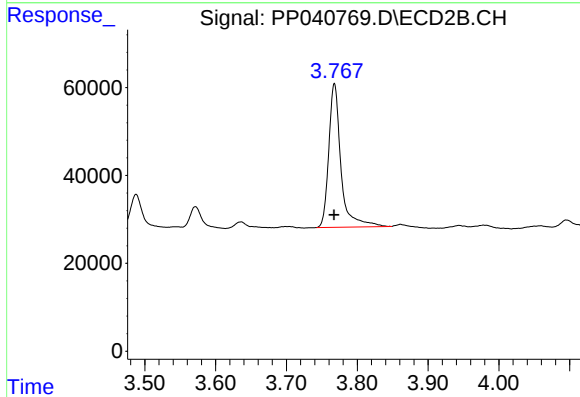


#1 Tetrachloro-m-xylene

R.T.: 3.768 min  
Delta R.T.: 0.000 min  
Response: 391651  
Conc: 16.32 ng/ml

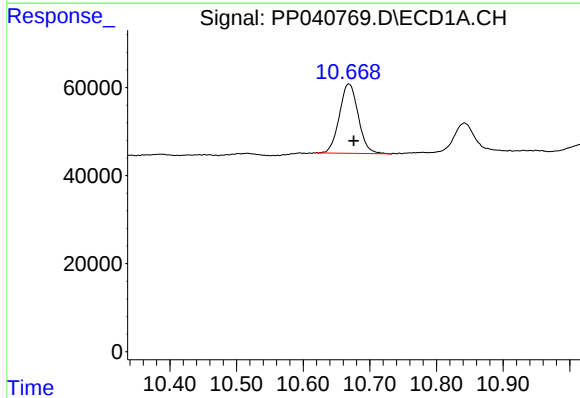

#2 Decachlorobiphenyl

R.T.: 10.669 min  
Delta R.T.: -0.007 min  
Response: 308986  
Conc: 14.51 ng/ml

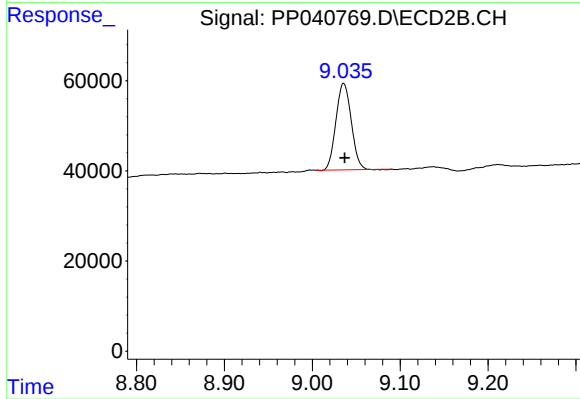

#2 Decachlorobiphenyl

R.T.: 9.036 min  
Delta R.T.: -0.001 min  
Response: 231704  
Conc: 13.27 ng/ml