

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110821\
 Data File : PP040776.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Nov 2021 15:19
 Operator : AJ\MA
 Sample : M4507-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BW-15-20211103

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 00:35:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 04 11:28:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.762	3.767	447731	550297	22.101	22.931
2)	SA Decachlor...	10.668	9.036	363803	300489	17.082	17.207

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110821\
Data File : PP040776.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Nov 2021 15:19
Operator : AJ\MA
Sample : M4507-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
BW-15-20211103

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 00:35:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 04 11:28:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

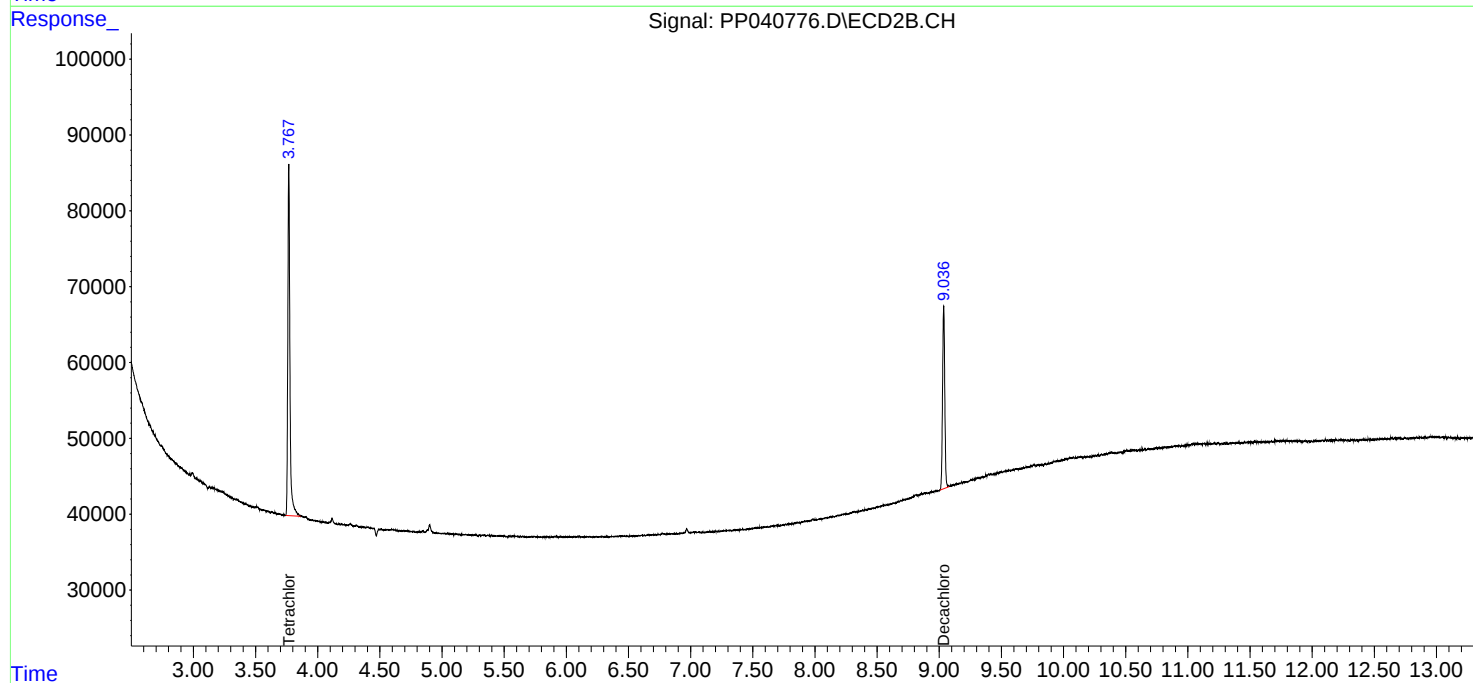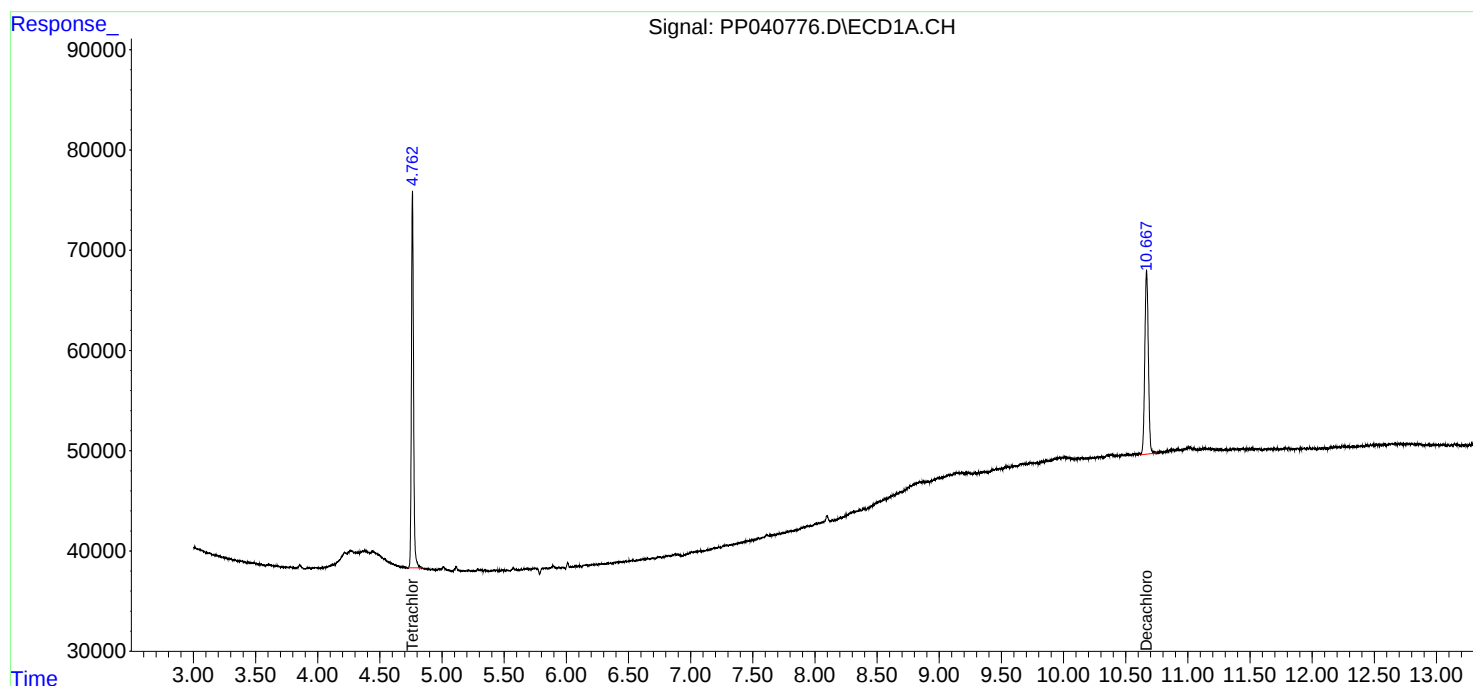


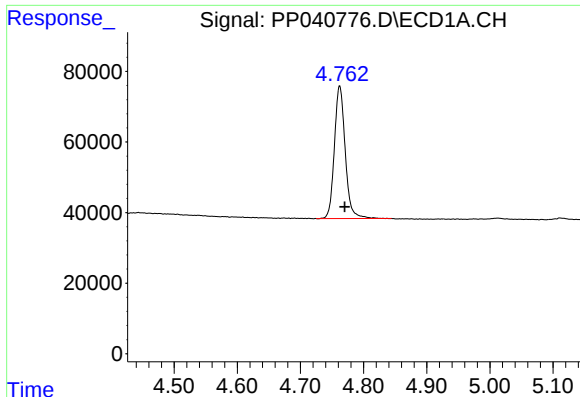

#1 Tetrachloro-m-xylene


R.T.: 4.762 min
Delta R.T.: -0.008 min
Response: 447731
Conc: 22.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
BW-15-20211103

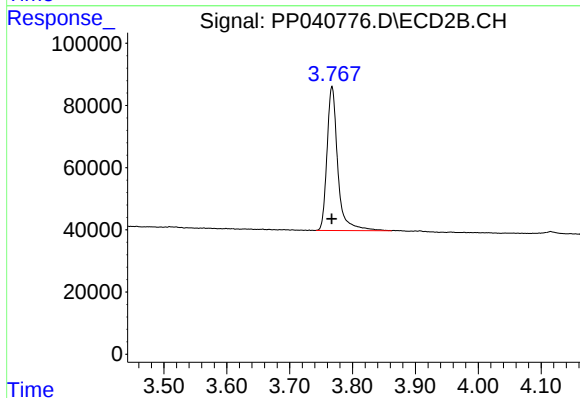


#1 Tetrachloro-m-xylene

R.T.: 3.767 min
Delta R.T.: 0.000 min
Response: 550297
Conc: 22.93 ng/ml

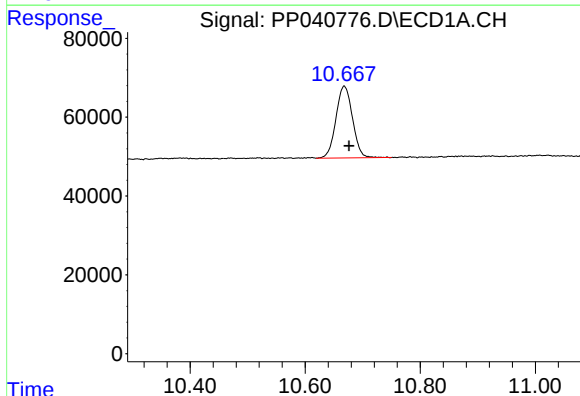

#2 Decachlorobiphenyl

R.T.: 10.668 min
Delta R.T.: -0.008 min
Response: 363803
Conc: 17.08 ng/ml

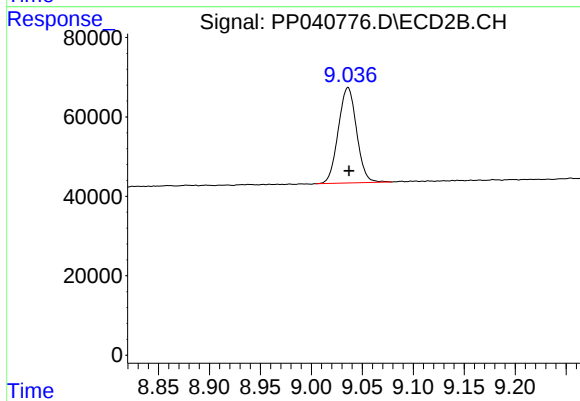

#2 Decachlorobiphenyl

R.T.: 9.036 min
Delta R.T.: 0.000 min
Response: 300489
Conc: 17.21 ng/ml