

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110921\
 Data File : PP040824.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Nov 2021 13:29
 Operator : AJ\MA
 Sample : M4506-08 20X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 01:14:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 04 11:28:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.762	3.765	14219	19384	0.702	0.808
2)	SA Decachlor...	10.671	9.035	14197	23427	0.667	1.342 #
Target Compounds							
33)	L7 AR-1260-3	8.426f	0.000	9009	0	10.203	N.D. #
34)	L7 AR-1260-4	8.635	0.000	9570	0	9.057	N.D. #
38)	L8 AR-1262-3	9.224	0.000	13903	0	13.076	N.D. #
39)	L8 AR-1262-4	9.274f	8.038	3744	11834	6.385	8.443 #
41)	L9 AR-1268-1	9.224	0.000	13903	0	5.100	N.D. #
42)	L9 AR-1268-2	0.000	8.038	0	11834	N.D.	5.937 #
45)	L9 AR-1268-5	0.000	8.824f	0	8390	N.D.	1.555 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110921\
Data File : PP040824.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Nov 2021 13:29
Operator : AJ\MA
Sample : M4506-08 20X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 01:14:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 04 11:28:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

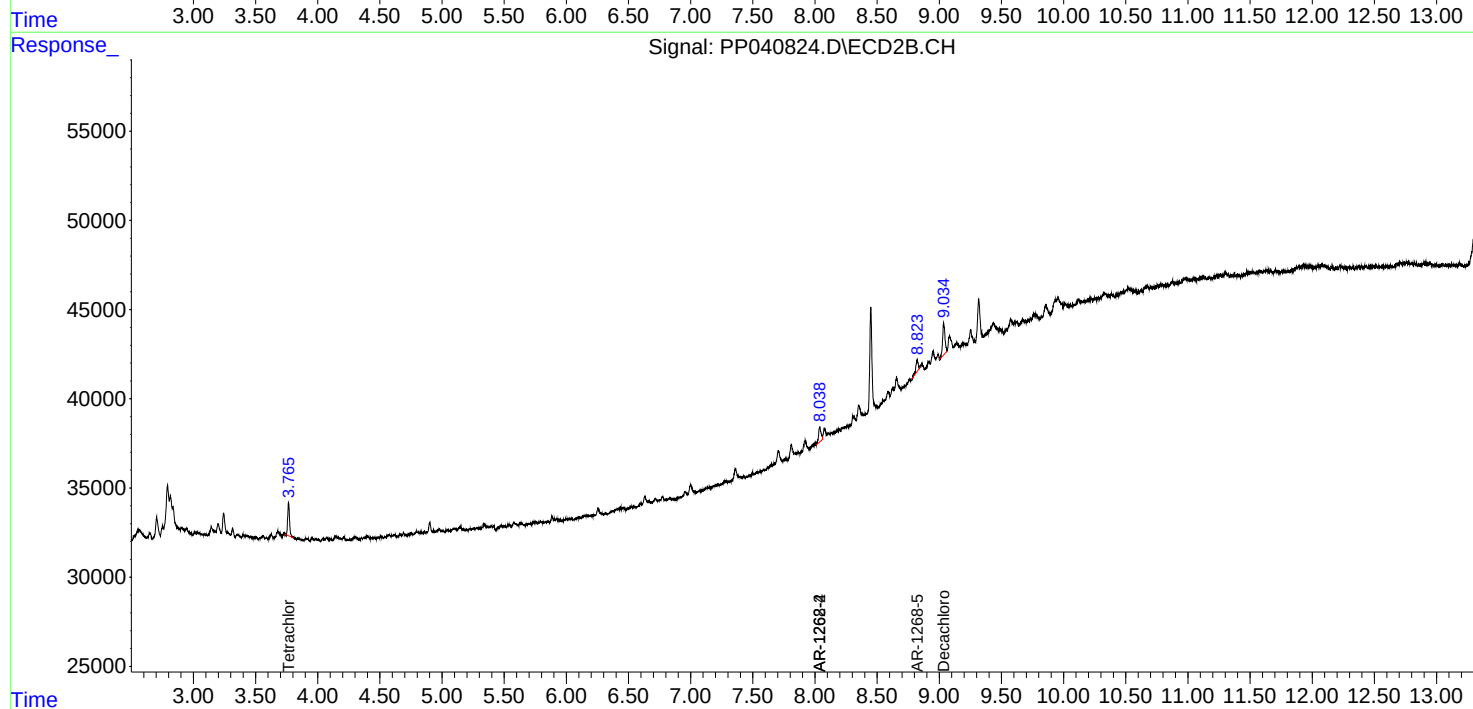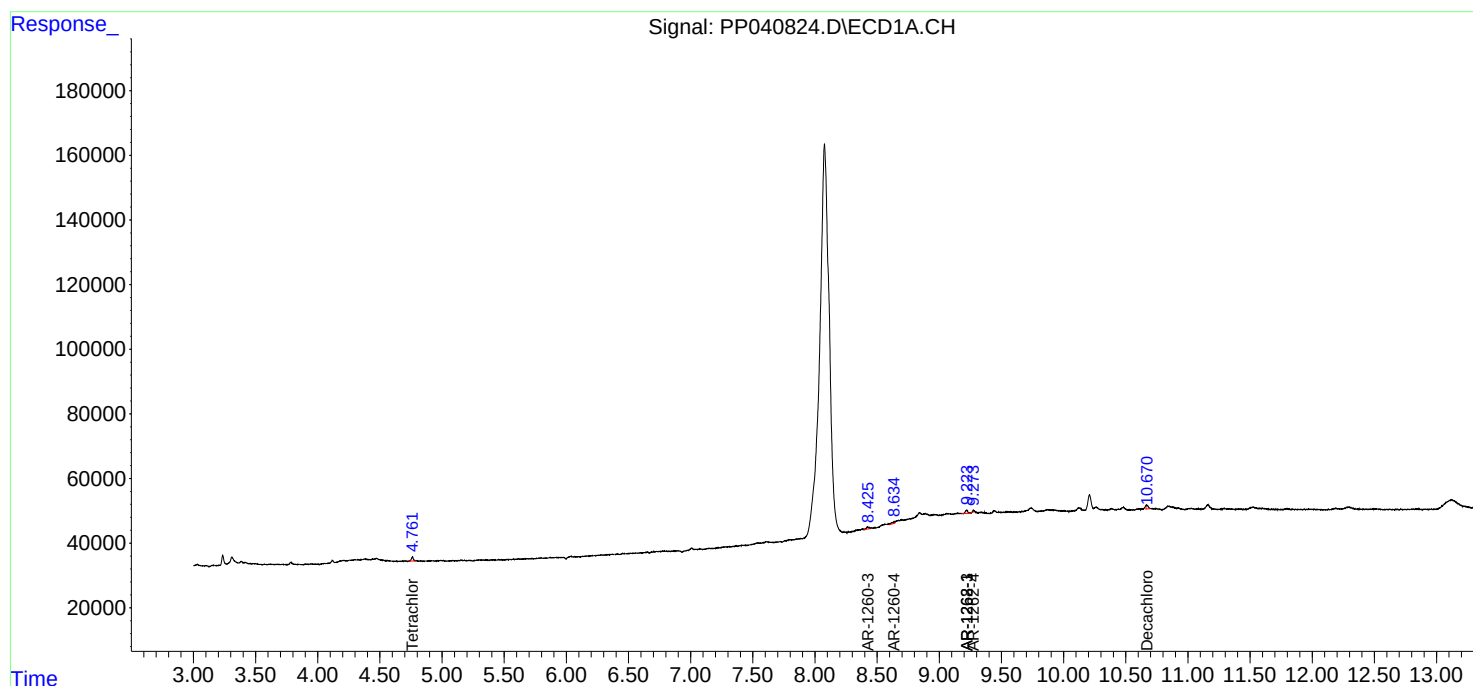


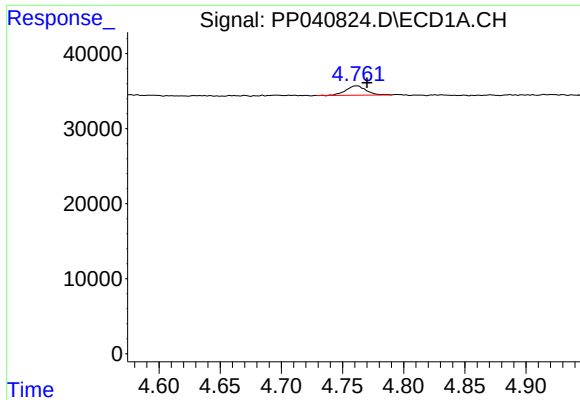

#1 Tetrachloro-m-xylene


R.T.: 4.762 min
Delta R.T.: -0.008 min
Response: 14219
Conc: 0.70 ng/ml

Instrument :
ECD_P
ClientSampleId :

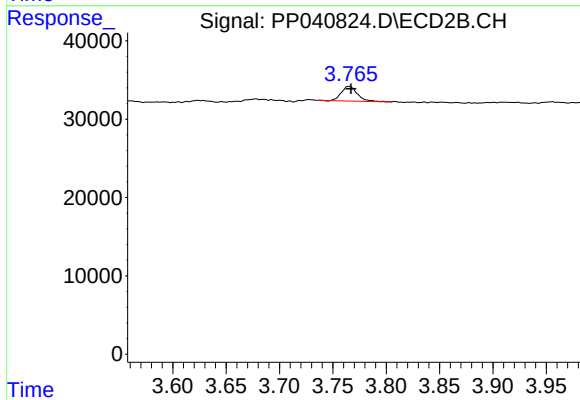


#1 Tetrachloro-m-xylene

R.T.: 3.765 min
Delta R.T.: -0.002 min
Response: 19384
Conc: 0.81 ng/ml

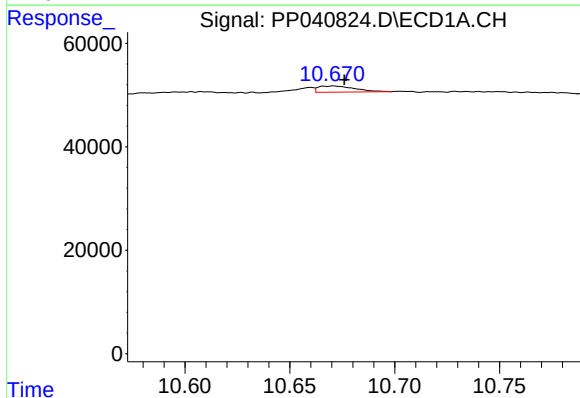


#2 Decachlorobiphenyl

R.T.: 10.671 min
Delta R.T.: -0.005 min
Response: 14197
Conc: 0.67 ng/ml

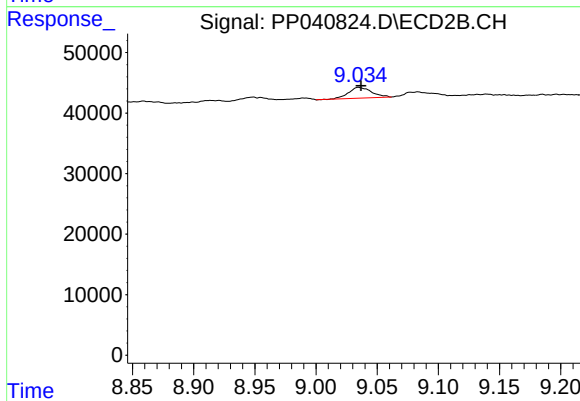

#2 Decachlorobiphenyl


R.T.: 9.035 min
Delta R.T.: -0.002 min
Response: 23427
Conc: 1.34 ng/ml

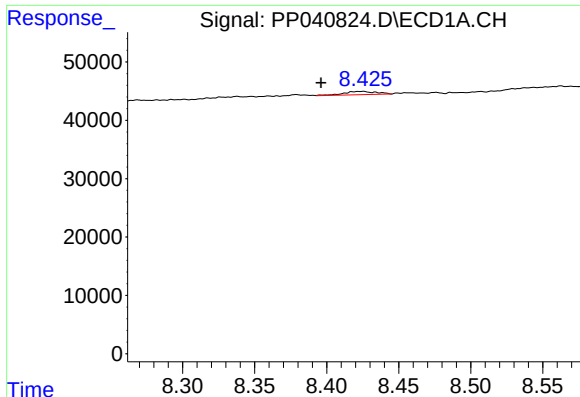

#33 AR-1260-3


R.T.: 8.426 min
Delta R.T.: 0.030 min
Response: 9009
Conc: 10.20 ng/ml

Instrument :
ECD_P
ClientSampleId :

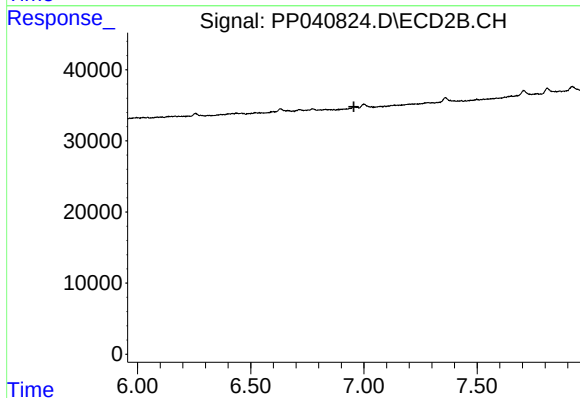


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 6.956 min
Response: 0
Conc: N.D.

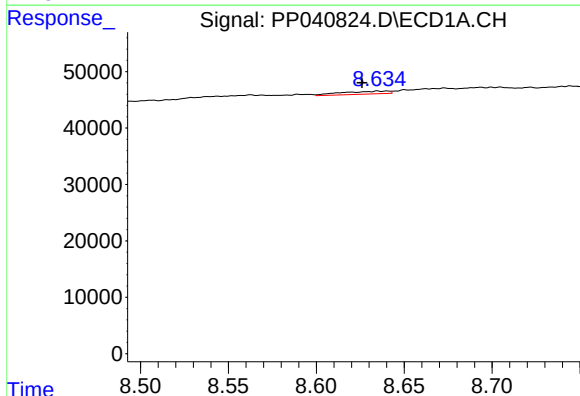


#34 AR-1260-4

R.T.: 8.635 min
Delta R.T.: 0.009 min
Response: 9570
Conc: 9.06 ng/ml

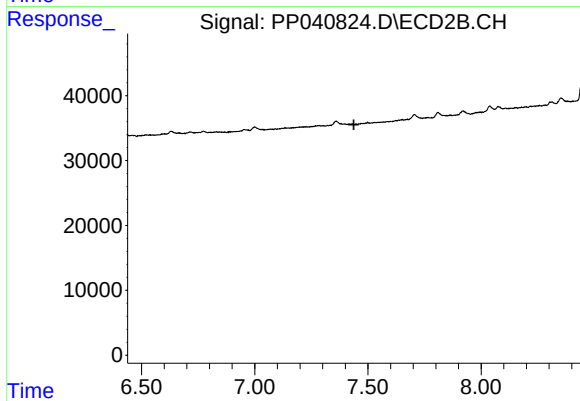

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.438 min
Response: 0
Conc: N.D.

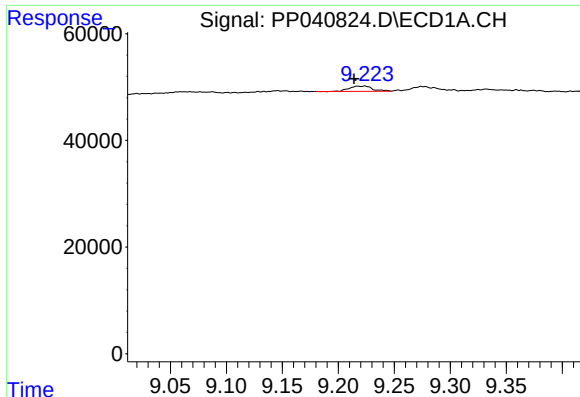

#38 AR-1262-3


R.T.: 9.224 min
Delta R.T.: 0.010 min
Response: 13903
Conc: 13.08 ng/ml

Instrument :
ECD_P
ClientSampleId :

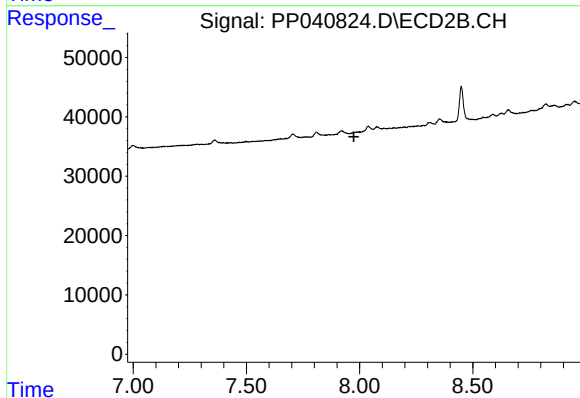


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 7.974 min
Response: 0
Conc: N.D.

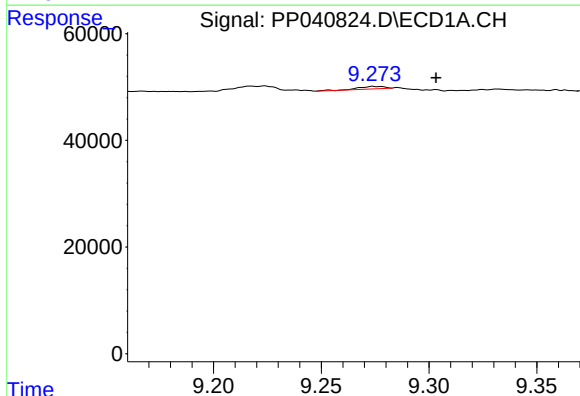


#39 AR-1262-4

R.T.: 9.274 min
Delta R.T.: -0.029 min
Response: 3744
Conc: 6.38 ng/ml

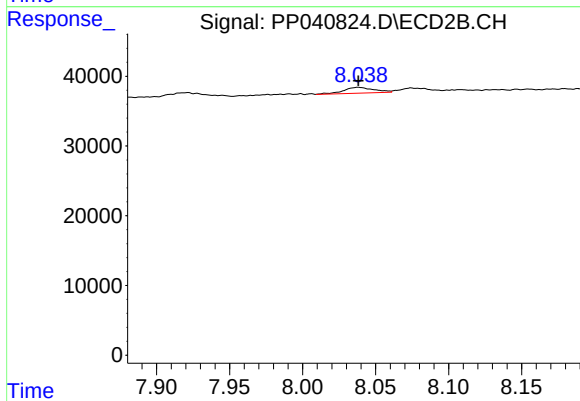

#39 AR-1262-4


R.T.: 8.038 min
Delta R.T.: 0.000 min
Response: 11834
Conc: 8.44 ng/ml

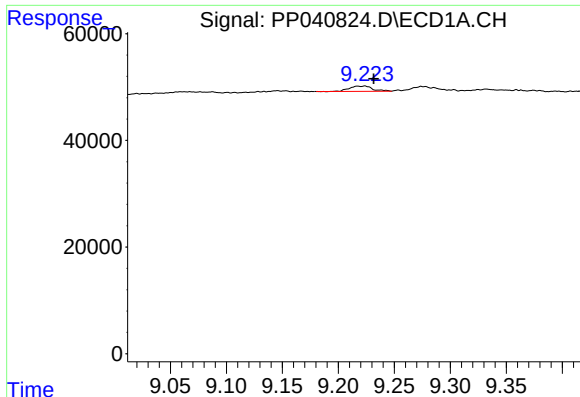

#41 AR-1268-1


R.T.: 9.224 min
Delta R.T.: -0.008 min
Response: 13903
Conc: 5.10 ng/ml

Instrument :
ECD_P
ClientSampleId :

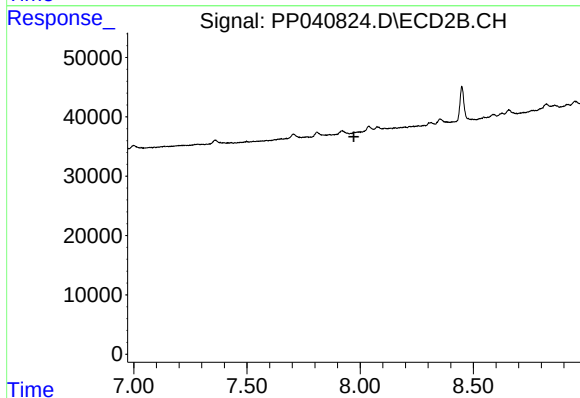


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 7.972 min
Response: 0
Conc: N.D.

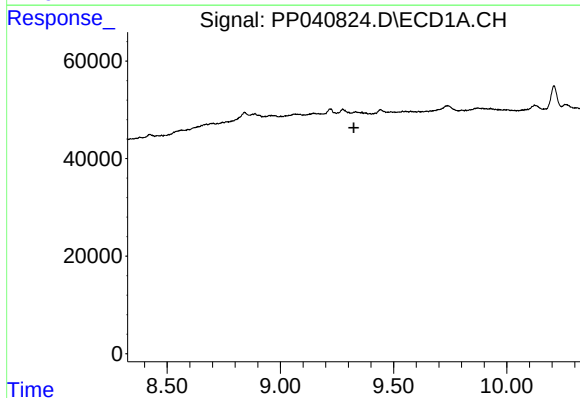


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 9.324 min
Response: 0
Conc: N.D.

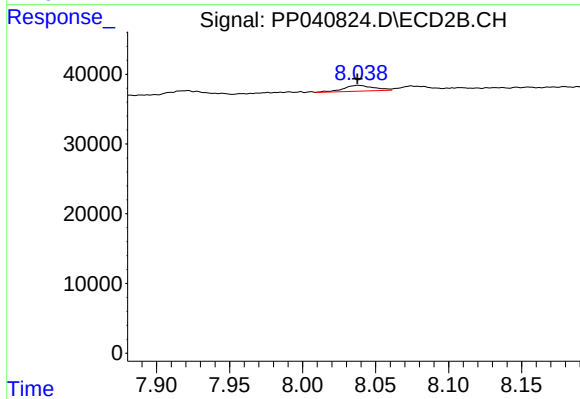

#42 AR-1268-2


R.T.: 8.038 min
Delta R.T.: 0.000 min
Response: 11834
Conc: 5.94 ng/ml

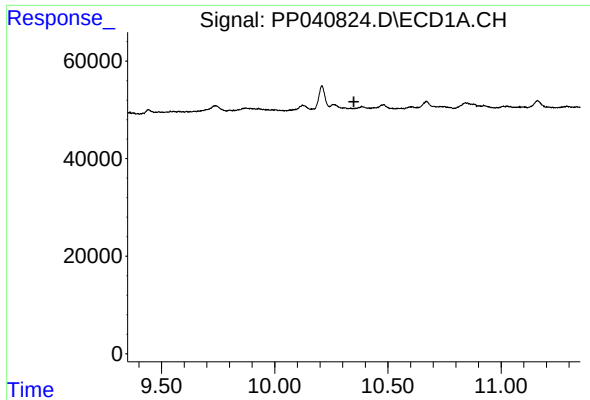

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.350 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

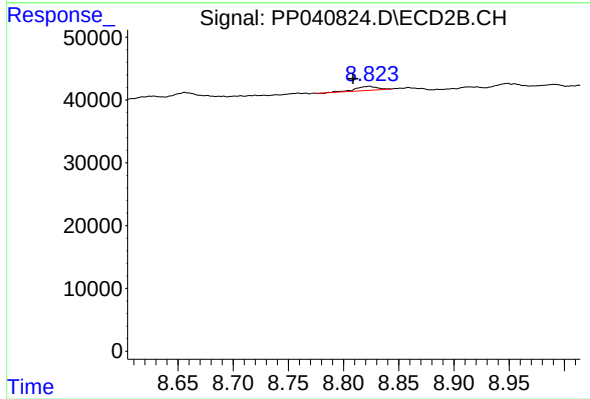

#45 AR-1268-5

R.T.: 8.824 min
Delta R.T.: 0.015 min
Response: 8390
Conc: 1.55 ng/ml