

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110921\
 Data File : PP040842.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Nov 2021 18:29
 Operator : AJ\MA
 Sample : M4570-11 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 01:20:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 04 11:28:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.762	3.766	40261	61102	1.987	2.546 #
2) SA Decachlor...	10.669	9.035	43212	32712	2.029	1.873
Target Compounds						
32) L7 AR-1260-2	0.000	6.819f	0	21616	N.D.	21.482 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110921\
Data File : PP040842.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Nov 2021 18:29
Operator : AJ\MA
Sample : M4570-11 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 01:20:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 04 11:28:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

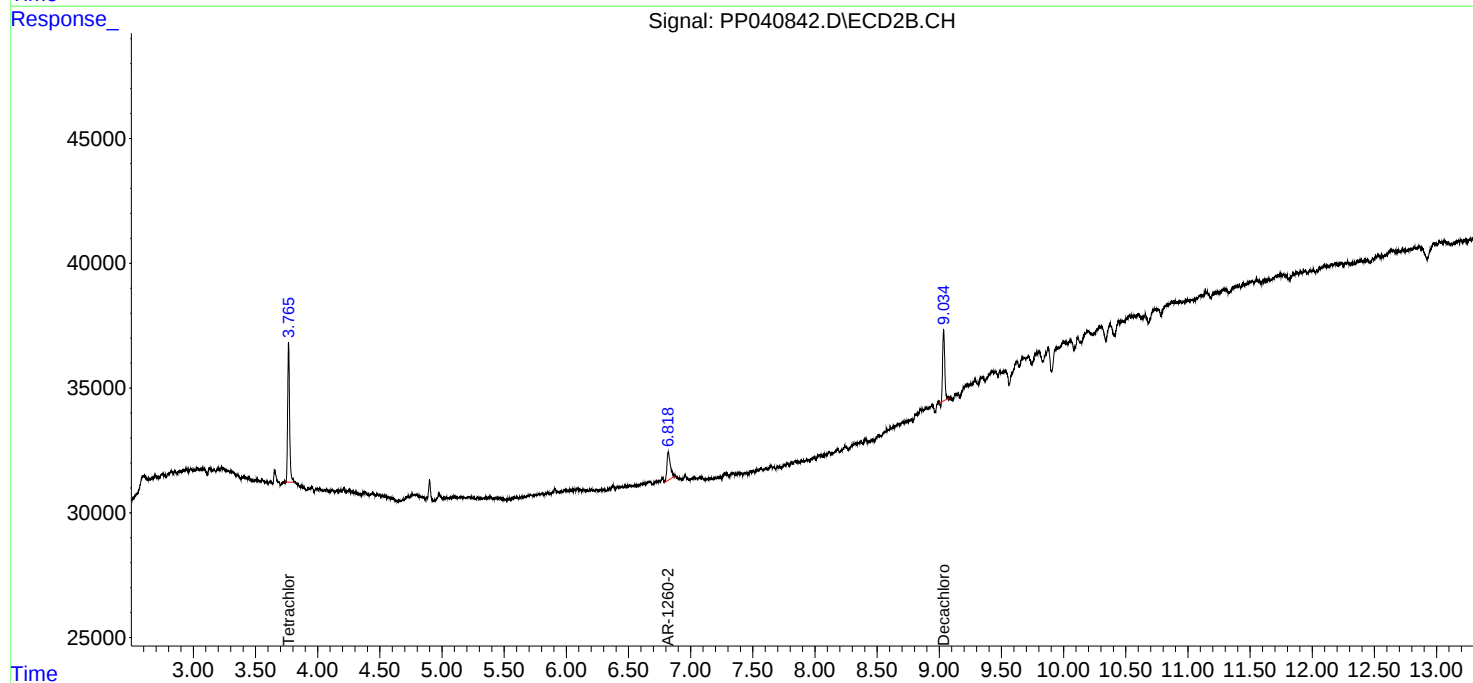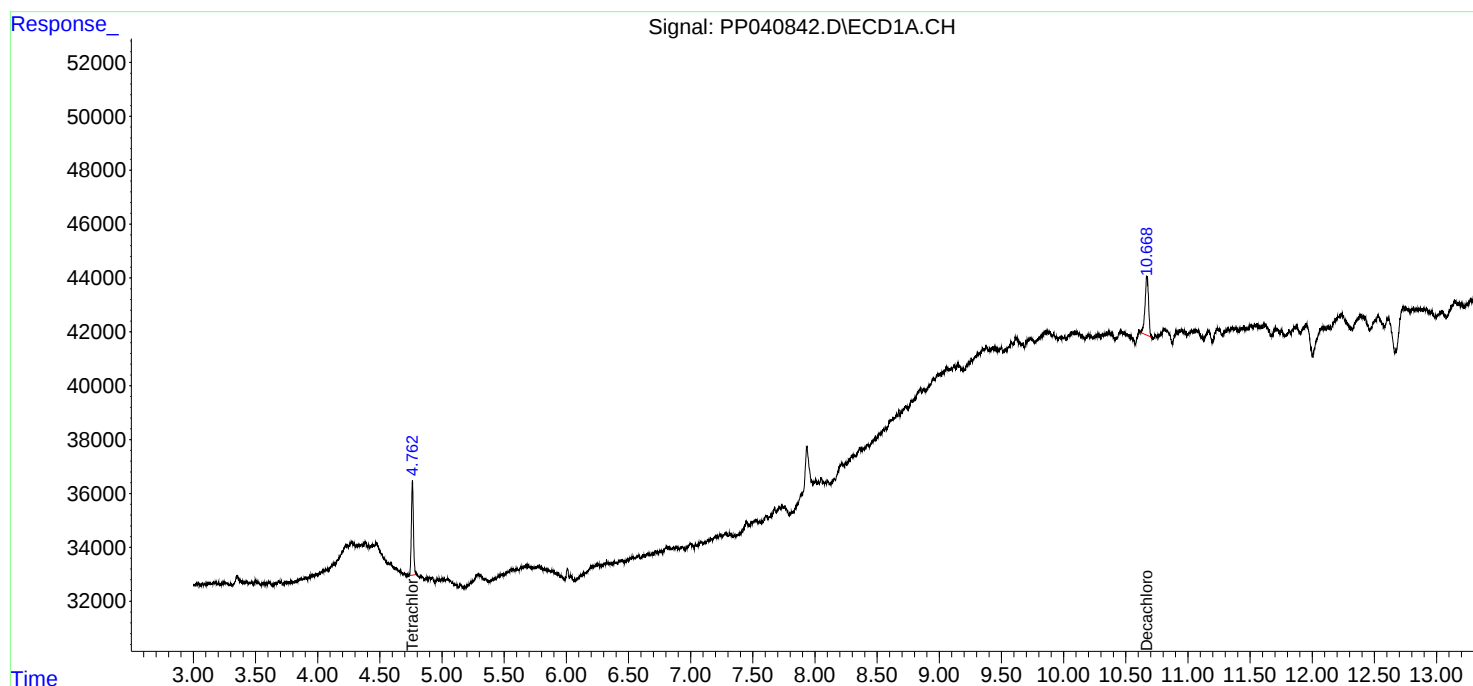


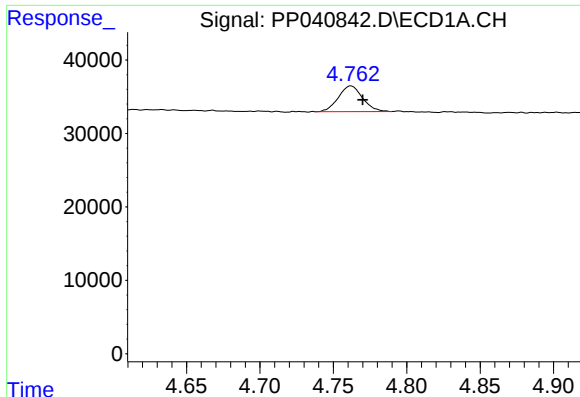

#1 Tetrachloro-m-xylene


R.T.: 4.762 min
Delta R.T.: -0.008 min
Response: 40261
Conc: 1.99 ng/ml

Instrument :
ECD_P
ClientSampleId :

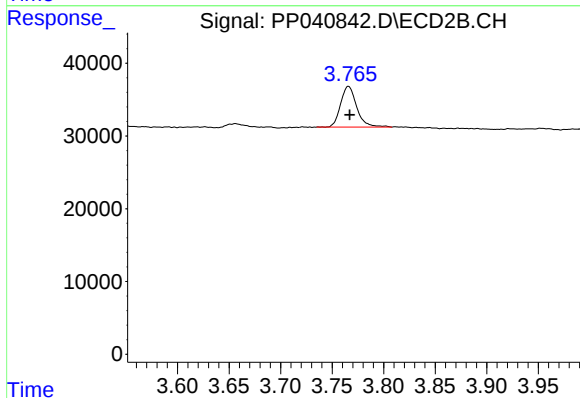


#1 Tetrachloro-m-xylene

R.T.: 3.766 min
Delta R.T.: -0.001 min
Response: 61102
Conc: 2.55 ng/ml

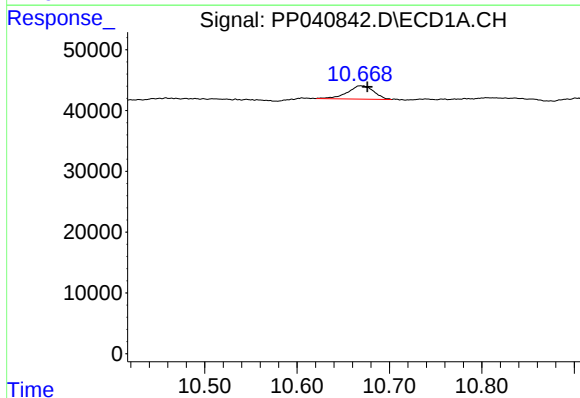


#2 Decachlorobiphenyl

R.T.: 10.669 min
Delta R.T.: -0.007 min
Response: 43212
Conc: 2.03 ng/ml

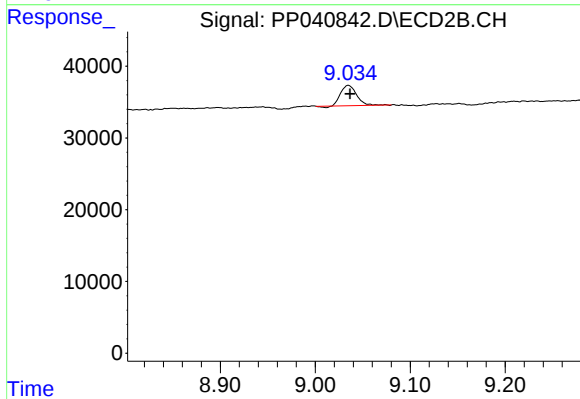

#2 Decachlorobiphenyl


R.T.: 9.035 min
Delta R.T.: -0.002 min
Response: 32712
Conc: 1.87 ng/ml

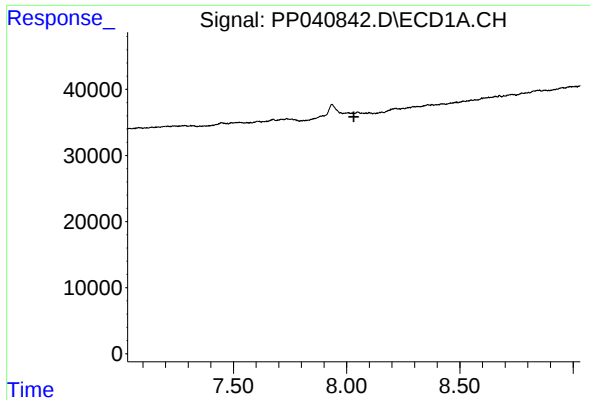

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 8.032 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

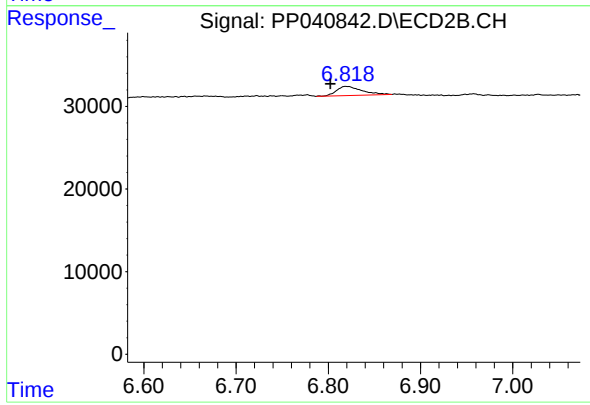

#32 AR-1260-2

R.T.: 6.819 min
Delta R.T.: 0.017 min
Response: 21616
Conc: 21.48 ng/ml