

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110921\
 Data File : PP040855.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Nov 2021 22:06
 Operator : AJ\MA
 Sample : M4544-02 10X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 01:24:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 04 11:28:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.763	3.767	31613	47059	1.560	1.961 #
2)	SA Decachlor...	10.670	9.035	40779	24566	1.915	1.407 #
Target Compounds							
28)	L6 AR-1254-3	7.609	0.000	16007	0	11.890	N.D. #
32)	L7 AR-1260-2	8.027	0.000	42358	0	36.588	N.D. #
38)	L8 AR-1262-3	0.000	7.986	0	35814	N.D.	46.191 #
39)	L8 AR-1262-4	0.000	8.025	0	252	N.D.	0.180 #
41)	L9 AR-1268-1	9.255f	7.986	1776	35814	0.651	16.703 #
42)	L9 AR-1268-2	0.000	8.025	0	252	N.D.	0.127 #
43)	L9 AR-1268-3	0.000	8.240	0	71372	N.D.	40.857 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110921\
Data File : PP040855.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Nov 2021 22:06
Operator : AJ\MA
Sample : M4544-02 10X
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 01:24:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 04 11:28:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

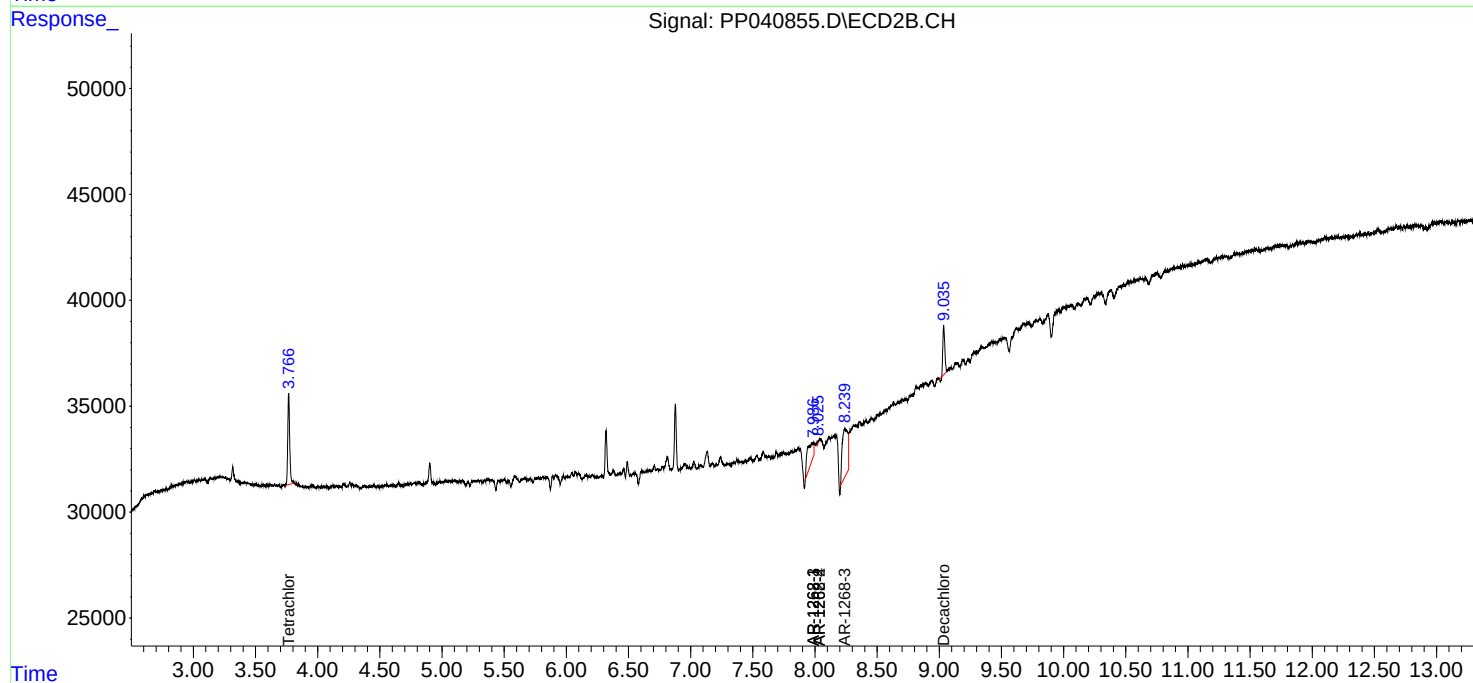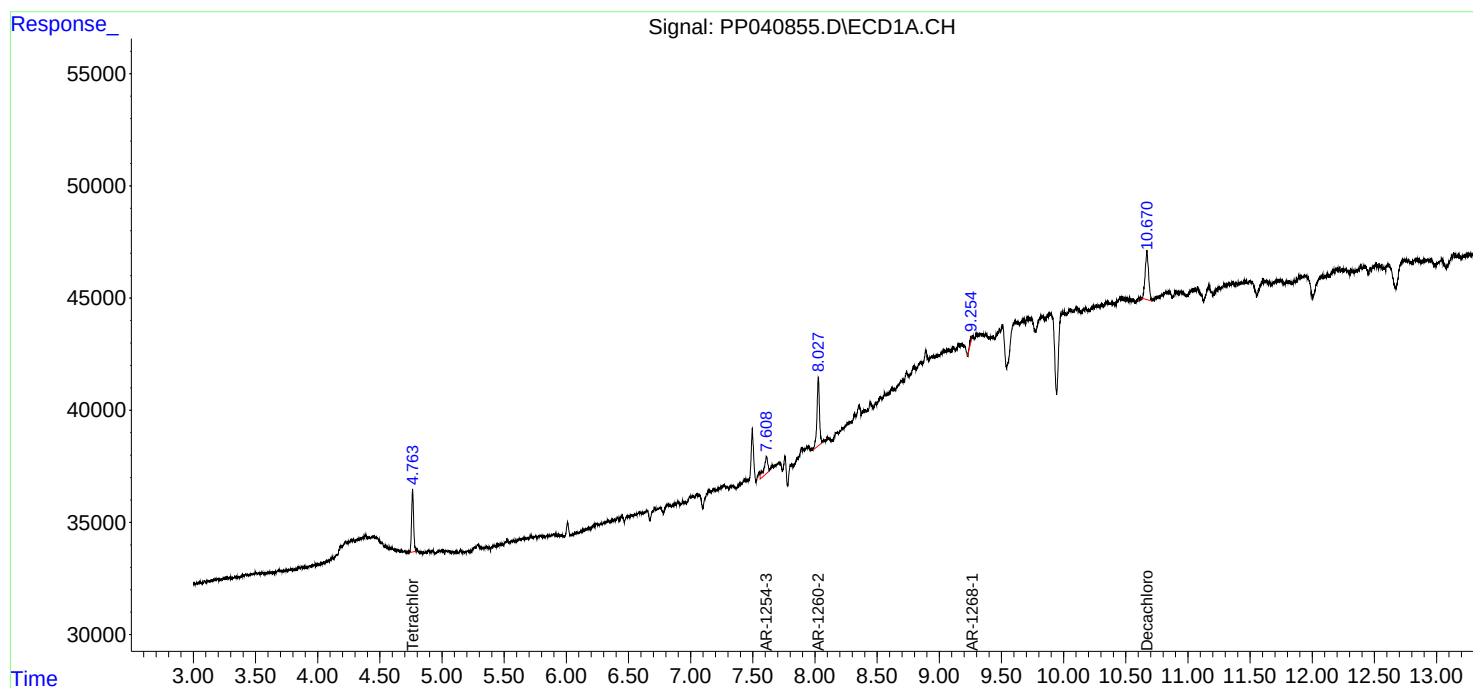


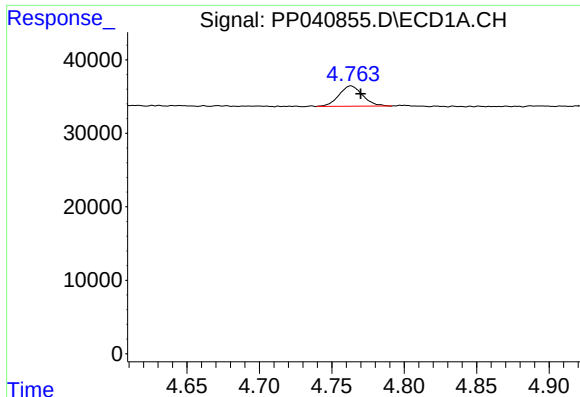

#1 Tetrachloro-m-xylene


R.T.: 4.763 min
Delta R.T.: -0.007 min
Response: 31613
Conc: 1.56 ng/ml

Instrument :
ECD_P
ClientSampleId :

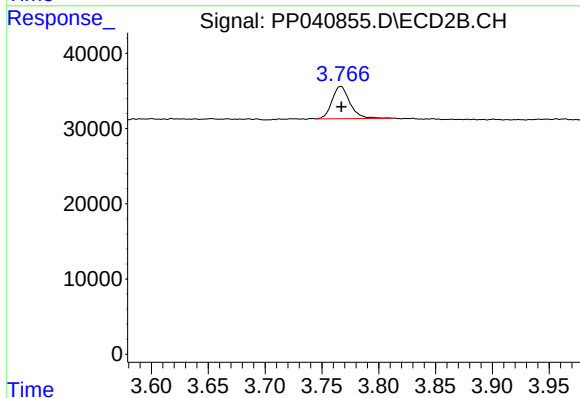


#1 Tetrachloro-m-xylene

R.T.: 3.767 min
Delta R.T.: 0.000 min
Response: 47059
Conc: 1.96 ng/ml

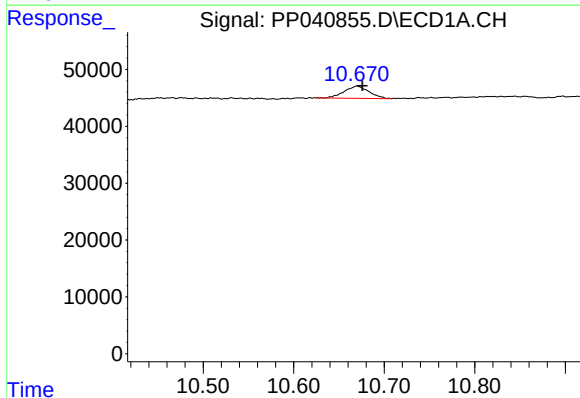


#2 Decachlorobiphenyl

R.T.: 10.670 min
Delta R.T.: -0.006 min
Response: 40779
Conc: 1.91 ng/ml

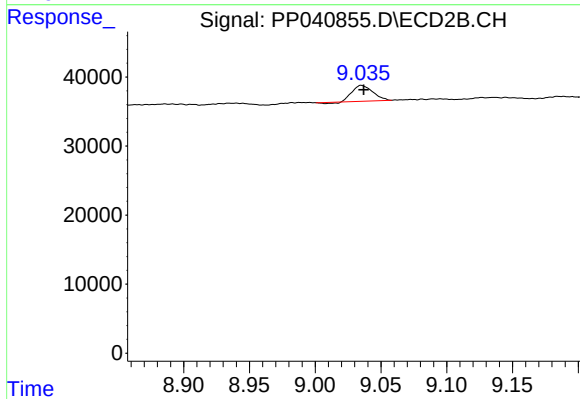

#2 Decachlorobiphenyl


R.T.: 9.035 min
Delta R.T.: -0.002 min
Response: 24566
Conc: 1.41 ng/ml

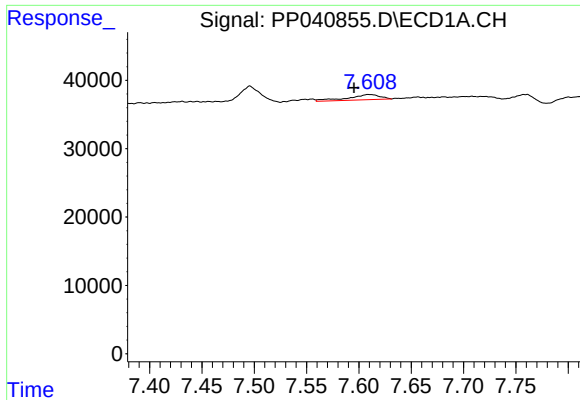

#28 AR-1254-3


R.T.: 7.609 min
Delta R.T.: 0.013 min
Response: 16007
Conc: 11.89 ng/ml

Instrument :
ECD_P
ClientSampleId :

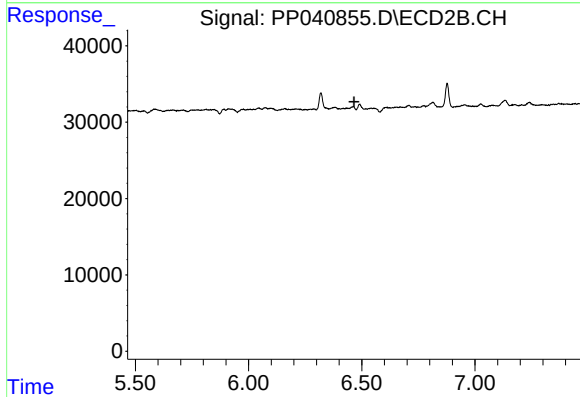


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.466 min
Response: 0
Conc: N.D.

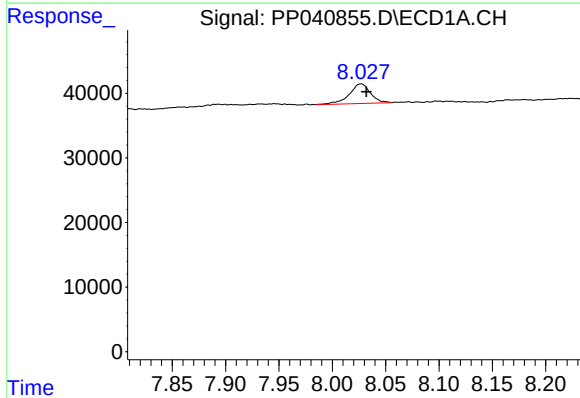


#32 AR-1260-2

R.T.: 8.027 min
Delta R.T.: -0.005 min
Response: 42358
Conc: 36.59 ng/ml

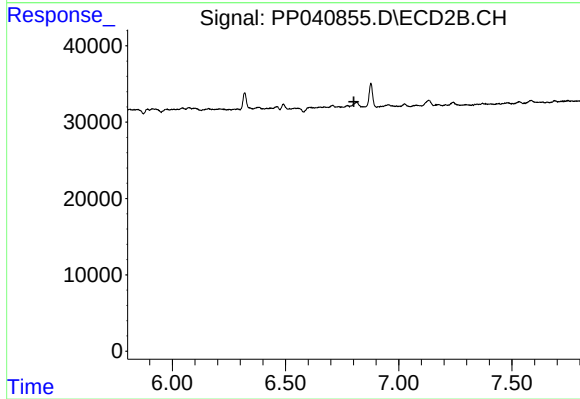

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.802 min
Response: 0
Conc: N.D.

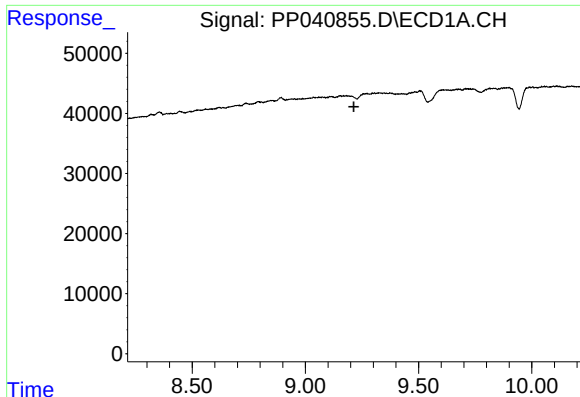

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 9.214 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

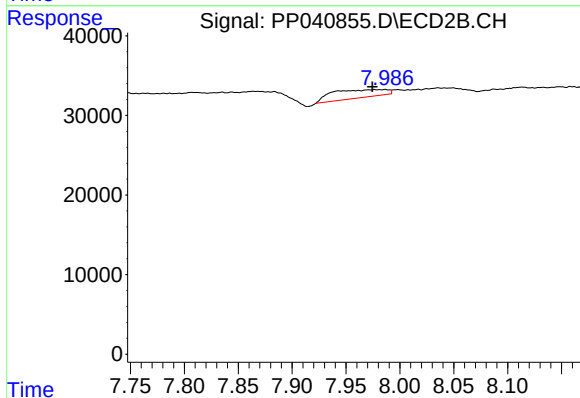


#38 AR-1262-3

R.T.: 7.986 min
Delta R.T.: 0.012 min
Response: 35814
Conc: 46.19 ng/ml

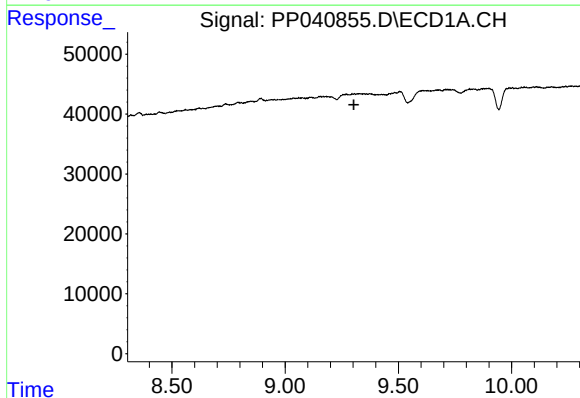


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T.: 9.303 min
Response: 0
Conc: N.D.

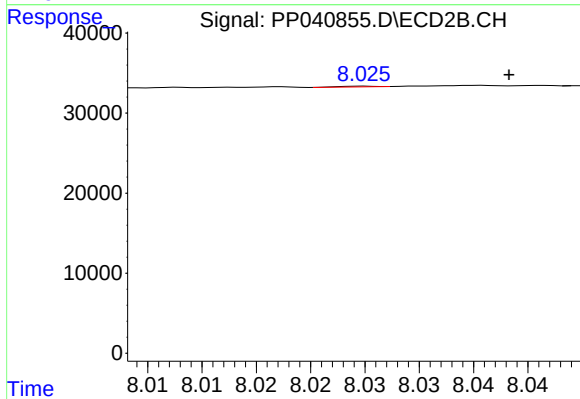

#39 AR-1262-4


R.T.: 8.025 min
Delta R.T.: -0.013 min
Response: 252
Conc: 0.18 ng/ml

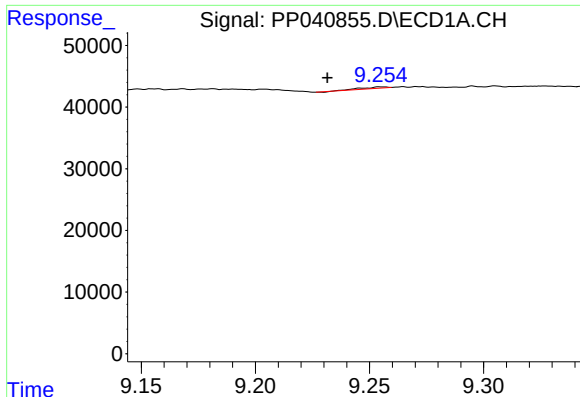

#41 AR-1268-1


R.T.: 9.255 min
Delta R.T.: 0.023 min
Response: 1776
Conc: 0.65 ng/ml

Instrument :
ECD_P
ClientSampleId :

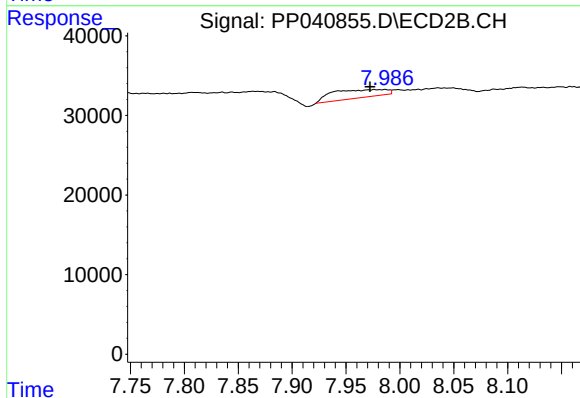


#41 AR-1268-1

R.T.: 7.986 min
Delta R.T.: 0.014 min
Response: 35814
Conc: 16.70 ng/ml

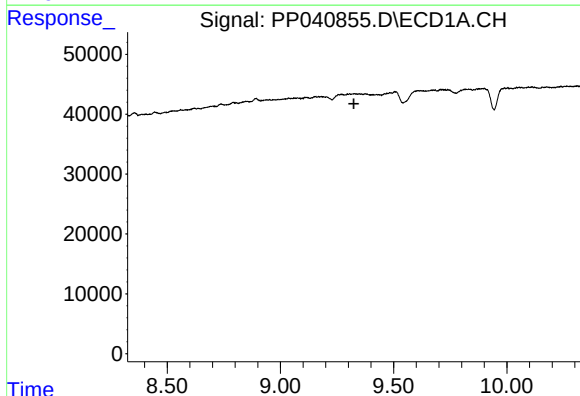


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 9.324 min
Response: 0
Conc: N.D.

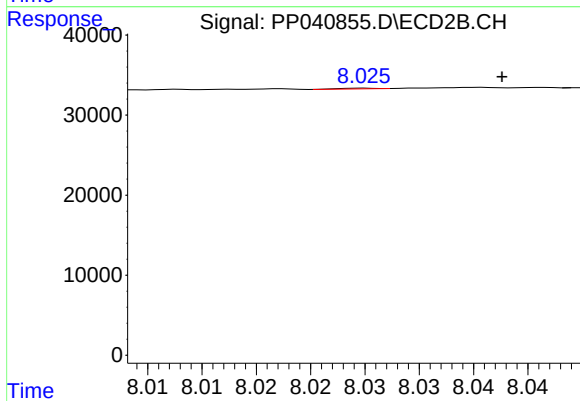

#42 AR-1268-2


R.T.: 8.025 min
Delta R.T.: -0.013 min
Response: 252
Conc: 0.13 ng/ml

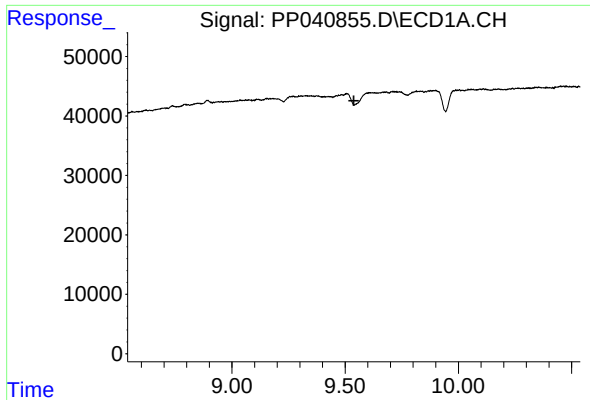

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 9.538 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

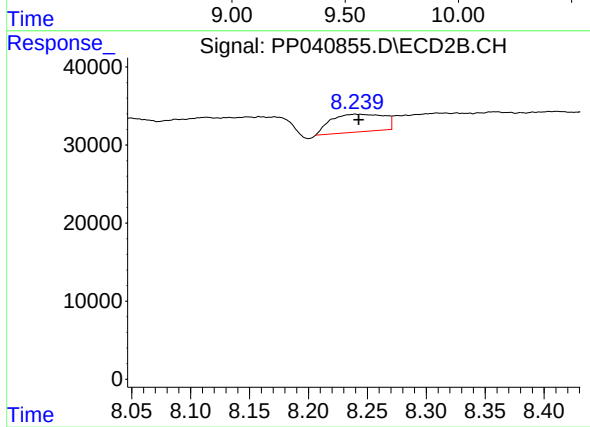

#43 AR-1268-3

R.T.: 8.240 min
Delta R.T.: -0.003 min
Response: 71372
Conc: 40.86 ng/ml