

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110921\
 Data File : PP040884.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Nov 2021 7:12
 Operator : AJ\MA
 Sample : M4544-03 20X
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MOO-2021-10C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 07:53:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 04 11:28:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.761	3.764	17306	27213	0.854	1.134m#
2) SA Decachlor...	10.666	9.032	25771	19812	1.210m	1.135m

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110921\
Data File : PP040884.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Nov 2021 7:12
Operator : AJ\MA
Sample : M4544-03 20X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MOO-2021-10C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 07:53:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 04 11:28:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

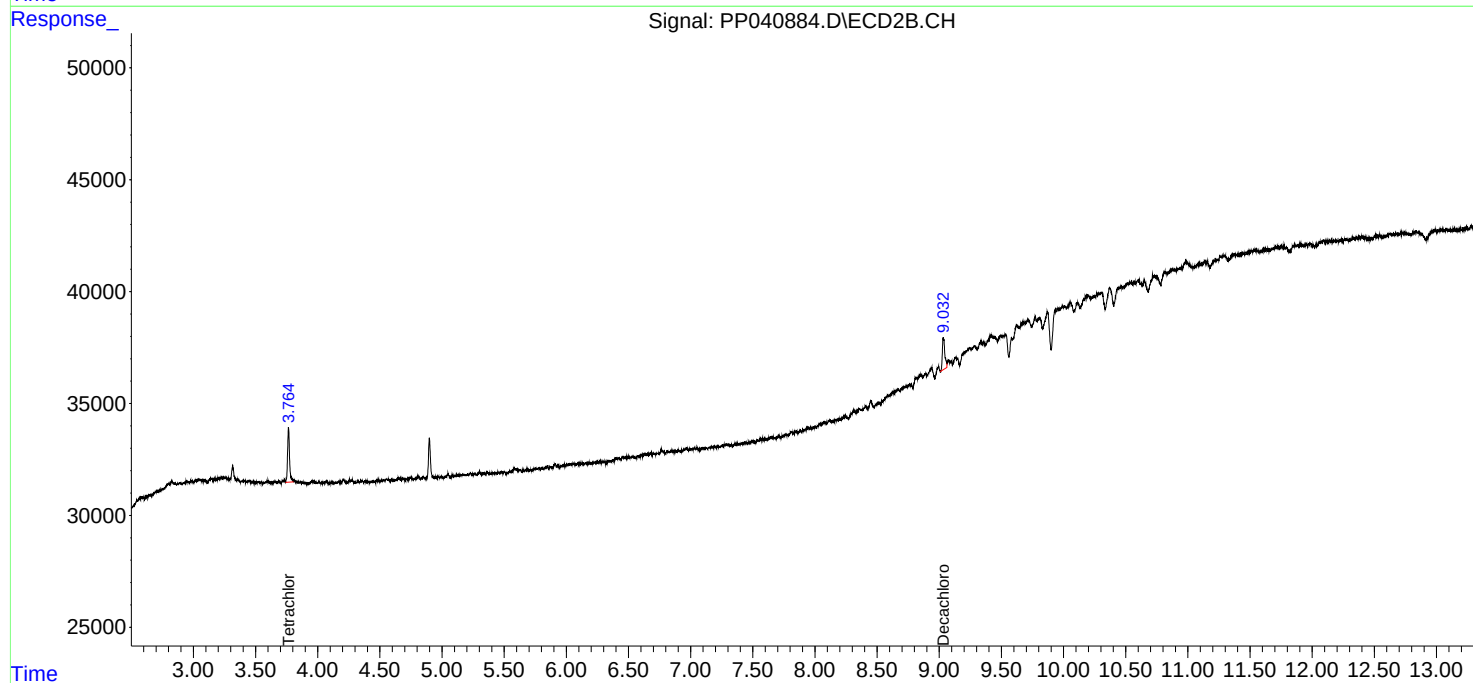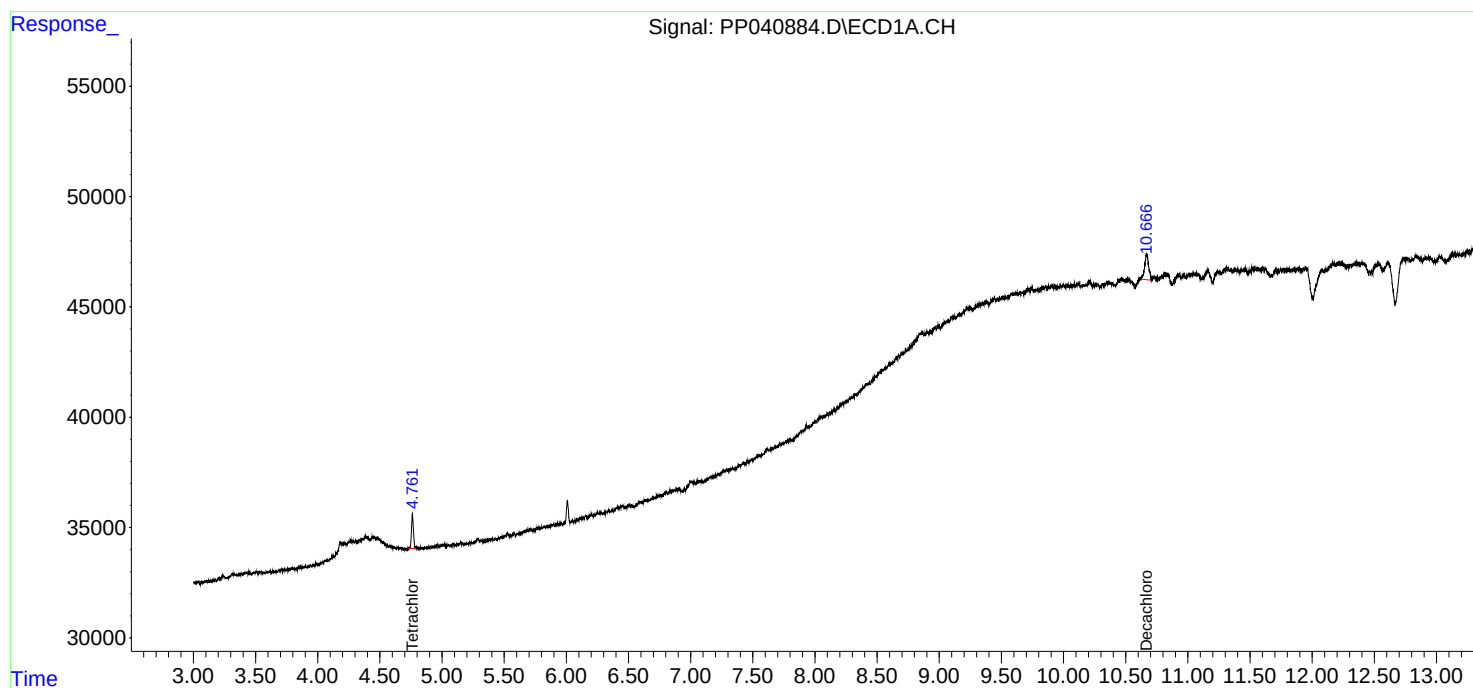


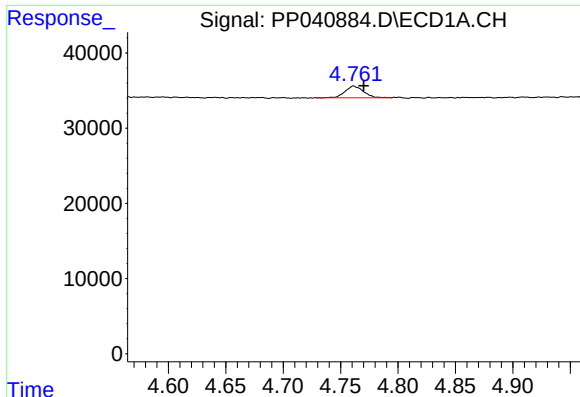

#1 Tetrachloro-m-xylene


R.T.: 4.761 min
Delta R.T.: -0.009 min
Response: 17306
Conc: 0.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2021-10C

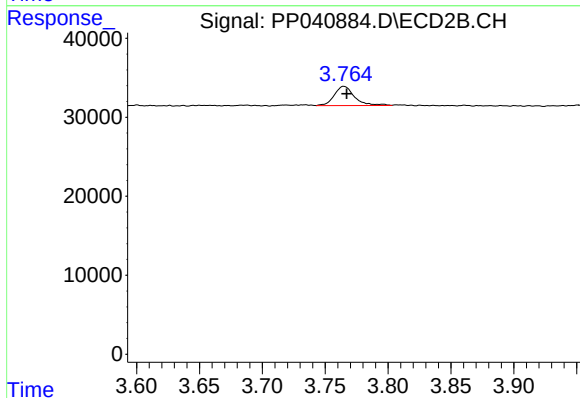


#1 Tetrachloro-m-xylene

R.T.: 3.764 min
Delta R.T.: -0.003 min
Response: 27213
Conc: 1.13 ng/ml m

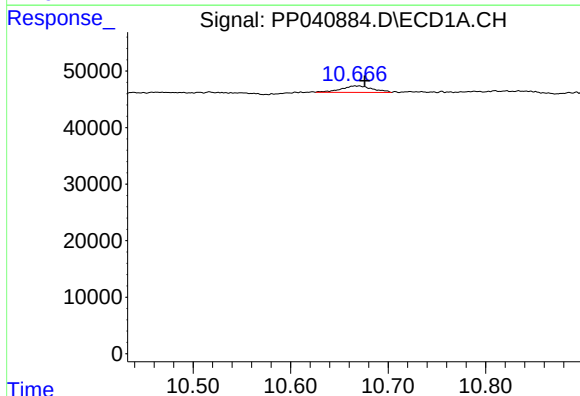

#2 Decachlorobiphenyl

R.T.: 10.666 min
Delta R.T.: -0.010 min
Response: 25771
Conc: 1.21 ng/ml m

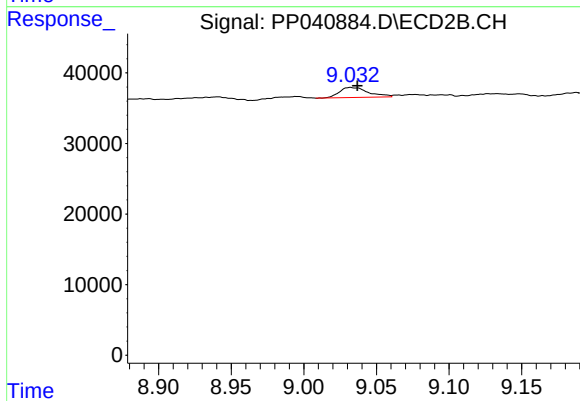

#2 Decachlorobiphenyl

R.T.: 9.032 min
Delta R.T.: -0.005 min
Response: 19812
Conc: 1.13 ng/ml m