

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110921\
 Data File : PP040886.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Nov 2021 7:45
 Operator : AJ\MA
 Sample : M4544-05 20X
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MOO-2021-11B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 07:54:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 04 11:28:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.764	3.765	8291	12731	0.409m	0.531m#
2) SA Decachlor...	10.669	9.038	14793	7264	0.695m	0.416 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110921\
Data File : PP040886.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Nov 2021 7:45
Operator : AJ\MA
Sample : M4544-05 20X
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MOO-2021-11B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 07:54:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 04 11:28:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

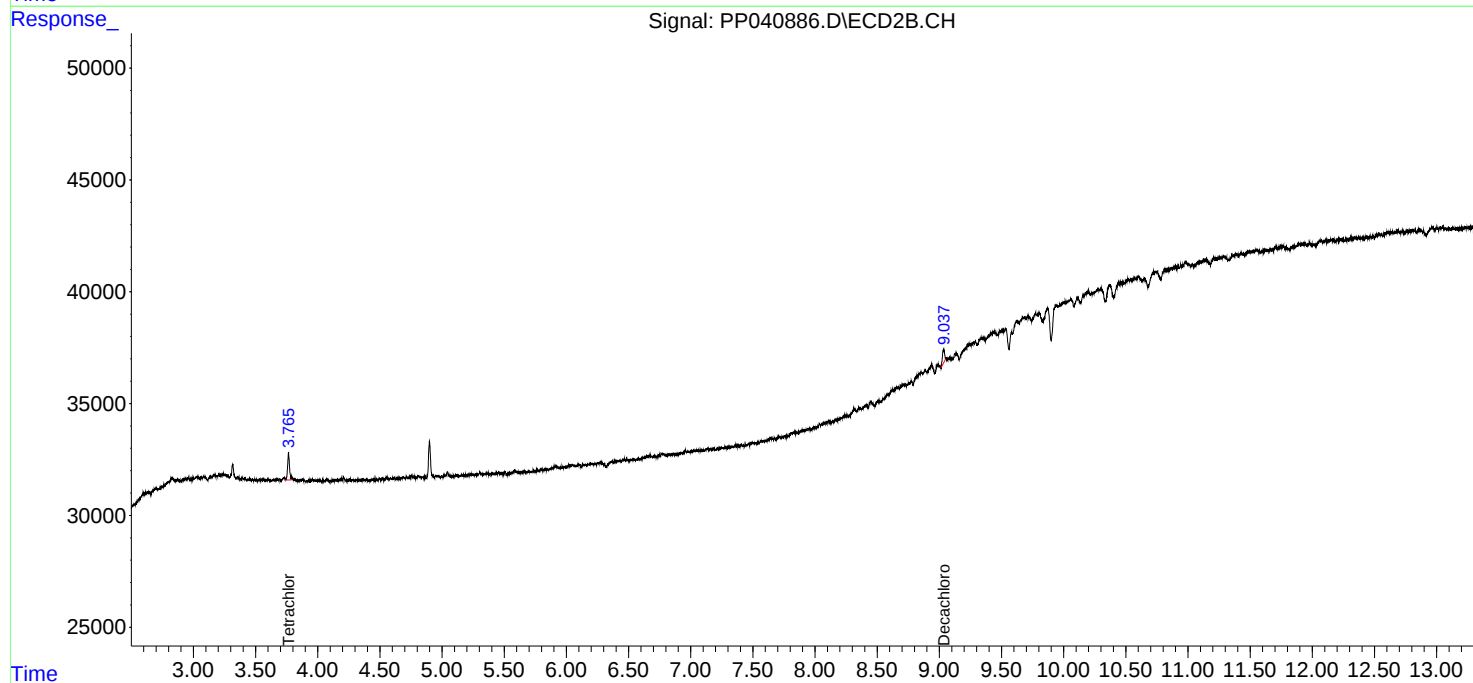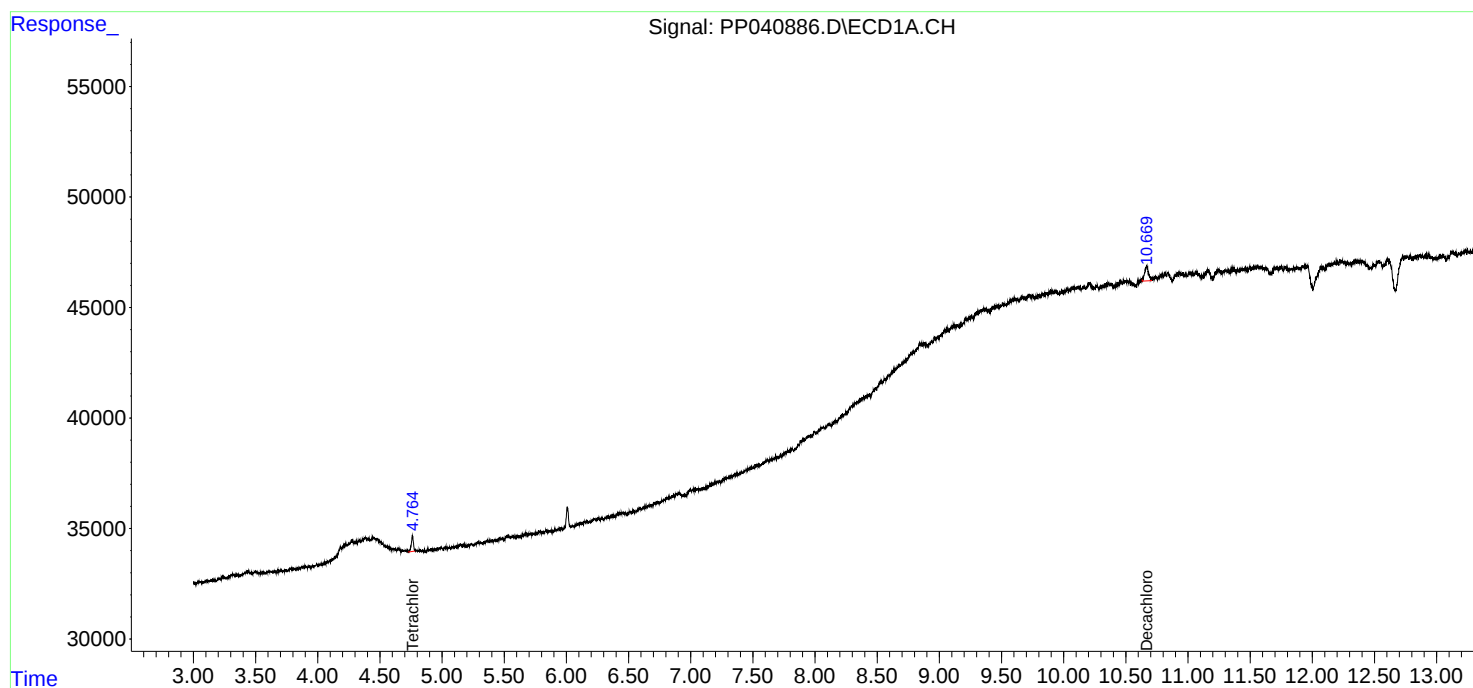


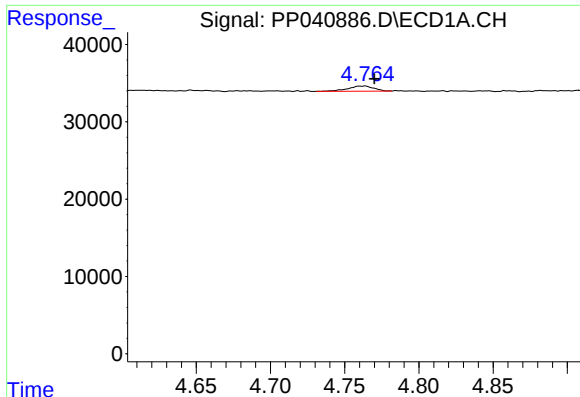

#1 Tetrachloro-m-xylene


R.T.: 4.764 min
Delta R.T.: -0.006 min
Response: 8291
Conc: 0.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2021-11B

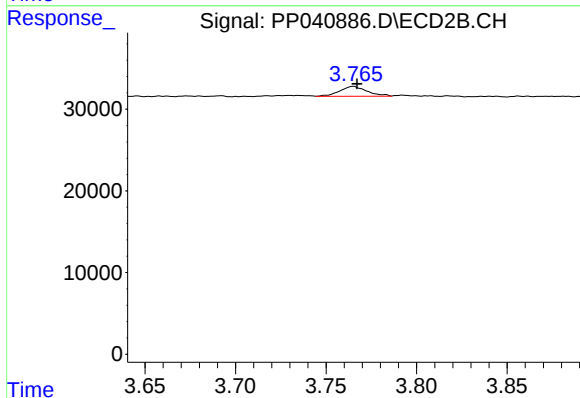


#1 Tetrachloro-m-xylene

R.T.: 3.765 min
Delta R.T.: -0.002 min
Response: 12731
Conc: 0.53 ng/ml m

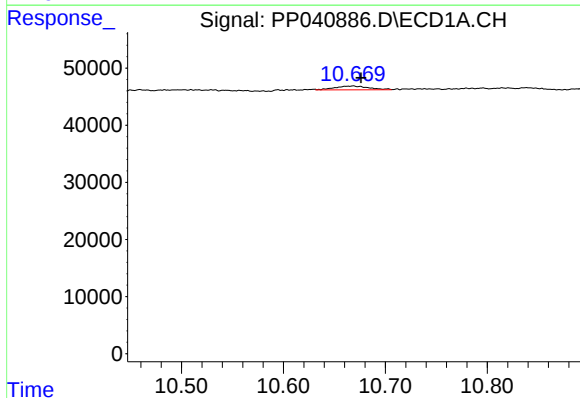

#2 Decachlorobiphenyl

R.T.: 10.669 min
Delta R.T.: -0.007 min
Response: 14793
Conc: 0.69 ng/ml m

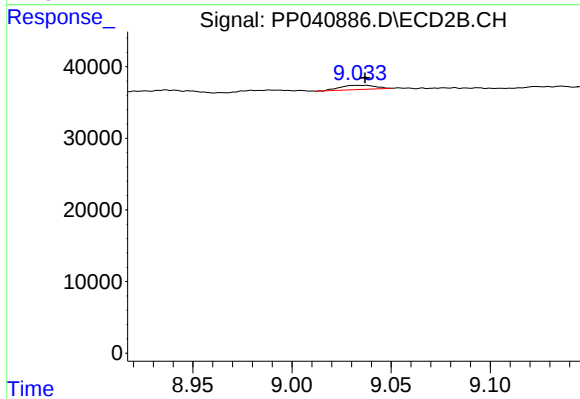

#2 Decachlorobiphenyl

R.T.: 9.038 min
Delta R.T.: 0.000 min
Response: 7264
Conc: 0.42 ng/ml