

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111020\
 Data File : PP031206.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Nov 2020 18:22
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 11 00:40:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 05 13:03:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
20)	L4	AR-1242-5	0.000	6.233f	0	38742 N.D. 38.916 #
25)	L5	AR-1248-5	0.000	6.233f	0	38742 N.D. 30.676 #
26)	L6	AR-1254-1	0.000	6.233f	0	38742 N.D. 19.699 #
28)	L6	AR-1254-3	0.000	6.770f	0	1095 N.D. 0.400 #
35)	L7	AR-1260-5	0.000	8.029f	0	627 N.D. 0.139 #
37)	L8	AR-1262-2	0.000	8.029f	0	627 N.D. 0.151 #
38)	L8	AR-1262-3	0.000	8.300	0	32850 N.D. 19.376 #
39)	L8	AR-1262-4	0.000	8.341f	0	899 N.D. 0.283 #
41)	L9	AR-1268-1	0.000	8.300	0	32850 N.D. 6.710 #
42)	L9	AR-1268-2	0.000	8.341f	0	899 N.D. 0.189 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111020\
Data File : PP031206.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Nov 2020 18:22
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 11 00:40:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110420.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 05 13:03:18 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

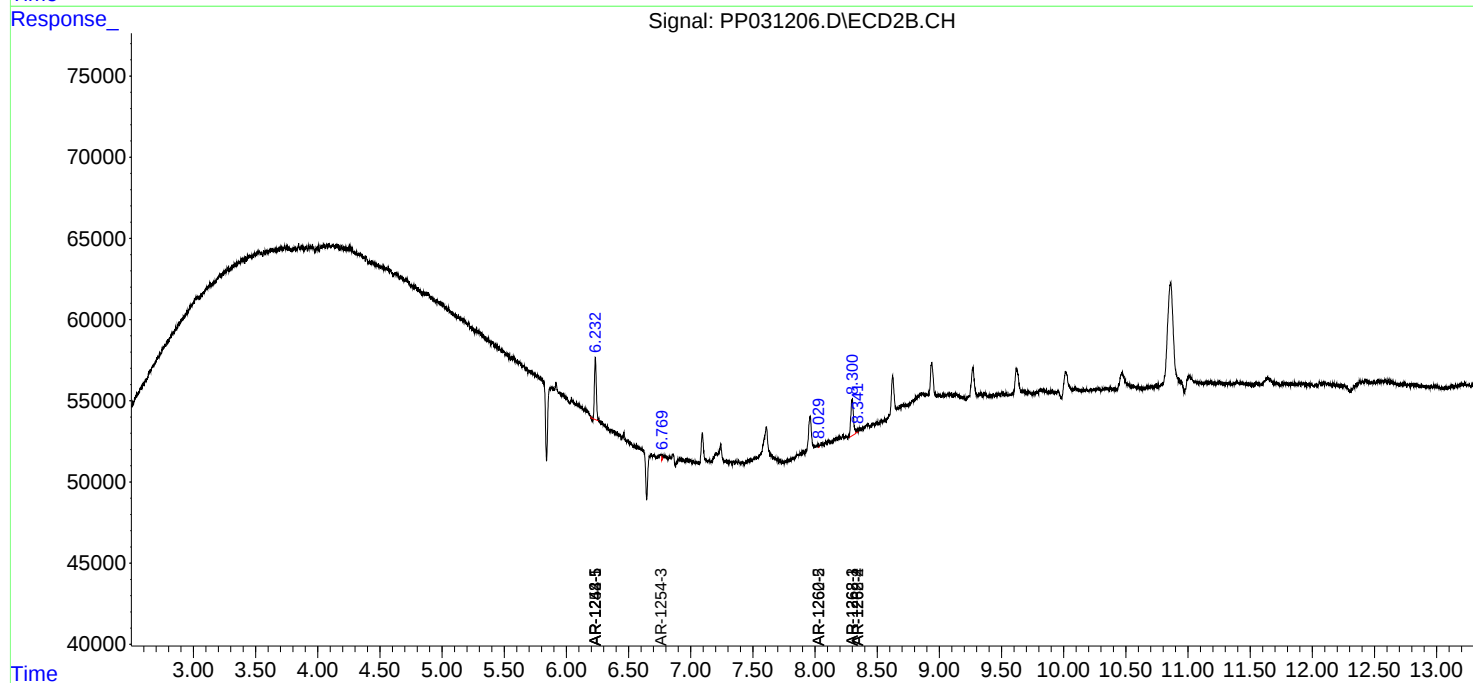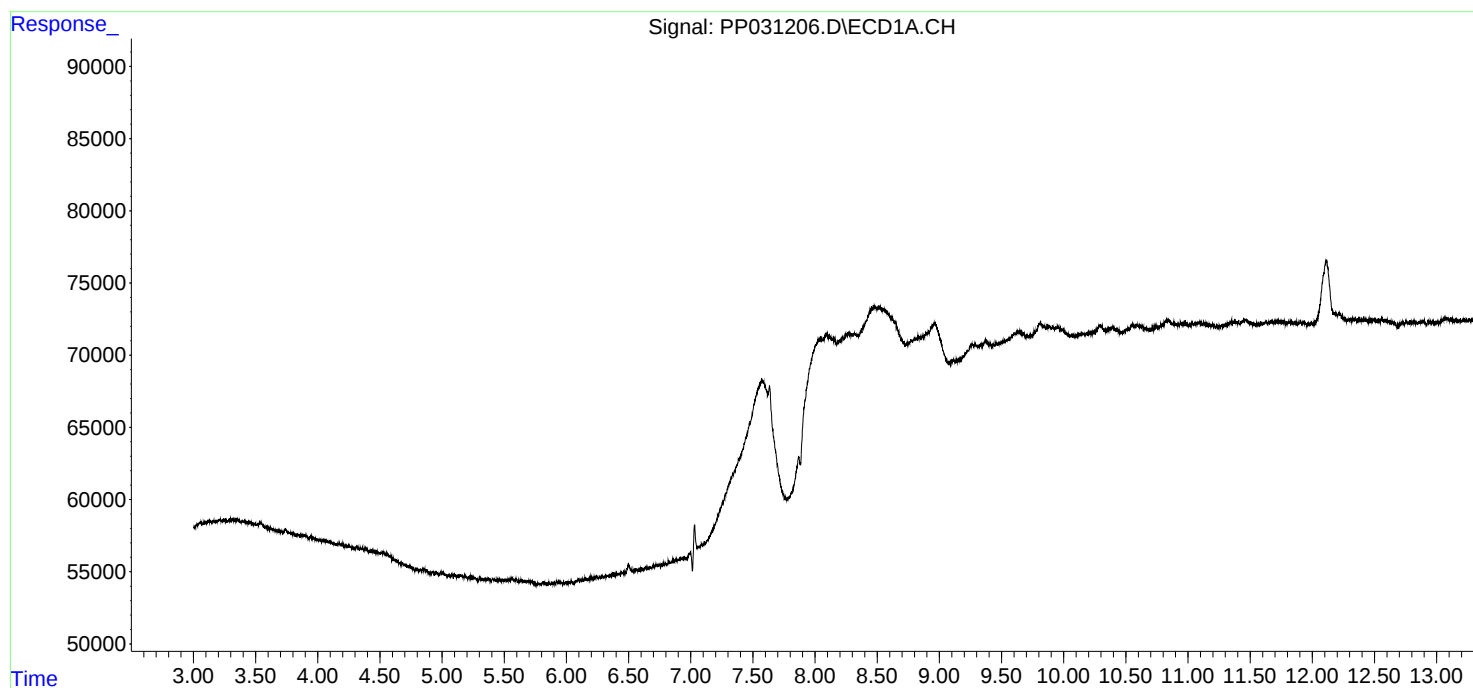


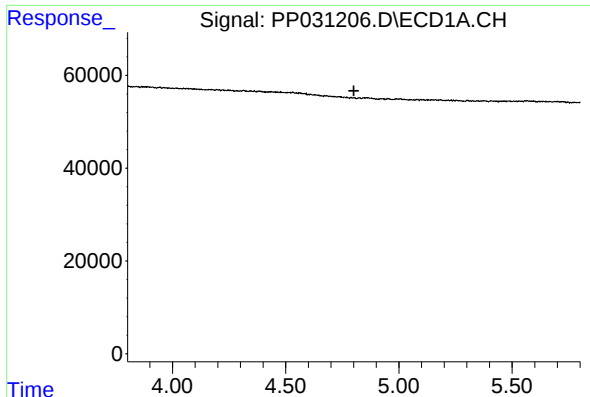

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.801 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

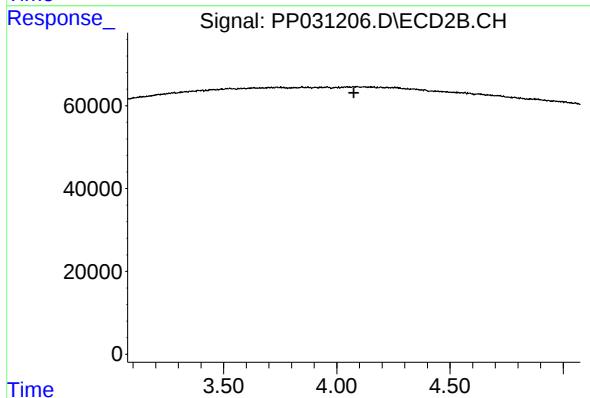


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.076 min
Response: 0
Conc: N.D.

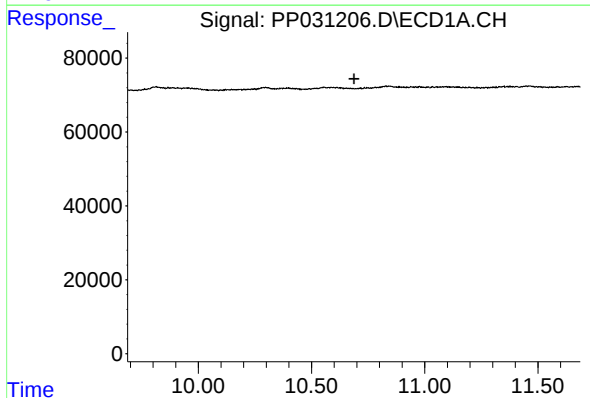


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.688 min
Response: 0
Conc: N.D.

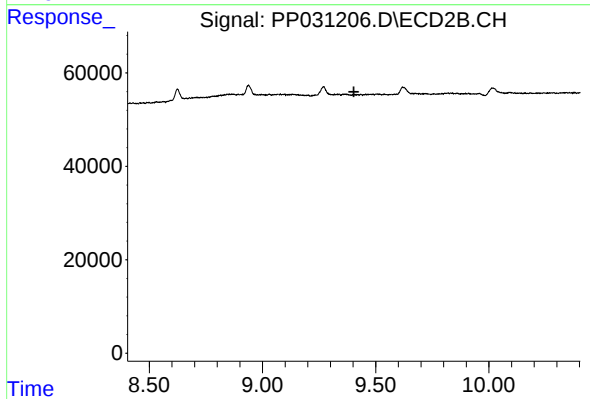

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 9.404 min
Response: 0
Conc: N.D.

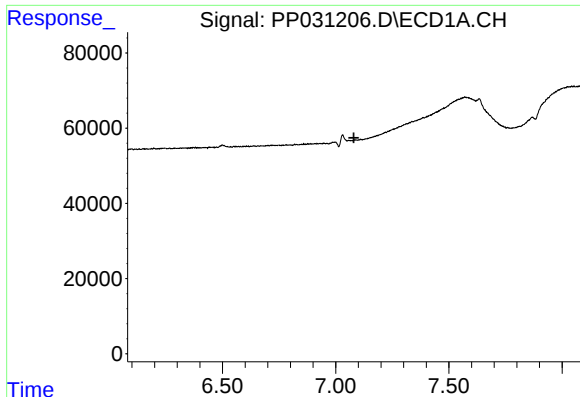

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 7.081 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

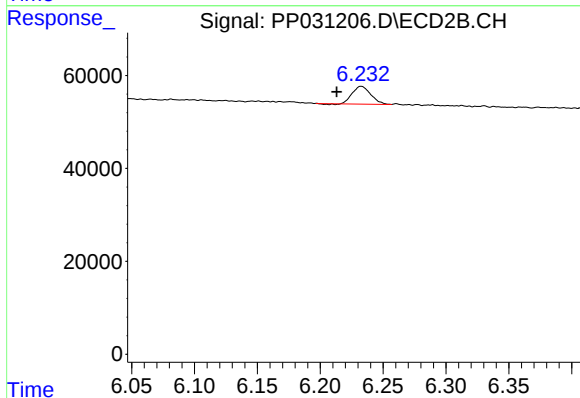


#20 AR-1242-5

R.T.: 6.233 min
Delta R.T.: 0.020 min
Response: 38742
Conc: 38.92 ng/ml

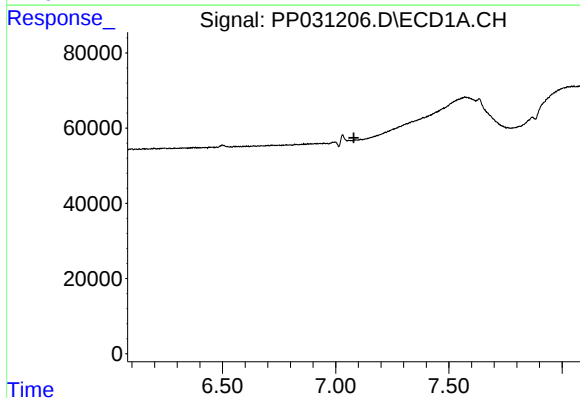


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 7.080 min
Response: 0
Conc: N.D.

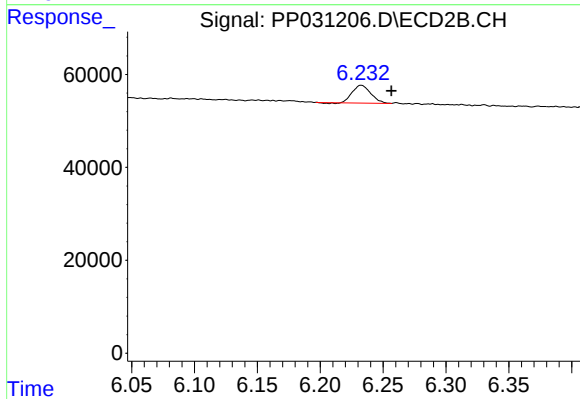

#25 AR-1248-5


R.T.: 6.233 min
Delta R.T.: -0.024 min
Response: 38742
Conc: 30.68 ng/ml

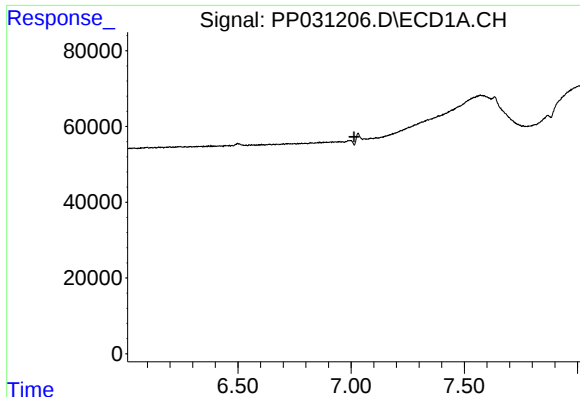

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T.: 7.013 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

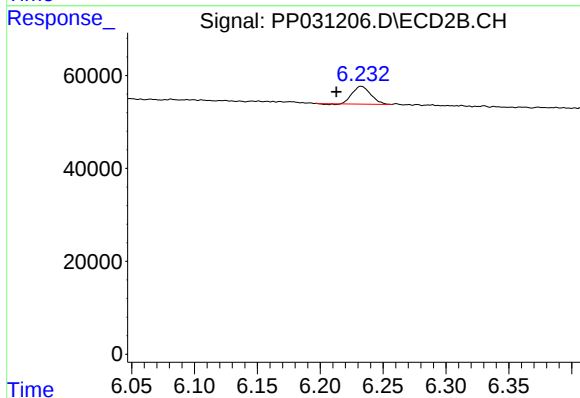


#26 AR-1254-1

R.T.: 6.233 min
Delta R.T.: 0.020 min
Response: 38742
Conc: 19.70 ng/ml

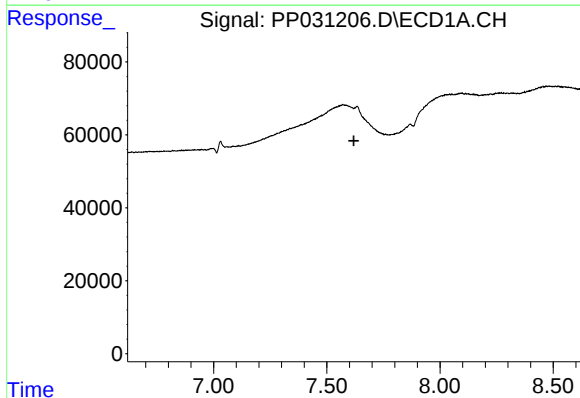


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T.: 7.620 min
Response: 0
Conc: N.D.

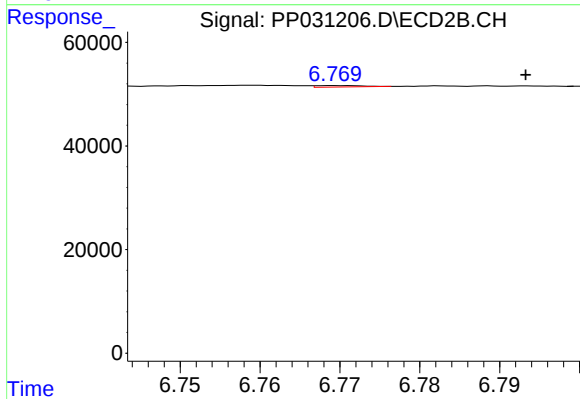

#28 AR-1254-3


R.T.: 6.770 min
Delta R.T.: -0.024 min
Response: 1095
Conc: 0.40 ng/ml

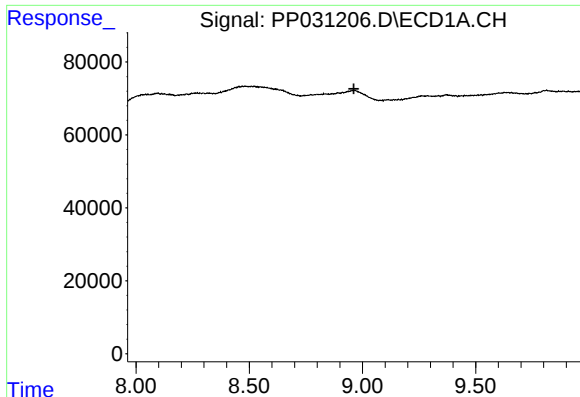

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 8.962 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

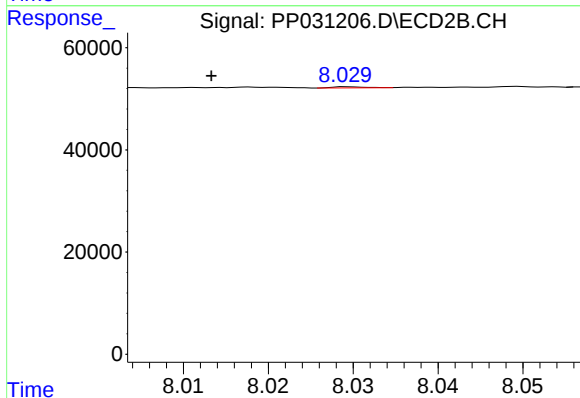


#35 AR-1260-5

R.T.: 8.029 min
Delta R.T.: 0.016 min
Response: 627
Conc: 0.14 ng/ml

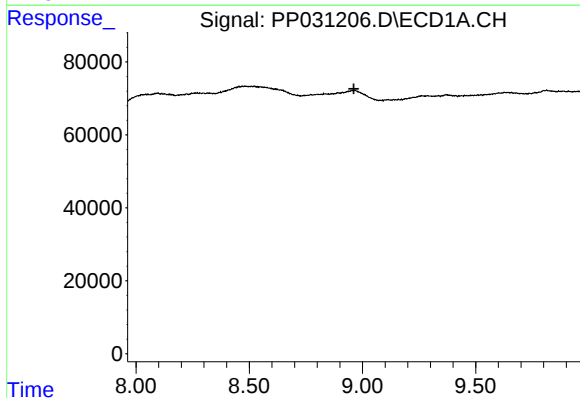


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 8.963 min
Response: 0
Conc: N.D.

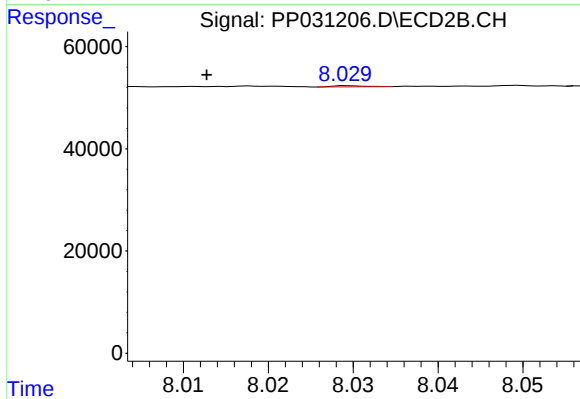

#37 AR-1262-2


R.T.: 8.029 min
Delta R.T.: 0.017 min
Response: 627
Conc: 0.15 ng/ml

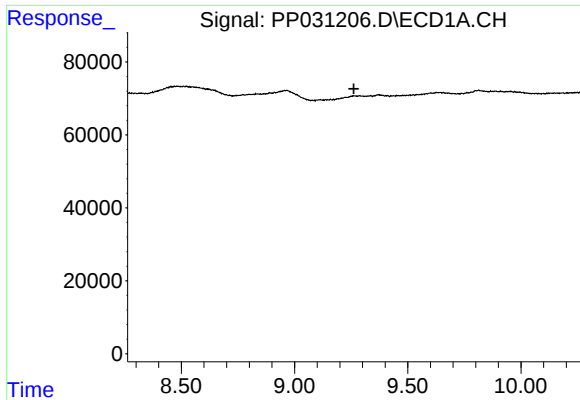

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 9.262 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

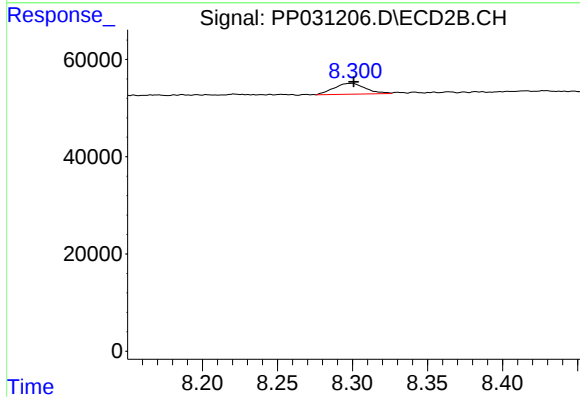


#38 AR-1262-3

R.T.: 8.300 min
Delta R.T.: 0.000 min
Response: 32850
Conc: 19.38 ng/ml

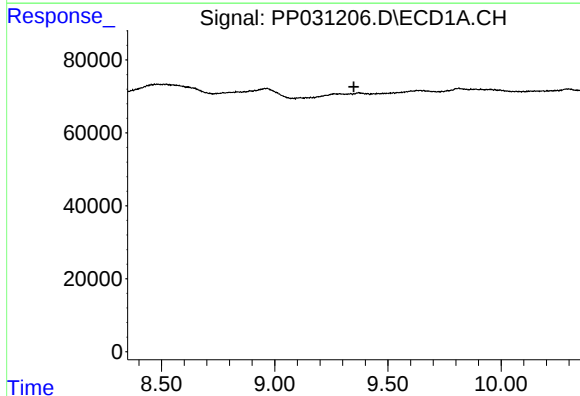


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T.: 9.350 min
Response: 0
Conc: N.D.

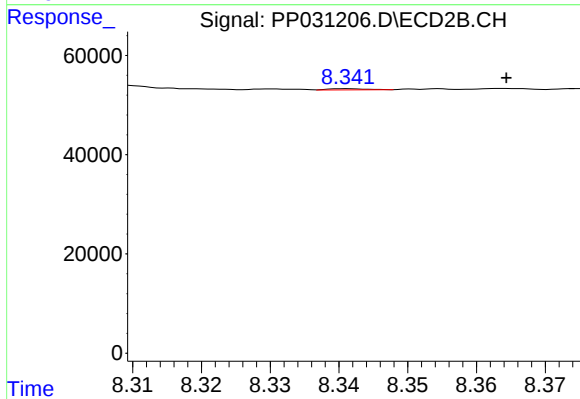

#39 AR-1262-4


R.T.: 8.341 min
Delta R.T.: -0.023 min
Response: 899
Conc: 0.28 ng/ml

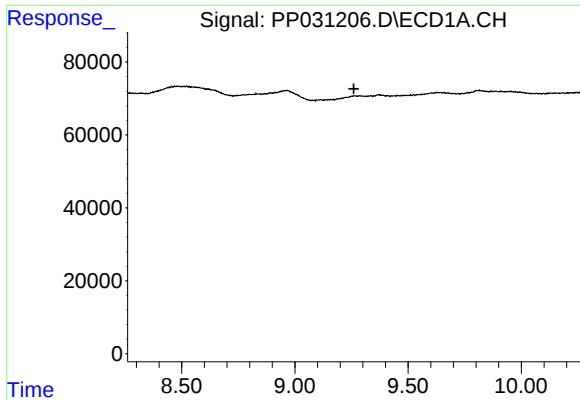

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 9.261 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

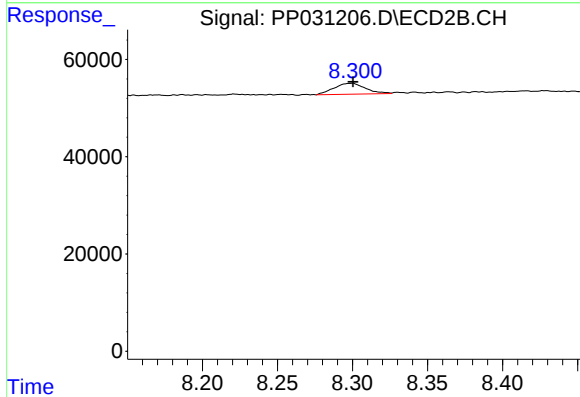


#41 AR-1268-1

R.T.: 8.300 min
Delta R.T.: 0.000 min
Response: 32850
Conc: 6.71 ng/ml

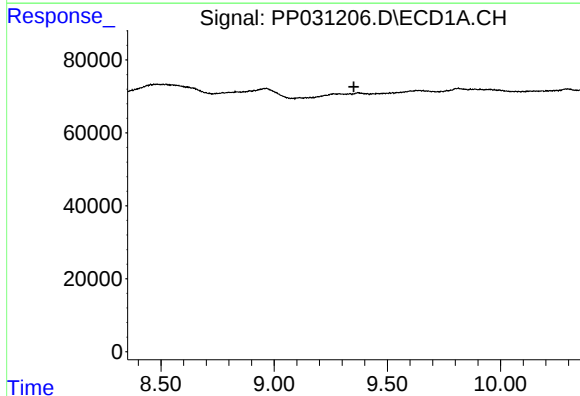

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 9.352 min
Response: 0
Conc: N.D.

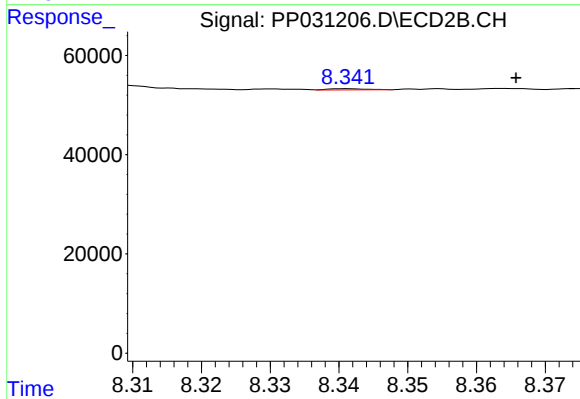

#42 AR-1268-2

R.T.: 8.341 min
Delta R.T.: -0.024 min
Response: 899
Conc: 0.19 ng/ml