

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111020\
 Data File : PP031214.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Nov 2020 20:53
 Operator : DD\AJ
 Sample : L4680-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PAV-B7-110520-0-10

Manual Integrations
 APPROVED

Ankita
 11/11/2020 9:01:06 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 11 00:43:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 05 13:03:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.797	4.071	1229876	1166140	18.414m	17.544m
2) SA Decachlor...	10.681	9.391	805423	838398	20.144	20.078

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111020\
Data File : PP031214.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Nov 2020 20:53
Operator : DD\AJ
Sample : L4680-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PAV-B7-110520-0-10


Manual Integrations
APPROVED

Ankita
11/11/2020 9:01:06 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 11 00:43:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110420.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 05 13:03:18 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

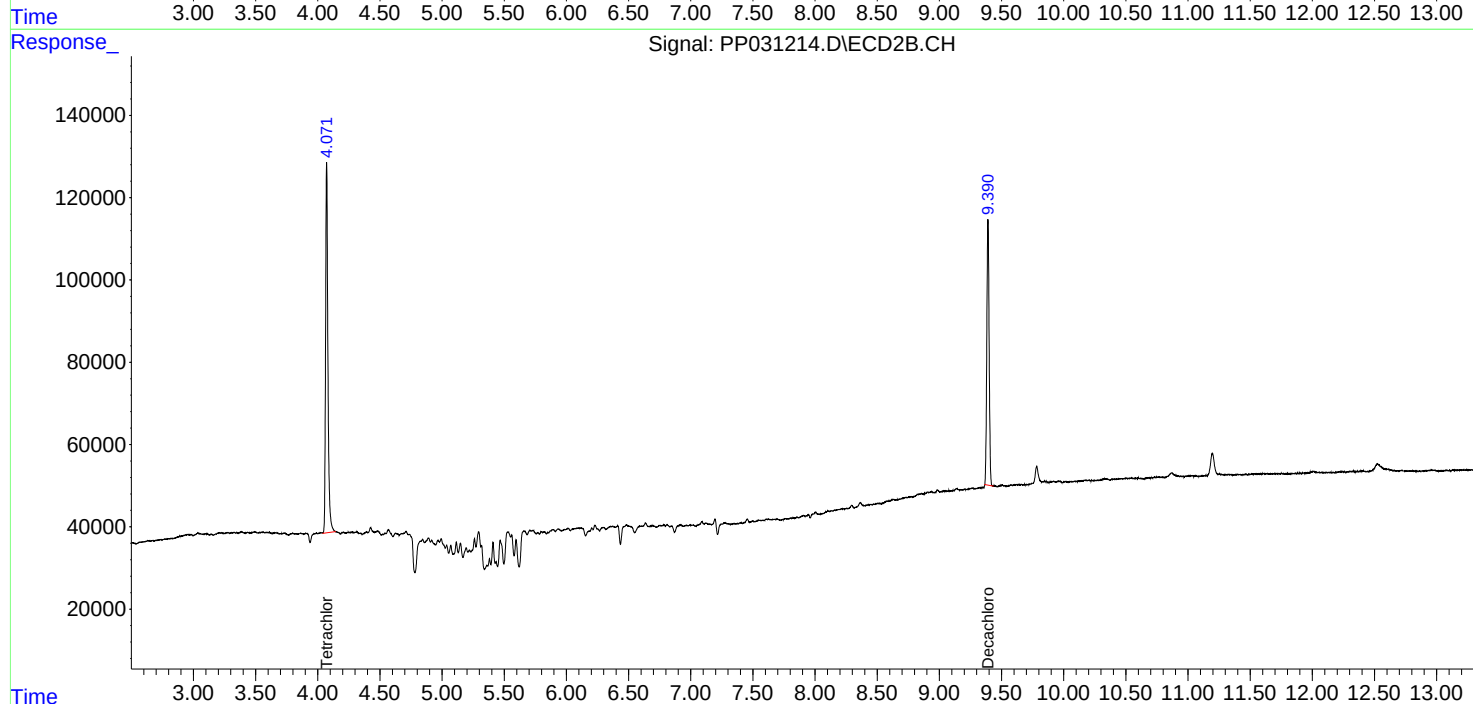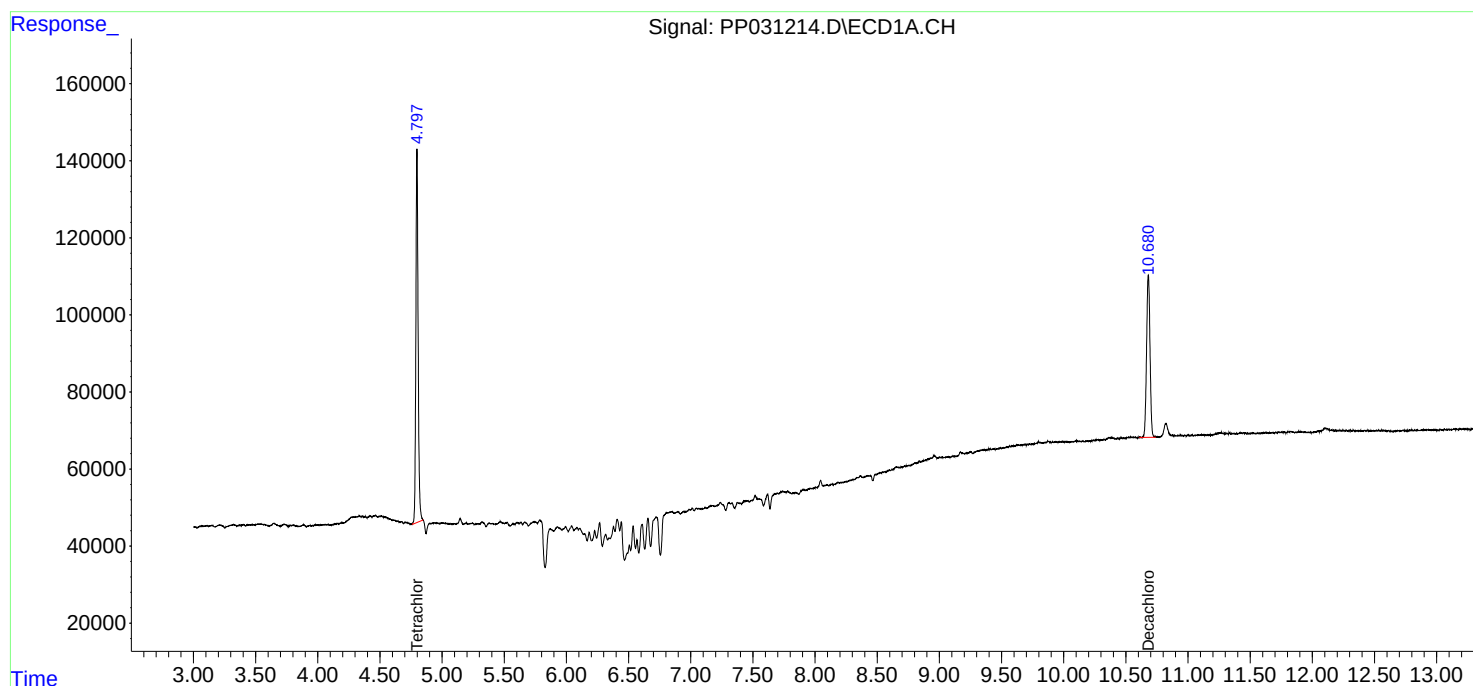

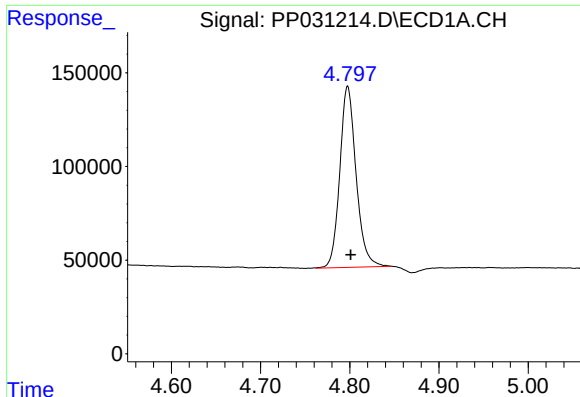


#1 Tetrachloro-m-xylene

R.T.: 4.797 min
Delta R.T.: -0.004 min
Response: 1229876
Conc: 18.41 ng/ml m

Instrument :
ECD_P
ClientSampleId :
PAV-B7-110520-0-10


Manual Integrations
APPROVED

Ankita
11/11/2020 9:01:06 AM

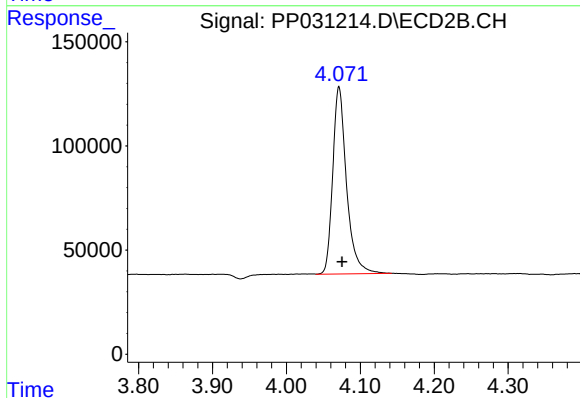


#1 Tetrachloro-m-xylene

R.T.: 4.071 min
Delta R.T.: -0.005 min
Response: 1166140
Conc: 17.54 ng/ml m

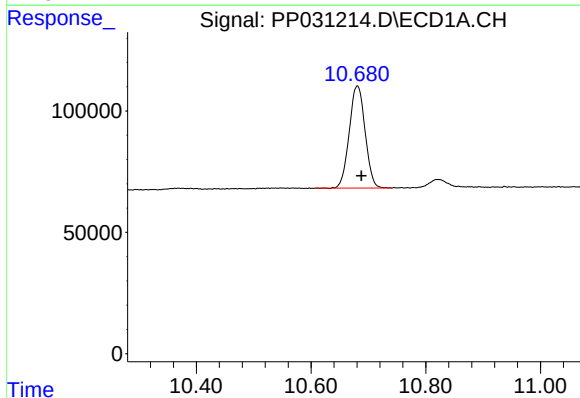

#2 Decachlorobiphenyl

R.T.: 10.681 min
Delta R.T.: -0.007 min
Response: 805423
Conc: 20.14 ng/ml

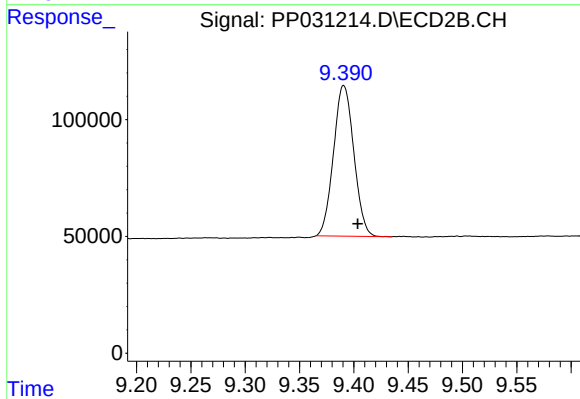

#2 Decachlorobiphenyl

R.T.: 9.391 min
Delta R.T.: -0.013 min
Response: 838398
Conc: 20.08 ng/ml