

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111020\
 Data File : PP031218.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Nov 2020 2:03
 Operator : DD\AJ
 Sample : L4680-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PAV-B7-110920-10-20

Manual Integrations
 APPROVED

Ankita
 11/11/2020 9:01:10 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 11 03:07:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 05 13:03:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.811	4.071	1132129	1004163	16.950	15.107m
2) SA Decachlor...	10.703f	9.397	648055	688125	16.208	16.480

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111020\
Data File : PP031218.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Nov 2020 2:03
Operator : DD\AJ
Sample : L4680-05
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PAV-B7-110920-10-20


Manual Integrations
APPROVED

Ankita
11/11/2020 9:01:10 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 11 03:07:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110420.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 05 13:03:18 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

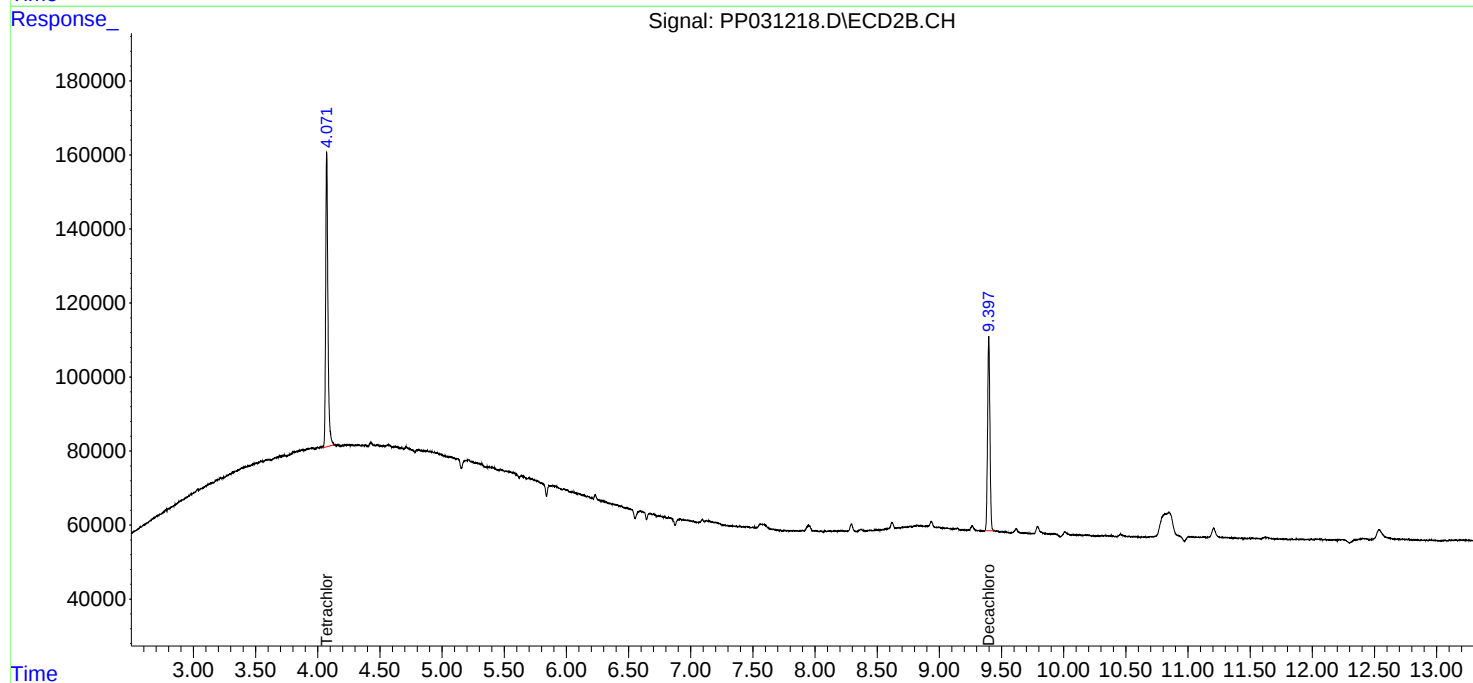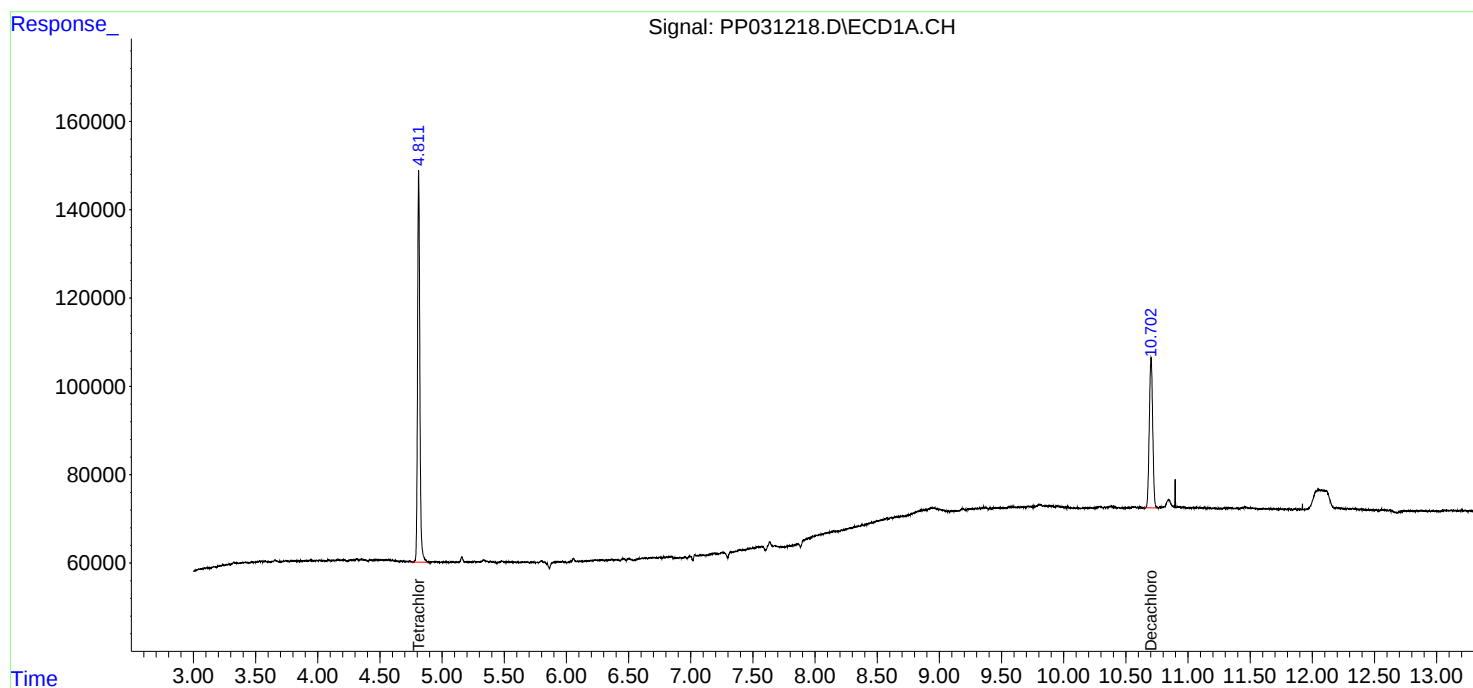

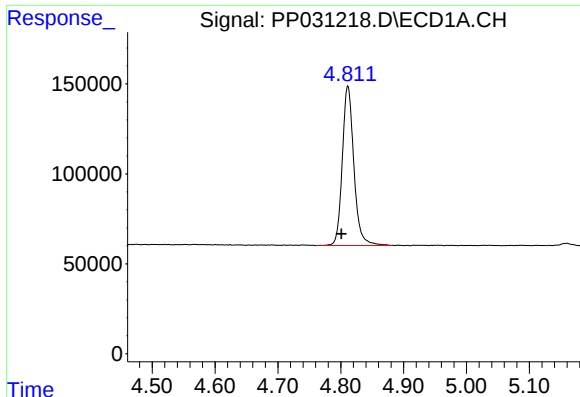


#1 Tetrachloro-m-xylene

R.T.: 4.811 min
Delta R.T.: 0.010 min
Response: 1132129
Conc: 16.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
PAV-B7-110920-10-20


Manual Integrations
APPROVED

Ankita
11/11/2020 9:01:10 AM

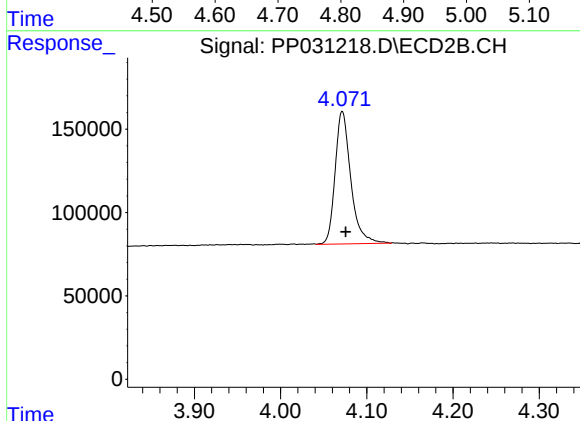


#1 Tetrachloro-m-xylene

R.T.: 4.071 min
Delta R.T.: -0.004 min
Response: 1004163
Conc: 15.11 ng/ml m

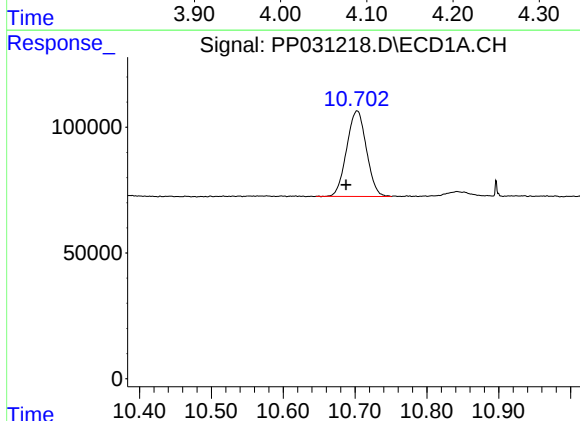

#2 Decachlorobiphenyl

R.T.: 10.703 min
Delta R.T.: 0.016 min
Response: 648055
Conc: 16.21 ng/ml

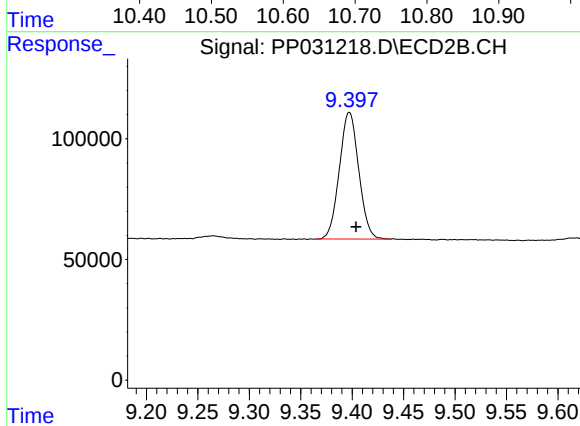

#2 Decachlorobiphenyl

R.T.: 9.397 min
Delta R.T.: -0.006 min
Response: 688125
Conc: 16.48 ng/ml