

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111021\
 Data File : PP040934.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Nov 2021 23:49
 Operator : AJ\MA
 Sample : M4588-07 10X
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 11 01:13:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 04 11:28:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.761	3.764	30110	48120	1.486	2.005 #
2) SA Decachlor...	10.664	9.031	29587	26895	1.389	1.540
Target Compounds						
29) L6 AR-1254-4	7.892	0.000	5484	0	5.620	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111021\
Data File : PP040934.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Nov 2021 23:49
Operator : AJ\MA
Sample : M4588-07 10X
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 11 01:13:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 04 11:28:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

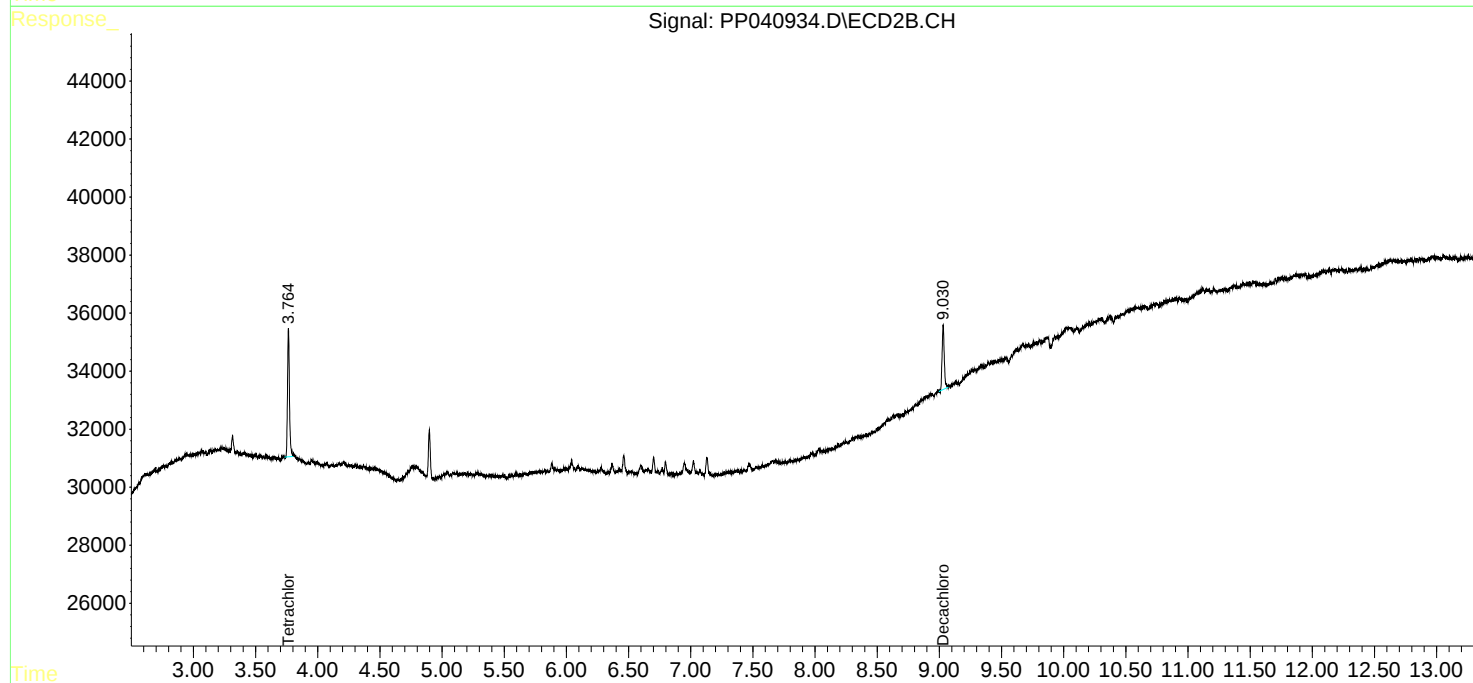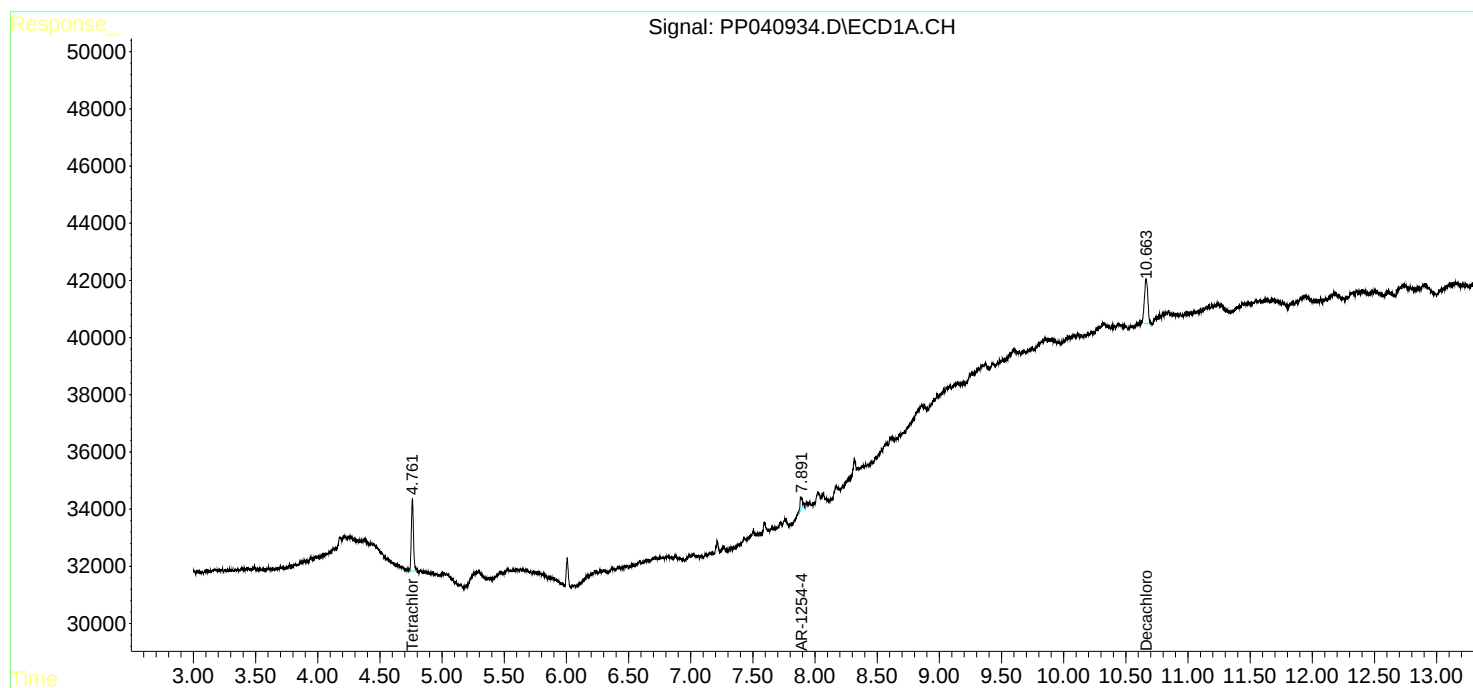


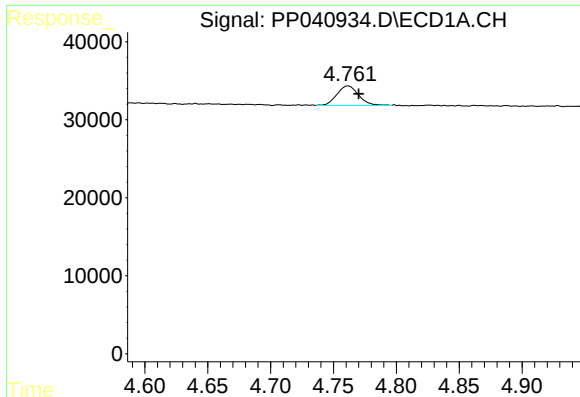

#1 Tetrachloro-m-xylene


R.T.: 4.761 min
Delta R.T.: -0.009 min
Response: 30110
Conc: 1.49 ng/ml

Instrument :
ECD_P
ClientSampleId :

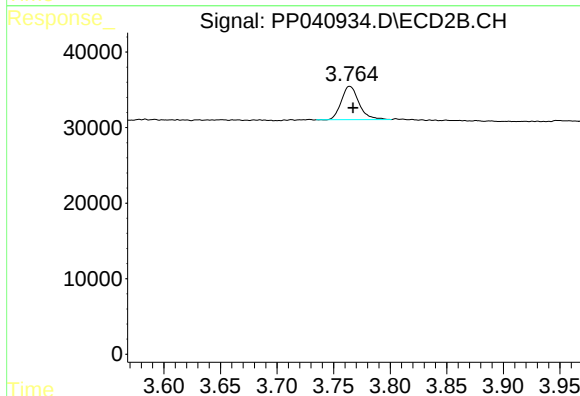


#1 Tetrachloro-m-xylene

R.T.: 3.764 min
Delta R.T.: -0.003 min
Response: 48120
Conc: 2.01 ng/ml

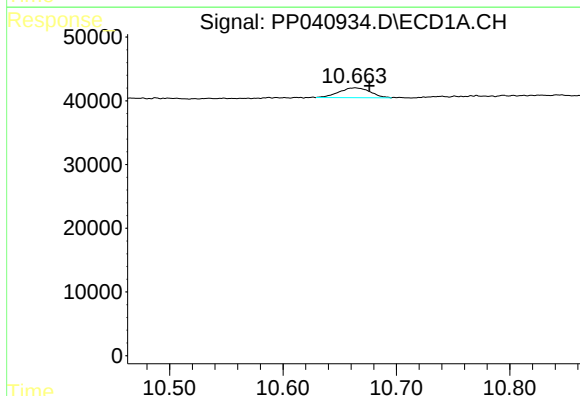


#2 Decachlorobiphenyl

R.T.: 10.664 min
Delta R.T.: -0.012 min
Response: 29587
Conc: 1.39 ng/ml

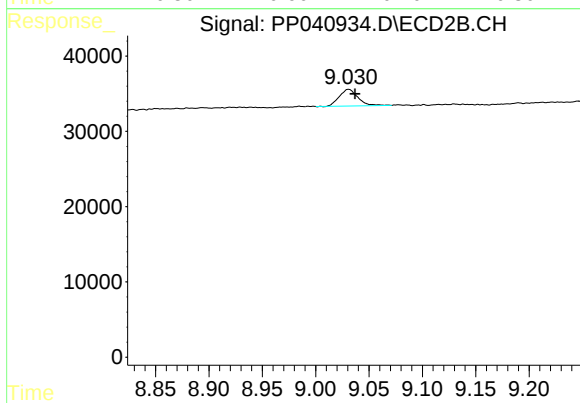

#2 Decachlorobiphenyl


R.T.: 9.031 min
Delta R.T.: -0.006 min
Response: 26895
Conc: 1.54 ng/ml

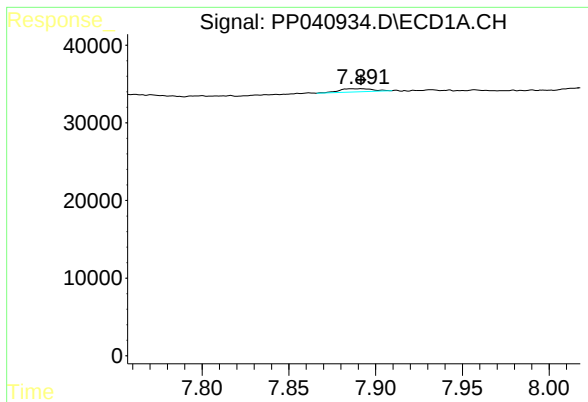

#29 AR-1254-4

R.T.: 7.892 min
Delta R.T.: 0.000 min
Response: 5484
Conc: 5.62 ng/ml

Instrument :
ECD_P
ClientSampleId :

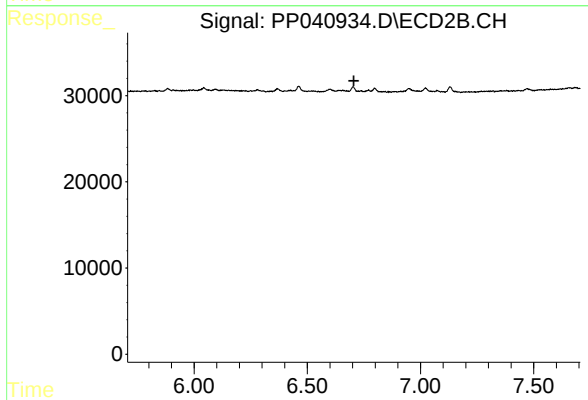

#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.706 min
Response: 0
Conc: N.D.